
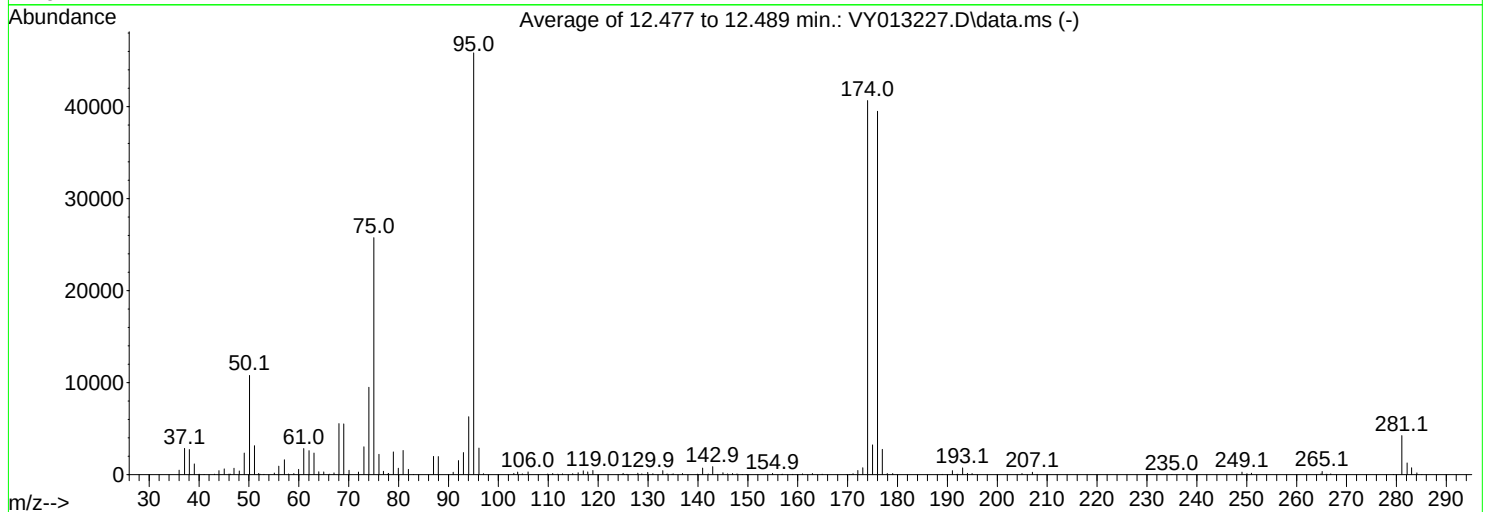


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041123\
Data File : VY013227.D
Acq On : 10 Apr 2023 14:10
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041123S.M
Title : SW846 8260
Last Update : Tue Apr 11 11:59:49 2023

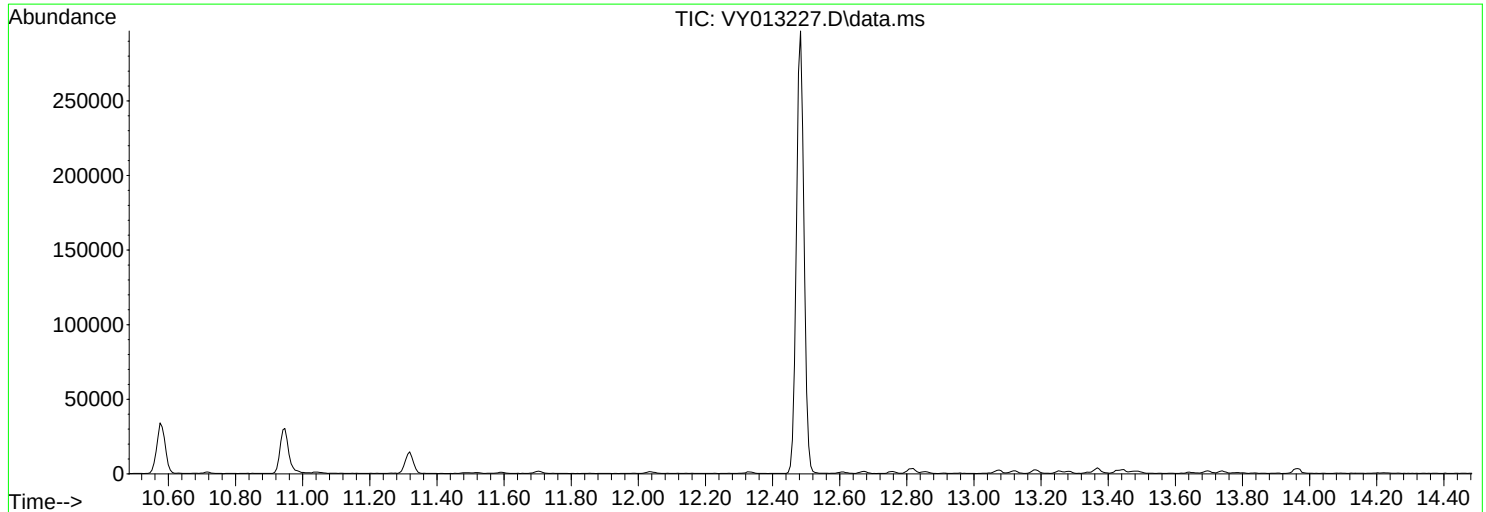

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	10784	PASS
75	95	30	60	56.2	25765	PASS
95	95	100	100	100.0	45848	PASS
96	95	5	9	6.3	2890	PASS
173	174	0.00	2	1.8	745	PASS
174	95	50	100	88.7	40664	PASS
175	174	5	9	7.9	3232	PASS
176	174	95	101	97.1	39491	PASS
177	176	5	9	7.0	2753	PASS