
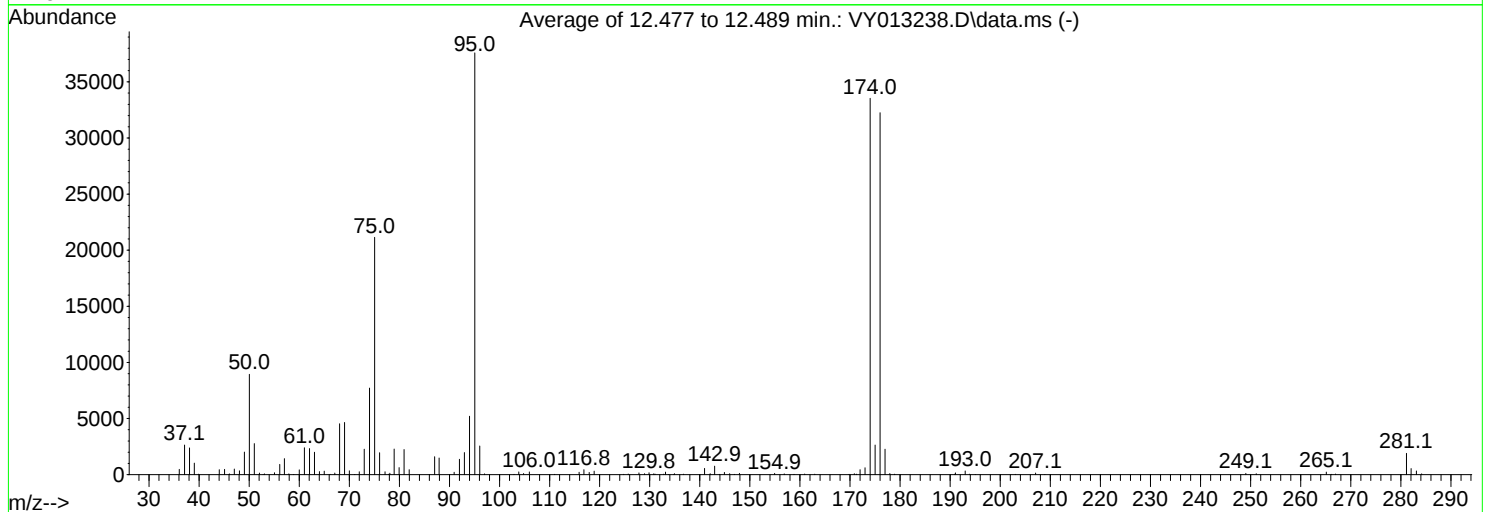


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041123\
 Data File : VY013238.D
 Acq On : 11 Apr 2023 09:59
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041123S.M
 Title : SW846 8260
 Last Update : Tue Apr 11 11:59:49 2023

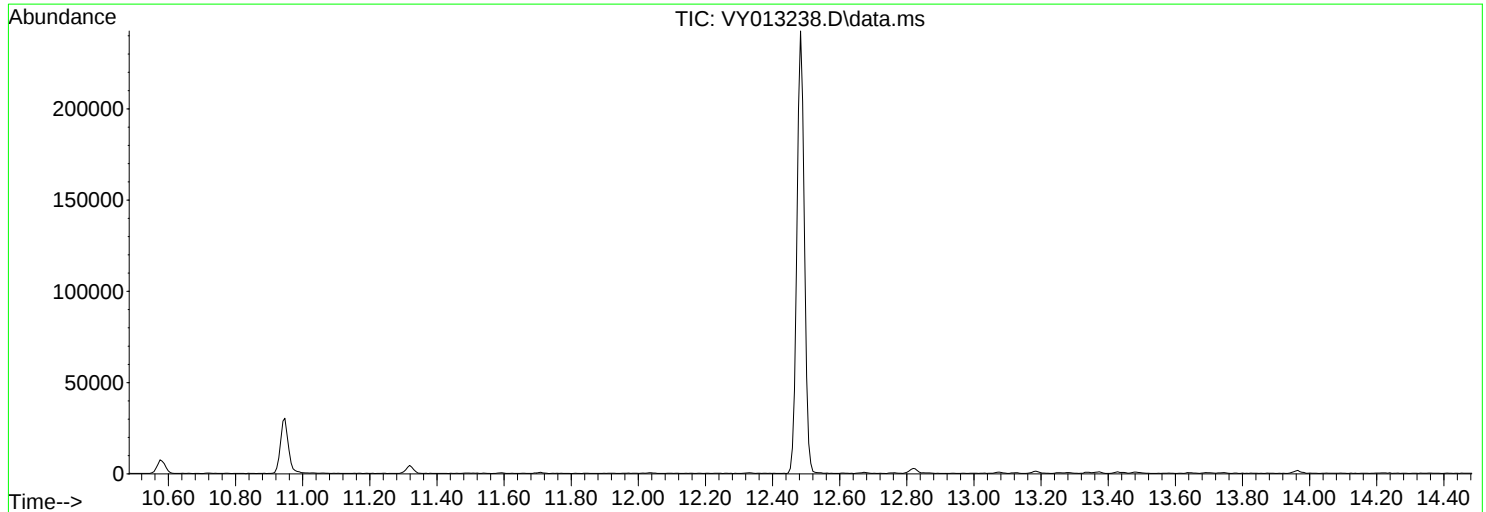

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	8947	PASS
75	95	30	60	56.2	21139	PASS
95	95	100	100	100.0	37587	PASS
96	95	5	9	6.8	2546	PASS
173	174	0.00	2	1.8	608	PASS
174	95	50	100	89.2	33533	PASS
175	174	5	9	7.9	2643	PASS
176	174	95	101	96.2	32251	PASS
177	176	5	9	7.0	2268	PASS