


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041125\
Data File : VY021849.D
Acq On : 11 Apr 2025 08:46
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Title : SW846 8260
Last Update : Fri Mar 28 02:30:29 2025

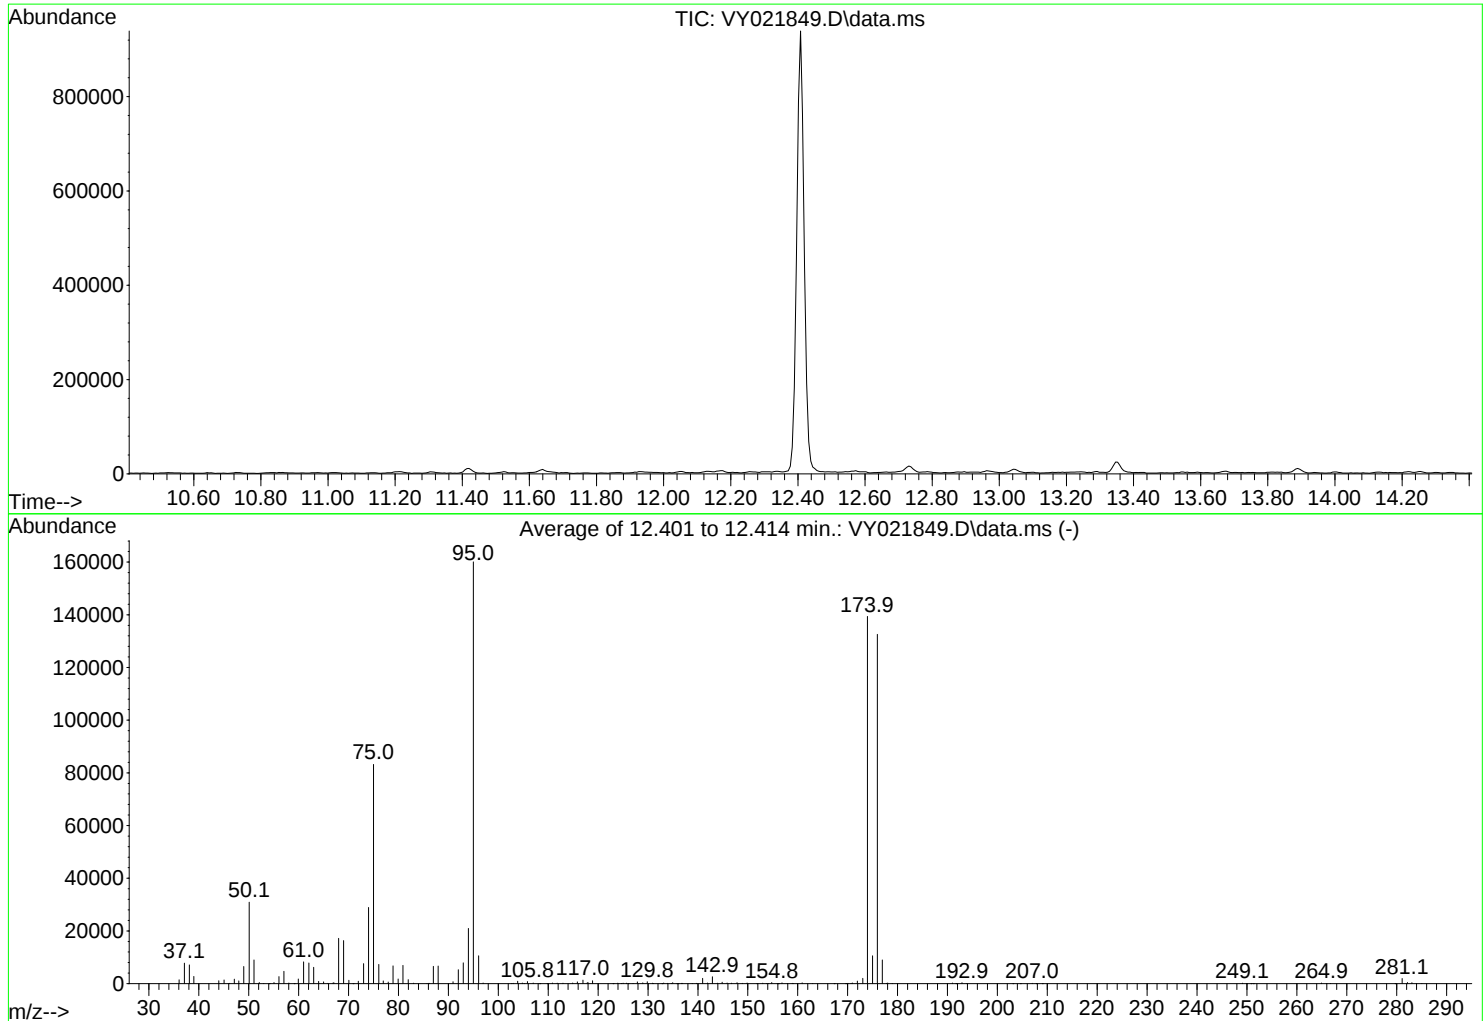

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	30925	PASS
75	95	30	60	52.0	83200	PASS
95	95	100	100	100.0	160096	PASS
96	95	5	9	6.6	10593	PASS
173	174	0.00	2	1.4	1977	PASS
174	95	50	100	87.0	139347	PASS
175	174	5	9	7.6	10569	PASS
176	174	95	101	95.1	132568	PASS
177	176	5	9	6.8	8980	PASS