

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041222\
 Data File : VY008292.D
 Acq On : 12 Apr 2022 16:56
 Operator : KP/MD
 Sample : N2364-01
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-01-14.5-15.0

Quant Time: Apr 13 08:14:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 08 16:02:50 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	7371	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	14212	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	14787	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	6633	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	5170	74.670	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 149.340%	
35) Dibromofluoromethane	7.716	113	4765	58.049	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 116.100%	
50) Toluene-d8	10.179	98	17027	60.620	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 121.240%	
62) 4-Bromofluorobenzene	12.483	95	6264	59.292	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 118.580%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.113	50	120	Below Cal	#	44
5) Bromomethane	2.656	94	266	Below Cal	#	62
10) Methyl Iodide	4.094	142	222	4.722	ug/l #	35
16) Acetone	3.930	43	42	2.522	ug/l #	47
20) Methylene Chloride	4.698	84	120	Below Cal	#	61
36) 1,1-Dichloropropene	7.789	75	446	3.403	ug/l #	42
38) Carbon Tetrachloride	7.789	117	837	5.935	ug/l #	11
48) Methyl methacrylate	9.264	41	123	2.307	ug/l #	77
51) 4-Methyl-2-Pentanone	10.093	43	242	3.736	ug/l #	40
55) 1,1,2-Trichloroethane	10.666	97	136	1.511	ug/l #	15
56) Ethyl methacrylate	10.496	69	184	1.667	ug/l #	39
58) 2-Chloroethyl Vinyl ether	9.715	63	89	2.047	ug/l	98
59) 2-Hexanone	10.843	43	76	1.705	ug/l #	28
60) Dibromochloromethane	10.746	129	114	1.084	ug/l	86
61) 1,2-Dibromoethane	11.087	107	101	1.147	ug/l #	52
66) 1,1,1,2-Tetrachloroethane	11.605	131	406	3.393	ug/l #	28
71) Bromoform	12.227	173	124	1.719	ug/l #	28
74) N-amyl acetate	12.123	43	428	3.998	ug/l #	53
75) 1,1,2,2-Tetrachloroethane	12.593	83	116	1.112	ug/l #	1
76) 1,2,3-Trichloropropane	12.483	75	3553	48.433	ug/l #	100
77) Bromobenzene	12.404	156	9135	75.592	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.373	75	110	3.355	ug/l #	69
82) 4-Chlorotoluene	12.843	91	372	1.108	ug/l #	66
84) 1,2,4-Trimethylbenzene	13.117	105	1283	3.206	ug/l #	31
85) sec-Butylbenzene	13.251	105	1420	2.640	ug/l	92
86) p-Isopropyltoluene	13.599	119	1139	2.538	ug/l	90
89) n-Butylbenzene	13.684	91	936	2.308	ug/l #	40
90) Hexachloroethane	13.971	117	329	3.922	ug/l #	6


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041222\
Data File : VY008292.D
Acq On : 12 Apr 2022 16:56
Operator : KP/MD
Sample : N2364-01
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0

Quant Time: Apr 13 08:14:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
Quant Title : SW846 8260
QLast Update : Fri Apr 08 16:02:50 2022
Response via : Initial Calibration




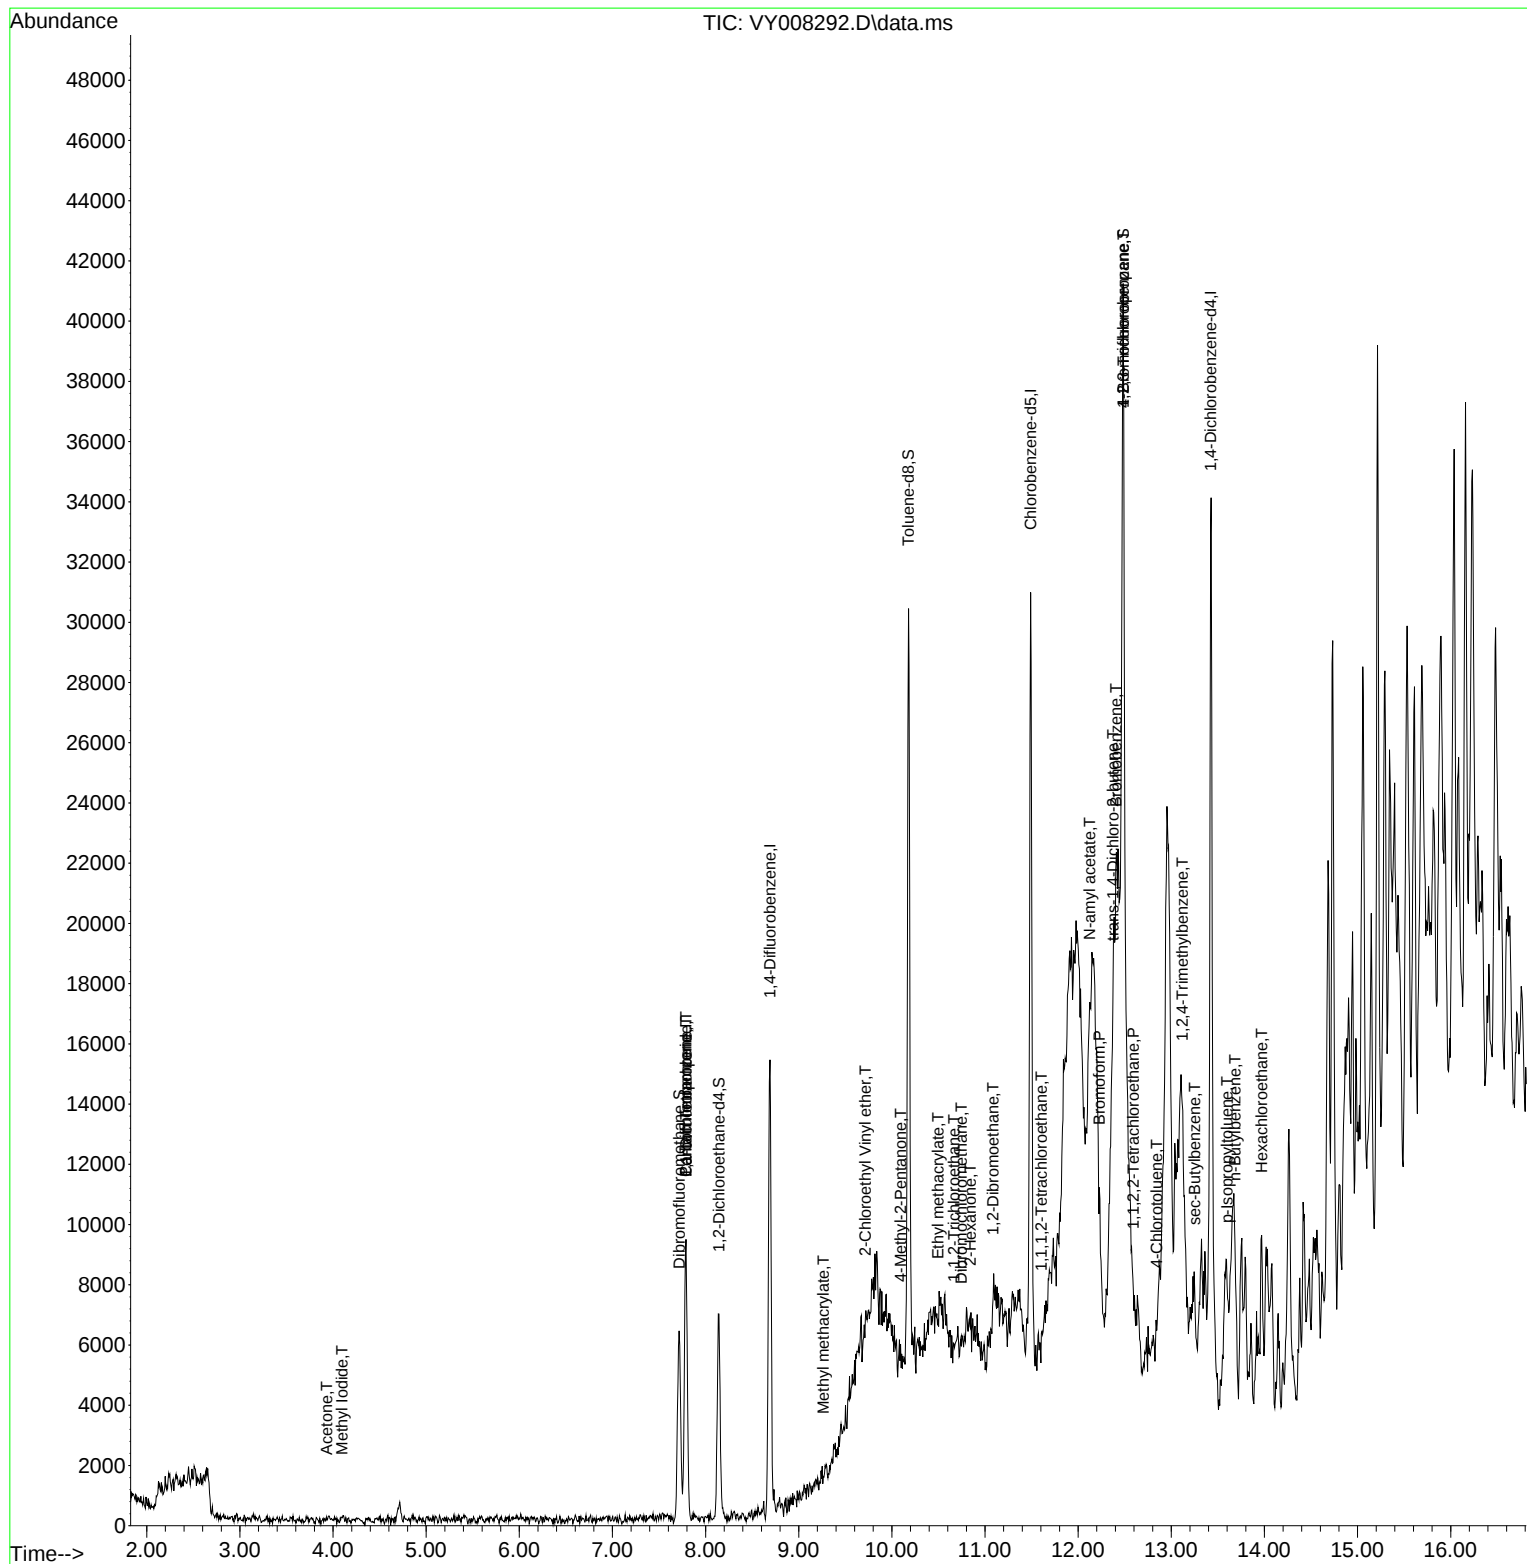




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0


Tgt Ion:168 Resp: 7371
Ion Ratio Lower Upper
168 100
99 64.2 46.9 70.3

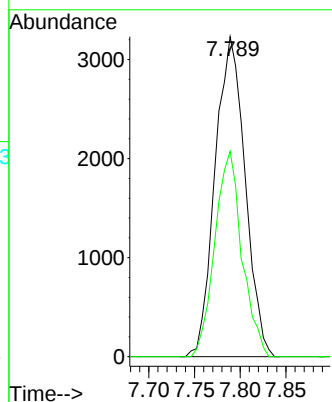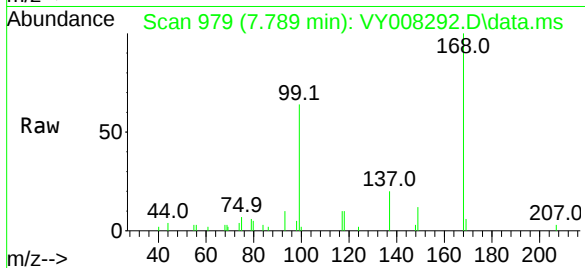

#3
Chloromethane
Concen: Below Cal
RT: 2.113 min Scan# 48
Delta R.T. 0.000 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Tgt Ion: 50 Resp: 120
Ion Ratio Lower Upper
50 100
52 0.0 24.6 37.0#


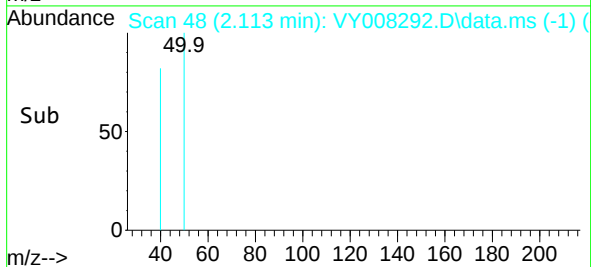
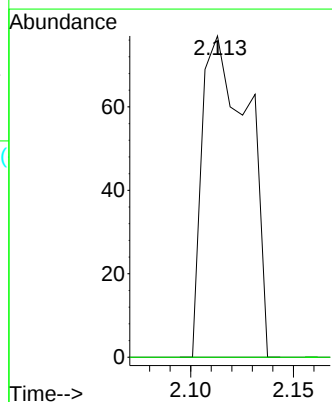
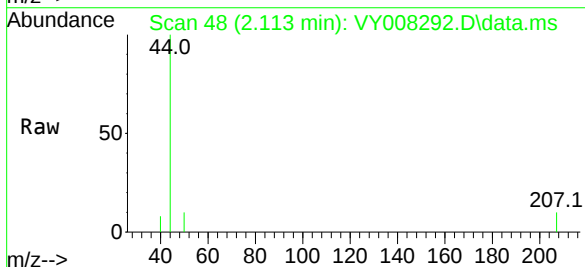




#5
Bromomethane
Concen: Below Cal
RT: 2.656 min Scan# 11
Delta R.T. 0.007 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0


Tgt Ion: 94 Resp: 266
Ion Ratio Lower Upper
94 100
96 55.4 73.5 110.3#

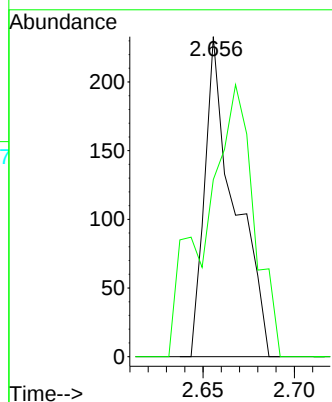

#10
Methyl Iodide
Concen: 4.722 ug/l
RT: 4.094 min Scan# 373
Delta R.T. 0.006 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Tgt Ion:142 Resp: 222
Ion Ratio Lower Upper
142 100
127 0.0 41.5 62.3#
141 0.0 11.9 17.9#


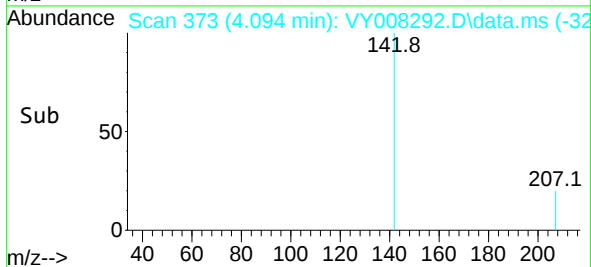
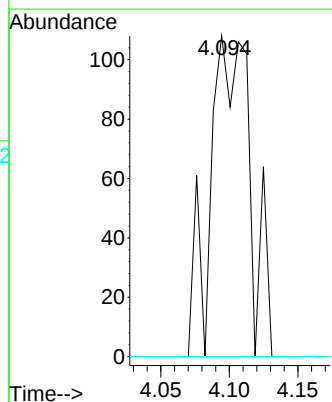
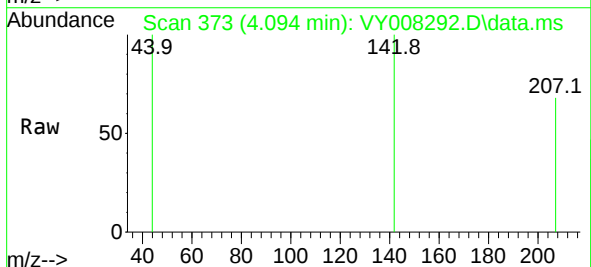


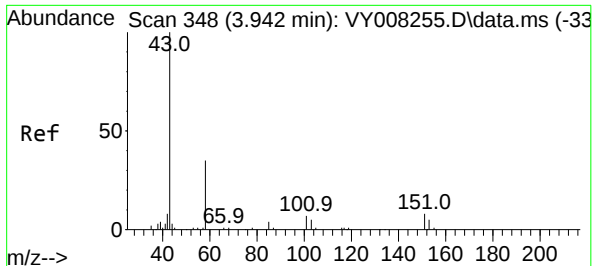

#16
Acetone
Concen: 2.522 ug/l
RT: 3.930 min Scan# 34
Delta R.T. -0.012 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0


Tgt Ion: 43 Resp: 42
Ion Ratio Lower Upper
43 100
58 0.0 22.0 33.0#

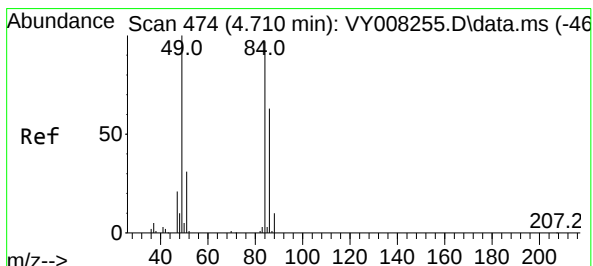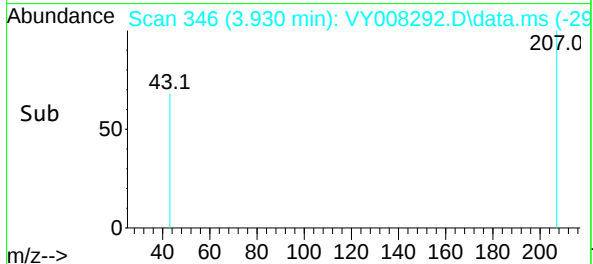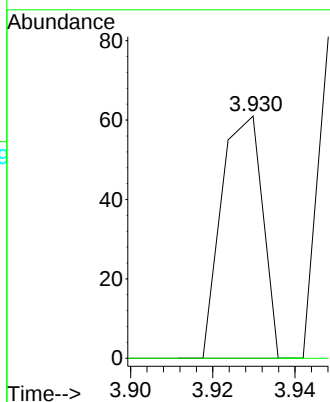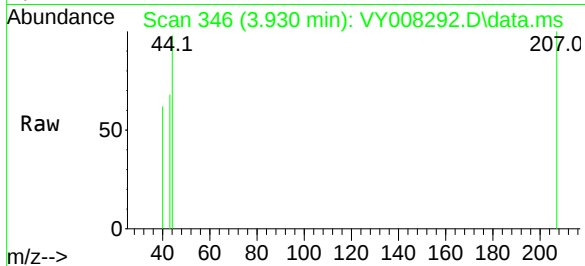

#20
Methylene Chloride
Concen: Below Cal
RT: 4.698 min Scan# 472
Delta R.T. -0.012 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Tgt Ion: 84 Resp: 120
Ion Ratio Lower Upper
84 100
49 86.3 114.4 171.6#
51 0.0 35.3 52.9#
86 62.9 53.7 80.5

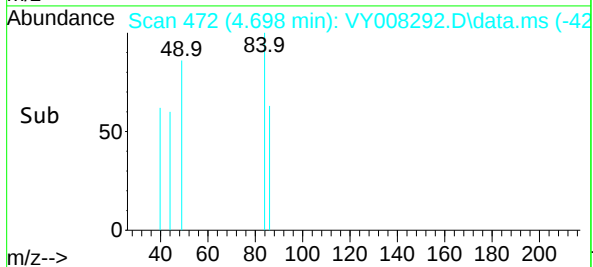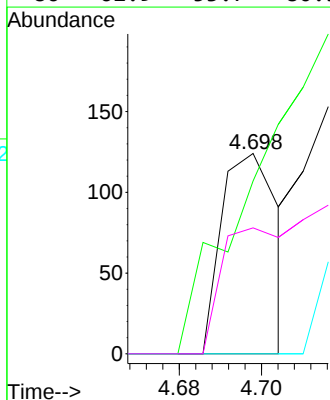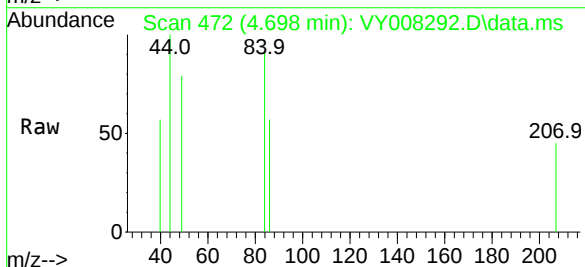

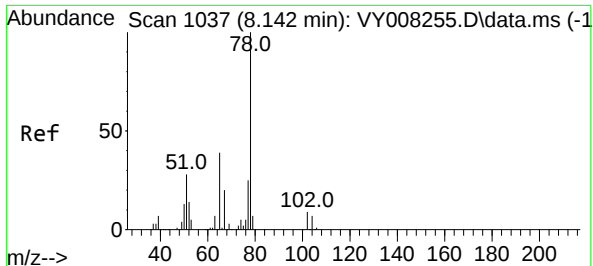

#33

1,2-Dichloroethane-d4

Concen: 74.670 ug/l

RT: 8.142 min Scan# 1037

Delta R.T. 0.000 min

Lab File: VY008292.D

Acq: 12 Apr 2022 16:56

Instrument :

MSVOA_Y

ClientSampleId :





SB-01-14.5-15.0

Tgt Ion: 65 Resp: 5170

Ion Ratio Lower Upper

65 100

67 55.4 0.0 99.4

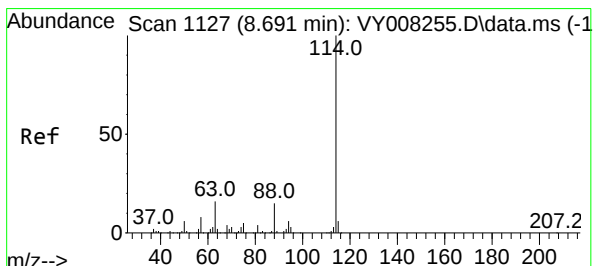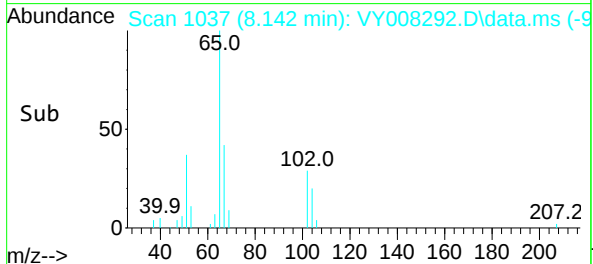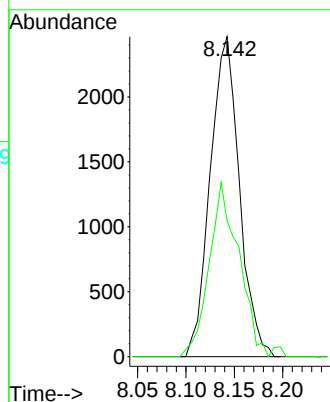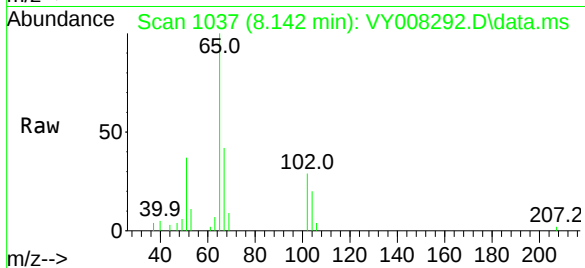

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY008292.D

Acq: 12 Apr 2022 16:56




Tgt Ion: 114 Resp: 14212


Ion Ratio Lower Upper

114 100

63 15.7 0.0 43.2

88 15.1 0.0 31.8


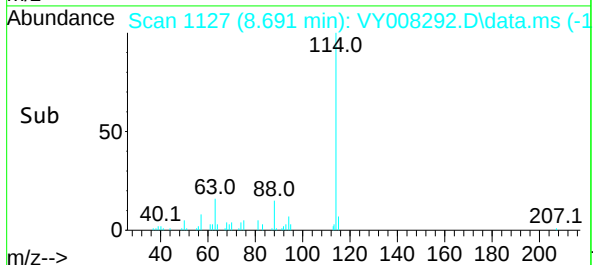
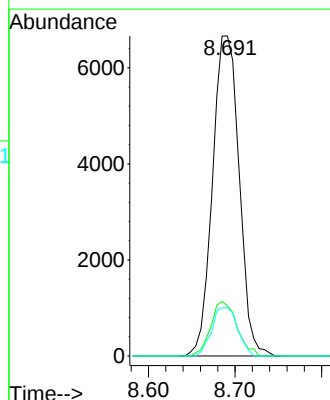
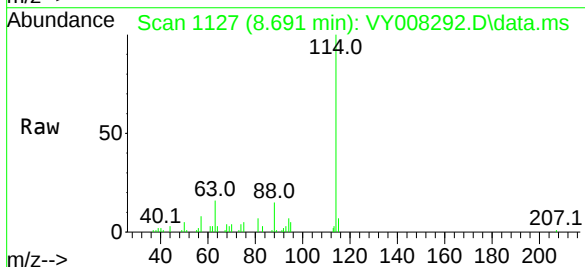




#35
Dibromofluoromethane
Concen: 58.049 ug/l
RT: 7.716 min Scan# 911
Delta R.T. 0.001 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0


Tgt Ion:113 Resp: 4765
Ion Ratio Lower Upper
113 100
111 99.5 82.6 124.0
192 20.2 17.6 26.4

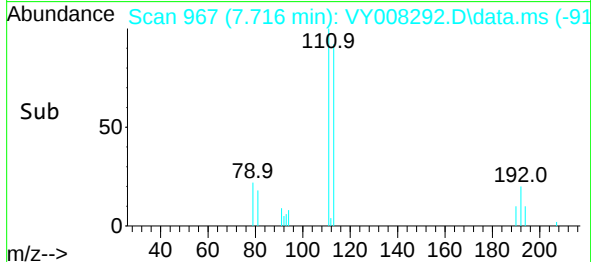

#36
1,1-Dichloropropene
Concen: 3.403 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.128 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56


Tgt Ion: 75 Resp: 446
Ion Ratio Lower Upper
75 100
110 0.0 17.1 51.2#
77 0.0 24.4 36.6#

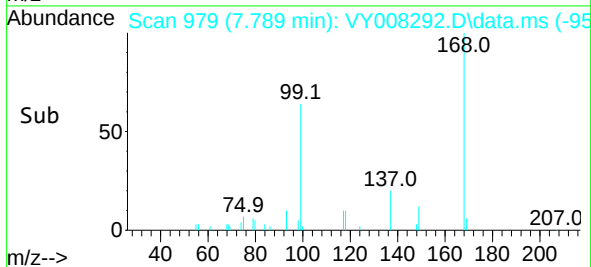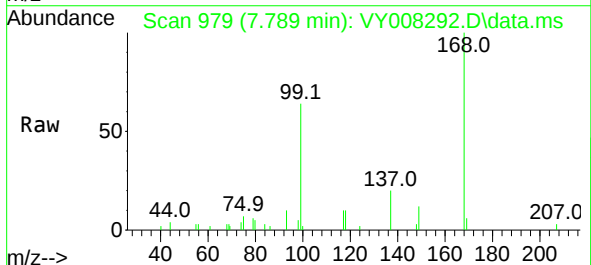






#38
Carbon Tetrachloride
Concen: 5.935 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.109 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0



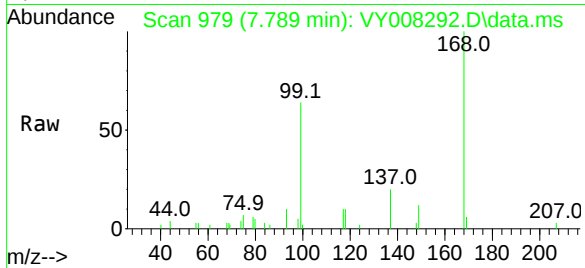



Tgt Ion: 117 Resp: 837
Ion Ratio Lower Upper
117 100
119 0.0 77.9 116.9#
121 0.0 24.8 37.2#

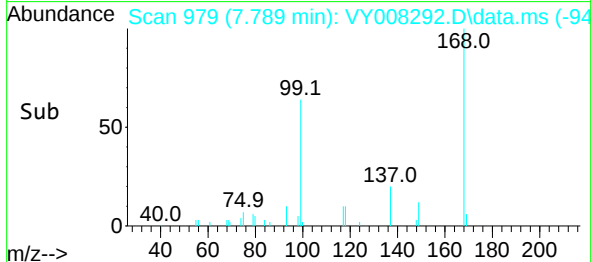

#48
Methyl methacrylate
Concen: 2.307 ug/l
RT: 9.264 min Scan# 1221
Delta R.T. -0.024 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Tgt Ion: 41 Resp: 123
Ion Ratio Lower Upper
41 100
69 42.3 58.2 87.2#
39 64.2 47.4 71.0

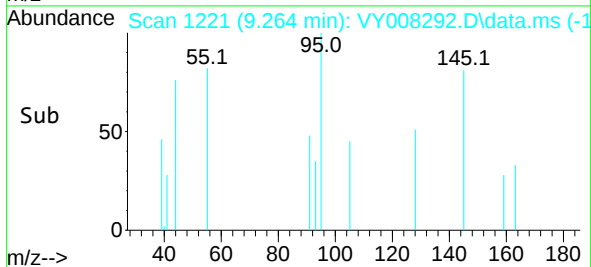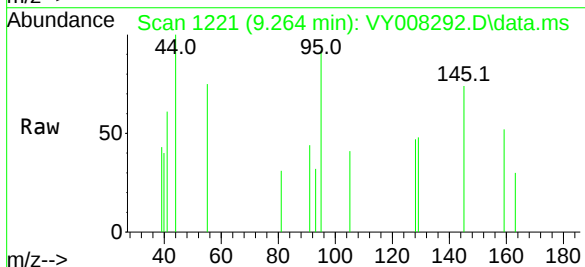



#50

Toluene-d8

Concen: 60.620 ug/l

RT: 10.179 min Scan# 11

Delta R.T. 0.001 min

Lab File: VY008292.D

Acq: 12 Apr 2022 16:56

Instrument :

MSVOA_Y

ClientSampleId :





SB-01-14.5-15.0

Tgt Ion: 98 Resp: 17027

Ion Ratio Lower Upper

98 100

100 64.5 50.2 75.2

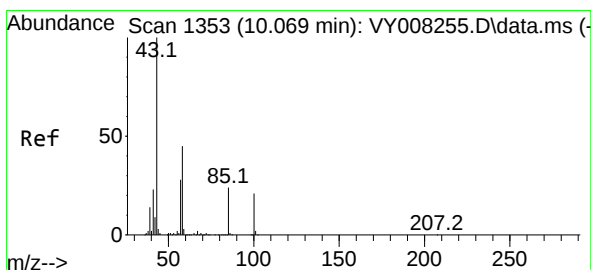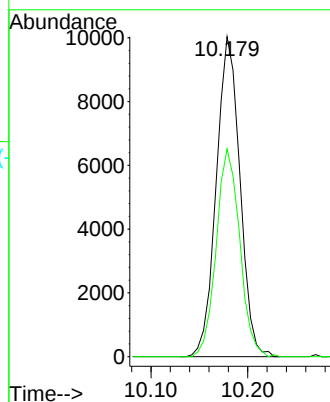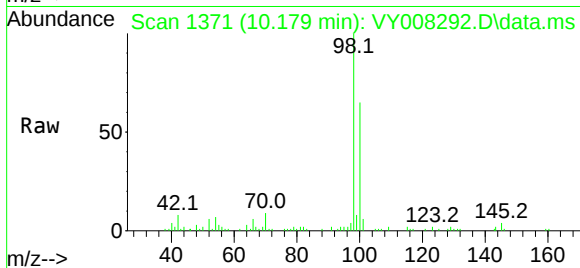

#51

4-Methyl-2-Pentanone

Concen: 3.736 ug/l

RT: 10.093 min Scan# 1357

Delta R.T. 0.024 min

Lab File: VY008292.D




Acq: 12 Apr 2022 16:56


Tgt Ion: 43 Resp: 242

Ion Ratio Lower Upper

43 100

58 0.0 28.1 42.1#


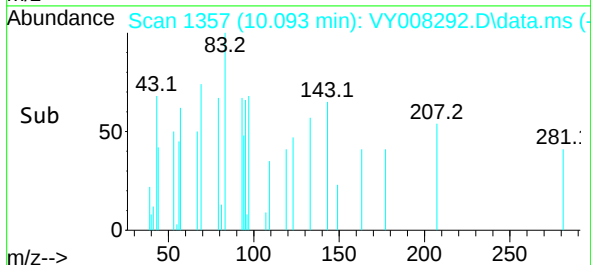
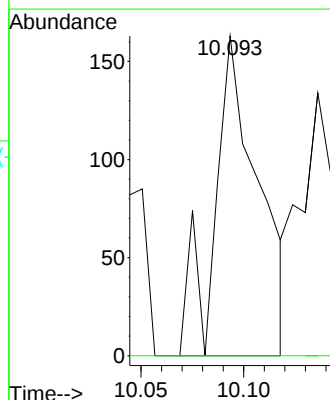
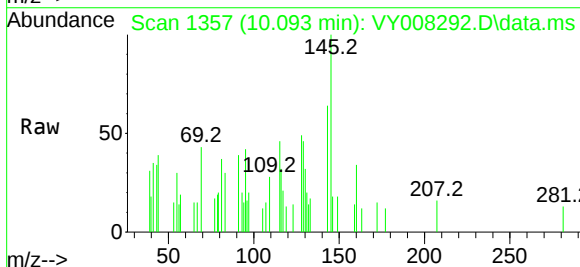




#55
 1,1,2-Trichloroethane
 Concen: 1.511 ug/l
 RT: 10.666 min Scan# 1448
 Delta R.T. 0.018 min
 Lab File: VY008292.D
 Acq: 12 Apr 2022 16:56




Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-01-14.5-15.0


Tgt Ion: 97	Resp:	136
Ion	Ratio	Lower Upper
97	100	
83	0.0	69.8 104.8#
85	0.0	44.3 66.5#
99	0.0	49.8 74.6#

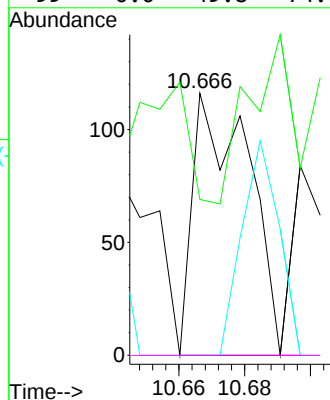

#56
 Ethyl methacrylate
 Concen: 1.667 ug/l
 RT: 10.496 min Scan# 1423
 Delta R.T. -0.012 min
 Lab File: VY008292.D
 Acq: 12 Apr 2022 16:56

Tgt Ion: 69	Resp: 184
Ion Ratio	Lower Upper
69 100	
41 0.0	63.4 95.0#
39 51.6	35.8 53.8


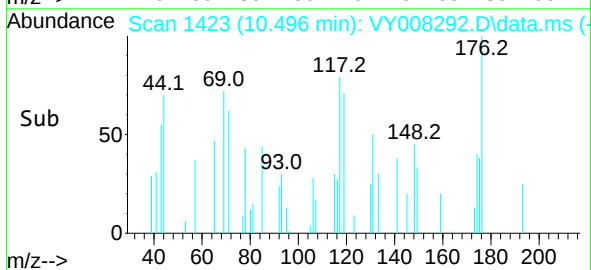
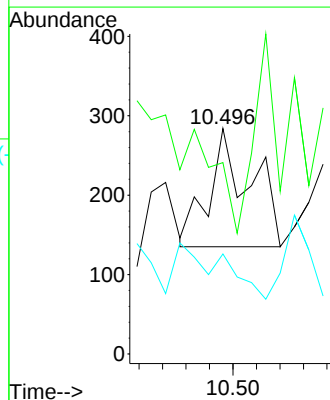





#58
 2-Chloroethyl Vinyl ether
 Concen: 2.047 ug/l
 RT: 9.715 min Scan# 11
 Delta R.T. -0.067 min
 Lab File: VY008292.D
 Acq: 12 Apr 2022 16:56




Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-01-14.5-15.0


Tgt Ion: 63 Resp: 89
 Ion Ratio Lower Upper
 63 100
 106 28.1 21.5 32.3

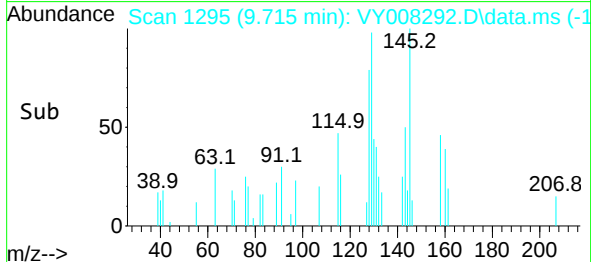

#59
 2-Hexanone
 Concen: 1.705 ug/l
 RT: 10.843 min Scan# 1480
 Delta R.T. 0.012 min
 Lab File: VY008292.D
 Acq: 12 Apr 2022 16:56

Tgt Ion: 43 Resp: 76
 Ion Ratio Lower Upper
 43 100
 58 0.0 24.4 73.4#


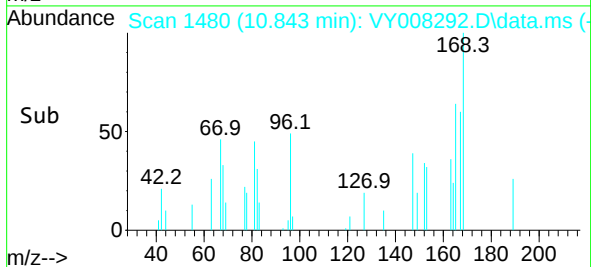

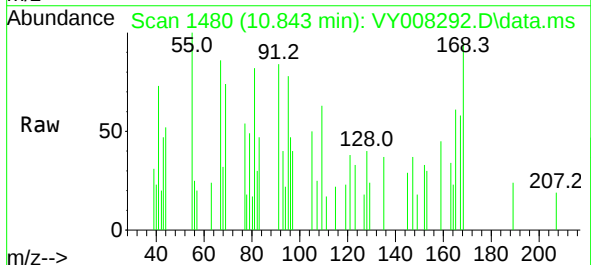




#60
Dibromochloromethane
Concen: 1.084 ug/l
RT: 10.746 min Scan# 1464
Delta R.T. -0.237 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0


Tgt Ion:129 Resp: 114
Ion Ratio Lower Upper
129 100
127 64.9 38.7 116.1

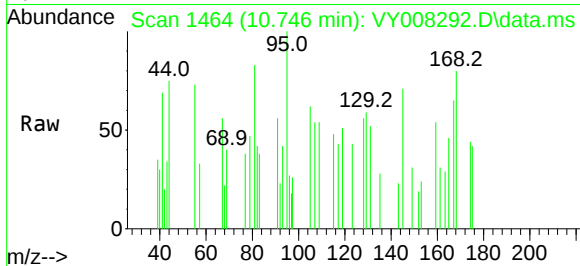

#61
1,2-Dibromoethane
Concen: 1.147 ug/l
RT: 11.087 min Scan# 1520
Delta R.T. 0.000 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Tgt Ion:107 Resp: 101
Ion Ratio Lower Upper
107 100
109 140.6 75.4 113.2#


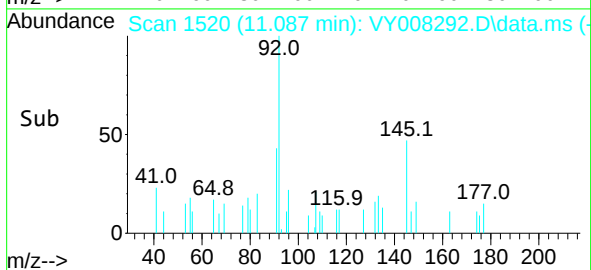

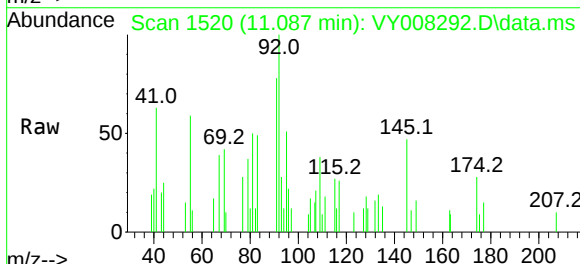




#62
4-Bromofluorobenzene
Concen: 59.292 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0


Tgt Ion: 95 Resp: 6264
Ion Ratio Lower Upper
95 100
174 92.5 0.0 177.0
176 80.9 0.0 175.8



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. 0.000 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Tgt Ion: 117 Resp: 14787
Ion Ratio Lower Upper
117 100
82 53.2 43.0 64.4
119 32.4 25.4 38.0


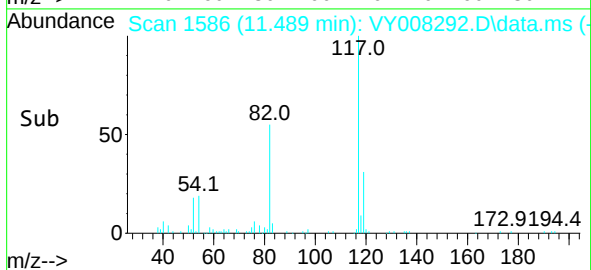

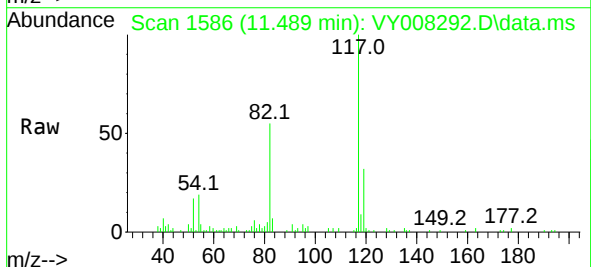




#66
1,1,1,2-Tetrachloroethane
Concen: 3.393 ug/l
RT: 11.605 min Scan# 11
Delta R.T. 0.012 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0


Tgt Ion:131 Resp: 406
Ion Ratio Lower Upper
131 100
133 30.0 47.9 143.6#
119 0.0 30.8 92.3#

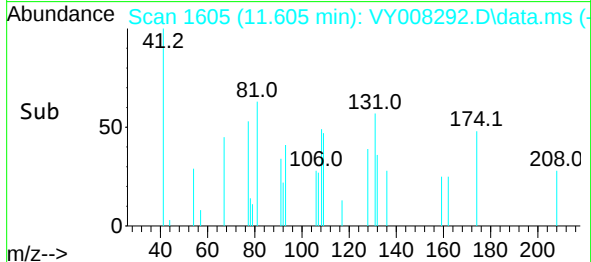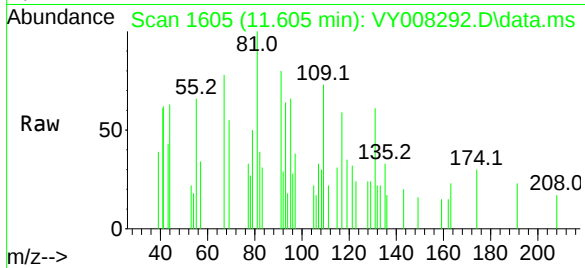

#71
Bromoform
Concen: 1.719 ug/l
RT: 12.227 min Scan# 1707
Delta R.T. 0.019 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Tgt Ion:173 Resp: 124
Ion Ratio Lower Upper
173 100
175 0.0 24.6 74.0#
254 0.0 0.0 0.0


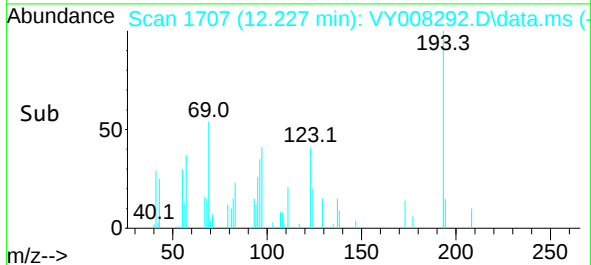

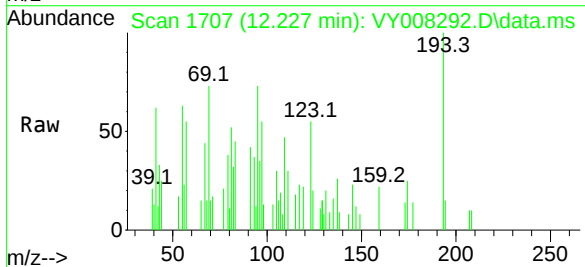




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1904
Delta R.T. -0.006 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0


Tgt Ion:152 Resp: 6633
Ion Ratio Lower Upper
152 100
115 64.1 28.2 84.7
150 147.6 0.0 347.6

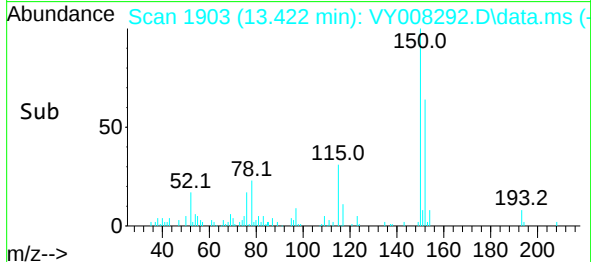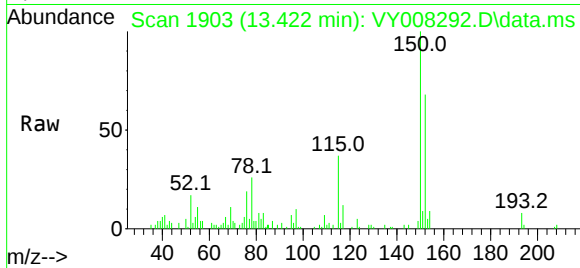

#74
N-ethyl acetate
Concen: 3.998 ug/l
RT: 12.123 min Scan# 1690
Delta R.T. -0.025 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Tgt Ion: 43 Resp: 428
Ion Ratio Lower Upper
43 100
70 23.4 28.7 43.1#
55 64.5 17.3 25.9#
61 0.0 17.0 25.6#

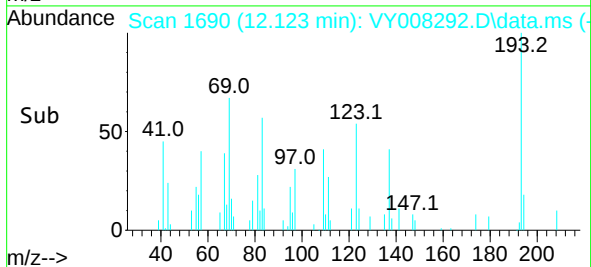

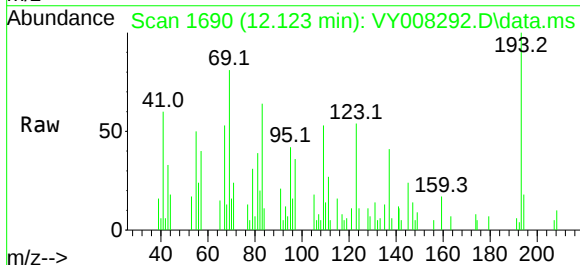


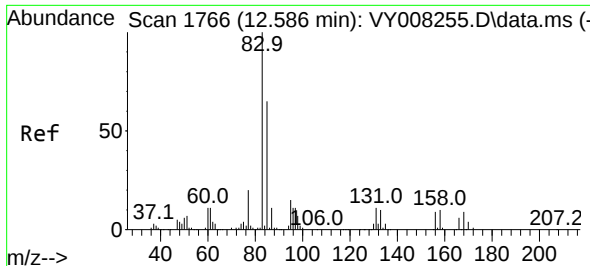

#75
 1,1,2,2-Tetrachloroethane
 Concen: 1.112 ug/l
 RT: 12.593 min Scan# 1767
 Delta R.T. 0.007 min
 Lab File: VY008292.D
 Acq: 12 Apr 2022 16:56




Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-01-14.5-15.0


Tgt Ion: 83 Resp: 116
 Ion Ratio Lower Upper
 83 100
 131 141.4 5.6 16.8#
 85 0.0 32.3 96.8#

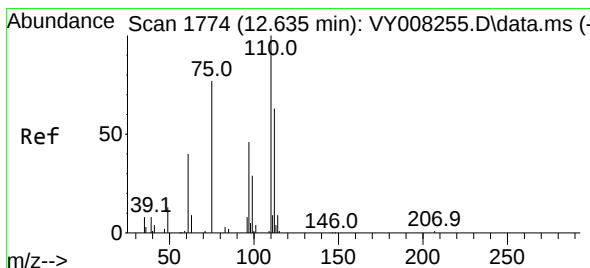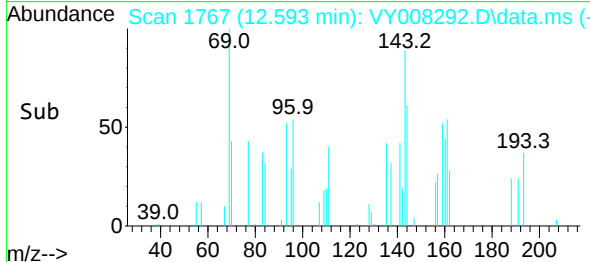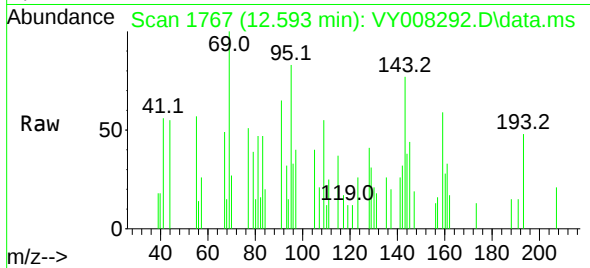

#76
 1,2,3-Trichloropropane
 Concen: 48.433 ug/l
 RT: 12.483 min Scan# 1749
 Delta R.T. -0.152 min
 Lab File: VY008292.D
 Acq: 12 Apr 2022 16:56

Tgt Ion: 75 Resp: 3553
 Ion Ratio Lower Upper
 75 100
 77 0.0 0.0 0.0

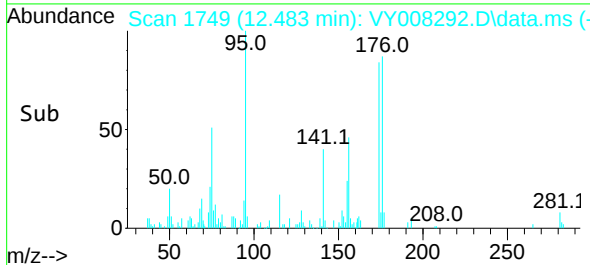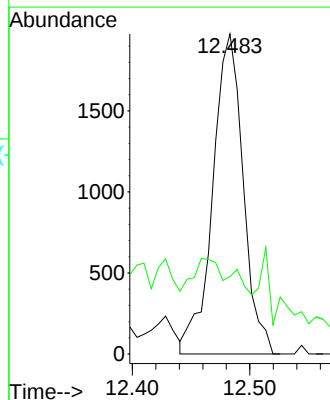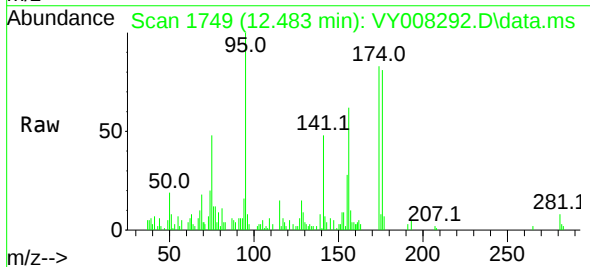



#77

Bromobenzene

Concen: 75.592 ug/l

RT: 12.404 min Scan# 1736

Delta R.T. -0.207 min

Lab File: VY008292.D

Acq: 12 Apr 2022 16:56





Instrument :

MSVOA_Y

ClientSampleId :

SB-01-14.5-15.0

Tgt Ion:	156	Resp:	9135
Ion Ratio	Lower	Upper	
156	100		
77	3.3	95.5	286.4#
158	3.4	48.0	144.0#

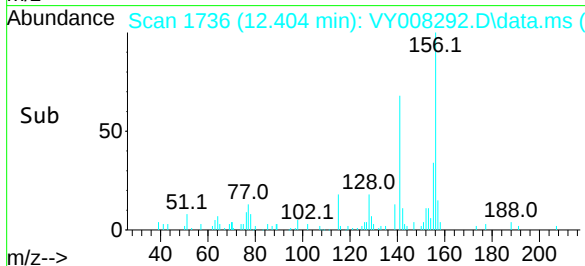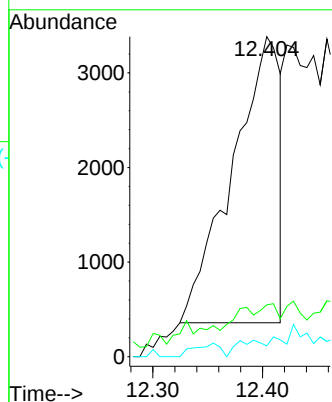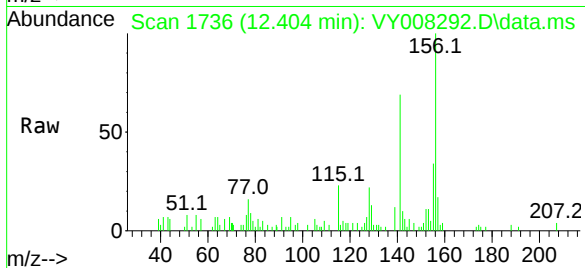

#81

trans-1,4-Dichloro-2-butene

Concen: 3.355 ug/l




RT: 12.373 min Scan# 1731


Delta R.T. -0.006 min

Lab File: VY008292.D

Acq: 12 Apr 2022 16:56

Tgt Ion:	75	Resp:	110
Ion Ratio	Lower	Upper	
75	100		
53	121.8	85.3	127.9
89	0.0	37.0	55.4#


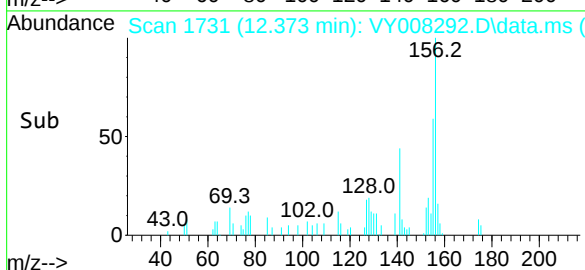

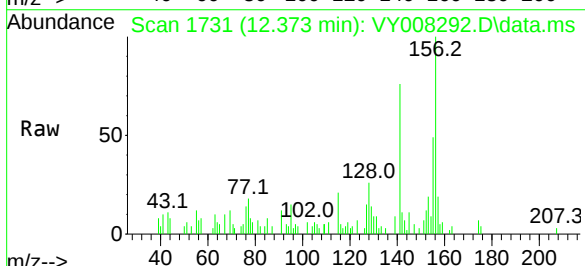




#82
4-Chlorotoluene
Concen: 1.108 ug/l
RT: 12.843 min Scan# 11
Delta R.T. -0.012 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0


Tgt Ion: 91 Resp: 372
Ion Ratio Lower Upper
91 100
126 14.8 17.0 51.0#

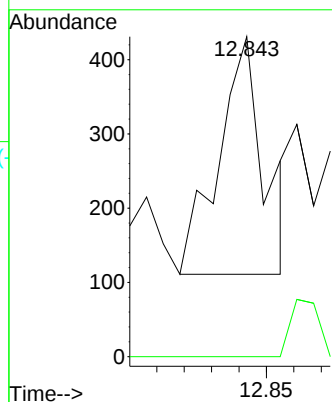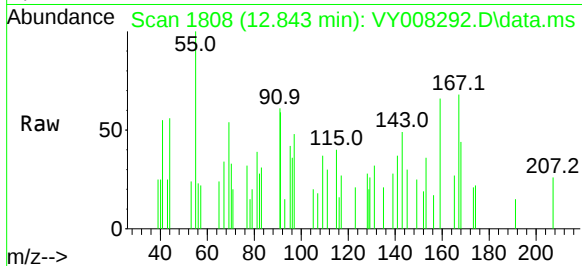

#84
1,2,4-Trimethylbenzene
Concen: 3.206 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. -0.006 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Tgt Ion: 105 Resp: 1283
Ion Ratio Lower Upper
105 100
120 0.0 22.3 66.9#


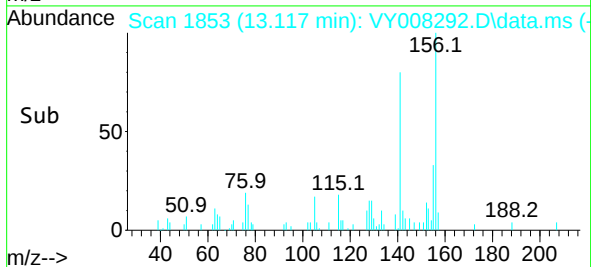
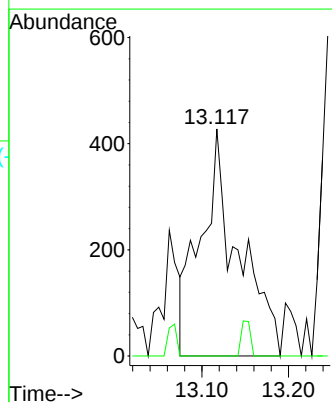
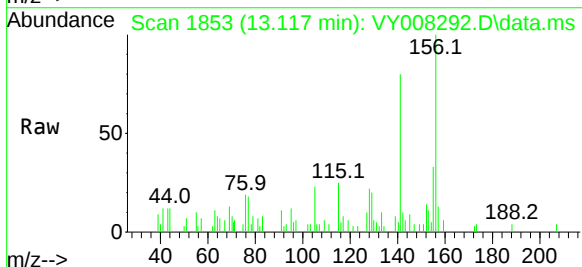




#85
 sec-Butylbenzene
 Concen: 2.640 ug/l
 RT: 13.251 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VY008292.D
 Acq: 12 Apr 2022 16:56




Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-01-14.5-15.0


Tgt Ion:105 Resp: 1420
 Ion Ratio Lower Upper
 105 100
 134 24.0 10.2 30.4

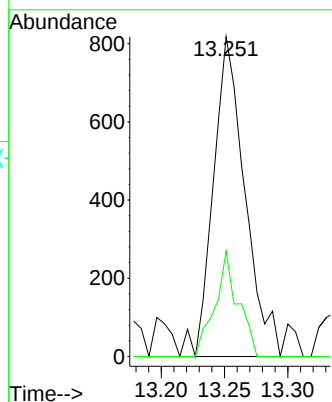

#86
 p-Isopropyltoluene
 Concen: 2.538 ug/l
 RT: 13.599 min Scan# 1932
 Delta R.T. 0.226 min
 Lab File: VY008292.D
 Acq: 12 Apr 2022 16:56

Tgt Ion:119 Resp: 1139
 Ion Ratio Lower Upper
 119 100
 134 33.5 13.2 39.5
 91 27.9 12.4 37.2


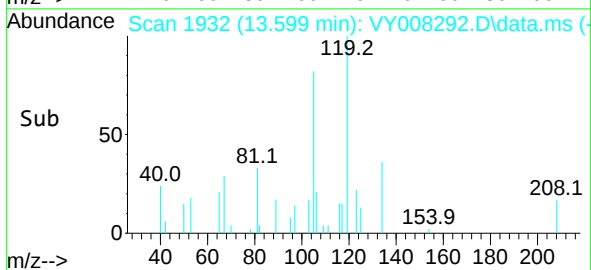






#89
n-Butylbenzene
Concen: 2.308 ug/l
RT: 13.684 min Scan# 1946
Delta R.T. -0.012 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Instrument :
MSVOA_Y
ClientSampleId :
SB-01-14.5-15.0

Tgt Ion: 91 Resp: 936
Ion Ratio Lower Upper
91 100
92 0.0 26.3 78.9#
134 41.5 13.0 38.9#

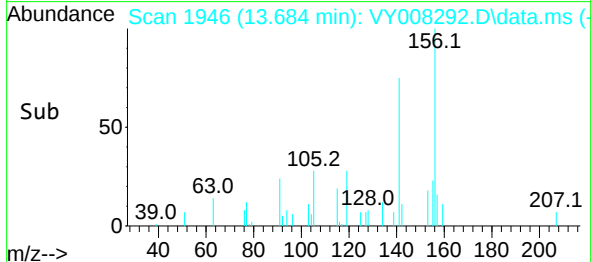

#90
Hexachloroethane
Concen: 3.922 ug/l
RT: 13.971 min Scan# 1993
Delta R.T. 0.007 min
Lab File: VY008292.D
Acq: 12 Apr 2022 16:56

Tgt Ion: 117 Resp: 329
Ion Ratio Lower Upper
117 100
201 0.0 43.0 128.8#

