
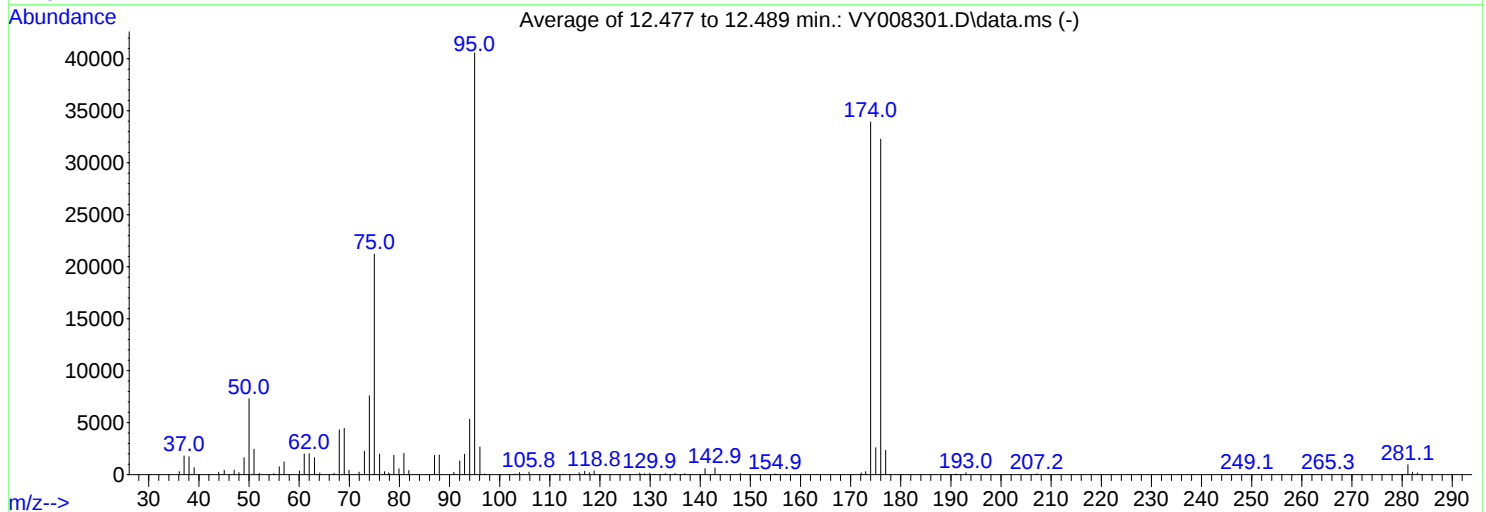


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041322\
 Data File : VY008301.D
 Acq On : 13 Apr 2022 09:18
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
 Title : SW846 8260
 Last Update : Fri Apr 08 16:02:50 2022

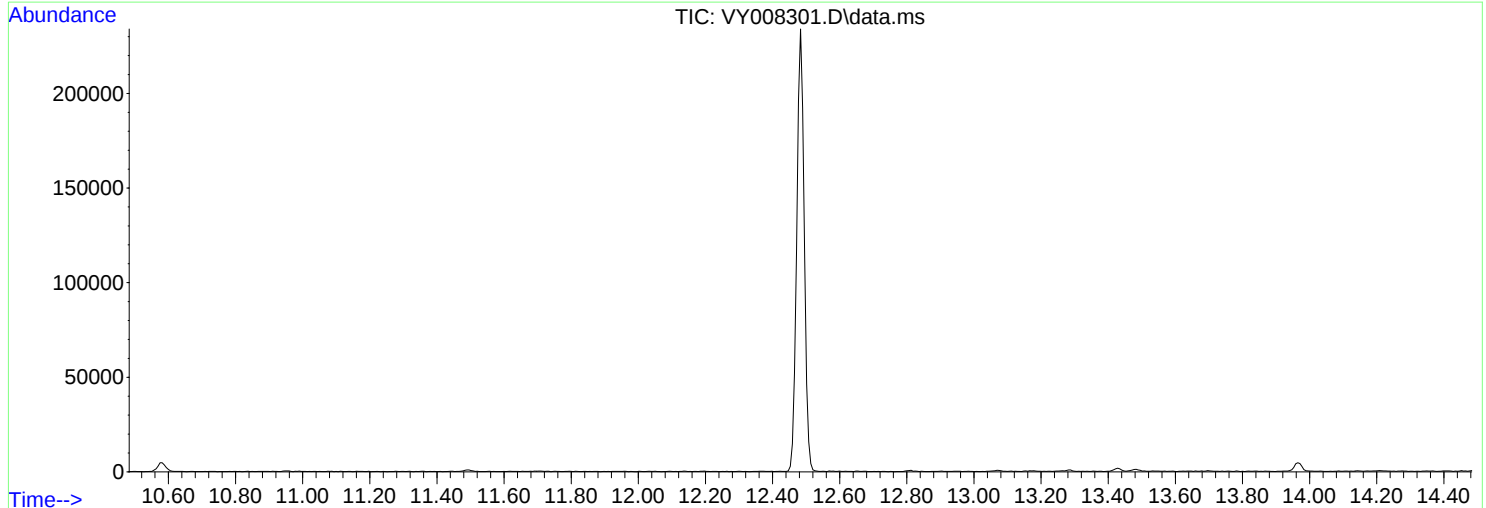

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	7314	PASS
75	95	30	60	52.3	21208	PASS
95	95	100	100	100.0	40579	PASS
96	95	5	9	6.6	2666	PASS
173	174	0.00	2	0.9	299	PASS
174	95	50	100	83.6	33931	PASS
175	174	5	9	7.6	2584	PASS
176	174	95	101	95.1	32285	PASS
177	176	5	9	7.2	2336	PASS