

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041425\
 Data File : VY021870.D
 Acq On : 14 Apr 2025 15:26
 Operator : SY/MD
 Sample : Q1784-01
 Misc : 5.08g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OR-01-41125

Quant Time: Apr 14 23:31:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 28 02:30:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	295671	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	536095	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	493540	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	206269	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	168192	52.502	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 105.000%			
35) Dibromofluoromethane	7.634	113	181225	52.113	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 104.220%			
50) Toluene-d8	10.109	98	652344	49.309	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery = 98.620%			
62) 4-Bromofluorobenzene	12.407	95	219972	49.157	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery = 98.320%			
Target Compounds					Qvalue	
16) Acetone	3.872	43	5630	8.587	ug/l	99
20) Methylene Chloride	4.610	84	1865	Below Cal	#	71
31) Cyclohexane	7.701	56	7519	1.330	ug/l #	25
36) 1,1-Dichloropropene	7.707	75	23678	4.470	ug/l #	51
38) Carbon Tetrachloride	7.713	117	30297	4.994	ug/l #	16
39) Methylcyclohexane	9.109	83	7925	1.252	ug/l	96
49) 1,4-Dioxane	9.115	88	26	1.122	ug/l #	1
51) 4-Methyl-2-Pentanone	10.103	43	3922	1.591	ug/l #	1
52) Toluene	10.170	92	54503	5.507	ug/l	95
55) 1,1,2-Trichloroethane	10.542	97	7364	2.644	ug/l #	20
59) 2-Hexanone	10.731	43	6818	4.153	ug/l #	31
67) Ethyl Benzene	11.517	91	226636	11.682	ug/l	99
68) m/p-Xylenes	11.627	106	384772	51.794	ug/l	99
69) o-Xylene	11.956	106	290354	42.341	ug/l	98
70) Styrene	11.956	104	15792	1.381	ug/l #	1
73) Isopropylbenzene	12.255	105	151852	9.912	ug/l	100
74) N-amyl acetate	12.048	43	27902	7.760	ug/l #	58
76) 1,2,3-Trichloropropane	12.657	75	10292	5.034	ug/l #	100
78) n-propylbenzene	12.596	91	383650	20.829	ug/l	100
79) 2-Chlorotoluene	12.694	91	49537	4.631	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.737	105	847933	67.720	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.407	75	114736	129.299	ug/l #	12
82) 4-Chlorotoluene	12.737	91	94957	8.514	ug/l #	43
83) tert-Butylbenzene	13.041	119	270432	24.248	ug/l #	65
84) 1,2,4-Trimethylbenzene	13.041	105	2213851	178.891	ug/l	99
85) sec-Butylbenzene	13.176	105	320362	19.656	ug/l	87
86) p-Isopropyltoluene	13.291	119	241739	17.946	ug/l	100
89) n-Butylbenzene	13.614	91	226625	18.191	ug/l #	71
90) Hexachloroethane	13.895	117	78118	26.463	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.255	75	5370	12.579	ug/l #	1
95) Naphthalene	15.145	128	239829	42.292	ug/l #	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041425\
Data File : VY021870.D
Acq On : 14 Apr 2025 15:26
Operator : SY/MD
Sample : Q1784-01
Misc : 5.08g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125

Quant Time: Apr 14 23:31:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 28 02:30:29 2025
Response via : Initial Calibration




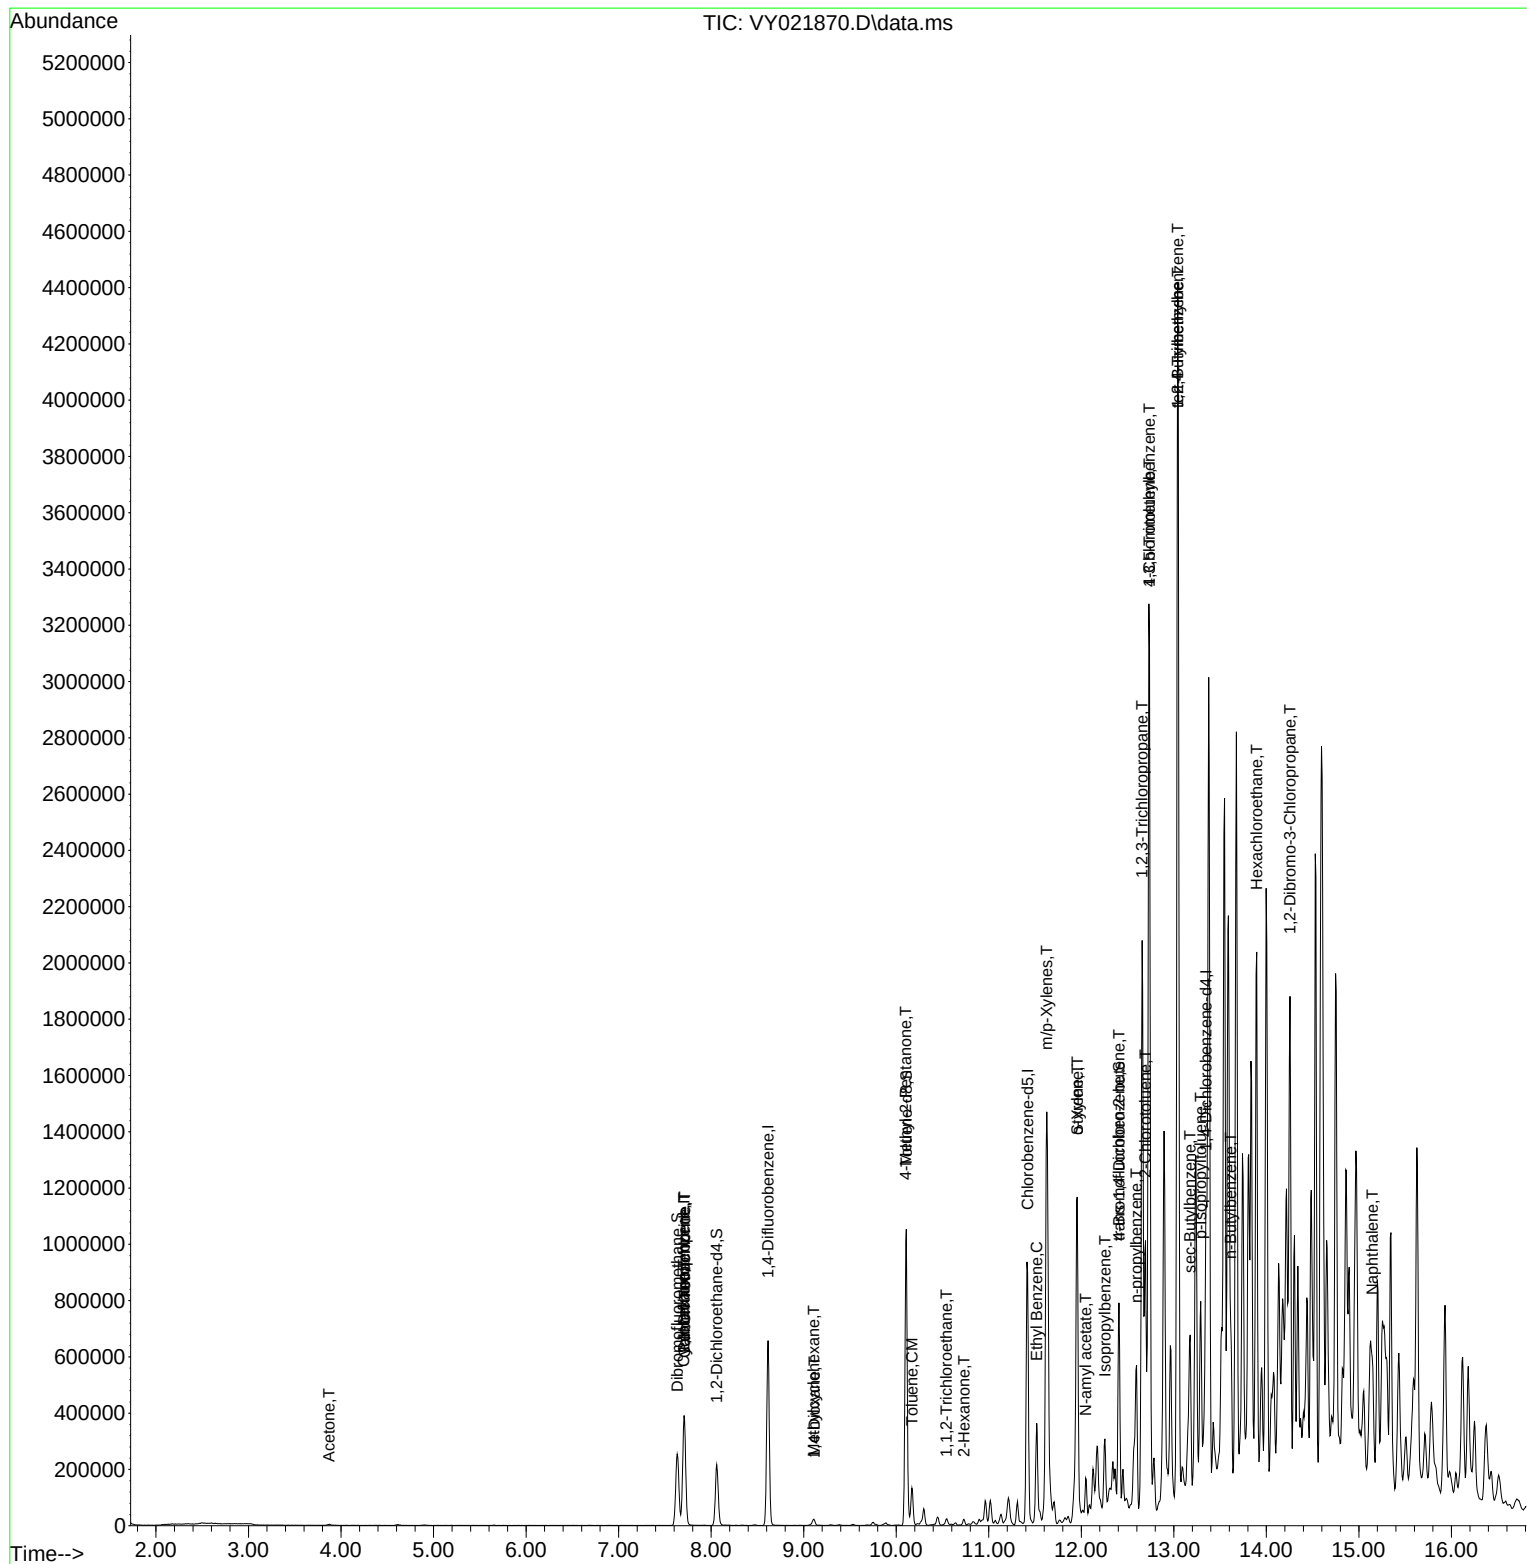




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 99
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion:168 Resp: 295671
Ion Ratio Lower Upper
168 100
99 56.0 46.7 70.1

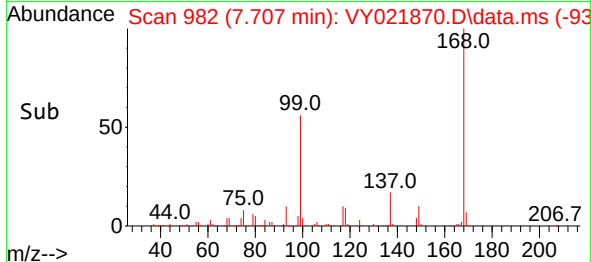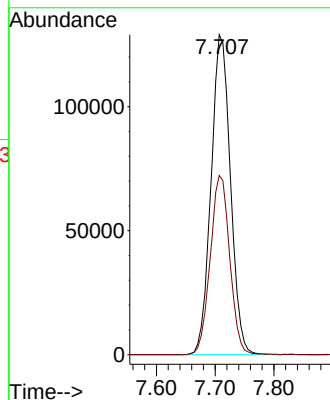

#16
Acetone
Concen: 8.587 ug/l
RT: 3.872 min Scan# 353
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion: 43 Resp: 5630
Ion Ratio Lower Upper
43 100
58 30.9 24.2 36.4


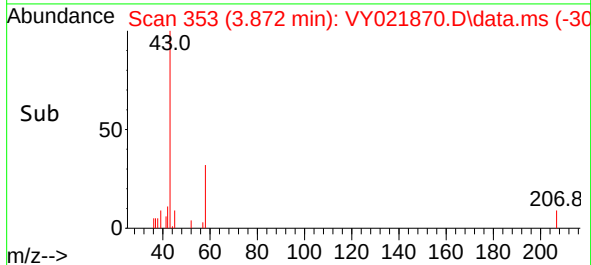
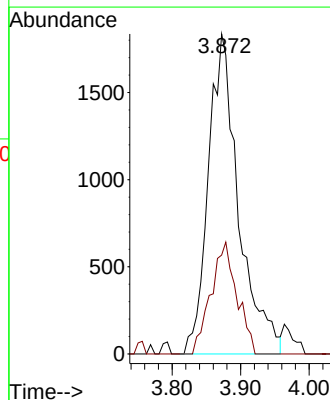
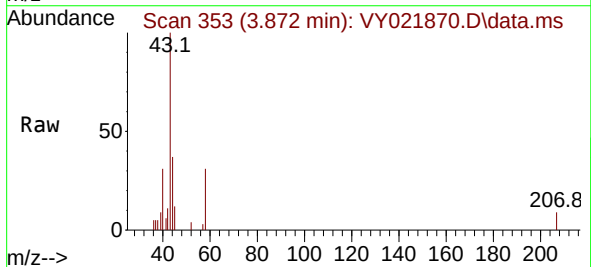




#20
Methylene Chloride
Concen: Below Cal
RT: 4.610 min Scan# 41
Delta R.T. -0.006 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion:	84	Resp:	1865
Ion	Ratio	Lower	Upper
84	100		
49	80.4	102.8	154.2#
51	42.9	33.5	50.3
86	46.3	52.0	78.0#

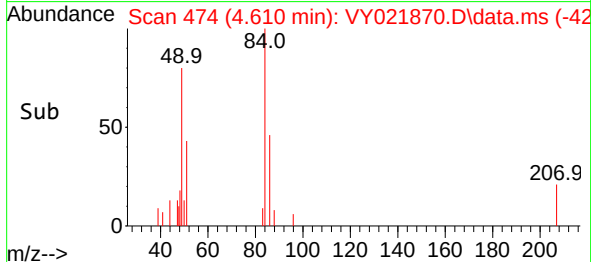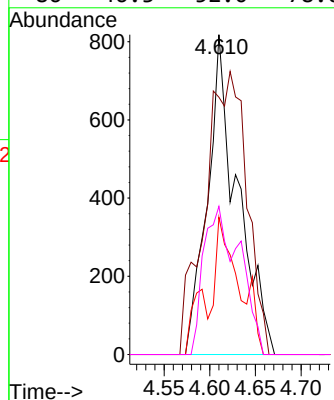

#31
Cyclohexane
Concen: 1.330 ug/l
RT: 7.701 min Scan# 981
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion:	56	Resp:	7519
Ion	Ratio	Lower	Upper
56	100		
69	144.5	26.6	40.0#
84	111.9	69.0	103.4#


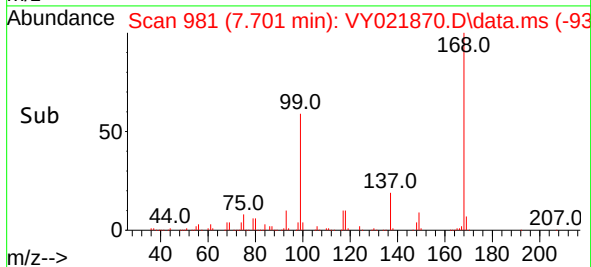
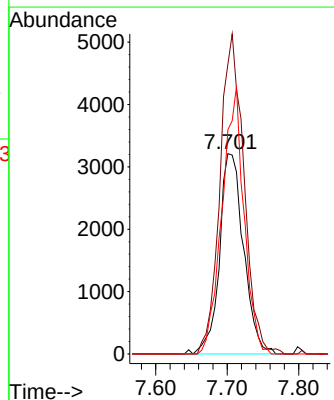
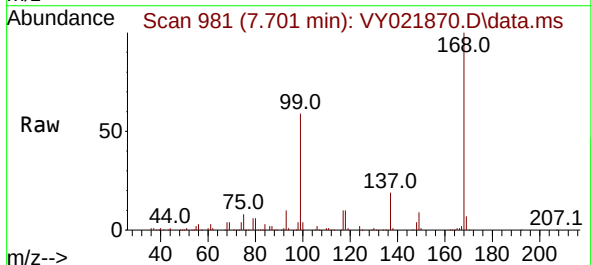




#33
 1,2-Dichloroethane-d4
 Concen: 52.502 ug/l
 RT: 8.061 min Scan# 1040
 Delta R.T. -0.000 min
 Lab File: VY021870.D
 Acq: 14 Apr 2025 15:26




Instrument :
 MSVOA_Y
 ClientSampleId :
 OR-01-41125


Tgt Ion: 65 Resp: 168192
 Ion Ratio Lower Upper
 65 100
 67 51.6 0.0 104.6

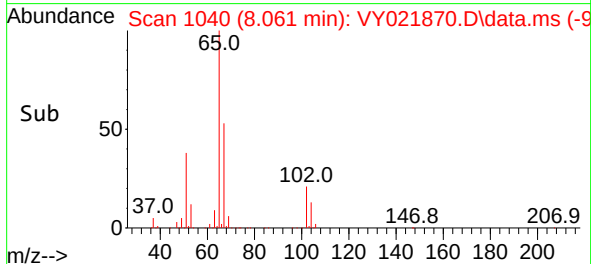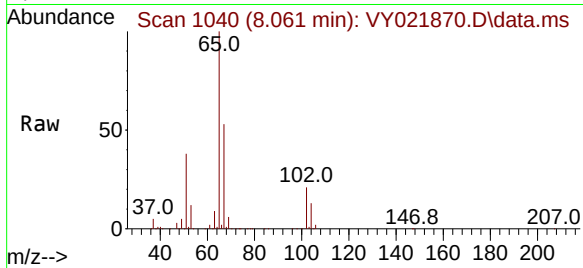

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.615 min Scan# 1131
 Delta R.T. -0.000 min
 Lab File: VY021870.D
 Acq: 14 Apr 2025 15:26

Tgt Ion: 114 Resp: 536095
 Ion Ratio Lower Upper
 114 100
 63 20.4 0.0 40.2
 88 15.6 0.0 29.8


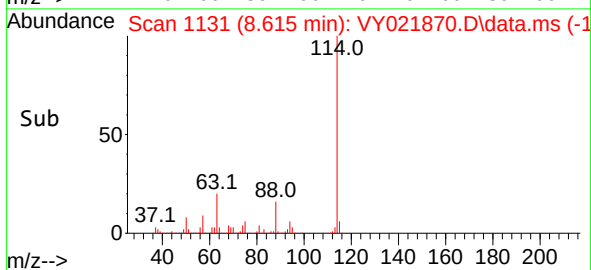

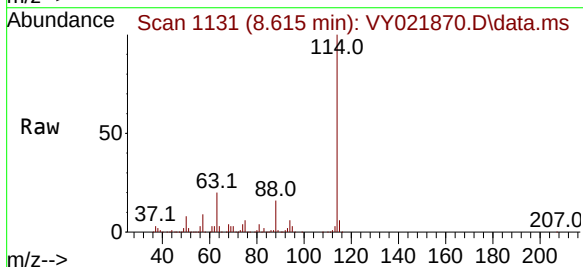




#35
Dibromofluoromethane
Concen: 52.113 ug/l
RT: 7.634 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion:113 Resp: 181225
Ion Ratio Lower Upper
113 100
111 102.6 82.6 123.8
192 20.1 16.2 24.4

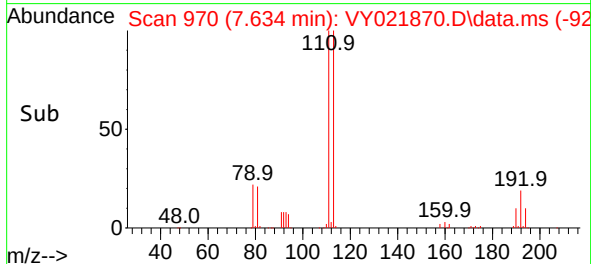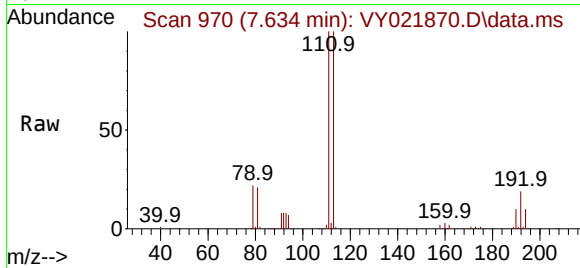

#36
1,1-Dichloropropene
Concen: 4.470 ug/l
RT: 7.707 min Scan# 982
Delta R.T. -0.128 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion: 75 Resp: 23678
Ion Ratio Lower Upper
75 100
110 9.4 17.0 50.9#
77 0.1 24.8 37.2#


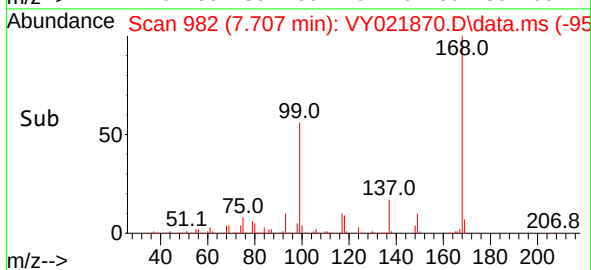

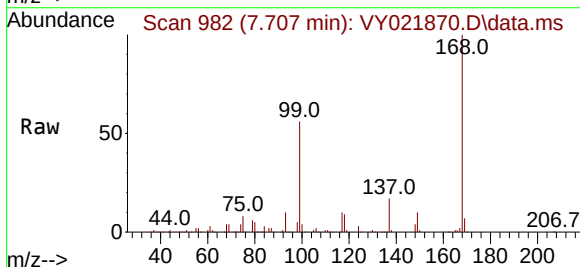


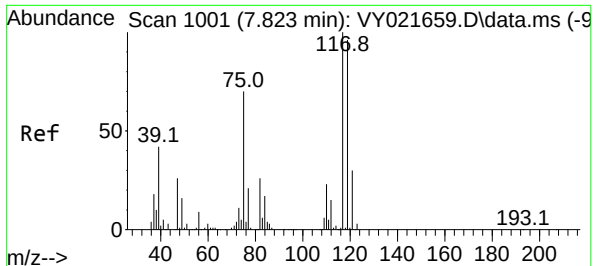

#38
Carbon Tetrachloride
Concen: 4.994 ug/l
RT: 7.713 min Scan# 91
Delta R.T. -0.110 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion:117 Resp: 30297
Ion Ratio Lower Upper
117 100
119 4.7 76.2 114.4#
121 0.0 24.2 36.4#

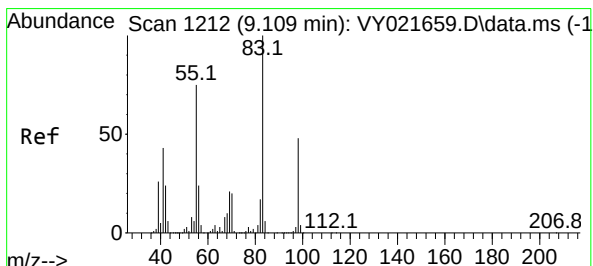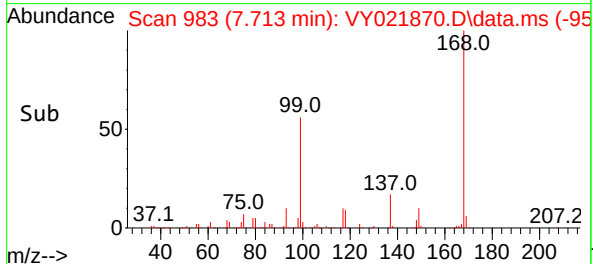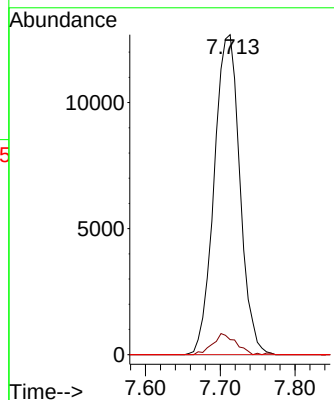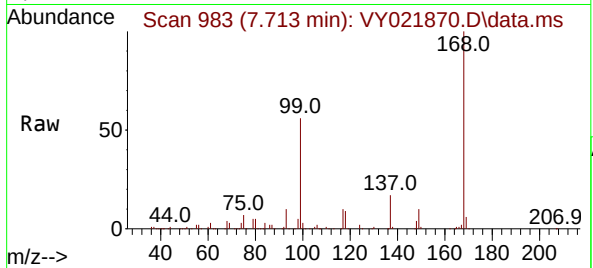

#39
Methylcyclohexane
Concen: 1.252 ug/l
RT: 9.109 min Scan# 1212
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion: 83 Resp: 7925
Ion Ratio Lower Upper
83 100
55 79.1 59.7 89.5
98 48.5 38.3 57.5

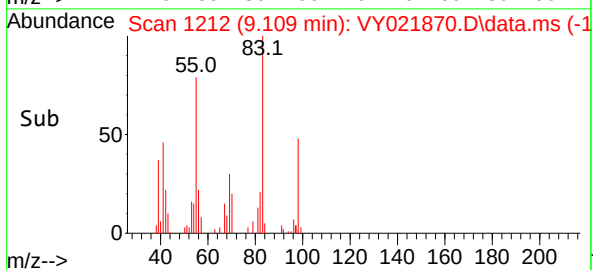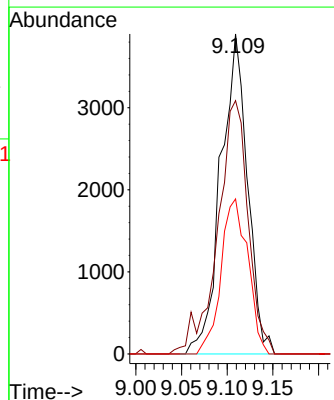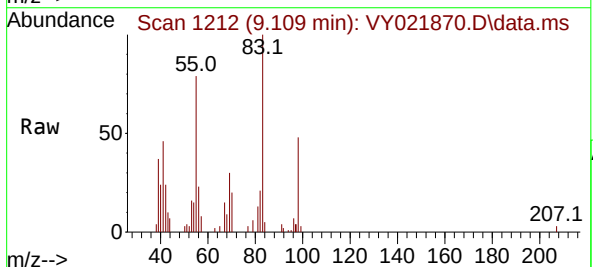



#49

1,4-Dioxane

Concen: 1.122 ug/l

RT: 9.115 min Scan# 11

Delta R.T. -0.110 min

Lab File: VY021870.D


Acq: 14 Apr 2025 15:26

Instrument :




MSVOA_Y

ClientSampleId :

OR-01-41125



Tgt Ion:	88	Resp:	26
Ion	Ratio	Lower	Upper
88	100		
43	3480.8	28.8	43.2#
58	0.0	59.4	89.2#

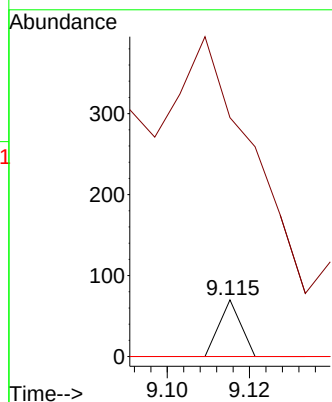

#50

Toluene-d8

Concen: 49.309 ug/l




RT: 10.109 min Scan# 1376


Delta R.T. -0.000 min

Lab File: VY021870.D

Acq: 14 Apr 2025 15:26

Tgt Ion:	98	Resp:	652344
Ion	Ratio	Lower	Upper
98	100		
100	64.7	52.1	78.1

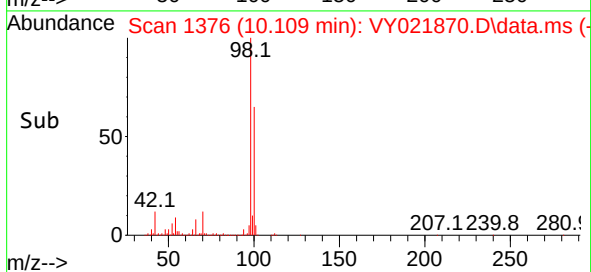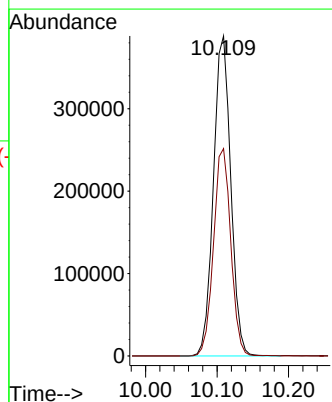



#51

4-Methyl-2-Pentanone

Concen: 1.591 ug/l

RT: 10.103 min Scan# 1375

Delta R.T. 0.104 min

Lab File: VY021870.D

Acq: 14 Apr 2025 15:26

Instrument :

MSVOA_Y

ClientSampleId :





OR-01-41125

Tgt Ion: 43 Resp: 3922

Ion Ratio Lower Upper

43 100

58 142.7 31.5 47.3#

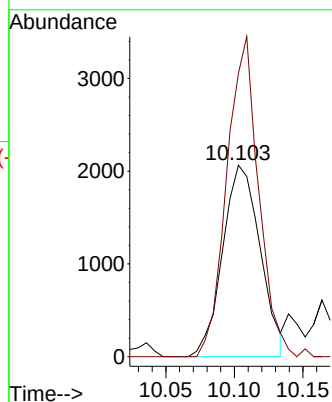

#52

Toluene

Concen: 5.507 ug/l

RT: 10.170 min Scan# 1386

Delta R.T. -0.000 min

Lab File: VY021870.D




Acq: 14 Apr 2025 15:26


Tgt Ion: 92 Resp: 54503

Ion Ratio Lower Upper

92 100

91 165.9 138.6 207.8


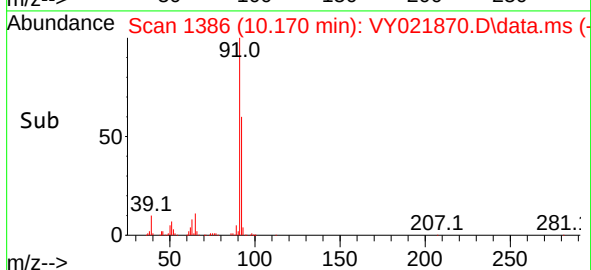






#55
1,1,2-Trichloroethane
Concen: 2.644 ug/l
RT: 10.542 min Scan# 1452
Delta R.T. -0.031 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion: 97 Resp: 7364
Ion Ratio Lower Upper
97 100
83 11.0 69.5 104.3#
85 0.0 43.9 65.9#
99 0.0 49.9 74.9#

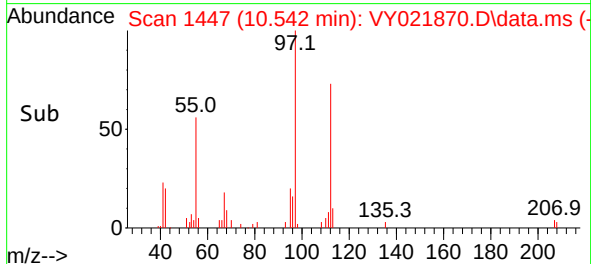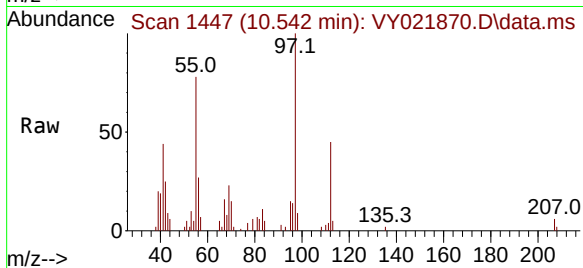

#59
2-Hexanone
Concen: 4.153 ug/l
RT: 10.731 min Scan# 1478
Delta R.T. -0.031 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion: 43 Resp: 6818
Ion Ratio Lower Upper
43 100
58 4.9 27.2 81.5#


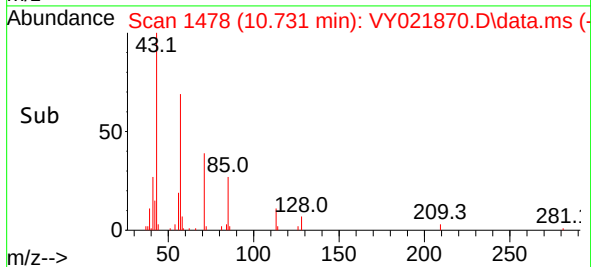

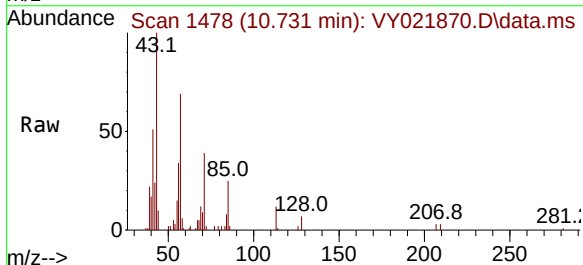




#62
4-Bromofluorobenzene
Concen: 49.157 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion: 95 Resp: 219972
Ion Ratio Lower Upper
95 100
174 84.1 0.0 170.8
176 80.6 0.0 162.0

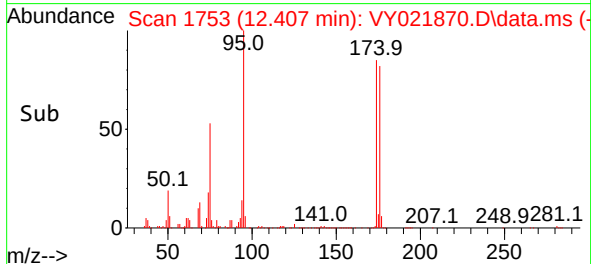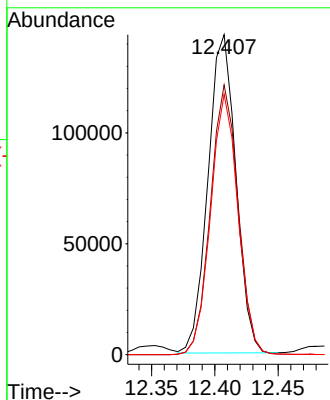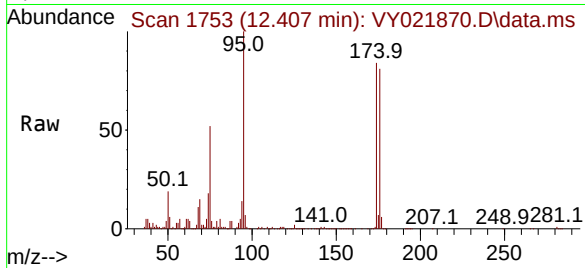

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 1591
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion: 117 Resp: 493540
Ion Ratio Lower Upper
117 100
82 54.0 42.8 64.2
119 32.4 25.7 38.5


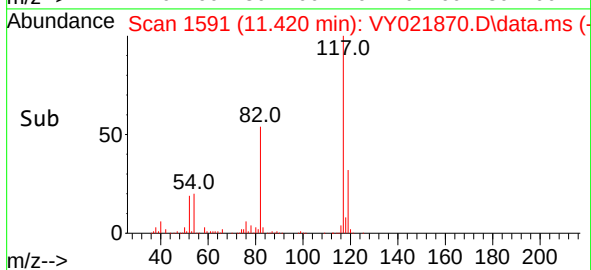
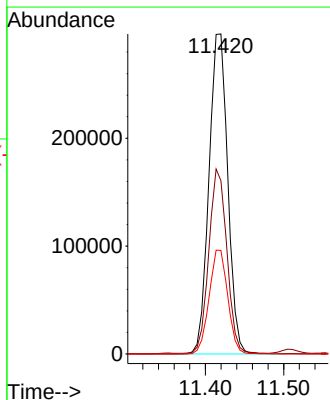
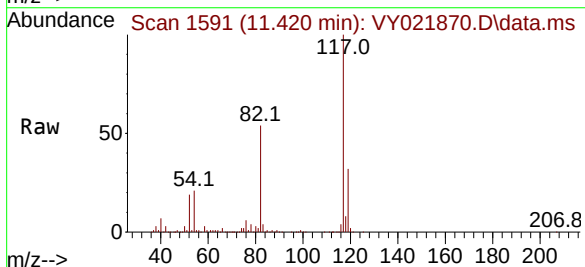




#67
Ethyl Benzene
Concen: 11.682 ug/l
RT: 11.517 min Scan# 1607
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion: 91 Resp: 226636
Ion Ratio Lower Upper
91 100
106 30.3 24.6 36.8

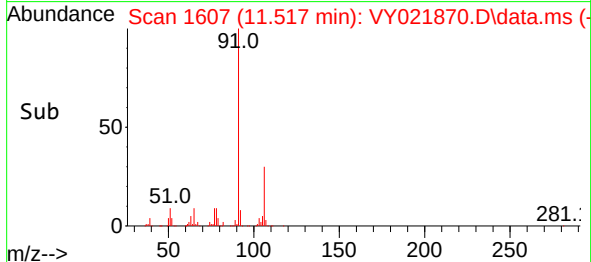

#68
m/p-Xylenes
Concen: 51.794 ug/l
RT: 11.627 min Scan# 1625
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion: 106 Resp: 384772
Ion Ratio Lower Upper
106 100
91 201.8 162.4 243.6


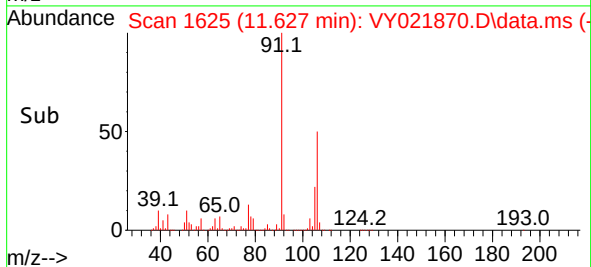

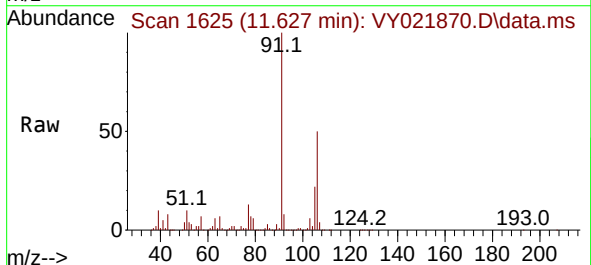




#69
o-Xylene
Concen: 42.341 ug/l
RT: 11.956 min Scan# 1679
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion:106 Resp: 290354
Ion Ratio Lower Upper
106 100
91 216.1 106.7 319.9

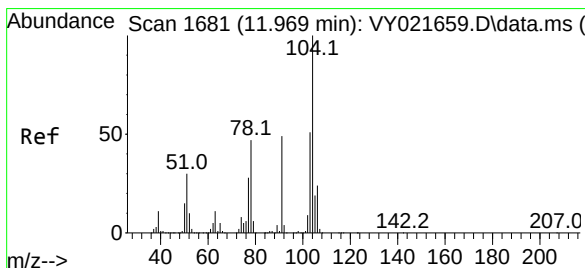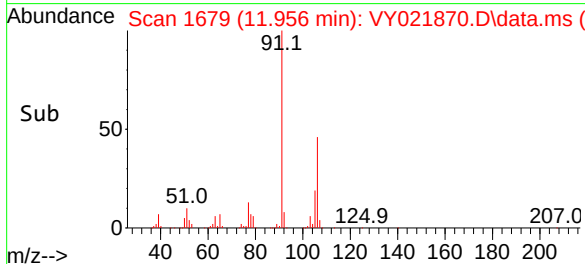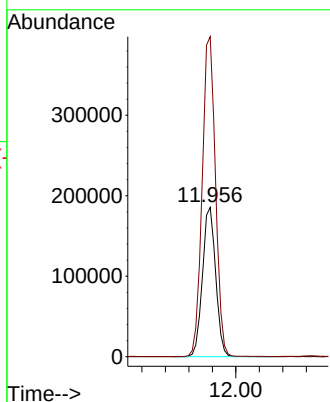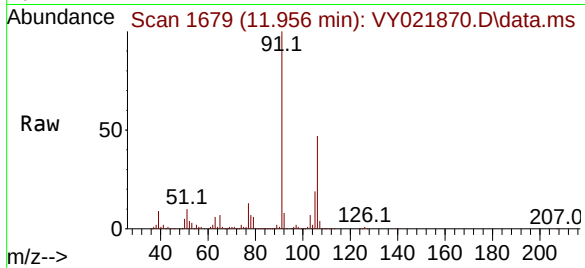

#70
Styrene
Concen: 1.381 ug/l
RT: 11.956 min Scan# 1679
Delta R.T. -0.012 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion:104 Resp: 15792
Ion Ratio Lower Upper
104 100
78 290.3 40.8 61.2#
103 258.8 44.2 66.2#


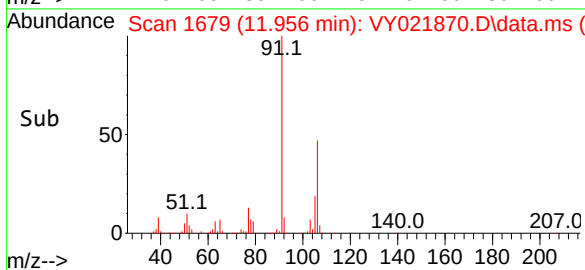
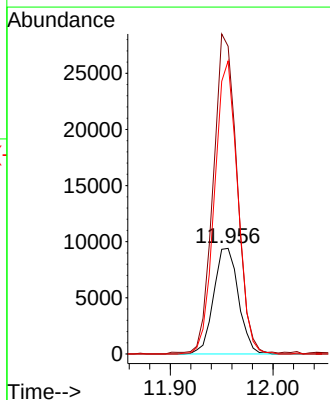
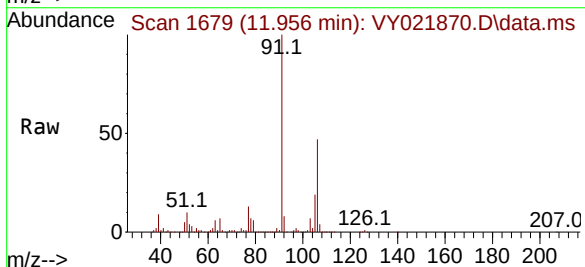


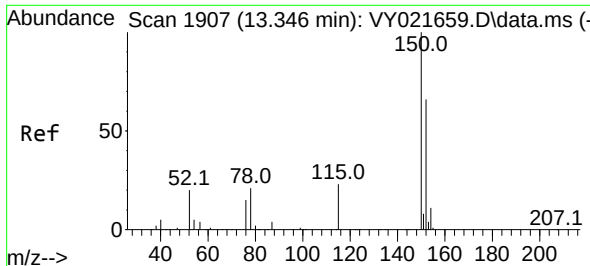

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion:152 Resp: 206269
Ion Ratio Lower Upper
152 100
115 58.4 28.8 86.5
150 154.3 0.0 348.4

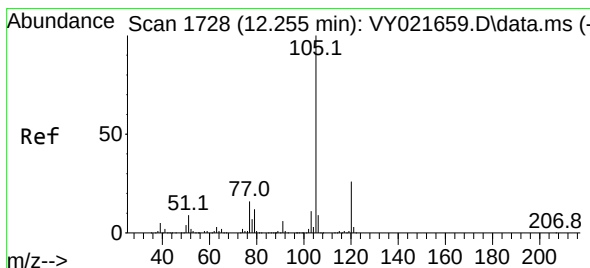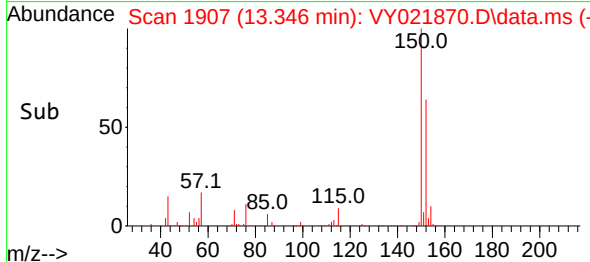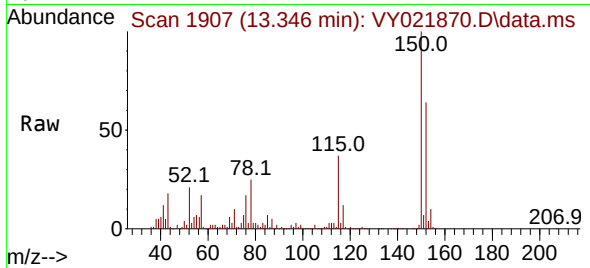

#73
Isopropylbenzene
Concen: 9.912 ug/l
RT: 12.255 min Scan# 1728
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion:105 Resp: 151852
Ion Ratio Lower Upper
105 100
120 26.3 13.2 39.5

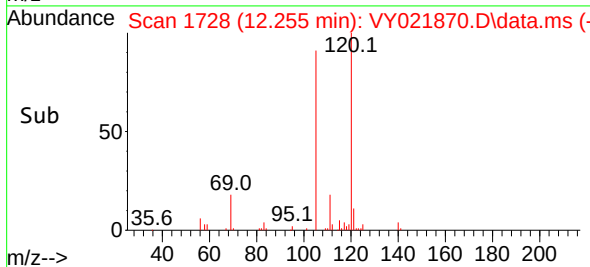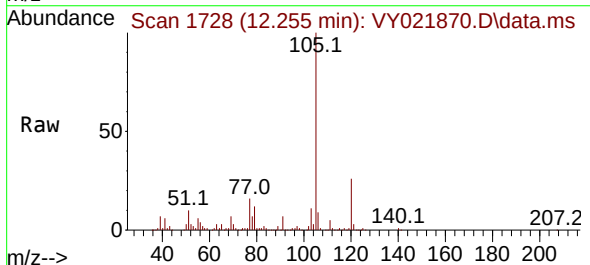



#74

N-amy1 acetate

Concen: 7.760 ug/l

RT: 12.048 min Scan# 1

Delta R.T. -0.024 min

Lab File: VY021870.D

Acq: 14 Apr 2025 15:26

Instrument :

MSVOA_Y

ClientSampleId :

OR-01-41125

Tgt Ion: 43 Resp: 27902





Ion Ratio Lower Upper

43 100

70 12.6 34.7 52.1#

55 13.0 21.2 31.8#

61 0.0 19.5 29.3#

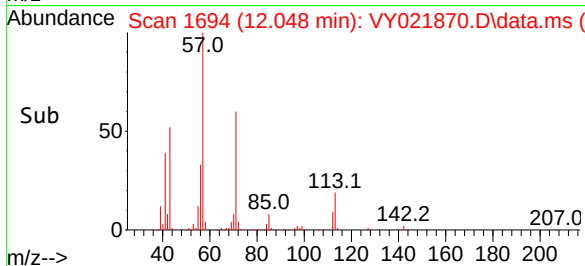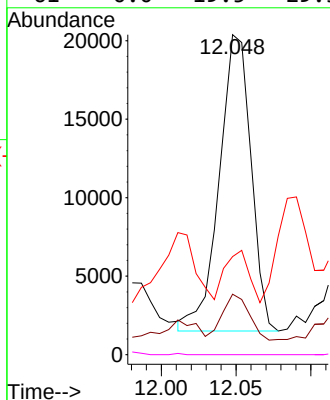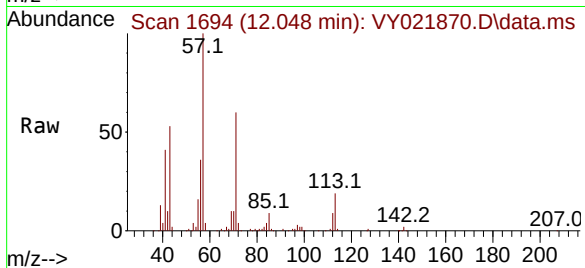

#76

1,2,3-Trichloropropane

Concen: 5.034 ug/l

RT: 12.657 min Scan# 1794

Delta R.T. 0.104 min

Lab File: VY021870.D




Acq: 14 Apr 2025 15:26


Tgt Ion: 75 Resp: 10292

Ion Ratio Lower Upper

75 100

77 1476.7 0.0 0.0#

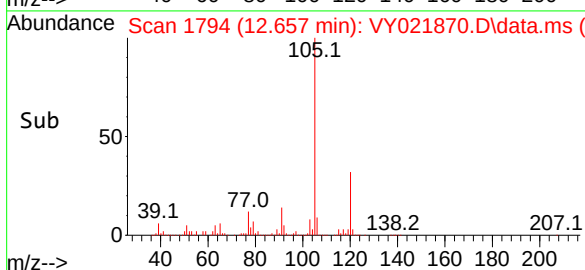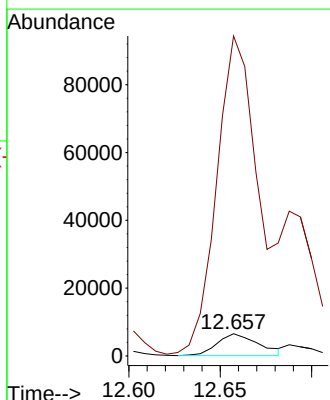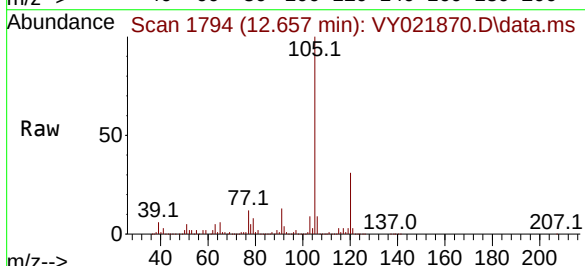

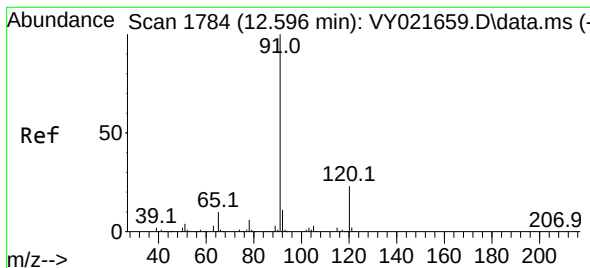

#78

n-propylbenzene

Concen: 20.829 ug/l

RT: 12.596 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY021870.D

Acq: 14 Apr 2025 15:26

Instrument :

MSVOA_Y

ClientSampleId :





OR-01-41125

Tgt Ion: 91 Resp: 383650

Ion Ratio Lower Upper

91 100

120 22.5 11.3 33.9

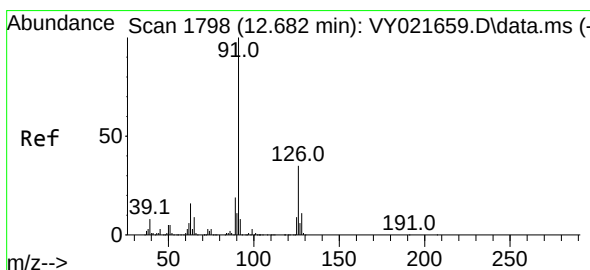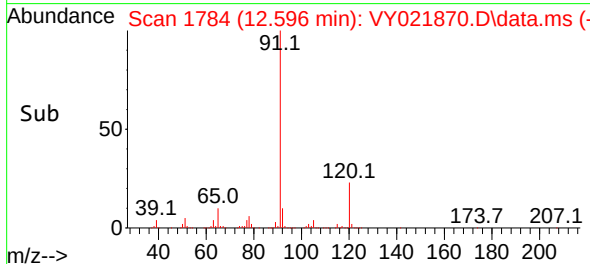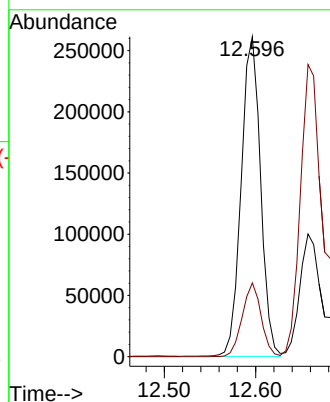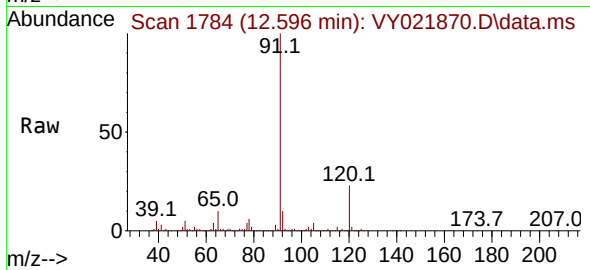

#79

2-Chlorotoluene

Concen: 4.631 ug/l

RT: 12.694 min Scan# 1800

Delta R.T. 0.012 min

Lab File: VY021870.D




Acq: 14 Apr 2025 15:26


Tgt Ion: 91 Resp: 49537

Ion Ratio Lower Upper

91 100

126 0.0 17.3 52.0#


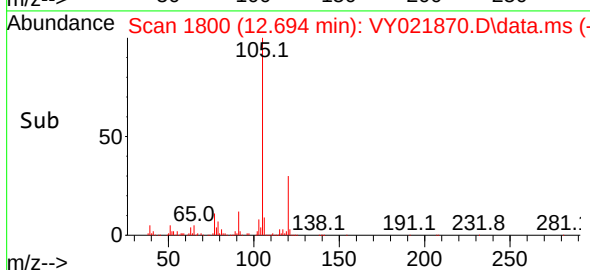
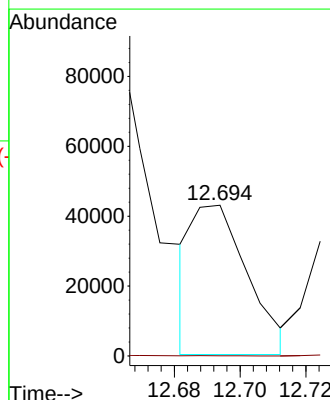
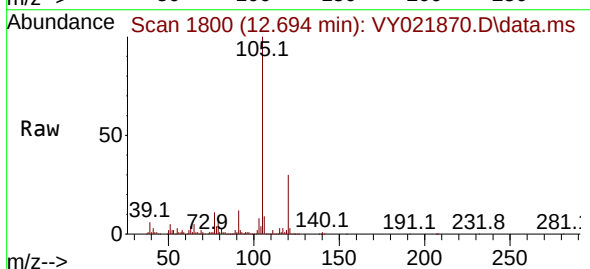




#80
 1,3,5-Trimethylbenzene
 Concen: 67.720 ug/l
 RT: 12.737 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VY021870.D
 Acq: 14 Apr 2025 15:26




Instrument :
 MSVOA_Y
 ClientSampleId :
 OR-01-41125


Tgt Ion:105 Resp: 847933
 Ion Ratio Lower Upper
 105 100
 120 48.5 24.5 73.5

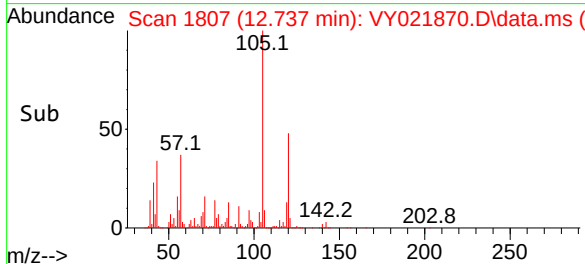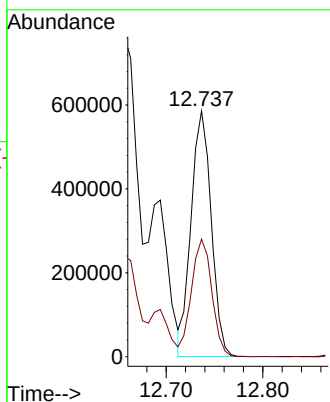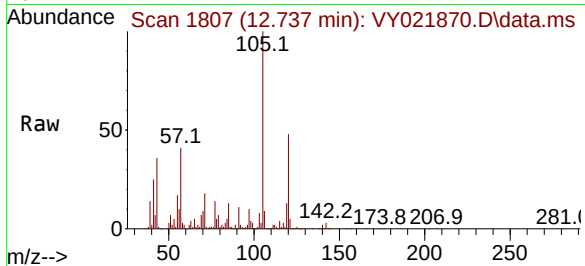

#81
 trans-1,4-Dichloro-2-butene
 Concen: 129.299 ug/l
 RT: 12.407 min Scan# 1753
 Delta R.T. 0.104 min
 Lab File: VY021870.D
 Acq: 14 Apr 2025 15:26

Tgt Ion: 75 Resp: 114736
 Ion Ratio Lower Upper
 75 100
 53 0.6 76.1 114.1#
 89 0.0 36.2 54.4#


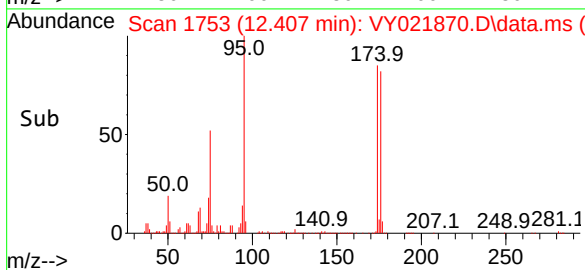
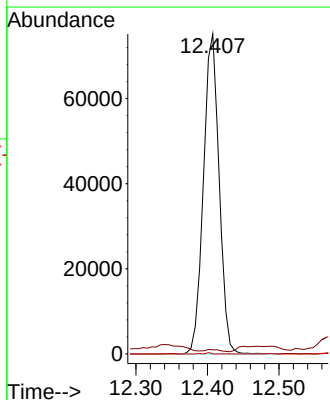
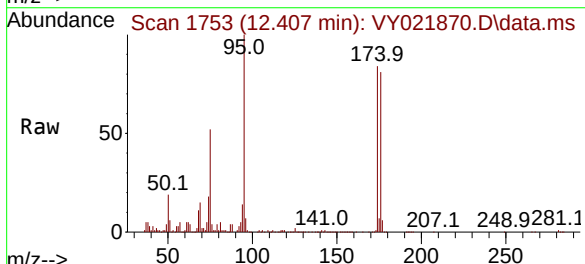




#82
4-Chlorotoluene
Concen: 8.514 ug/l
RT: 12.737 min Scan# 1807
Delta R.T. -0.043 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion: 91 Resp: 94957
Ion Ratio Lower Upper
91 100
126 1.5 17.0 50.9#

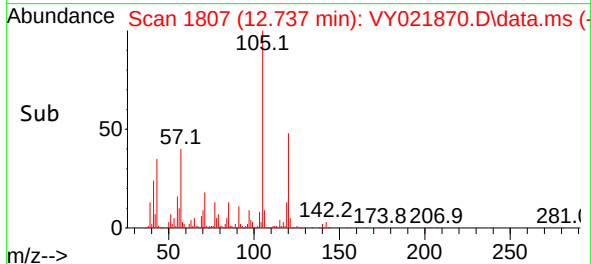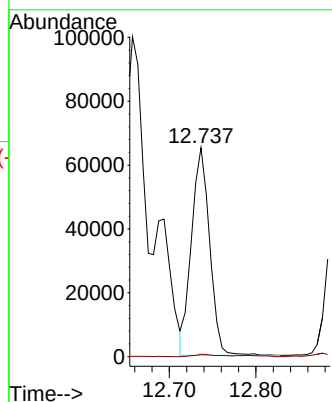

#83
tert-Butylbenzene
Concen: 24.248 ug/l
RT: 13.041 min Scan# 1857
Delta R.T. 0.043 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion: 119 Resp: 270432
Ion Ratio Lower Upper
119 100
91 87.7 32.6 97.7
134 0.0 13.2 39.6#


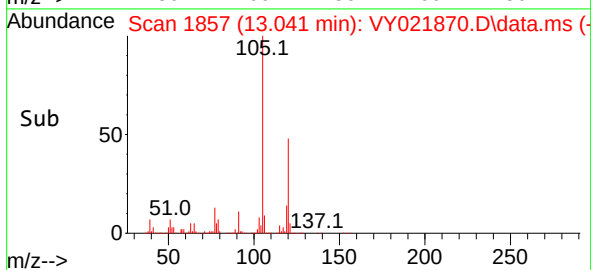

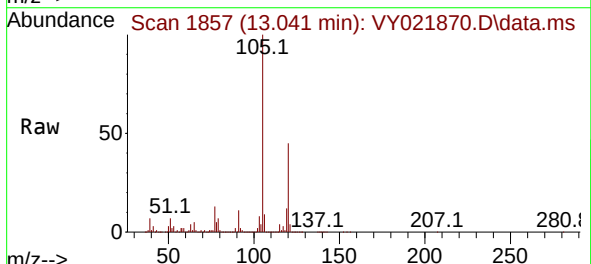




#84
1,2,4-Trimethylbenzene
Concen: 178.891 ug/l
RT: 13.041 min Scan# 1857
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26




Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125


Tgt Ion:105 Resp: 2213851
Ion Ratio Lower Upper
105 100
120 45.7 22.7 68.1

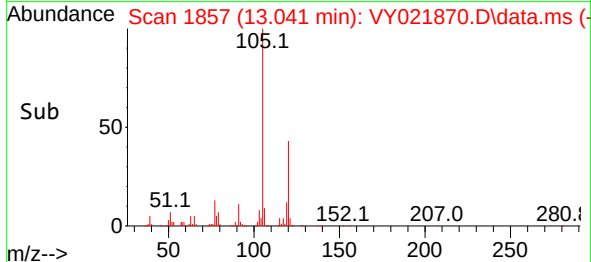

#85
sec-Butylbenzene
Concen: 19.656 ug/l
RT: 13.176 min Scan# 1879
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Tgt Ion:105 Resp: 320362
Ion Ratio Lower Upper
105 100
134 25.9 10.1 30.1


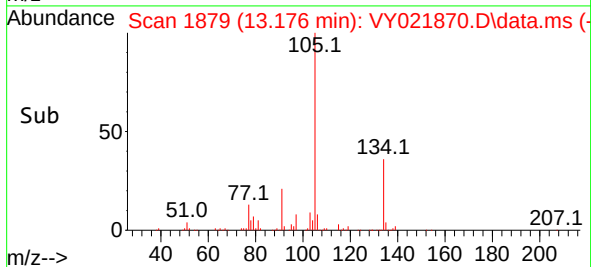

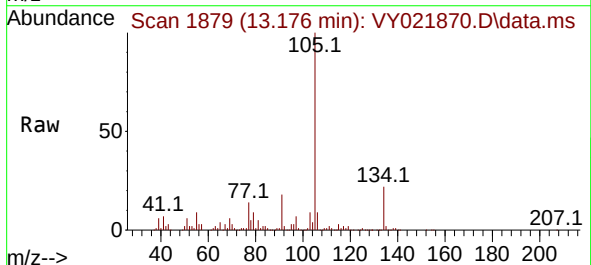


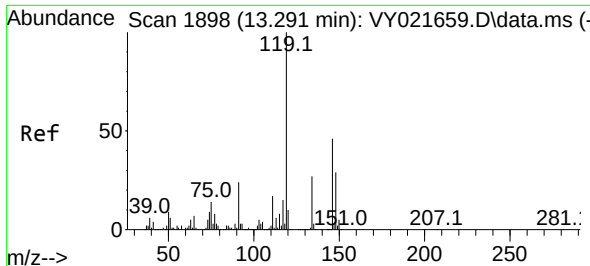

#86
 p-Isopropyltoluene
 Concen: 17.946 ug/l
 RT: 13.291 min Scan# 1898
 Delta R.T. -0.000 min
 Lab File: VY021870.D
 Acq: 14 Apr 2025 15:26




Instrument :
 MSVOA_Y
 ClientSampleId :
 OR-01-41125


Tgt Ion:119 Resp: 241739
 Ion Ratio Lower Upper
 119 100
 134 26.3 13.2 39.5
 91 23.6 12.0 36.0

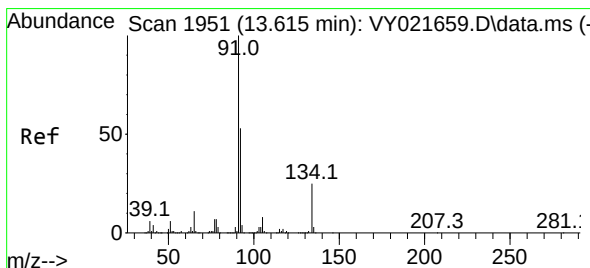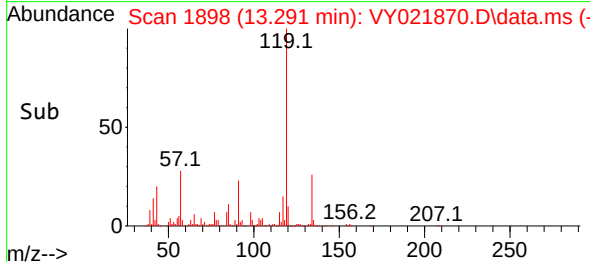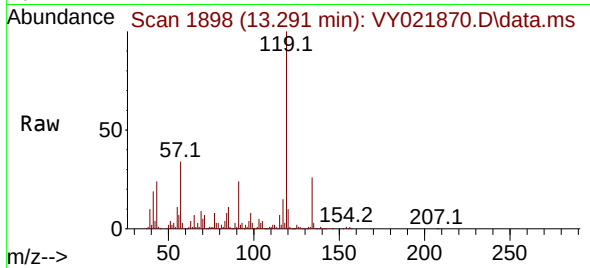

#89
 n-Butylbenzene
 Concen: 18.191 ug/l
 RT: 13.614 min Scan# 1951
 Delta R.T. -0.000 min
 Lab File: VY021870.D
 Acq: 14 Apr 2025 15:26

Tgt Ion: 91 Resp: 226625
 Ion Ratio Lower Upper
 91 100
 92 66.3 26.4 79.2
 134 0.0 12.8 38.4#

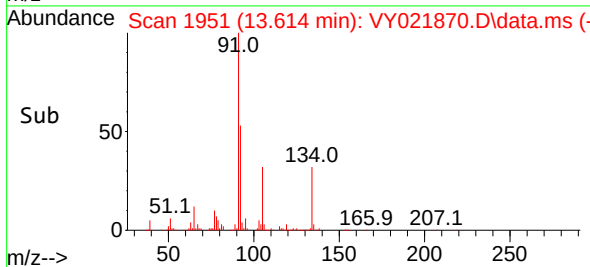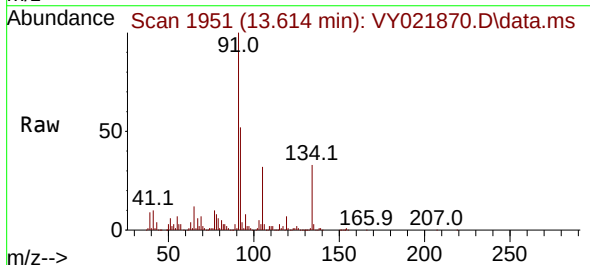



#90

Hexachloroethane

Concen: 26.463 ug/l

RT: 13.895 min Scan# 1997

Delta R.T. 0.018 min

Lab File: VY021870.D

Acq: 14 Apr 2025 15:26

Instrument :

MSVOA_Y

ClientSampleId :





OR-01-41125

Tgt Ion:117 Resp: 78118

Ion Ratio Lower Upper

117 100

201 0.0 37.4 112.1#

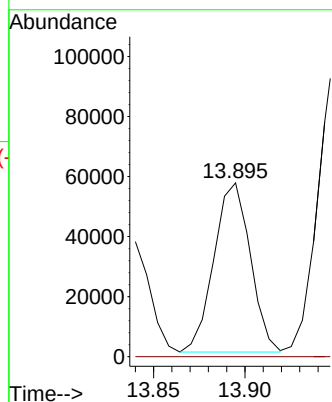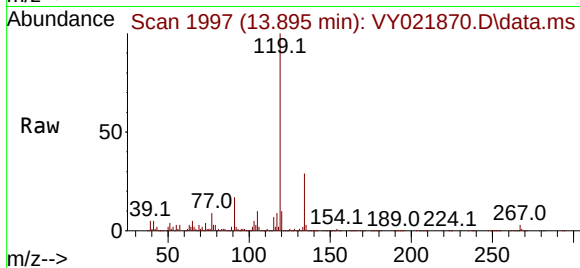

#92

1,2-Dibromo-3-Chloropropane

Concen: 12.579 ug/l

RT: 14.255 min Scan# 2056

Delta R.T. -0.018 min

Lab File: VY021870.D

Acq: 14 Apr 2025 15:26




Tgt Ion: 75 Resp: 5370


Ion Ratio Lower Upper

75 100

155 0.0 43.0 128.8#


157 0.0 54.0 162.0#

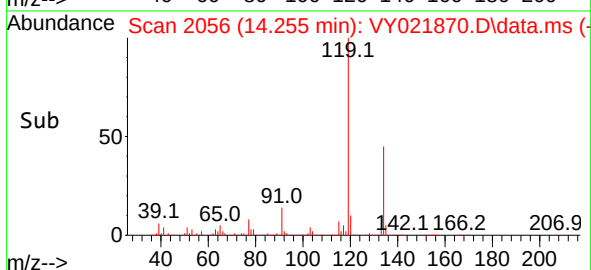

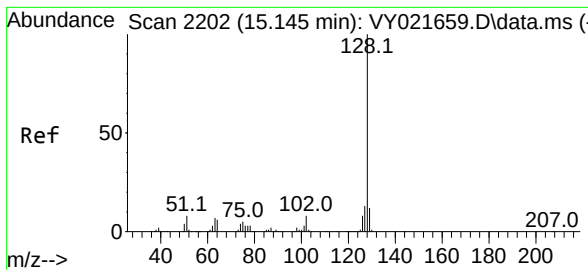

#95
Naphthalene
Concen: 42.292 ug/l
RT: 15.145 min Scan# 21
Delta R.T. -0.000 min
Lab File: VY021870.D
Acq: 14 Apr 2025 15:26

Instrument :
MSVOA_Y
ClientSampleId :
OR-01-41125

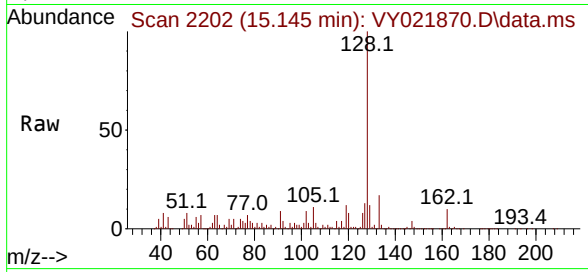

Tgt Ion:128 Resp: 239829
Ion Ratio Lower Upper
128 100
127 14.2 10.8 16.2
129 13.4 8.8 13.2#

