
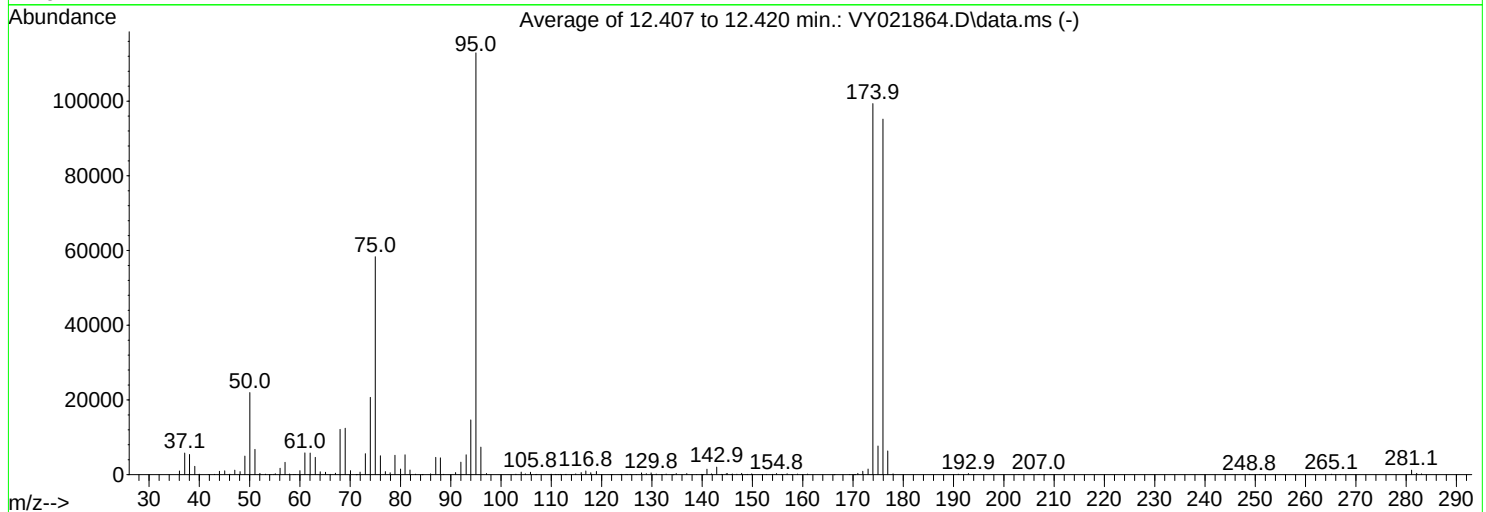


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041425\
Data File : VY021864.D
Acq On : 14 Apr 2025 08:27
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Title : SW846 8260
Last Update : Fri Mar 28 02:30:29 2025

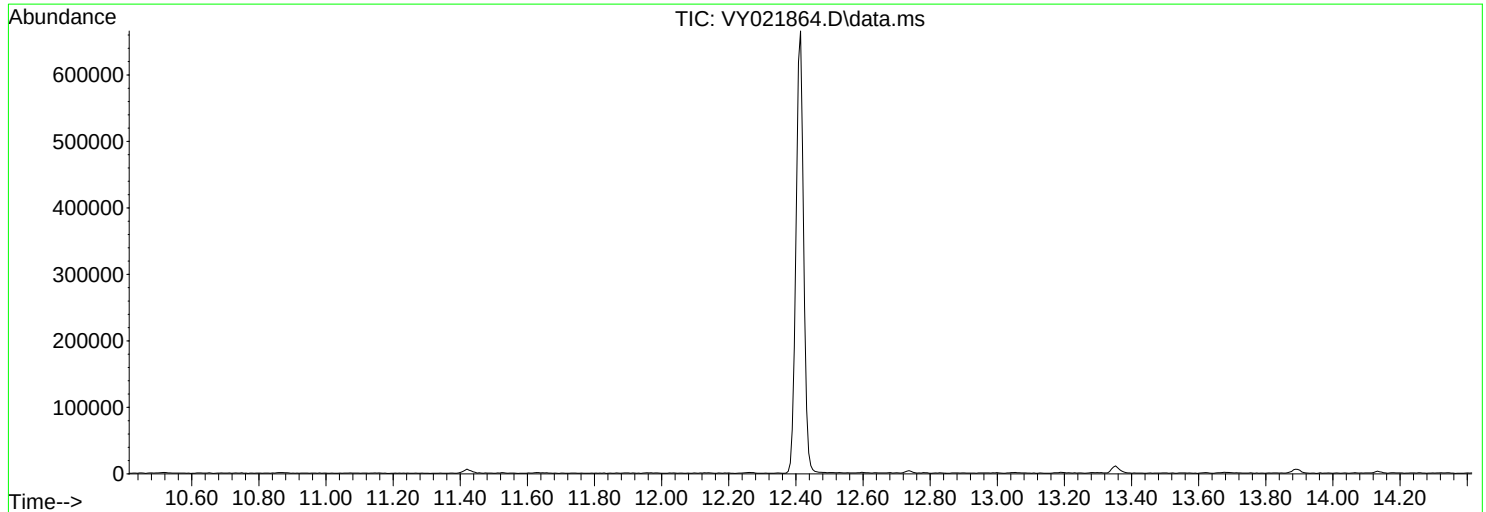

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	21992	PASS
75	95	30	60	51.7	58347	PASS
95	95	100	100	100.0	112928	PASS
96	95	5	9	6.5	7376	PASS
173	174	0.00	2	1.5	1511	PASS
174	95	50	100	87.9	99320	PASS
175	174	5	9	7.7	7648	PASS
176	174	95	101	95.9	95200	PASS
177	176	5	9	6.7	6348	PASS