
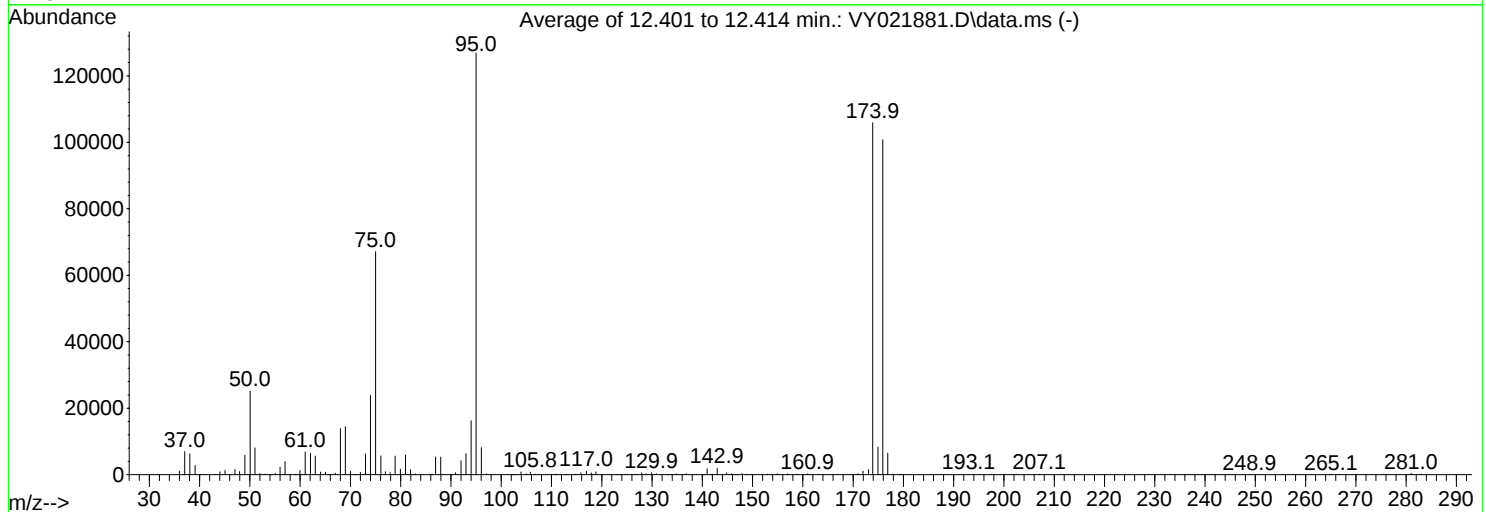


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041525\
Data File : VY021881.D
Acq On : 15 Apr 2025 08:33
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Title : SW846 8260
Last Update : Fri Mar 28 02:30:29 2025

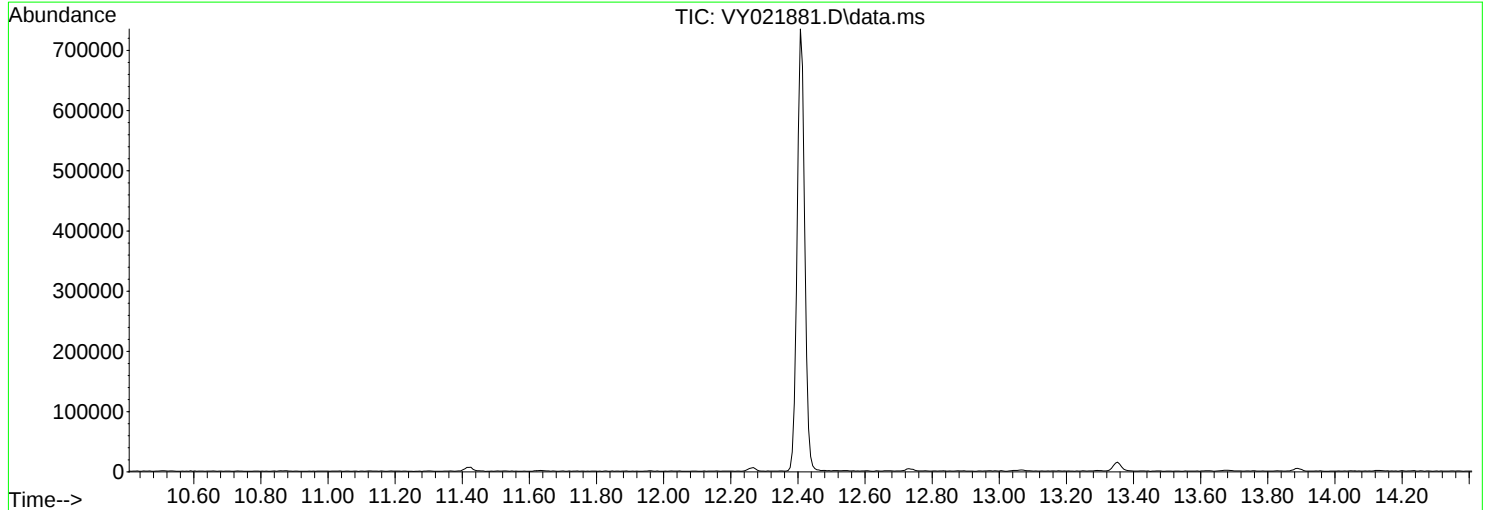

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	25117	PASS
75	95	30	60	52.9	67123	PASS
95	95	100	100	100.0	126925	PASS
96	95	5	9	6.4	8125	PASS
173	174	0.00	2	1.4	1494	PASS
174	95	50	100	83.4	105883	PASS
175	174	5	9	7.8	8305	PASS
176	174	95	101	95.2	100765	PASS
177	176	5	9	6.4	6476	PASS