

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041725\
 Data File : VY021911.D
 Acq On : 17 Apr 2025 15:15
 Operator : SY/MD
 Sample : Q1821-01
 Misc : 5.10g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SOIL-CUTTING

Quant Time: Apr 18 03:59:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 28 02:30:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	227478	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	423982	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	360344	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	133716	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.060	65	121753	49.400	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	98.800%
35) Dibromofluoromethane	7.634	113	139287	50.644	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.280%
50) Toluene-d8	10.109	98	504494	48.217	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.440%
62) 4-Bromofluorobenzene	12.407	95	139357	39.377	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	78.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041725\
Data File : VY021911.D
Acq On : 17 Apr 2025 15:15
Operator : SY/MD
Sample : Q1821-01
Misc : 5.10g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SOIL-CUTTING

Quant Time: Apr 18 03:59:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 28 02:30:29 2025
Response via : Initial Calibration




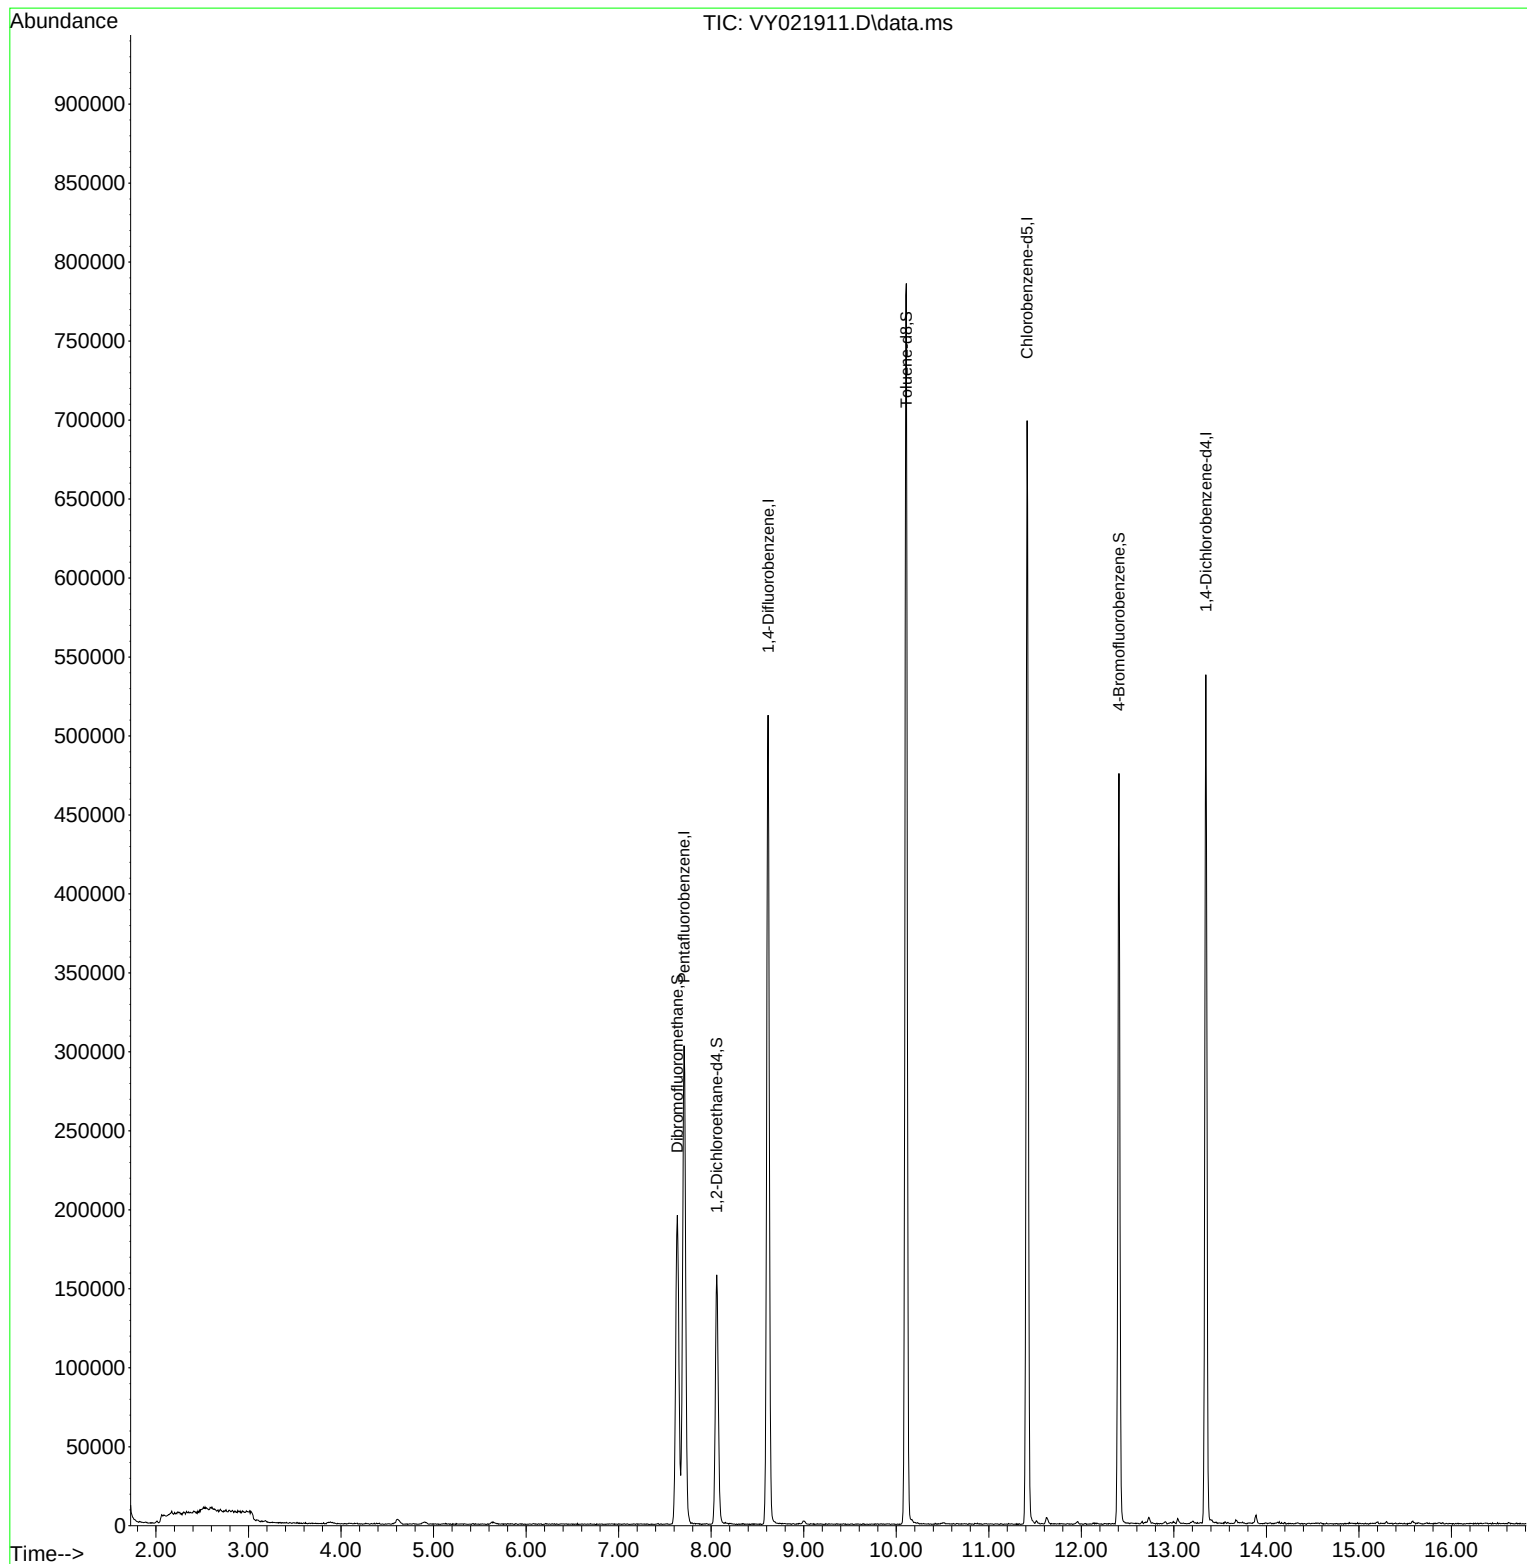


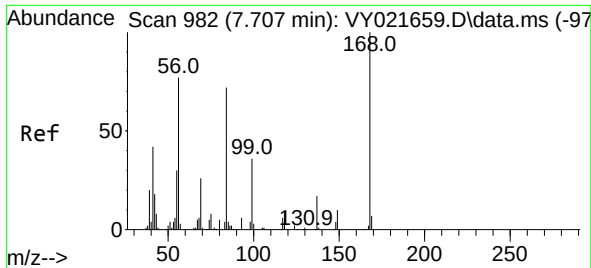

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. -0.000 min
Lab File: VY021911.D
Acq: 17 Apr 2025 15:15




Instrument :
MSVOA_Y
ClientSampleId :
SOIL-CUTTING


Tgt Ion:168 Resp: 227478
Ion Ratio Lower Upper
168 100
99 57.0 46.7 70.1

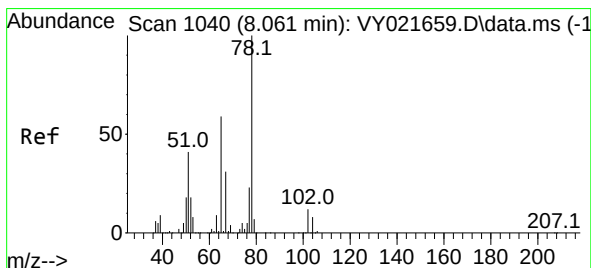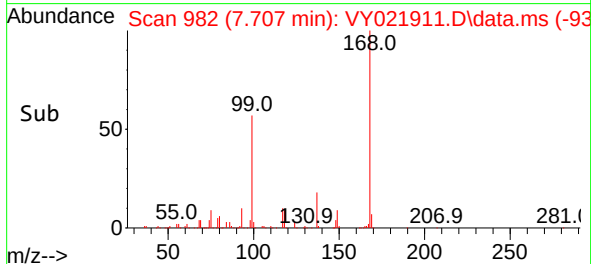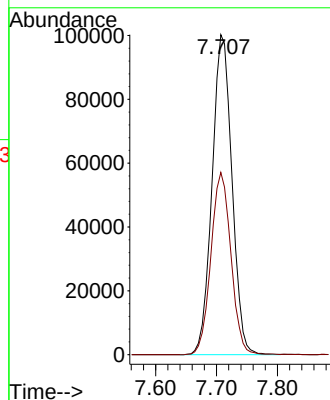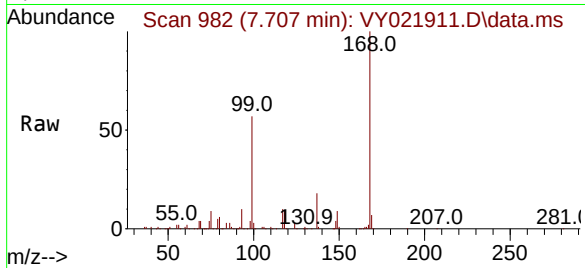

#33
1,2-Dichloroethane-d4
Concen: 49.400 ug/l
RT: 8.060 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY021911.D
Acq: 17 Apr 2025 15:15

Tgt Ion: 65 Resp: 121753
Ion Ratio Lower Upper
65 100
67 52.6 0.0 104.6


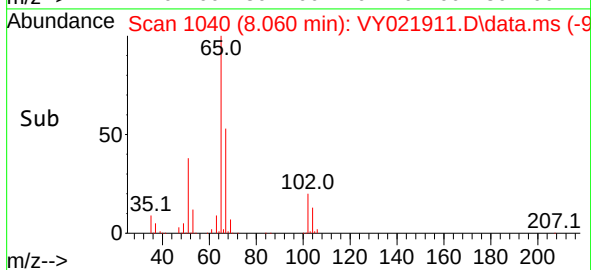
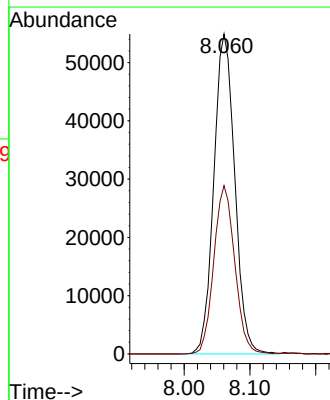
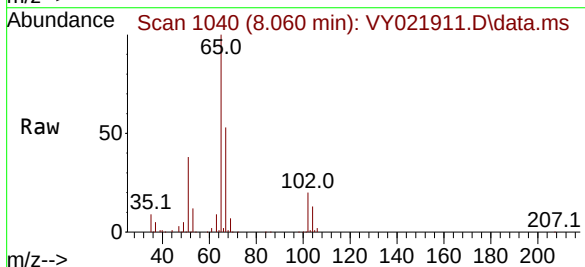


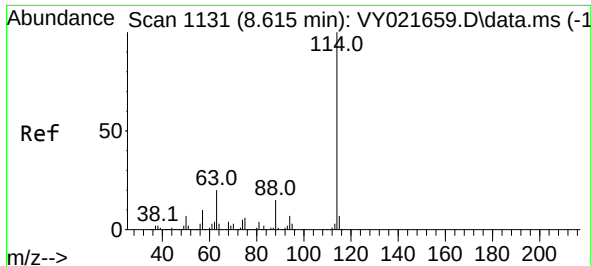

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.615 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VY021911.D
Acq: 17 Apr 2025 15:15




Instrument :
MSVOA_Y
ClientSampleId :
SOIL-CUTTING


Tgt Ion:114 Resp: 423982
Ion Ratio Lower Upper
114 100
63 20.3 0.0 40.2
88 15.1 0.0 29.8

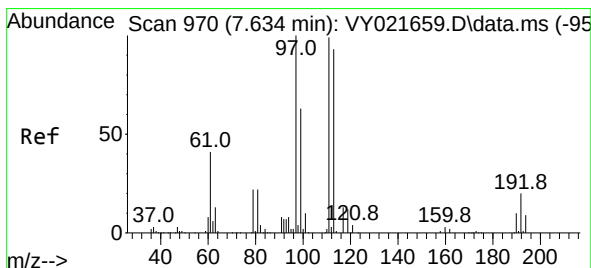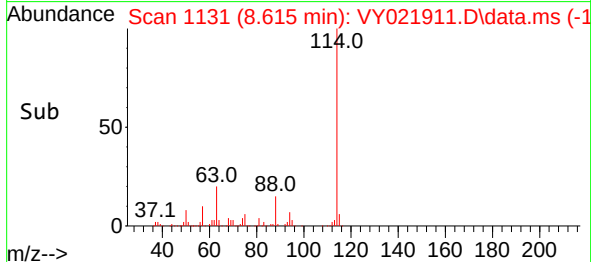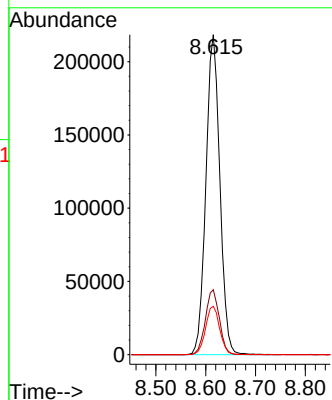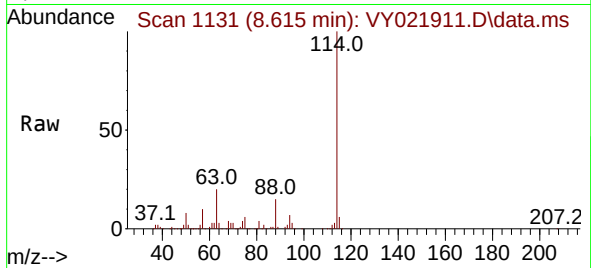

#35
Dibromofluoromethane
Concen: 50.644 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.000 min
Lab File: VY021911.D
Acq: 17 Apr 2025 15:15

Tgt Ion:113 Resp: 139287
Ion Ratio Lower Upper
113 100
111 102.3 82.6 123.8
192 19.7 16.2 24.4


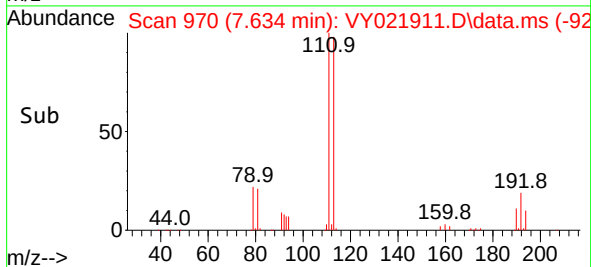
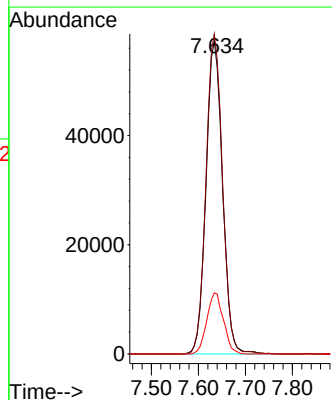
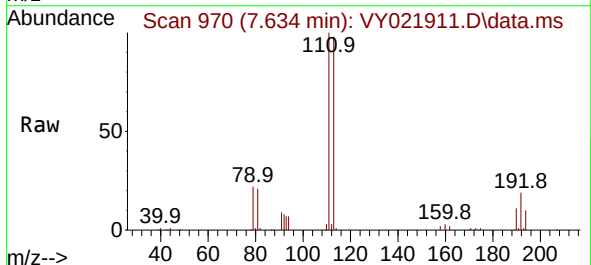


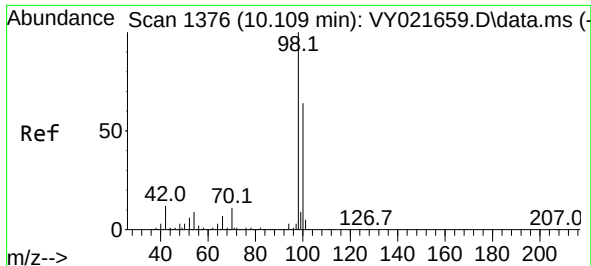

#50
Toluene-d8
Concen: 48.217 ug/l
RT: 10.109 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY021911.D
Acq: 17 Apr 2025 15:15




Instrument :
MSVOA_Y
ClientSampleId :
SOIL-CUTTING


Tgt Ion: 98 Resp: 504494
Ion Ratio Lower Upper
98 100
100 64.6 52.1 78.1

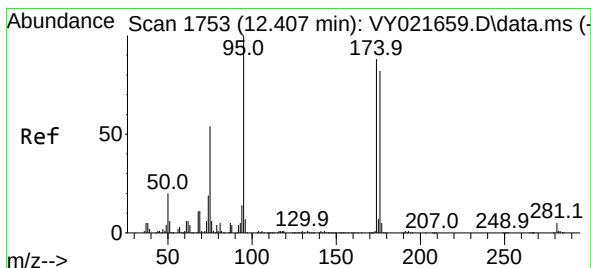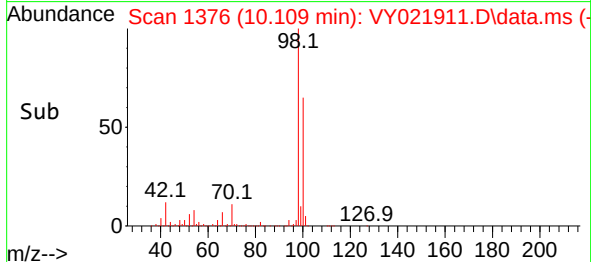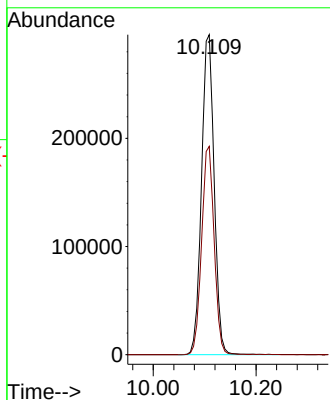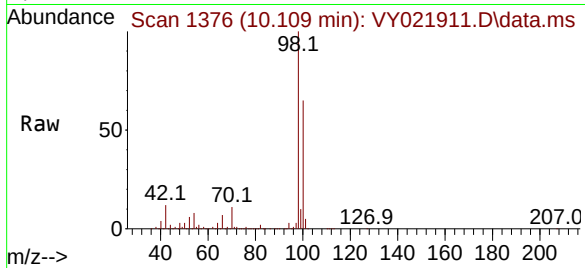

#62
4-Bromofluorobenzene
Concen: 39.377 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY021911.D
Acq: 17 Apr 2025 15:15

Tgt Ion: 95 Resp: 139357
Ion Ratio Lower Upper
95 100
174 83.9 0.0 170.8
176 81.5 0.0 162.0

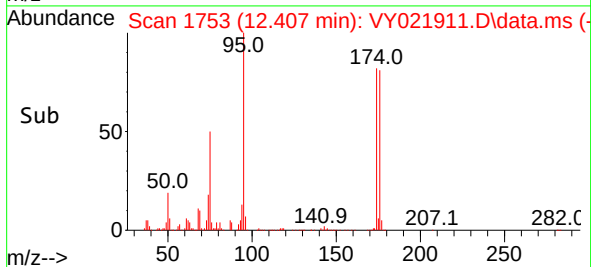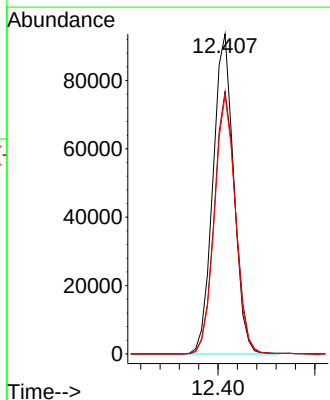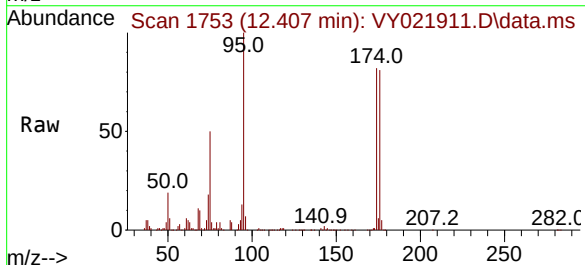

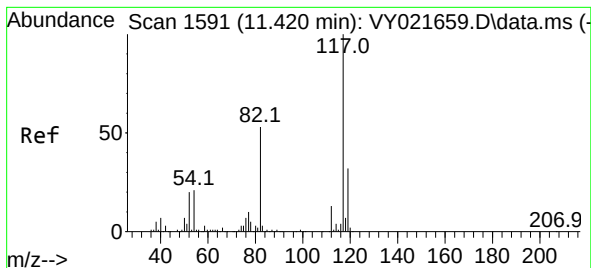

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY021911.D


Acq: 17 Apr 2025 15:15

Instrument :

MSVOA_Y

ClientSampleId :

SOIL-CUTTING

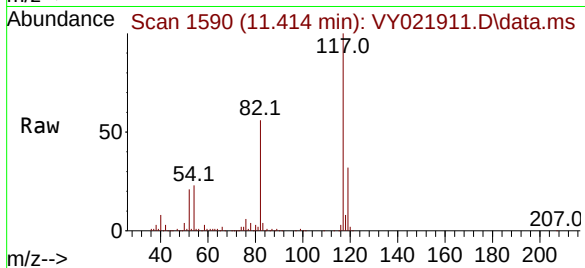




Tgt Ion:117 Resp: 360344

Ion Ratio Lower Upper

117 100

82 56.0 42.8 64.2

119 32.0 25.7 38.5

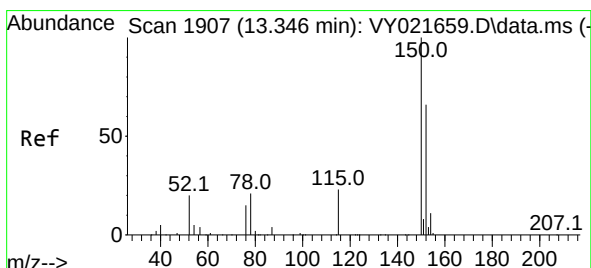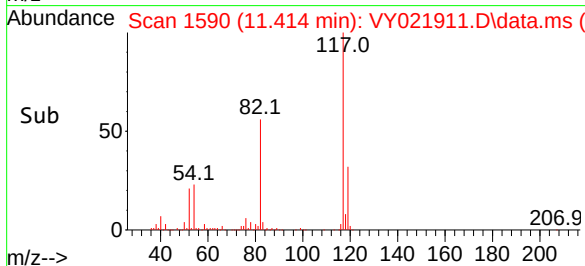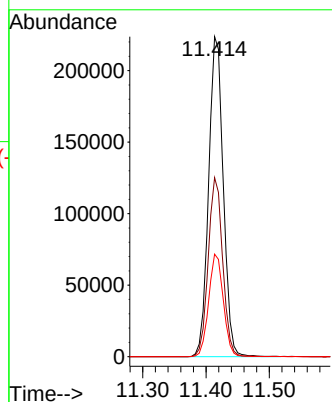

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VY021911.D

Acq: 17 Apr 2025 15:15

Tgt Ion:152 Resp: 133716

Ion Ratio Lower Upper

152 100

115 57.4 28.8 86.5

150 157.4 0.0 348.4

