

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041825\
 Data File : VY021923.D
 Acq On : 18 Apr 2025 12:13
 Operator : SY/MD
 Sample : Q1830-11
 Misc : 3.87g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SOIL-2

Quant Time: Apr 19 01:11:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 28 02:30:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	221474	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	412378	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	342774	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	122489	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	117585	49.002	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	98.000%
35) Dibromofluoromethane	7.634	113	135042	50.482	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.960%
50) Toluene-d8	10.109	98	494787	48.620	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.240%
62) 4-Bromofluorobenzene	12.407	95	130686	37.966	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	75.940%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041825\
Data File : VY021923.D
Acq On : 18 Apr 2025 12:13
Operator : SY/MD
Sample : Q1830-11
Misc : 3.87g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SOIL-2

Quant Time: Apr 19 01:11:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 28 02:30:29 2025
Response via : Initial Calibration




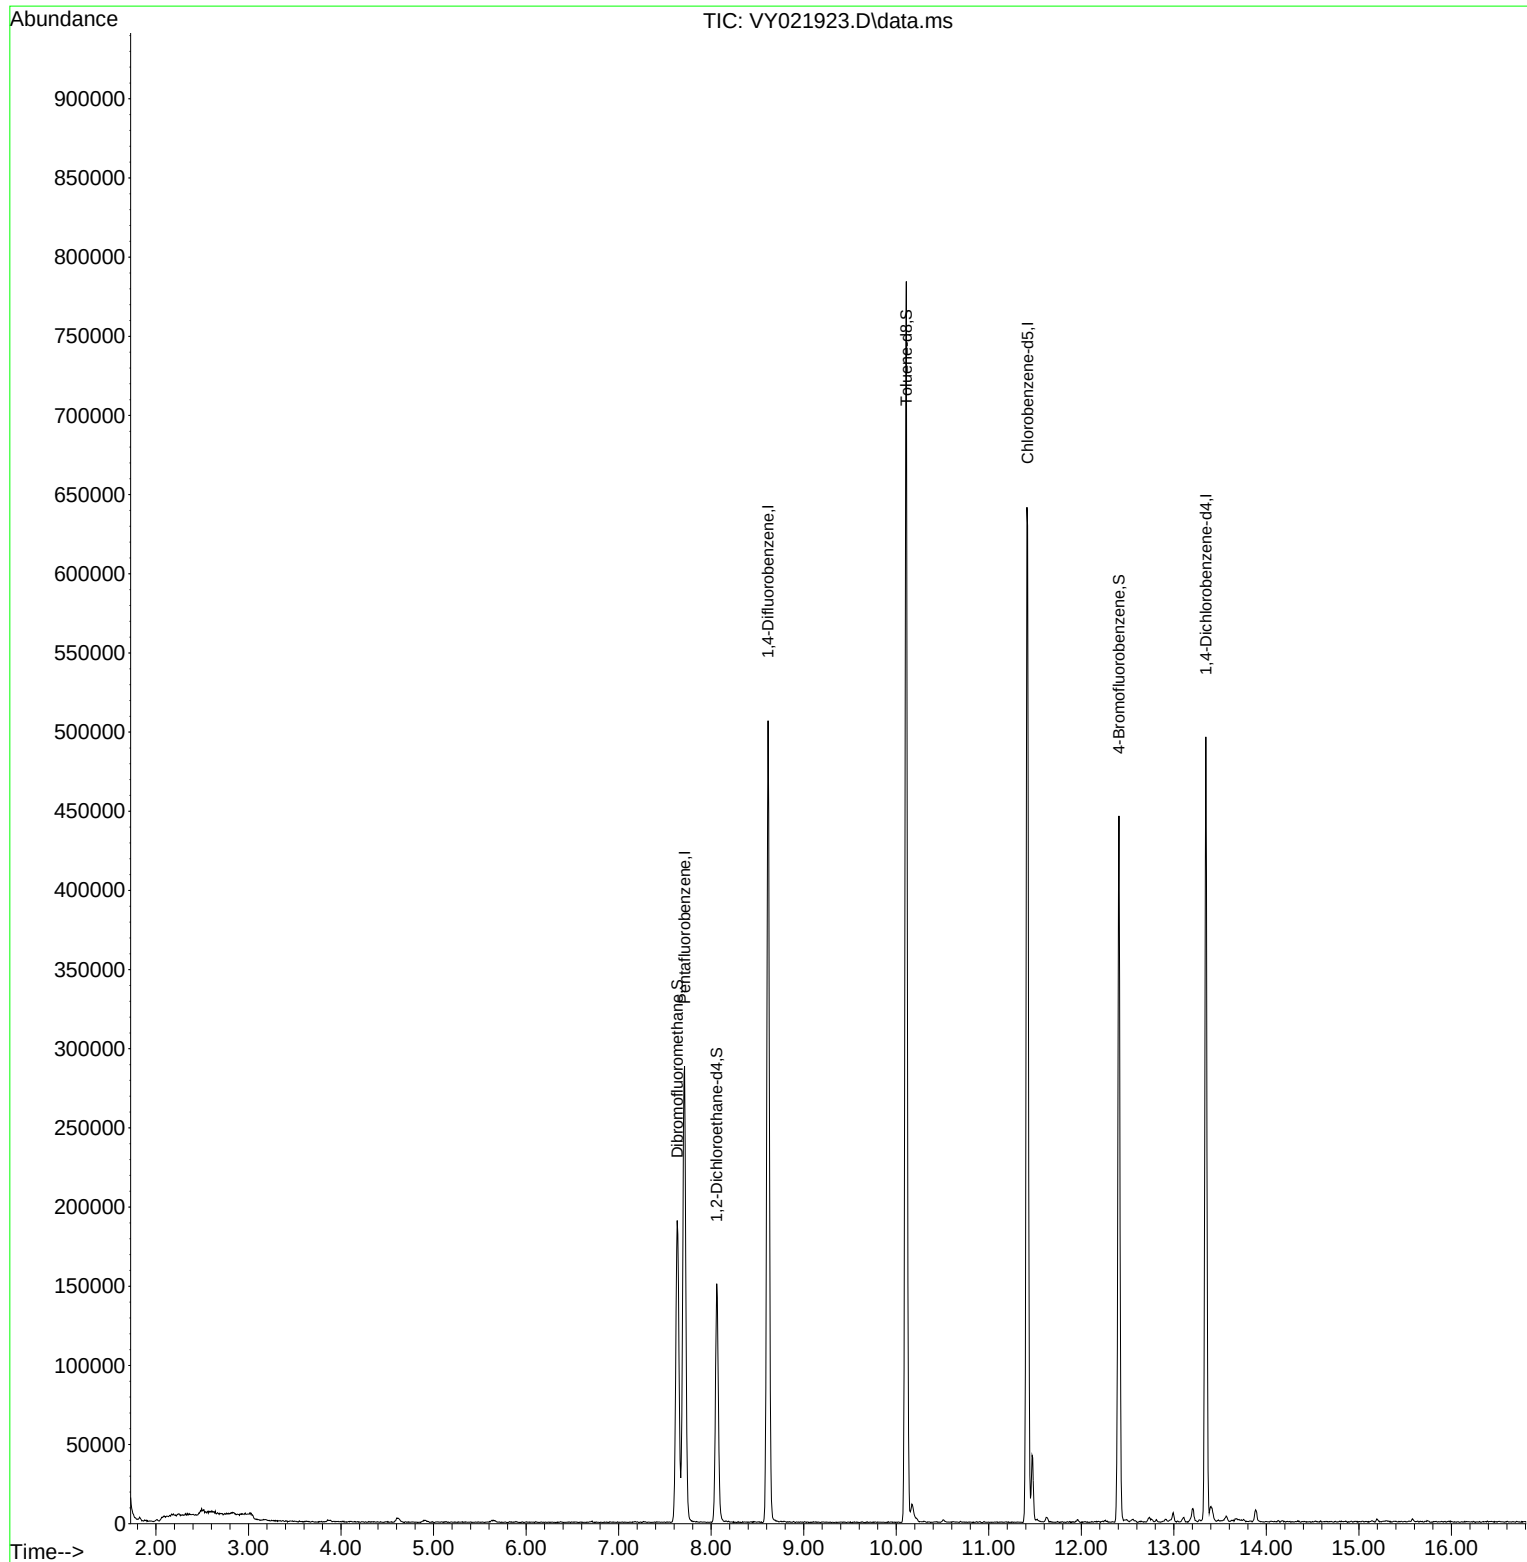


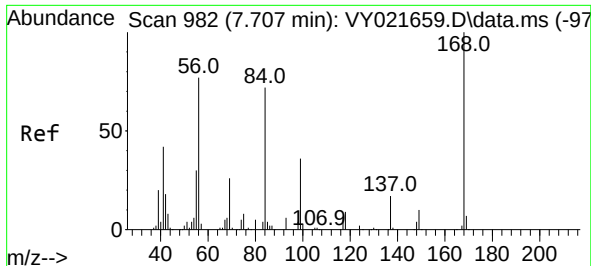

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY021923.D
Acq: 18 Apr 2025 12:13




Instrument :
MSVOA_Y
ClientSampleId :
SOIL-2


Tgt Ion:168 Resp: 221474
Ion Ratio Lower Upper
168 100
99 54.4 46.7 70.1

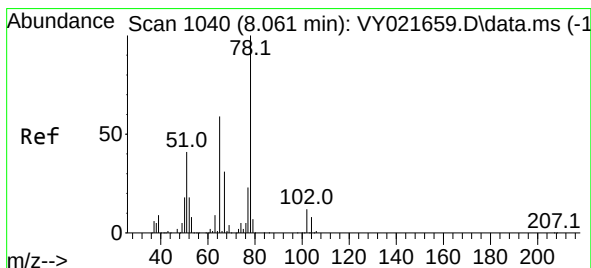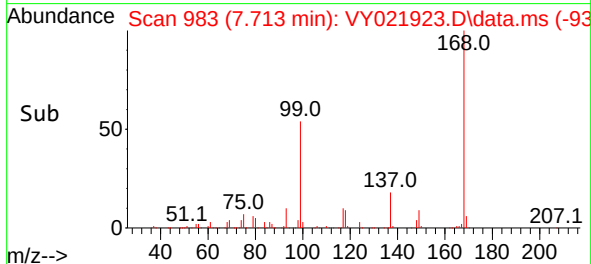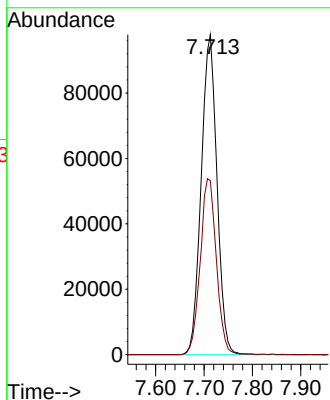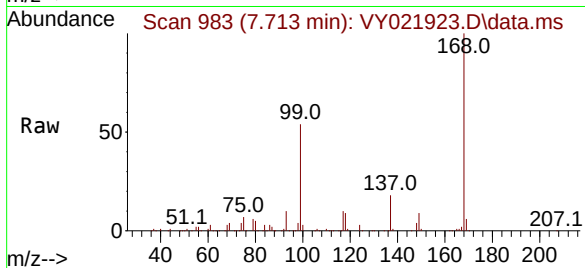

#33
1,2-Dichloroethane-d4
Concen: 49.002 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY021923.D
Acq: 18 Apr 2025 12:13

Tgt Ion: 65 Resp: 117585
Ion Ratio Lower Upper
65 100
67 52.2 0.0 104.6

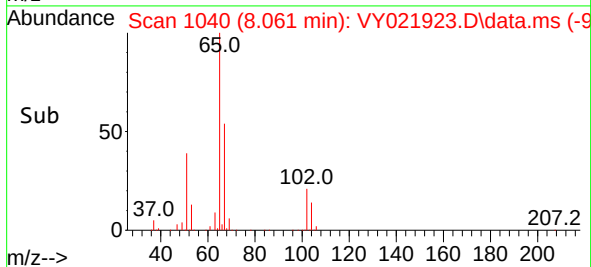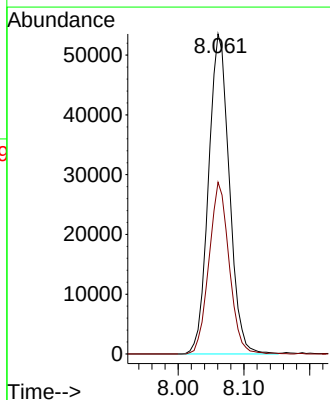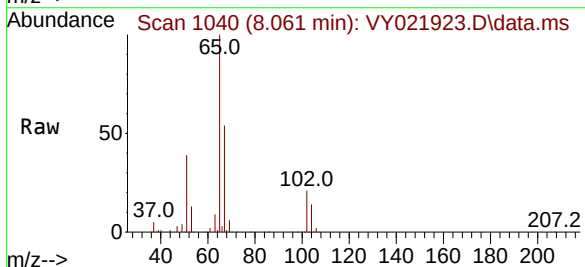

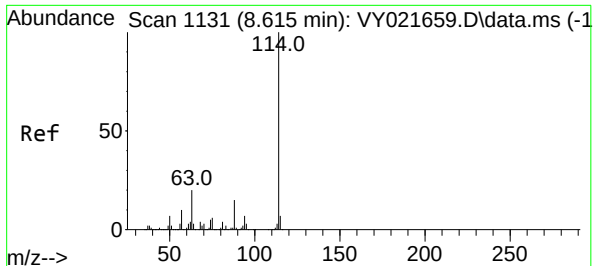

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.615 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VY021923.D

Acq: 18 Apr 2025 12:13

Instrument :

MSVOA_Y

ClientSampleId :

SOIL-2





Tgt Ion:114 Resp: 412378

Ion Ratio Lower Upper

114 100

63 21.0 0.0 40.2

88 15.2 0.0 29.8

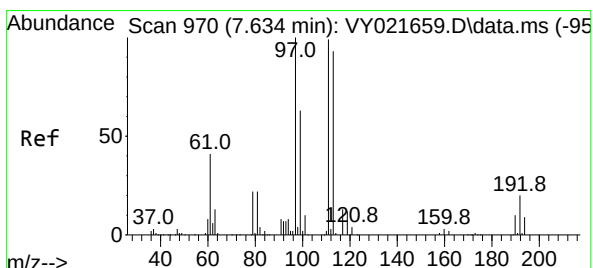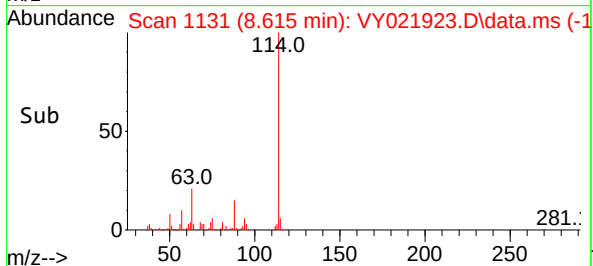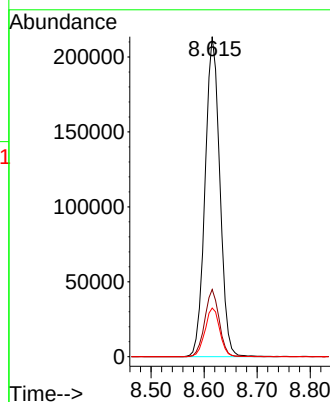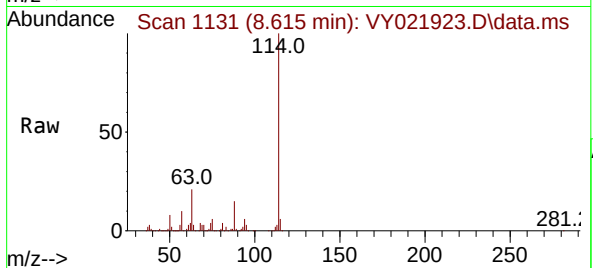

#35

Dibromofluoromethane

Concen: 50.482 ug/l

RT: 7.634 min Scan# 970

Delta R.T. -0.000 min

Lab File: VY021923.D

Acq: 18 Apr 2025 12:13




Tgt Ion:113 Resp: 135042


Ion Ratio Lower Upper

113 100

111 103.7 82.6 123.8

192 19.6 16.2 24.4


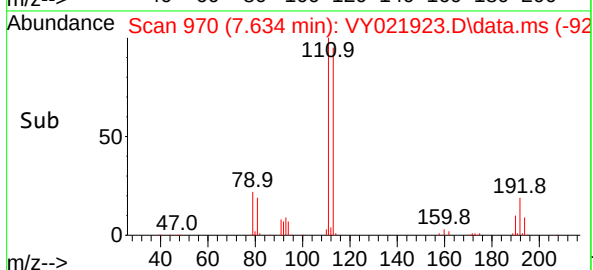
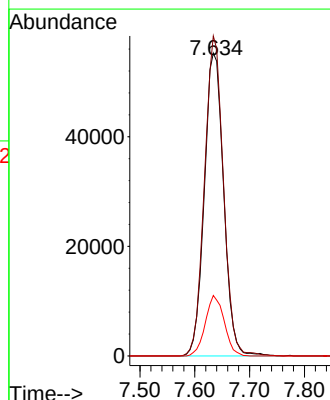
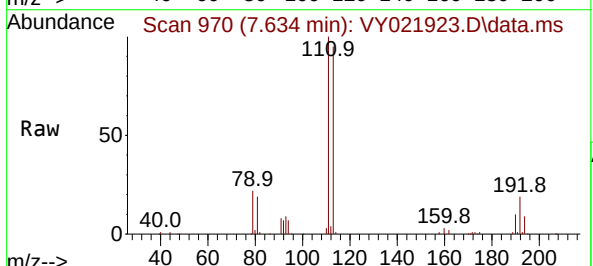


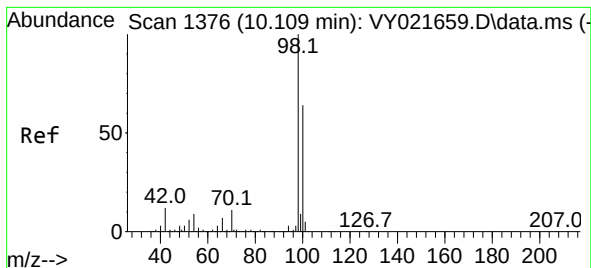

#50
Toluene-d8
Concen: 48.620 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. -0.000 min
Lab File: VY021923.D
Acq: 18 Apr 2025 12:13




Instrument :
MSVOA_Y
ClientSampleId :
SOIL-2


Tgt Ion: 98 Resp: 494787
Ion Ratio Lower Upper
98 100
100 64.4 52.1 78.1

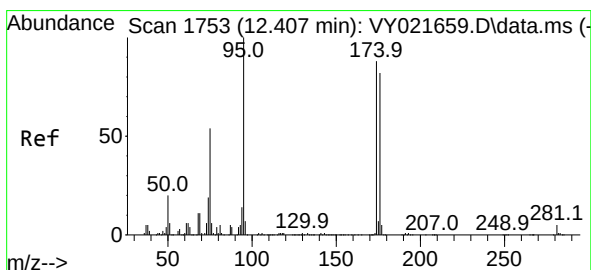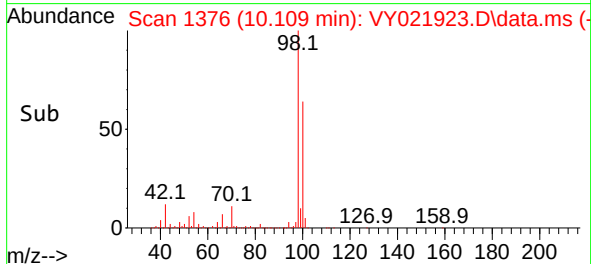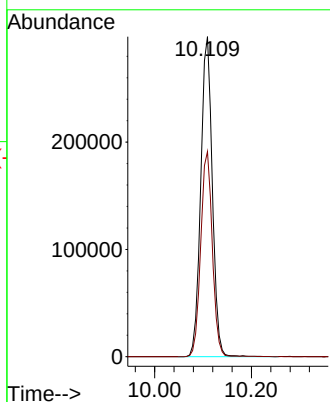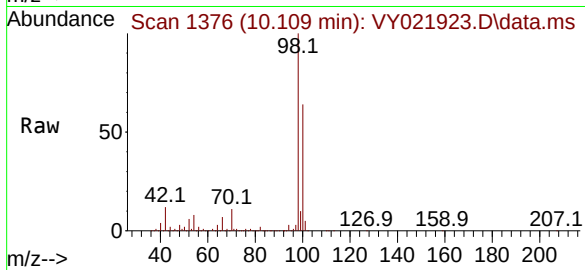

#62
4-Bromofluorobenzene
Concen: 37.966 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY021923.D
Acq: 18 Apr 2025 12:13

Tgt Ion: 95 Resp: 130686
Ion Ratio Lower Upper
95 100
174 85.0 0.0 170.8
176 80.7 0.0 162.0

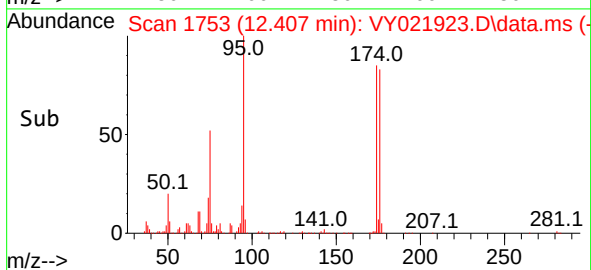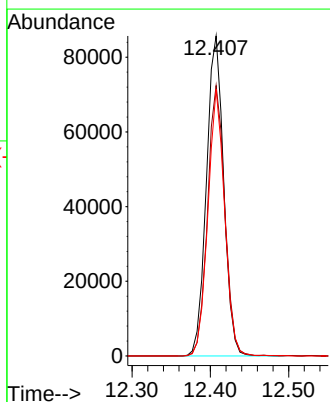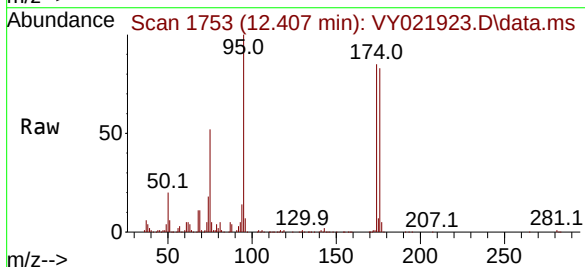

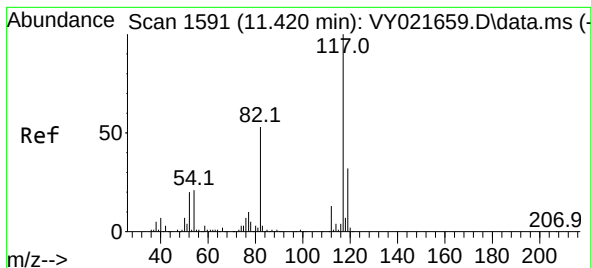

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY021923.D

Acq: 18 Apr 2025 12:13

Instrument :

MSVOA_Y

ClientSampleId :

SOIL-2





Tgt Ion:117 Resp: 342774

Ion Ratio Lower Upper

117 100

82 52.5 42.8 64.2

119 32.2 25.7 38.5

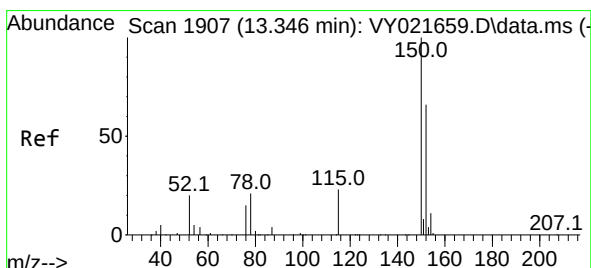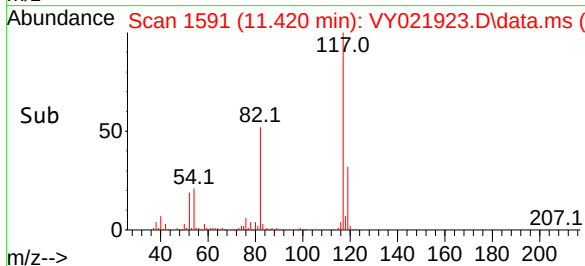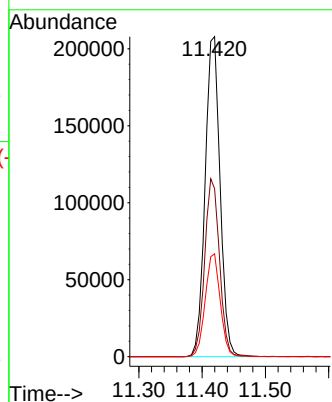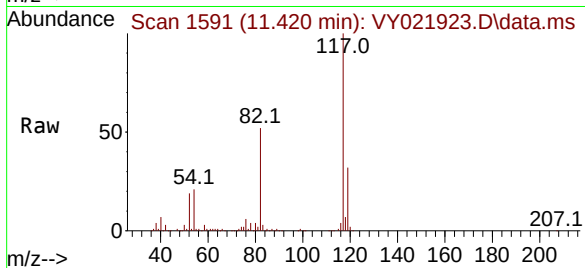

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VY021923.D

Acq: 18 Apr 2025 12:13

Tgt Ion:152 Resp: 122489

Ion Ratio Lower Upper

152 100

115 58.2 28.8 86.5

150 157.0 0.0 348.4

