


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041825\
Data File : VY021915.D
Acq On : 18 Apr 2025 08:15
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Title : SW846 8260
Last Update : Fri Mar 28 02:30:29 2025

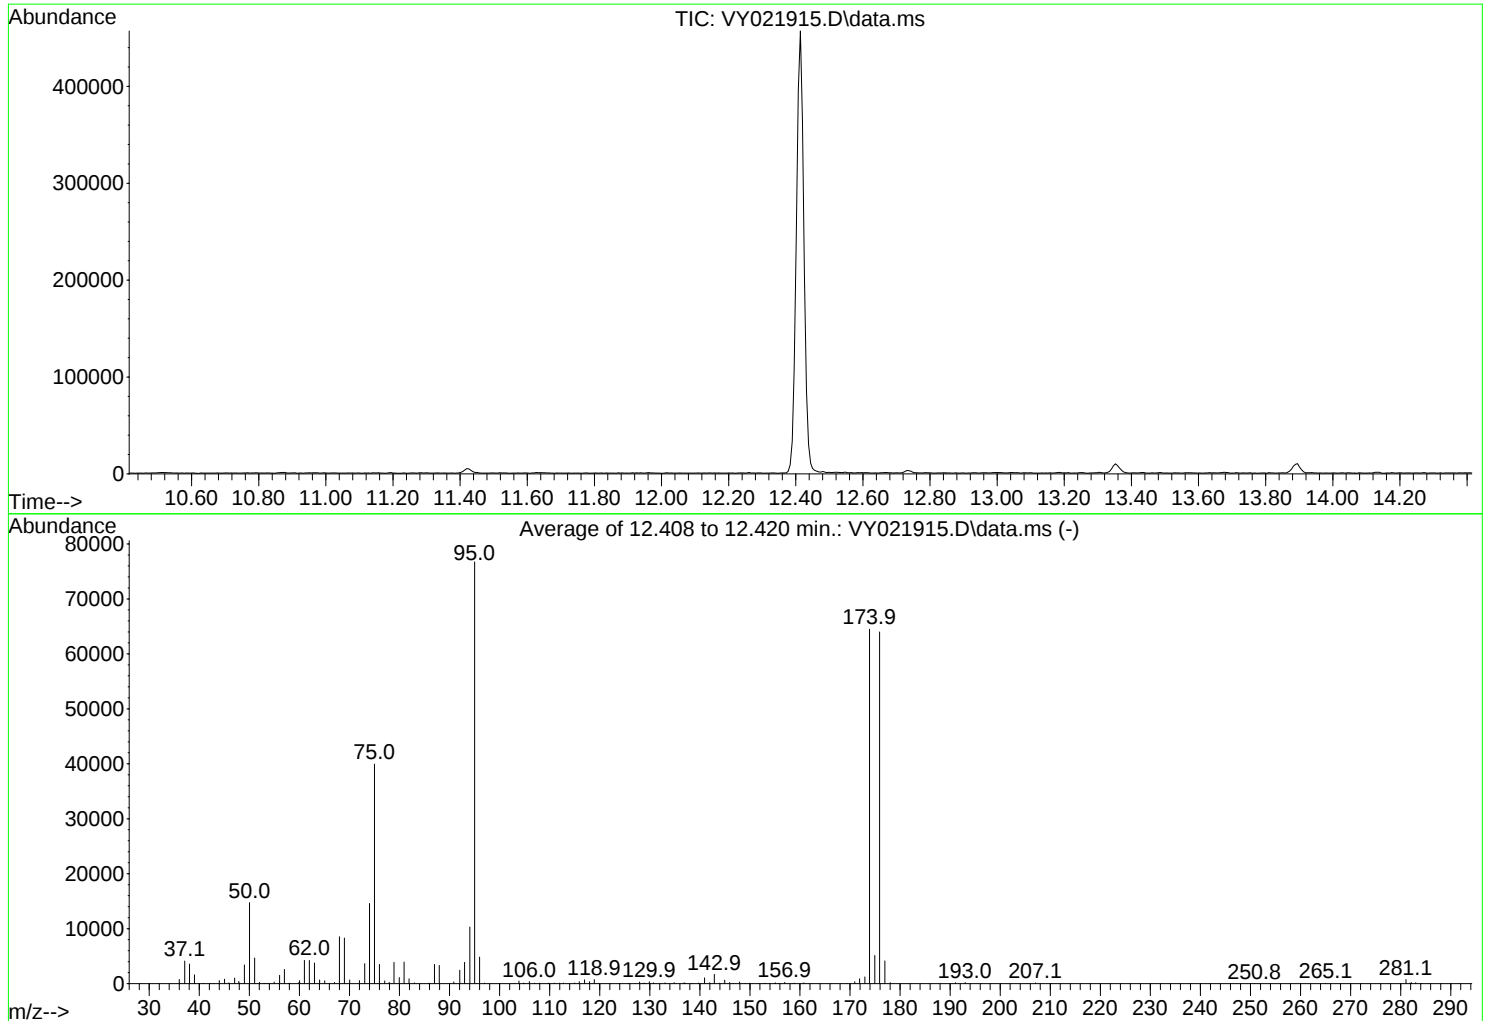

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	14722	PASS
75	95	30	60	52.0	39941	PASS
95	95	100	100	100.0	76747	PASS
96	95	5	9	6.3	4823	PASS
173	174	0.00	2	1.9	1235	PASS
174	95	50	100	84.0	64475	PASS
175	174	5	9	8.0	5132	PASS
176	174	95	101	99.2	63987	PASS
177	176	5	9	6.5	4138	PASS