

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042022\
 Data File : VY008426.D
 Acq On : 20 Apr 2022 18:15
 Operator : KP/MD
 Sample : N2507-01
 Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 PL-01-042022

Quant Time: Apr 21 02:41:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 08 16:02:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	94620	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	175161	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	172802	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	76917	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	56145	63.170	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	126.340%
35) Dibromofluoromethane	7.716	113	54831	54.197	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.400%
50) Toluene-d8	10.179	98	214811	62.051	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	124.100%
62) 4-Bromofluorobenzene	12.483	95	72828	55.932	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	111.860%
Target Compounds						
11) Tert butyl alcohol	4.948	59	2200	23.153	ug/l #	85
16) Acetone	3.948	43	5722	26.767	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042022\
Data File : VY008426.D
Acq On : 20 Apr 2022 18:15
Operator : KP/MD
Sample : N2507-01
Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
PL-01-042022


Quant Time: Apr 21 02:41:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
Quant Title : SW846 8260
QLast Update : Fri Apr 08 16:02:50 2022
Response via : Initial Calibration

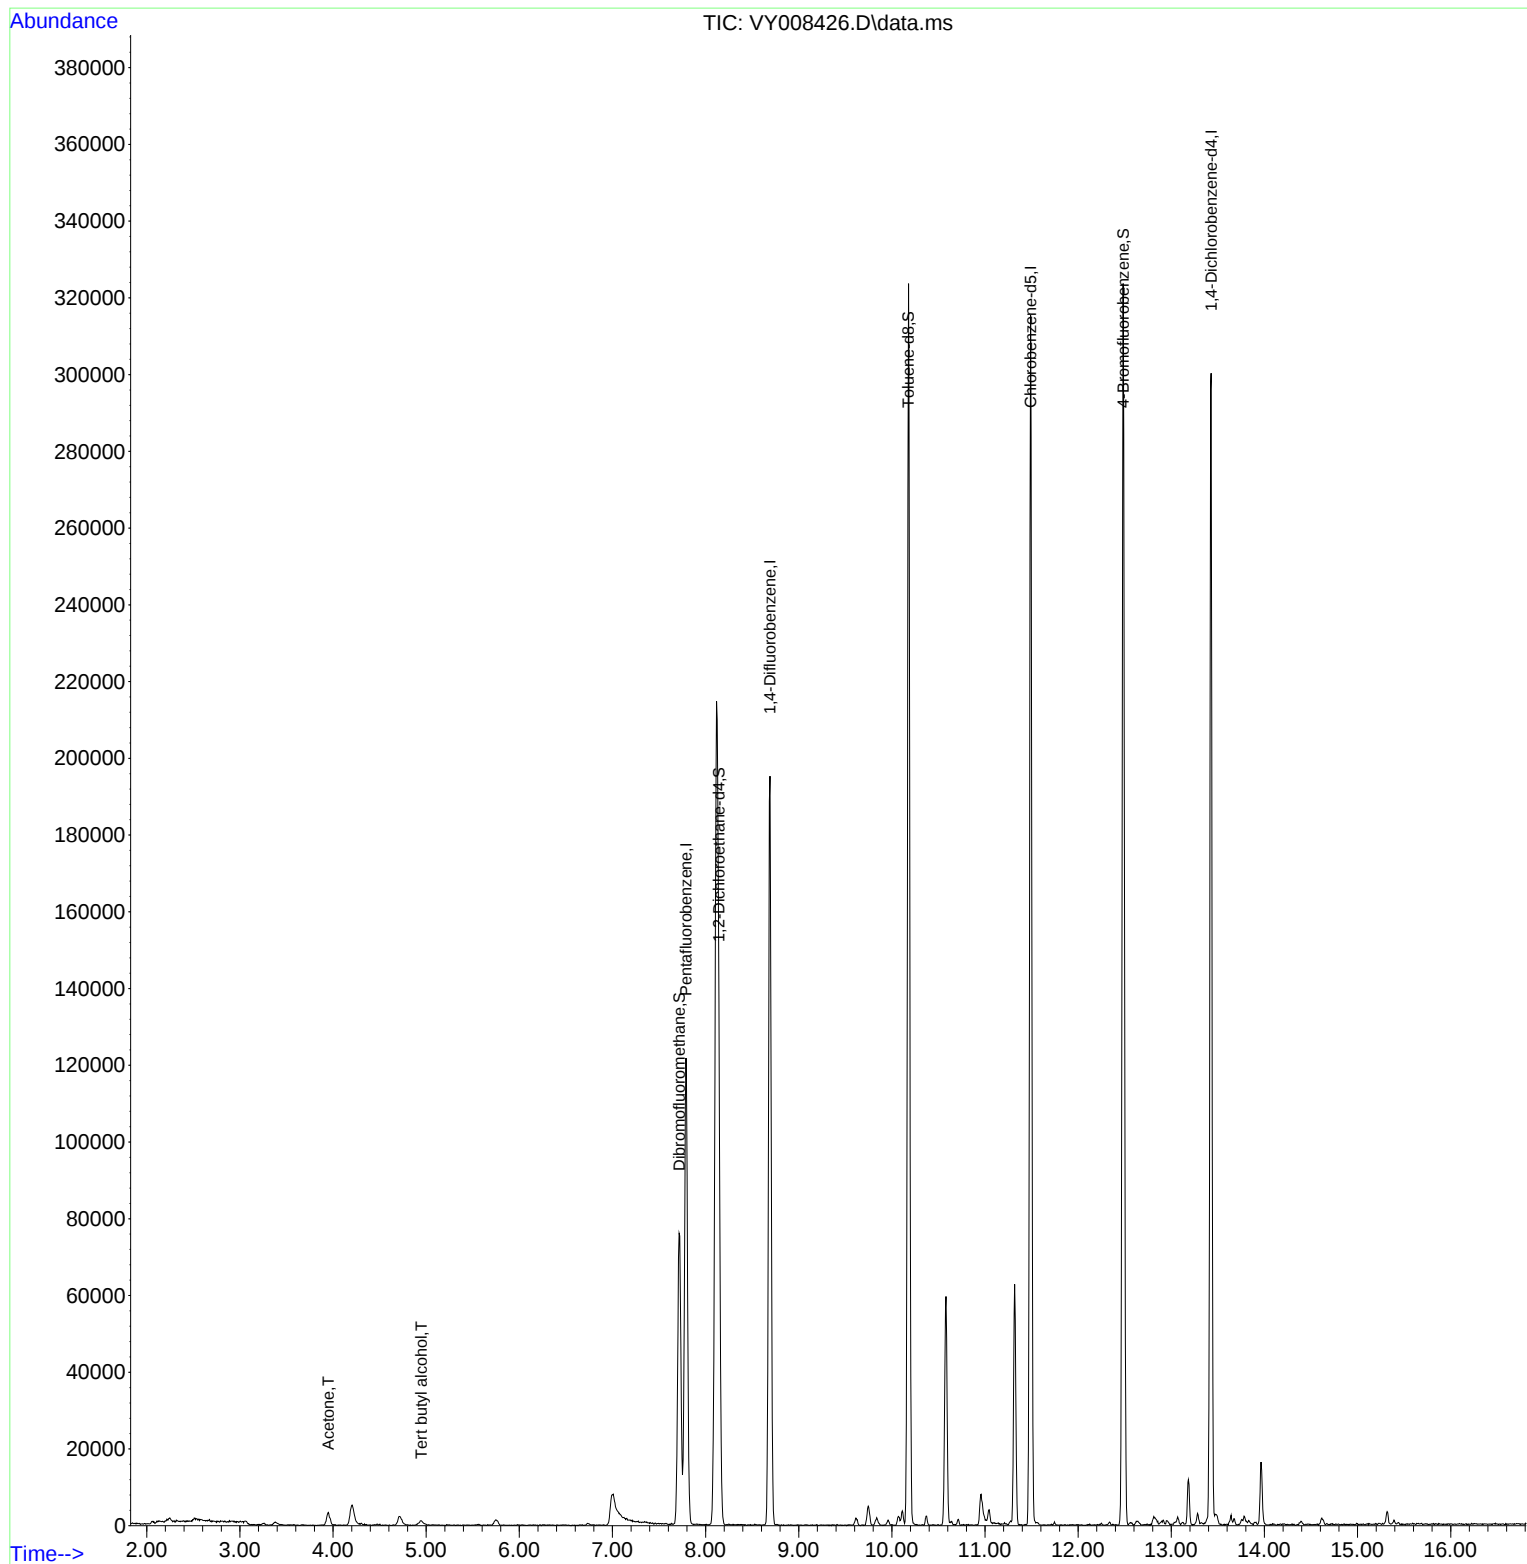






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008426.D
Acq: 20 Apr 2022 18:15

Instrument :
MSVOA_Y
ClientSampleId :
PL-01-042022



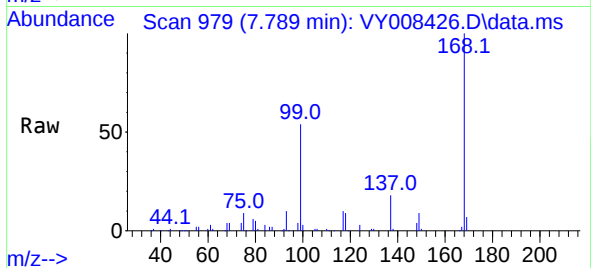



Tgt Ion:168 Resp: 94620
Ion Ratio Lower Upper
168 100
99 54.2 46.9 70.3

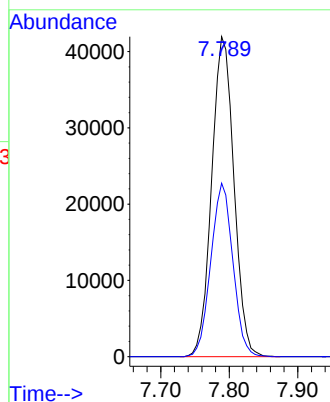

#11
Tert butyl alcohol
Concen: 23.153 ug/l
RT: 4.948 min Scan# 513
Delta R.T. -0.006 min
Lab File: VY008426.D
Acq: 20 Apr 2022 18:15

Tgt Ion: 59 Resp: 2200
Ion Ratio Lower Upper
59 100
57 2.8 6.4 9.6#


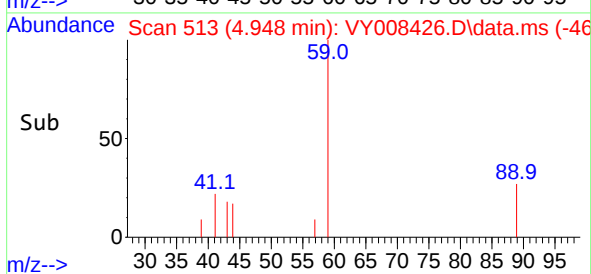
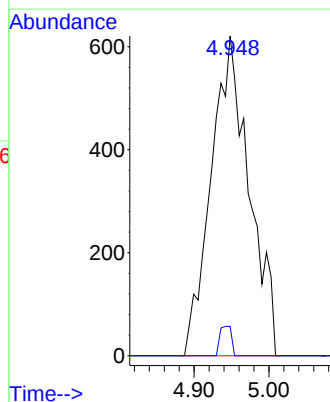
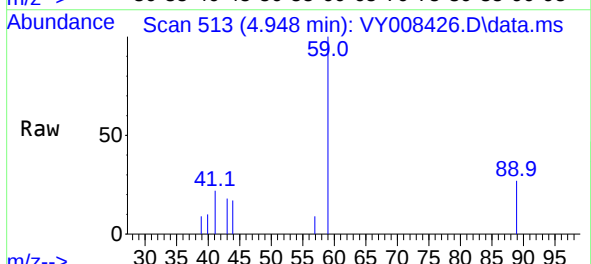




#16
Acetone
Concen: 26.767 ug/l
RT: 3.948 min Scan# 34
Delta R.T. 0.006 min
Lab File: VY008426.D
Acq: 20 Apr 2022 18:15




Instrument :
MSVOA_Y
ClientSampleId :
PL-01-042022


Tgt Ion: 43 Resp: 5722
Ion Ratio Lower Upper
43 100
58 29.5 22.0 33.0

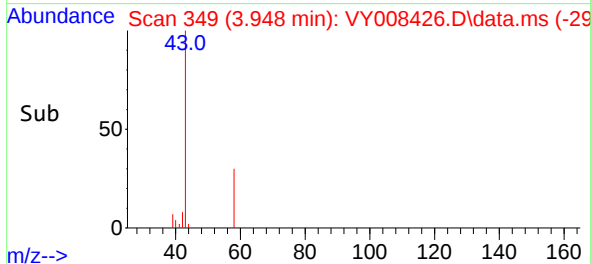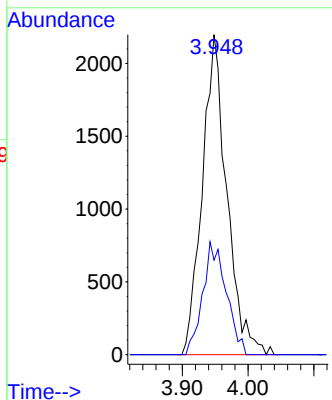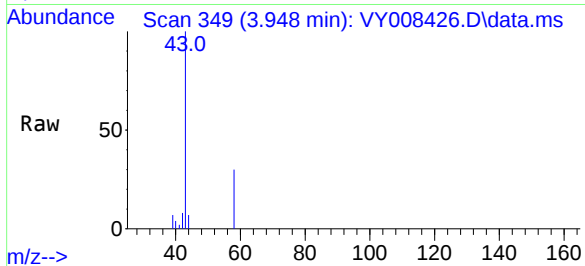

#33
1,2-Dichloroethane-d4
Concen: 63.170 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.001 min
Lab File: VY008426.D
Acq: 20 Apr 2022 18:15

Tgt Ion: 65 Resp: 56145
Ion Ratio Lower Upper
65 100
67 56.0 0.0 99.4

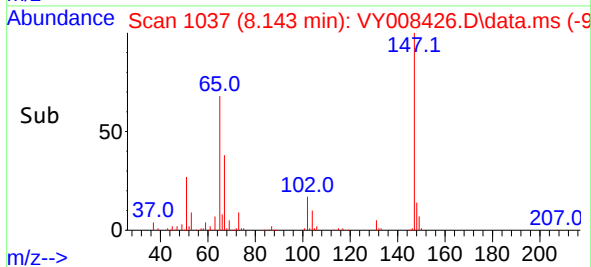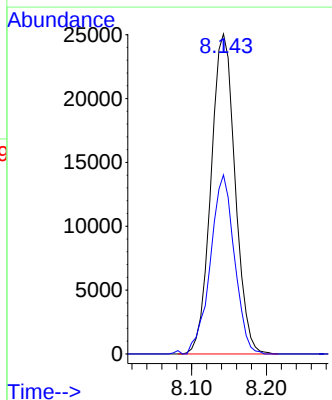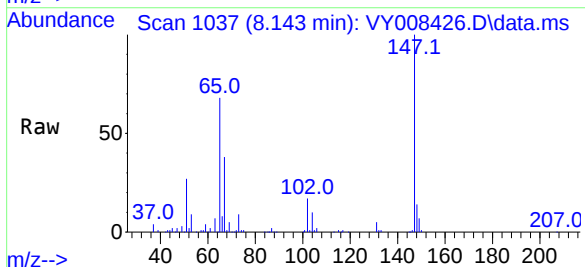

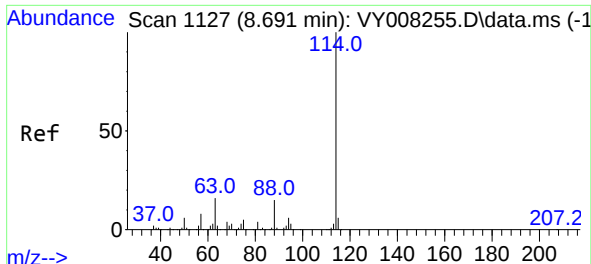

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY008426.D

Acq: 20 Apr 2022 18:15

Instrument :

MSVOA_Y

ClientSampleId :

PL-01-042022





Tgt Ion:114 Resp: 175161

Ion Ratio Lower Upper

114 100

63 18.0 0.0 43.2

88 14.3 0.0 31.8

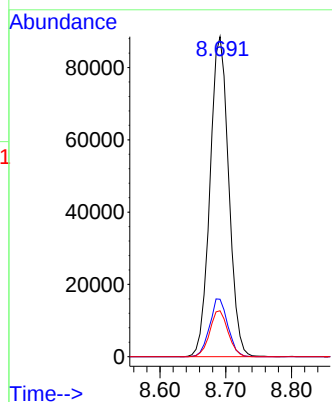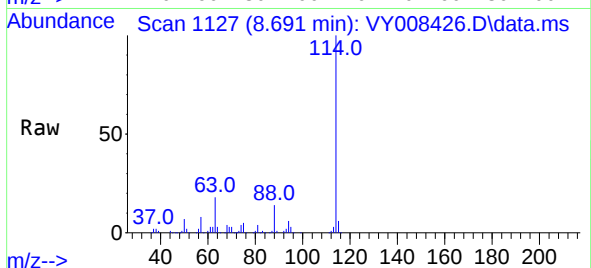

#35

Dibromofluoromethane

Concen: 54.197 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.001 min

Lab File: VY008426.D

Acq: 20 Apr 2022 18:15




Tgt Ion:113 Resp: 54831


Ion Ratio Lower Upper

113 100

111 103.8 82.6 124.0

192 18.8 17.6 26.4


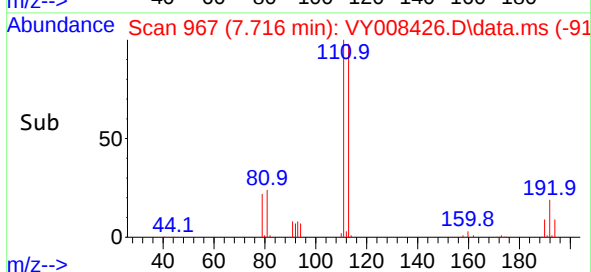
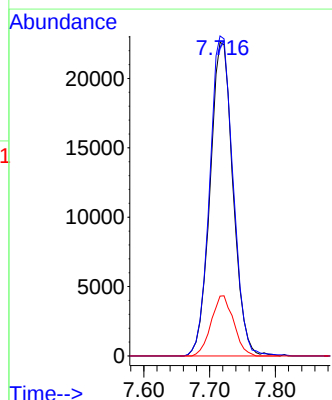
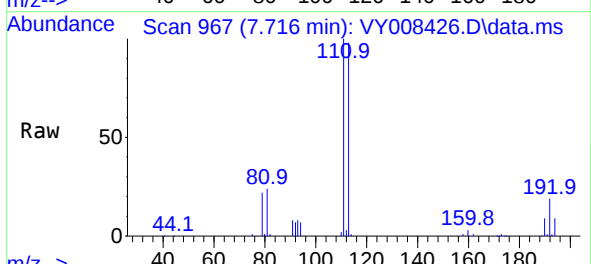




#50
Toluene-d8
Concen: 62.051 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.001 min
Lab File: VY008426.D
Acq: 20 Apr 2022 18:15




Instrument :
MSVOA_Y
ClientSampleId :
PL-01-042022


Tgt Ion: 98 Resp: 214811
Ion Ratio Lower Upper
98 100
100 65.4 50.2 75.2

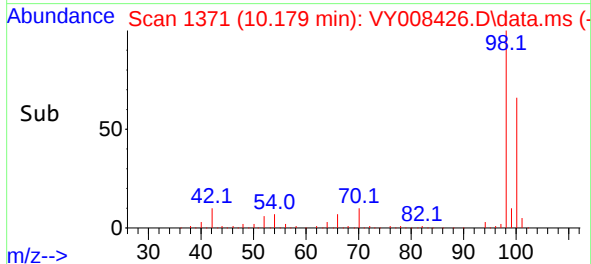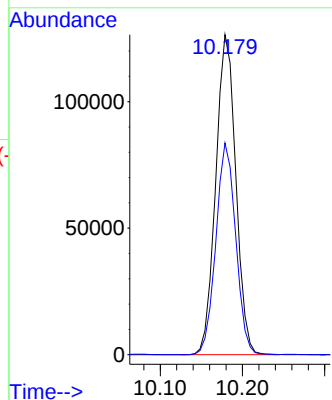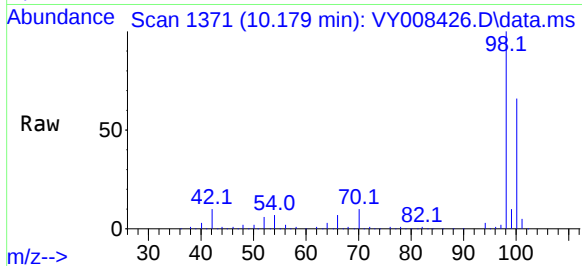

#62
4-Bromofluorobenzene
Concen: 55.932 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008426.D
Acq: 20 Apr 2022 18:15

Tgt Ion: 95 Resp: 72828
Ion Ratio Lower Upper
95 100
174 85.9 0.0 177.0
176 83.1 0.0 175.8


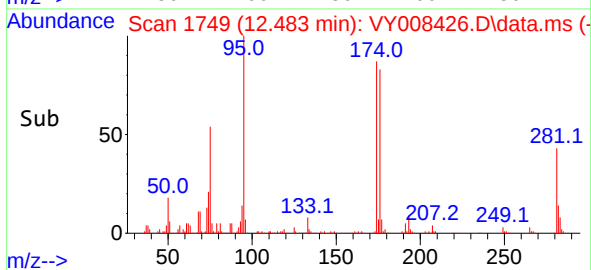
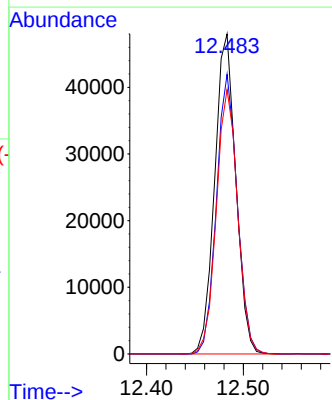
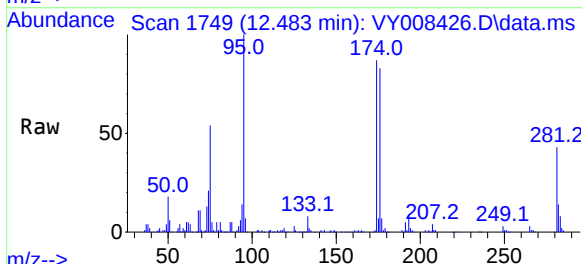




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY008426.D
Acq: 20 Apr 2022 18:15

Instrument :
MSVOA_Y
ClientSampleId :
PL-01-042022

Tgt Ion:117 Resp: 172802
Ion Ratio Lower Upper
117 100
82 52.1 43.0 64.4
119 31.5 25.4 38.0

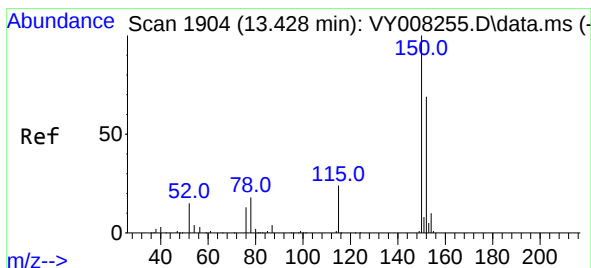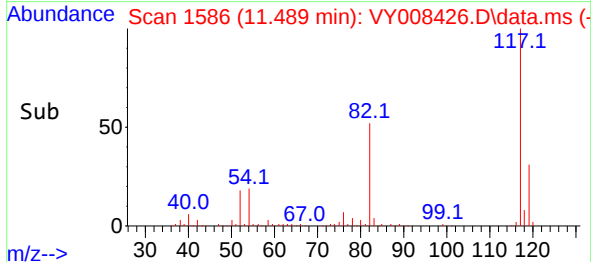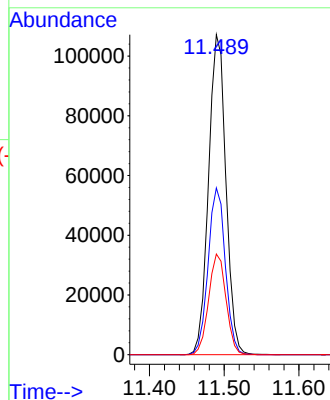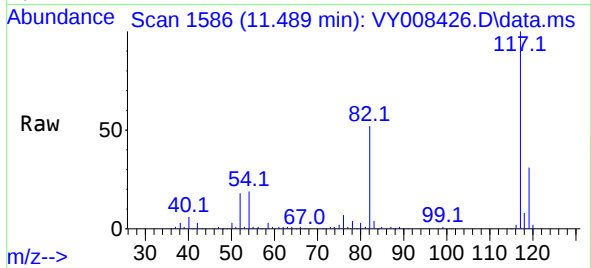

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008426.D
Acq: 20 Apr 2022 18:15

Tgt Ion:152 Resp: 76917
Ion Ratio Lower Upper
152 100
115 57.2 28.2 84.7
150 155.7 0.0 347.6

