

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042125\
 Data File : VY021944.D
 Acq On : 21 Apr 2025 13:34
 Operator : SY/MD
 Sample : Q1842-20
 Misc : 5.78g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 PL-714-VOC-11

Quant Time: Apr 22 02:45:04 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 28 02:30:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	145852	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	258170	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	219959	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	79291	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	81416	51.521	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 103.040%	
35) Dibromofluoromethane	7.634	113	89136	53.225	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 106.440%	
50) Toluene-d8	10.109	98	315183	49.471	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 98.940%	
62) 4-Bromofluorobenzene	12.408	95	80645	37.422	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 74.840%	
Target Compounds						Qvalue
11) Tert butyl alcohol	4.878	59	103	1.003	ug/l #	70
16) Acetone	3.879	43	394	1.218	ug/l #	44
20) Methylene Chloride	4.604	84	1639	Below Cal	#	77
31) Cyclohexane	7.707	56	3413	1.224	ug/l #	1
36) 1,1-Dichloropropene	7.707	75	12370	4.849	ug/l #	50
38) Carbon Tetrachloride	7.713	117	15059	5.154	ug/l #	15
76) 1,2,3-Trichloropropane	12.408	75	42941	54.634	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.408	75	42941	125.886	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042125\
Data File : VY021944.D
Acq On : 21 Apr 2025 13:34
Operator : SY/MD
Sample : Q1842-20
Misc : 5.78g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-11

Quant Time: Apr 22 02:45:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 28 02:30:29 2025
Response via : Initial Calibration




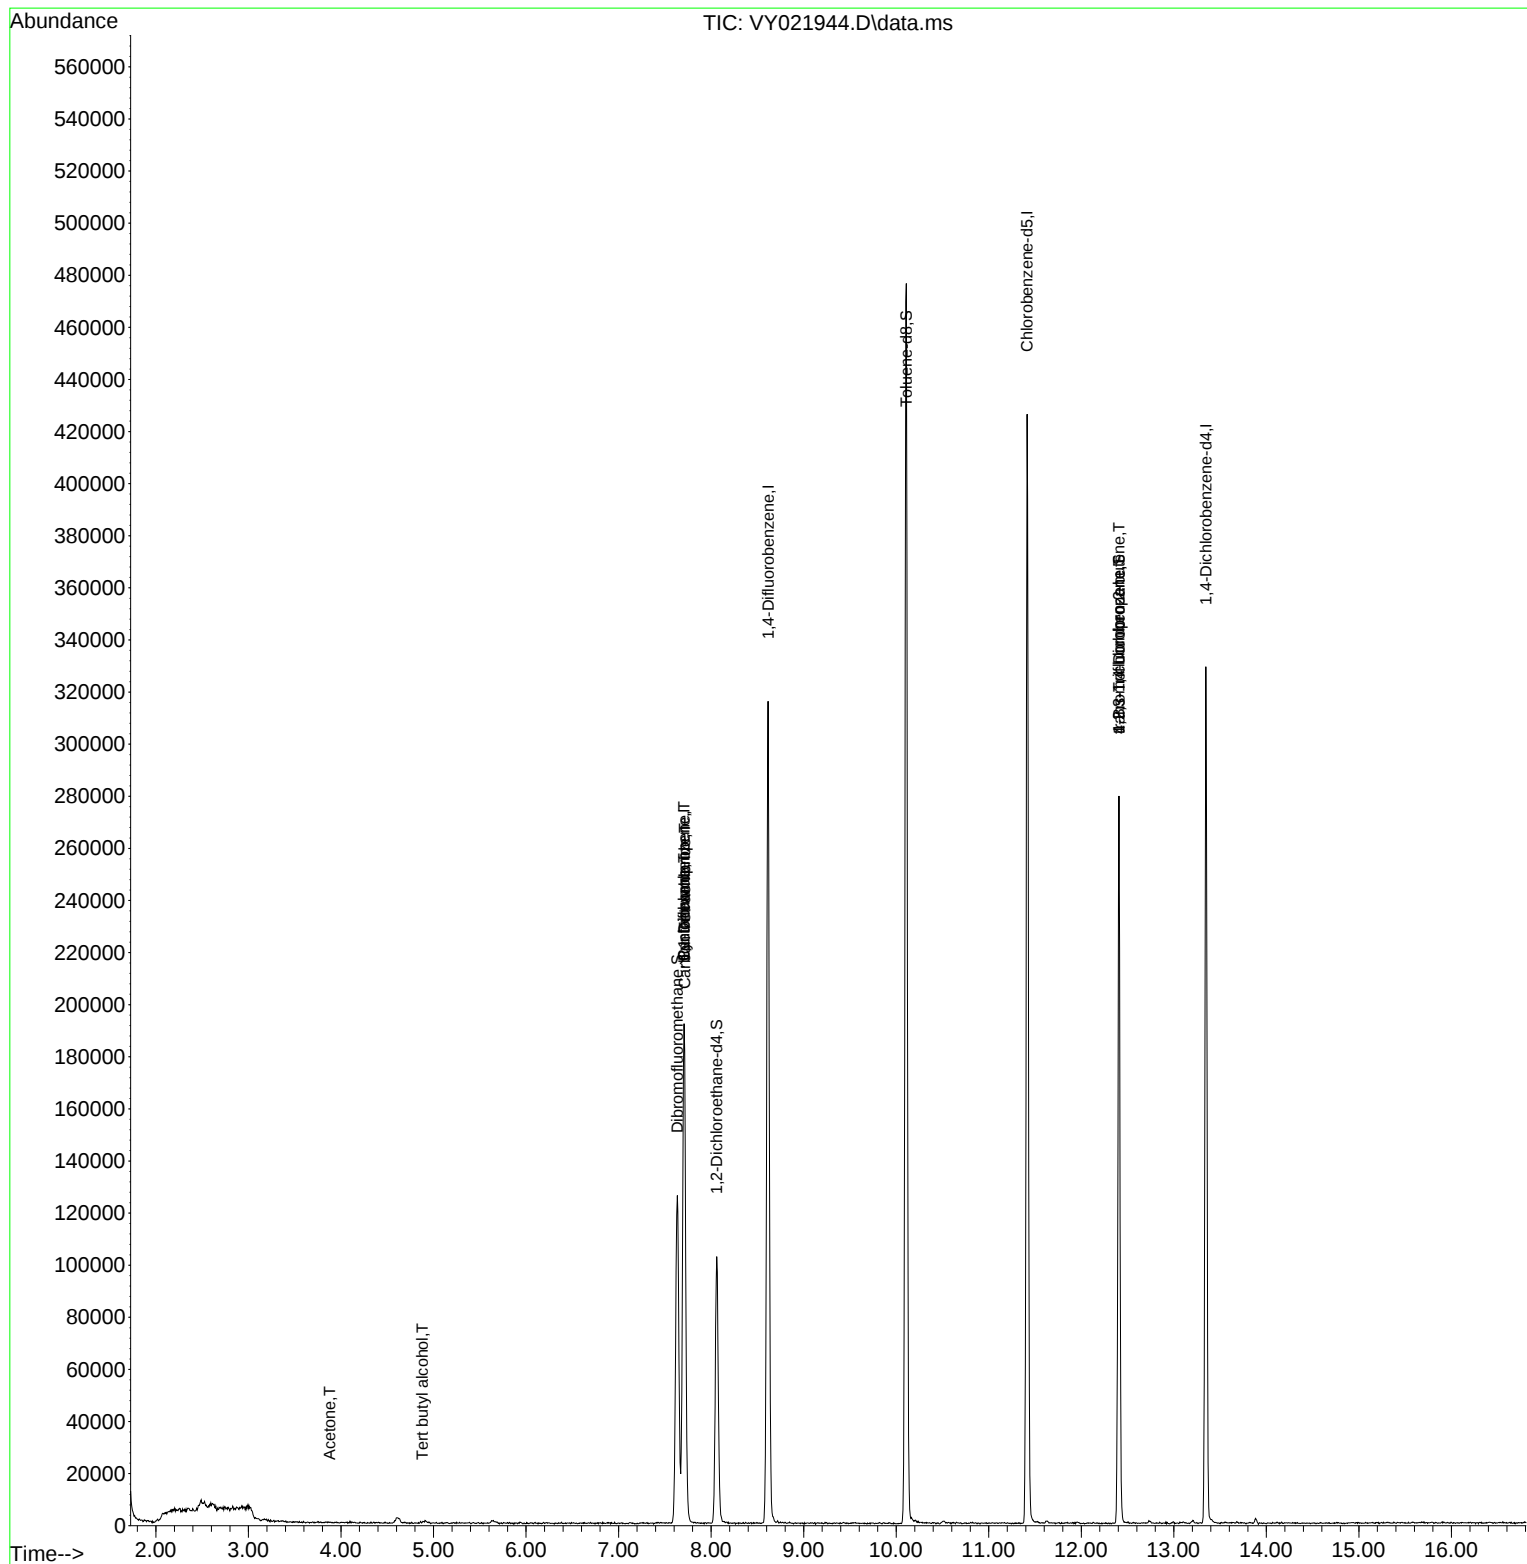


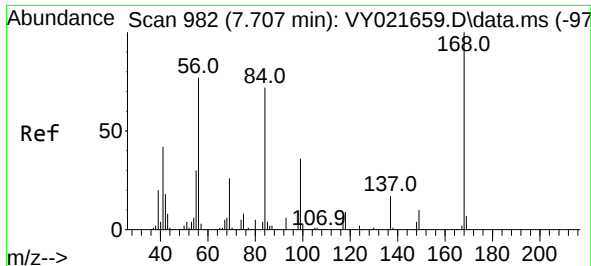

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-11


Tgt Ion:168 Resp: 145852
Ion Ratio Lower Upper
168 100
99 55.1 46.7 70.1

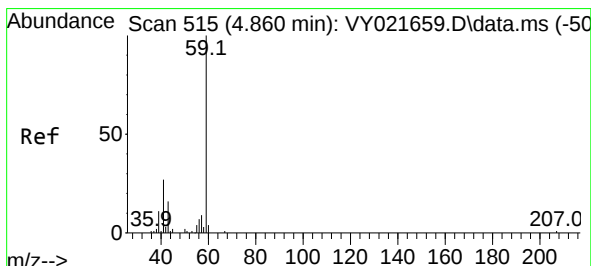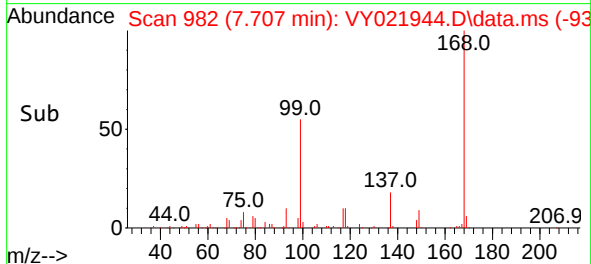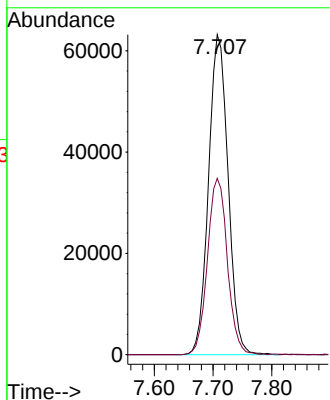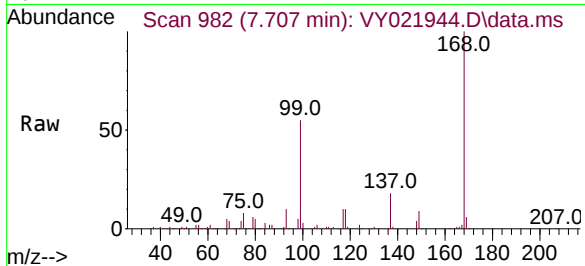

#11
Tert butyl alcohol
Concen: 1.003 ug/l
RT: 4.878 min Scan# 518
Delta R.T. 0.018 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34

Tgt Ion: 59 Resp: 103
Ion Ratio Lower Upper
59 100
57 0.0 9.2 13.8#


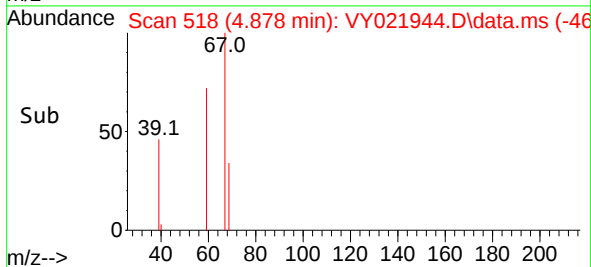
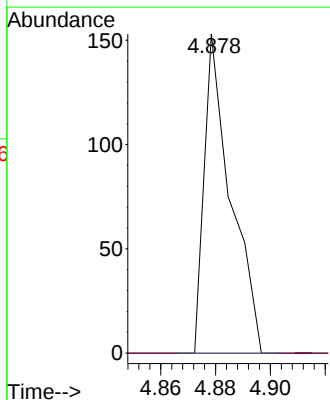
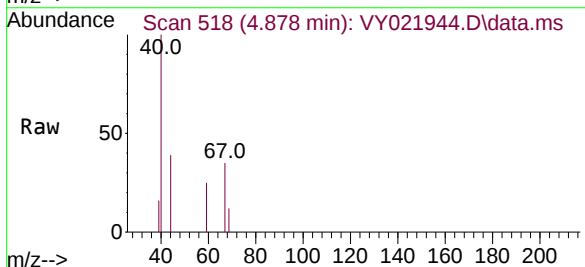


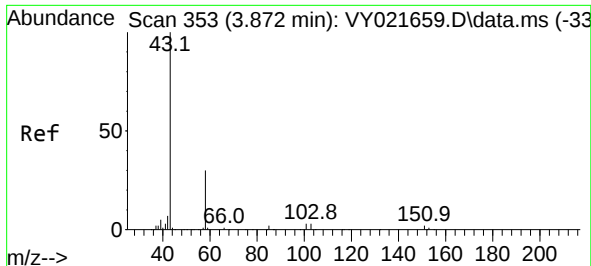

#16
Acetone
Concen: 1.218 ug/l
RT: 3.879 min Scan# 31
Delta R.T. 0.006 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-11


Tgt Ion: 43 Resp: 394
Ion Ratio Lower Upper
43 100
58 0.0 24.2 36.4#

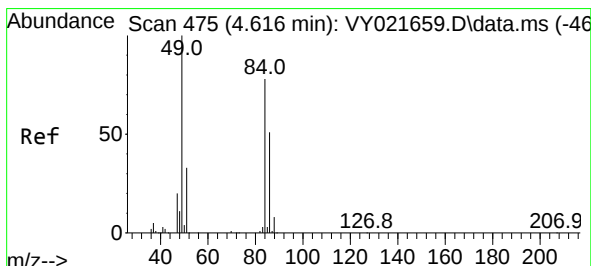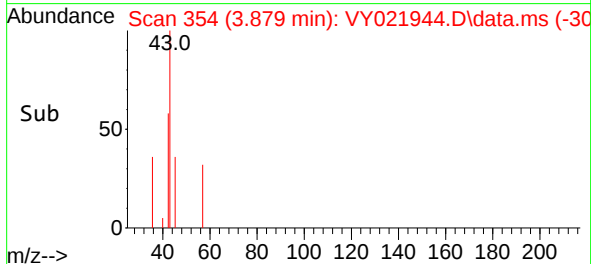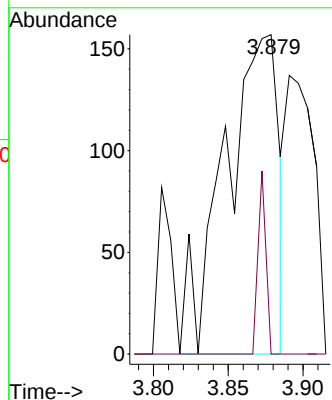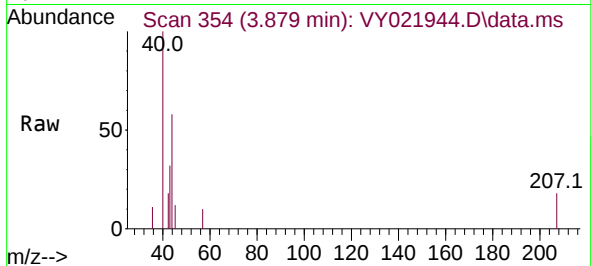

#20
Methylene Chloride
Concen: Below Cal
RT: 4.604 min Scan# 473
Delta R.T. -0.012 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34

Tgt Ion: 84 Resp: 1639
Ion Ratio Lower Upper
84 100
49 104.1 102.8 154.2
51 21.2 33.5 50.3#
86 81.1 52.0 78.0#


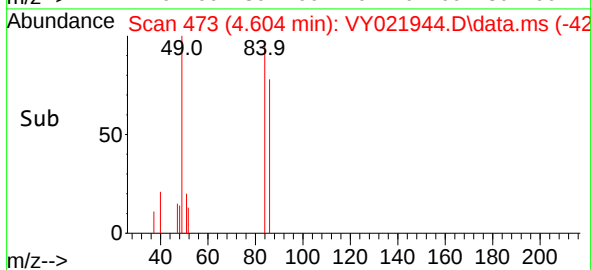
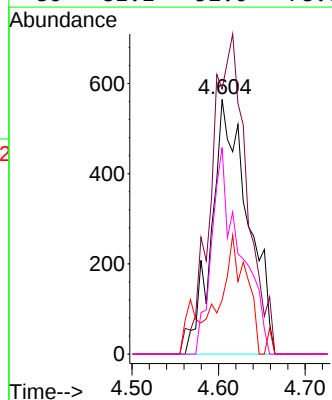
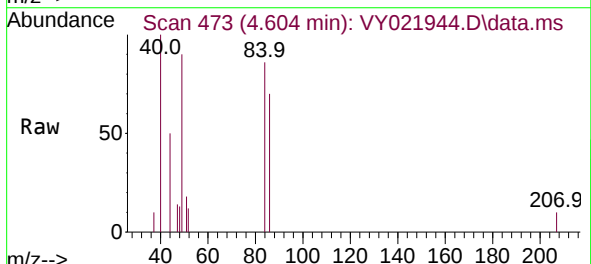


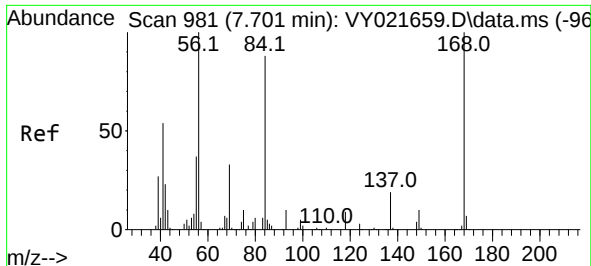

#31
Cyclohexane
Concen: 1.224 ug/l
RT: 7.707 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-11


Tgt Ion: 56 Resp: 3413
Ion Ratio Lower Upper
56 100
69 183.5 26.6 40.0#
84 140.6 69.0 103.4#

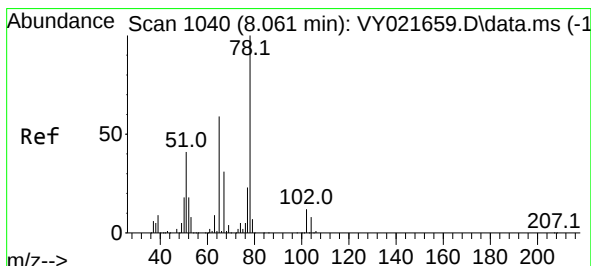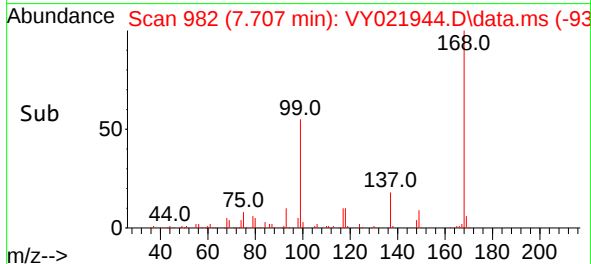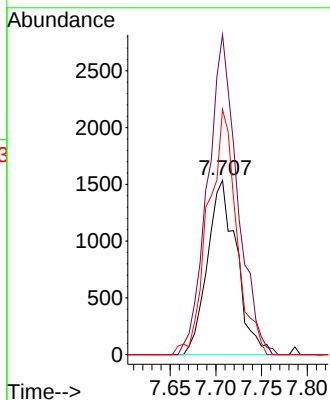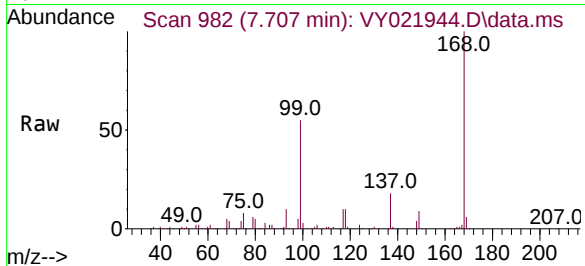

#33
1,2-Dichloroethane-d4
Concen: 51.521 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34

Tgt Ion: 65 Resp: 81416
Ion Ratio Lower Upper
65 100
67 51.8 0.0 104.6

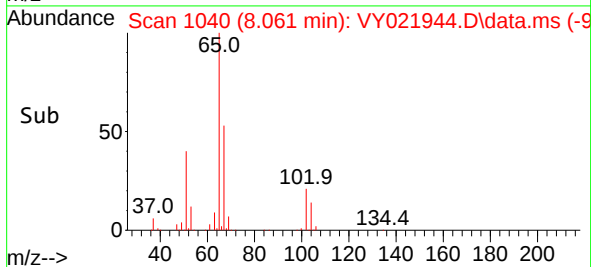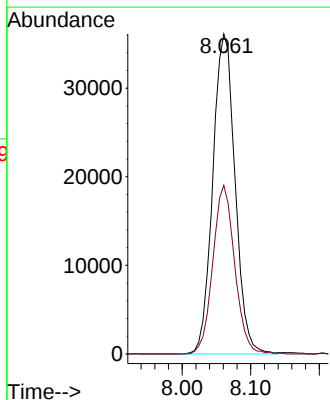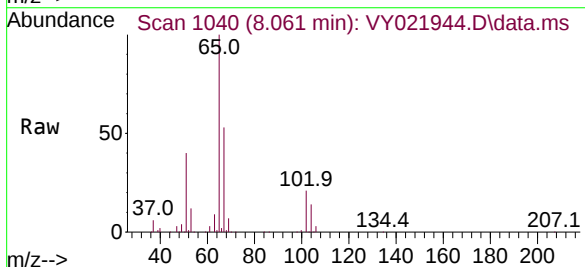

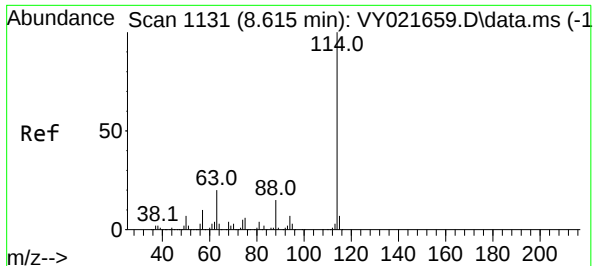

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY021944.D

Acq: 21 Apr 2025 13:34

Instrument :

MSVOA_Y

ClientSampleId :

PL-714-VOC-11





Tgt Ion:114 Resp: 258170

Ion Ratio Lower Upper

114 100

63 20.0 0.0 40.2

88 15.1 0.0 29.8

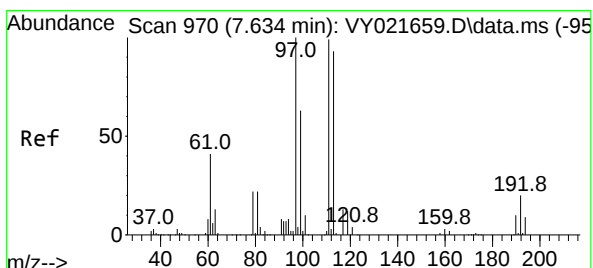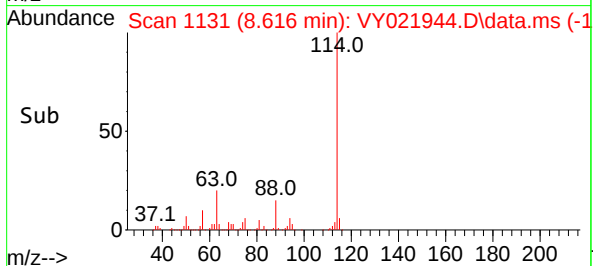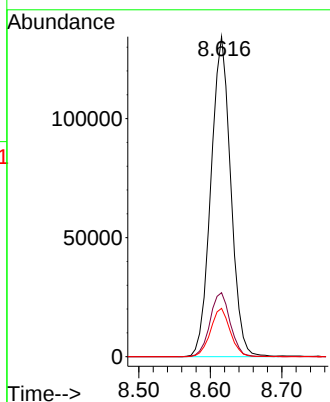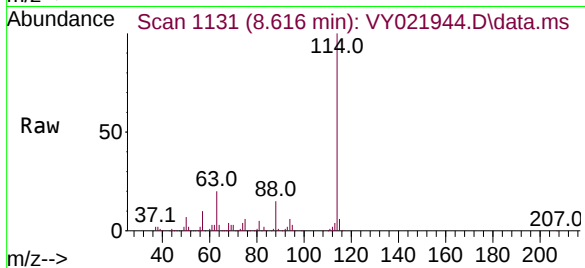

#35

Dibromofluoromethane

Concen: 53.225 ug/l

RT: 7.634 min Scan# 970

Delta R.T. 0.000 min

Lab File: VY021944.D

Acq: 21 Apr 2025 13:34




Tgt Ion:113 Resp: 89136


Ion Ratio Lower Upper

113 100

111 103.8 82.6 123.8

192 19.8 16.2 24.4


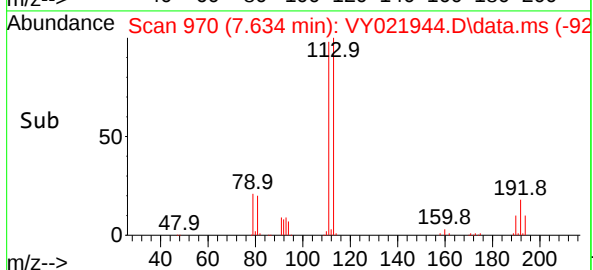
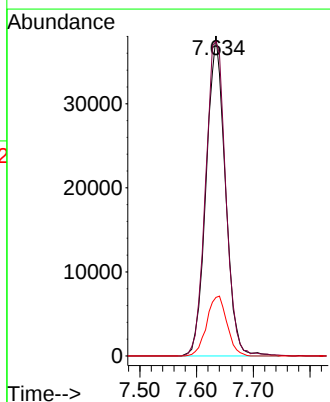
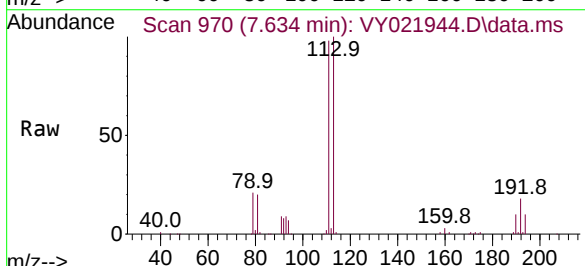


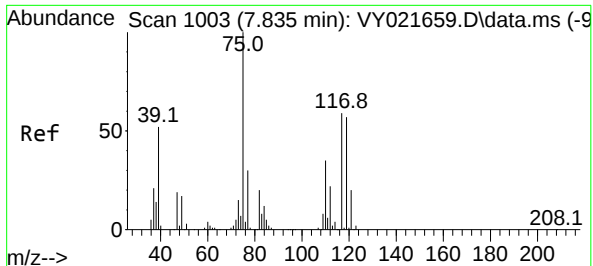

#36
1,1-Dichloropropene
Concen: 4.849 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.128 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-11


Tgt Ion: 75 Resp: 12370
Ion Ratio Lower Upper
75 100
110 8.9 17.0 50.9#
77 0.0 24.8 37.2#

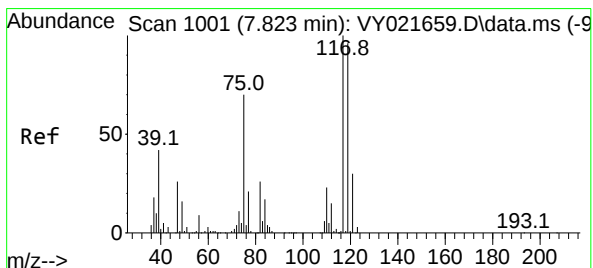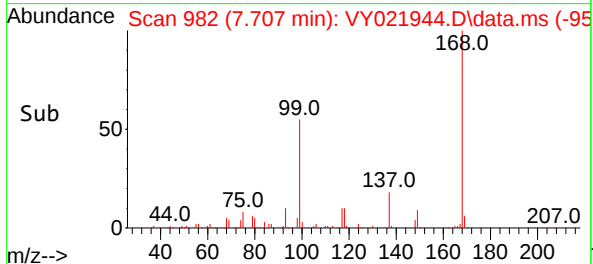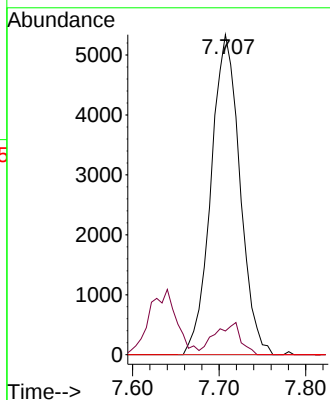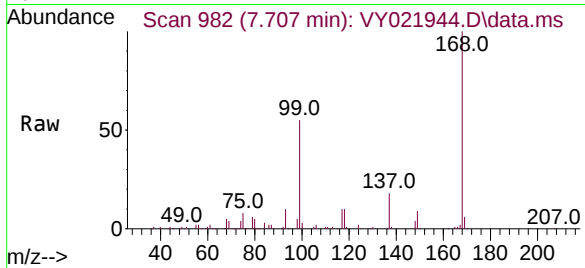

#38
Carbon Tetrachloride
Concen: 5.154 ug/l
RT: 7.713 min Scan# 983
Delta R.T. -0.110 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34

Tgt Ion: 117 Resp: 15059
Ion Ratio Lower Upper
117 100
119 3.3 76.2 114.4#
121 0.0 24.2 36.4#


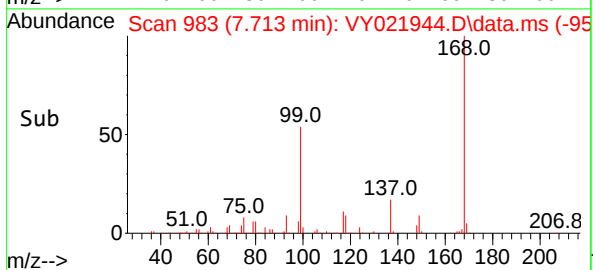
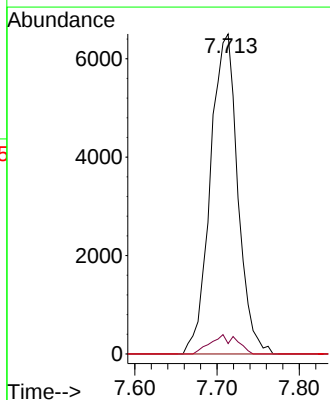
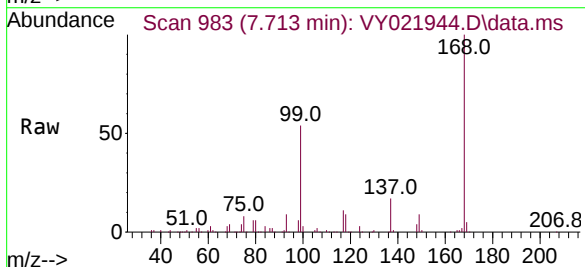


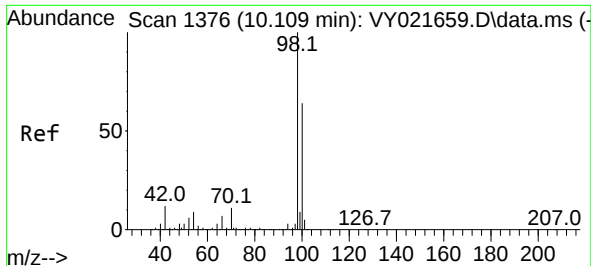

#50
Toluene-d8
Concen: 49.471 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-11


Tgt Ion: 98 Resp: 315183
Ion Ratio Lower Upper
98 100
100 63.0 52.1 78.1

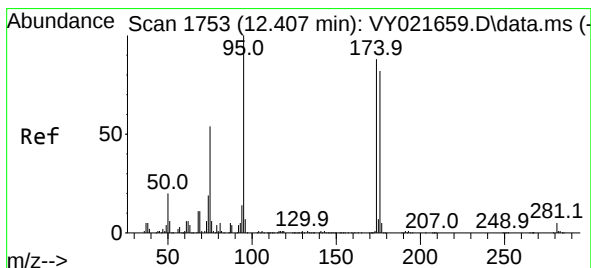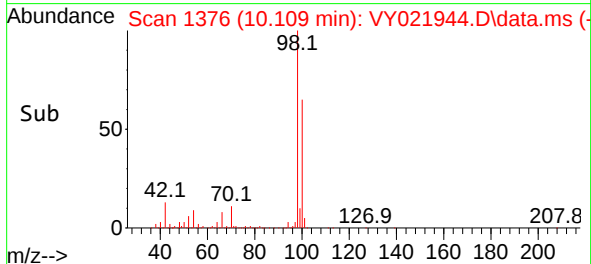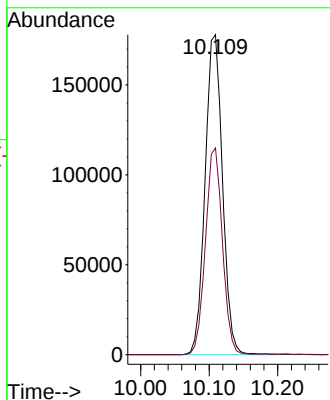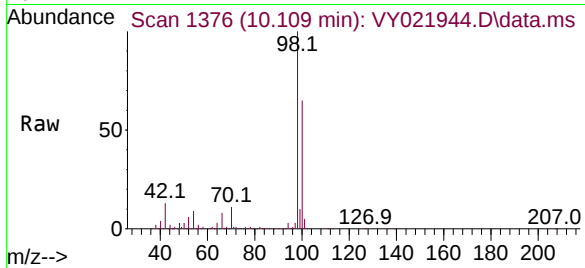

#62
4-Bromofluorobenzene
Concen: 37.422 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34

Tgt Ion: 95 Resp: 80645
Ion Ratio Lower Upper
95 100
174 85.5 0.0 170.8
176 82.6 0.0 162.0

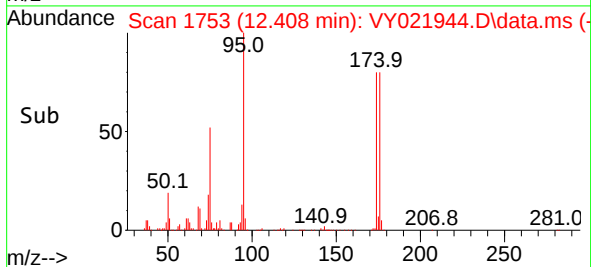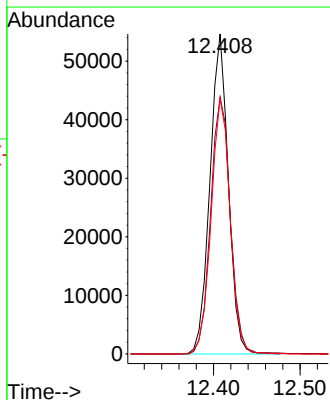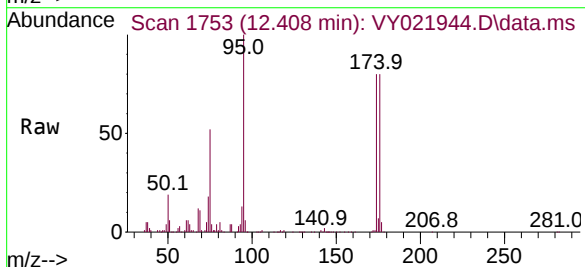

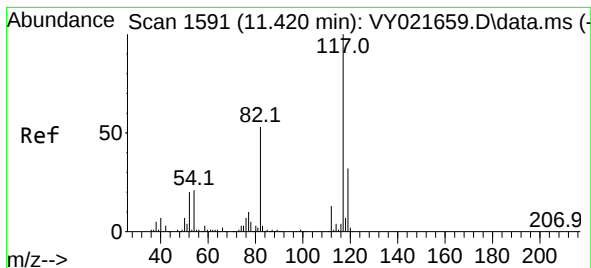

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY021944.D

Acq: 21 Apr 2025 13:34

Instrument :

MSVOA_Y

ClientSampleId :

PL-714-VOC-11





Tgt Ion:117 Resp: 219959

Ion Ratio Lower Upper

117 100

82 56.0 42.8 64.2

119 32.1 25.7 38.5

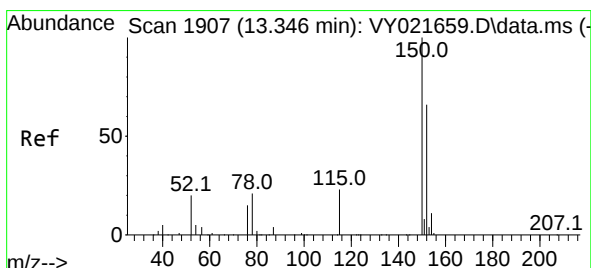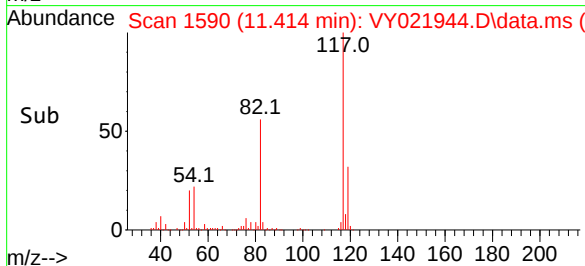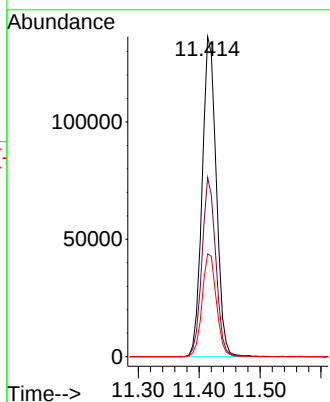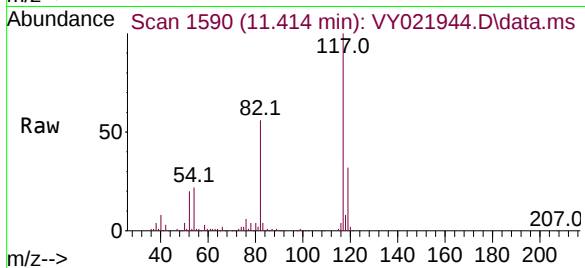

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY021944.D

Acq: 21 Apr 2025 13:34




Tgt Ion:152 Resp: 79291


Ion Ratio Lower Upper

152 100

115 58.8 28.8 86.5

150 159.0 0.0 348.4


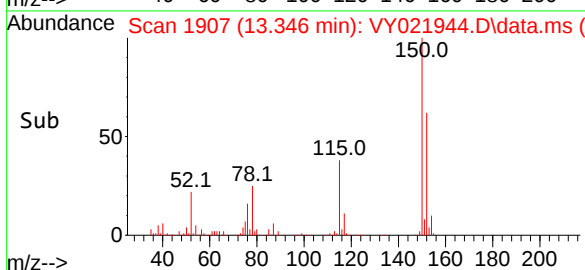
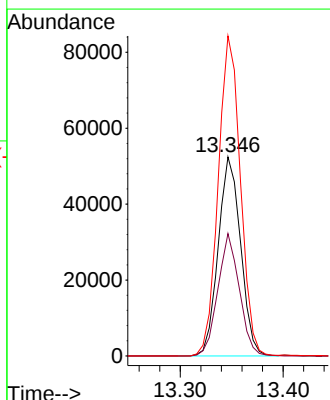
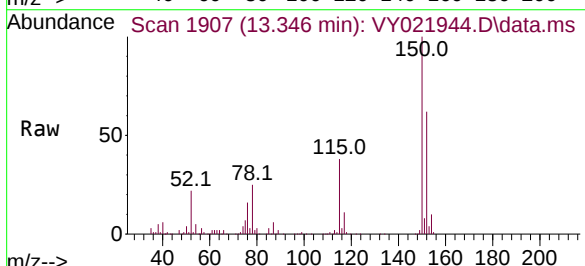


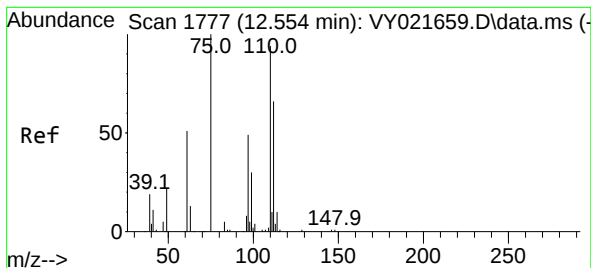

#76
1,2,3-Trichloropropane
Concen: 54.634 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. -0.146 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34

Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-11

Tgt Ion: 75 Resp: 42941
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#

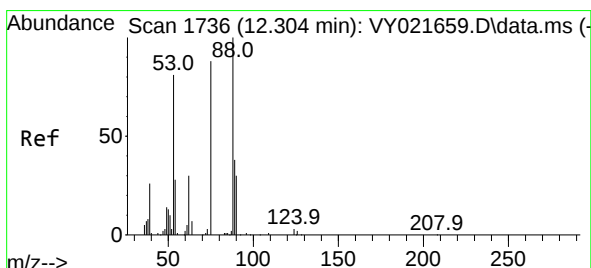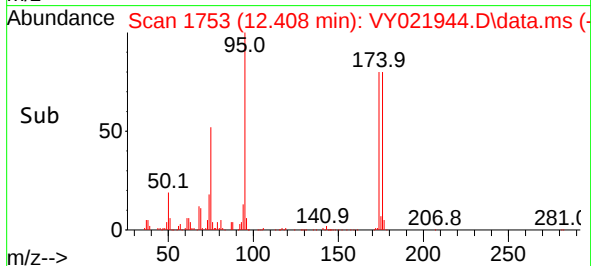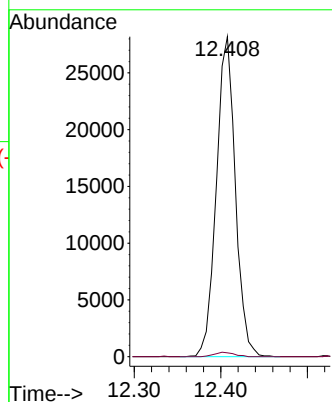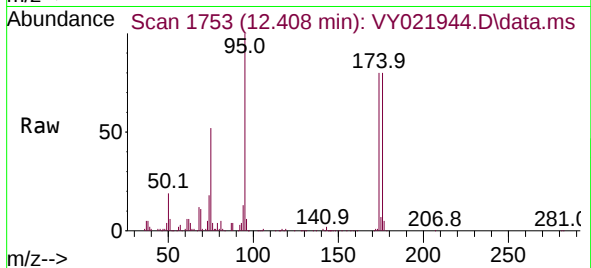

#81
trans-1,4-Dichloro-2-butene
Concen: 125.886 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.104 min
Lab File: VY021944.D
Acq: 21 Apr 2025 13:34

Tgt Ion: 75 Resp: 42941
Ion Ratio Lower Upper
75 100
53 0.4 76.1 114.1#
89 0.1 36.2 54.4#

