

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042125\
 Data File : VY021946.D
 Acq On : 21 Apr 2025 14:21
 Operator : SY/MD
 Sample : Q1842-32
 Misc : 5.27g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 PL-714-VOC-13

Quant Time: Apr 22 02:45:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 28 02:30:29 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	200754	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	379227	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	337671	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	129799	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	119295	54.845	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 109.700%	
35) Dibromofluoromethane	7.634	113	131285	53.368	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 106.740%	
50) Toluene-d8	10.109	98	467477	49.952	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 99.900%	
62) 4-Bromofluorobenzene	12.408	95	132582	41.884	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 83.760%	
Target Compounds						
					Qvalue	
20) Methylene Chloride	4.616	84	2650	Below Cal	#	74
31) Cyclohexane	7.707	56	4941	1.287	ug/l #	1
36) 1,1-Dichloropropene	7.707	75	16547	4.416	ug/l #	51
38) Carbon Tetrachloride	7.707	117	20395	4.752	ug/l #	17
51) 4-Methyl-2-Pentanone	10.115	43	2062	1.182	ug/l #	1
76) 1,2,3-Trichloropropane	12.408	75	69833	54.275	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.408	75	69833	125.060	ug/l #	12

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 22 02:45:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 28 02:30:29 2025
Response via : Initial Calibration







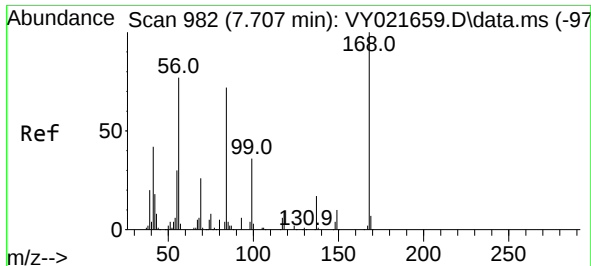

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-13


Tgt Ion:168 Resp: 200754
Ion Ratio Lower Upper
168 100
99 54.6 46.7 70.1

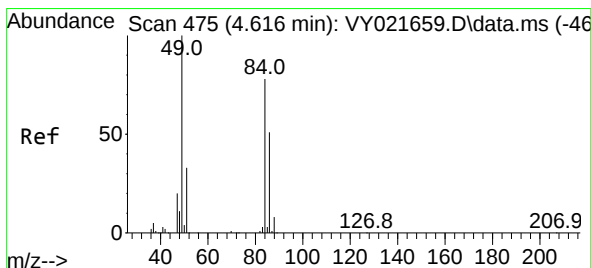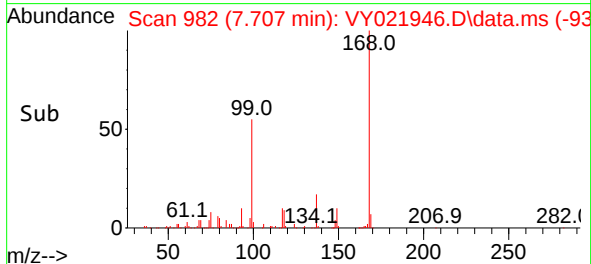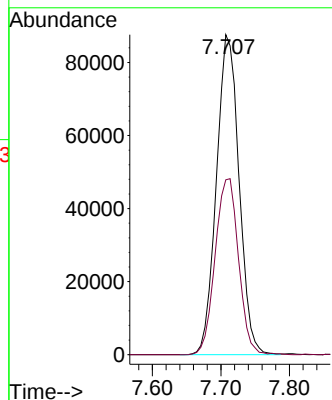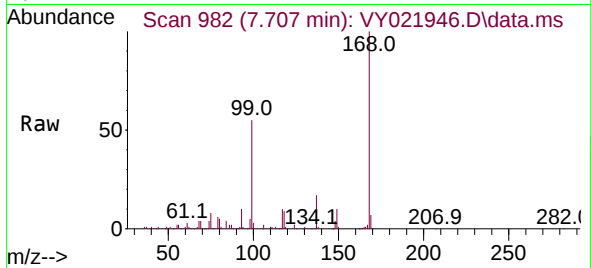

#20
Methylene Chloride
Concen: Below Cal
RT: 4.616 min Scan# 475
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21

Tgt Ion: 84 Resp: 2650
Ion Ratio Lower Upper
84 100
49 98.5 102.8 154.2#
51 27.1 33.5 50.3#
86 42.3 52.0 78.0#


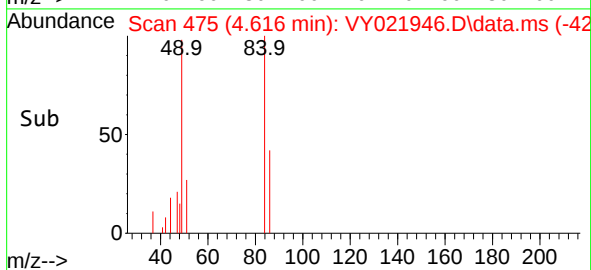
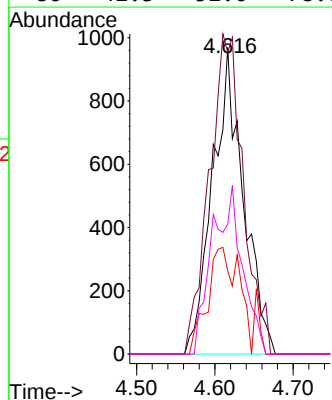
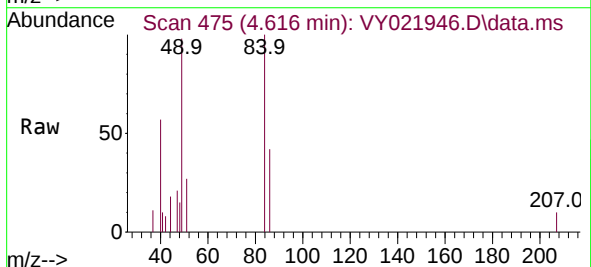


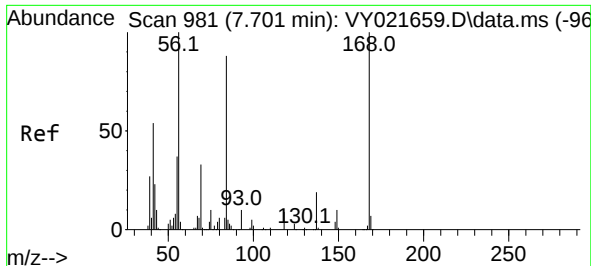

#31
Cyclohexane
Concen: 1.287 ug/l
RT: 7.707 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-13


Tgt Ion: 56 Resp: 4941
Ion Ratio Lower Upper
56 100
69 205.3 26.6 40.0#
84 166.0 69.0 103.4#

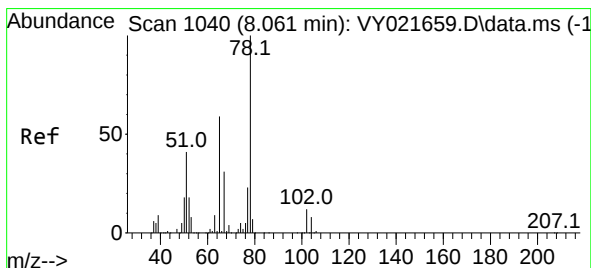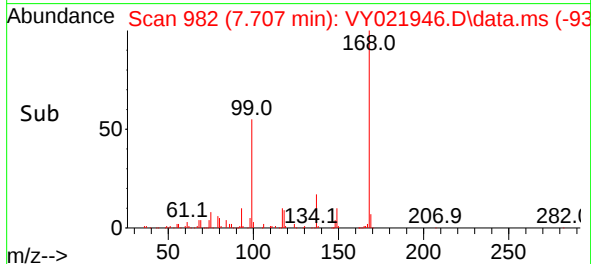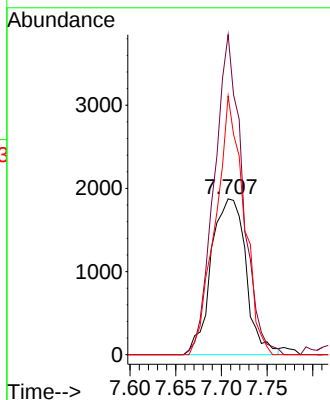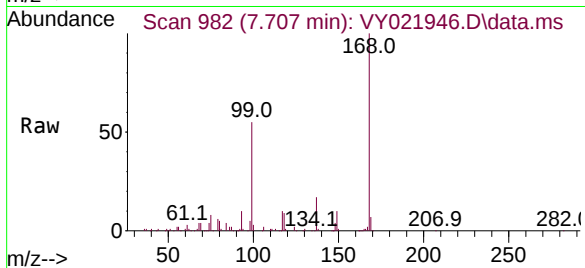

#33
1,2-Dichloroethane-d4
Concen: 54.845 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21

Tgt Ion: 65 Resp: 119295
Ion Ratio Lower Upper
65 100
67 52.9 0.0 104.6


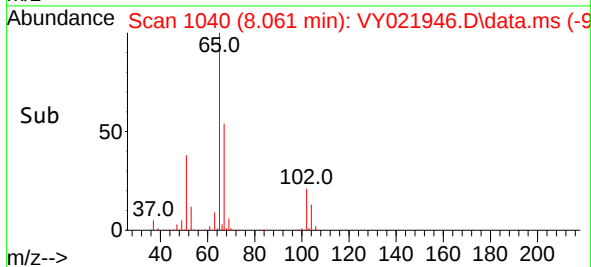
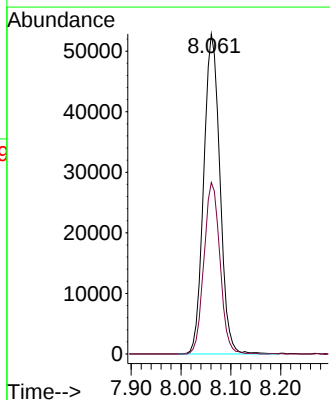
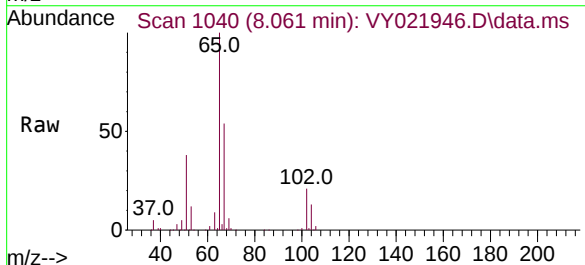


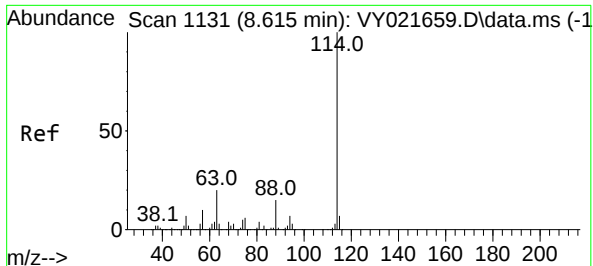

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-13


Tgt Ion:114 Resp: 379227
Ion Ratio Lower Upper
114 100
63 20.2 0.0 40.2
88 15.9 0.0 29.8

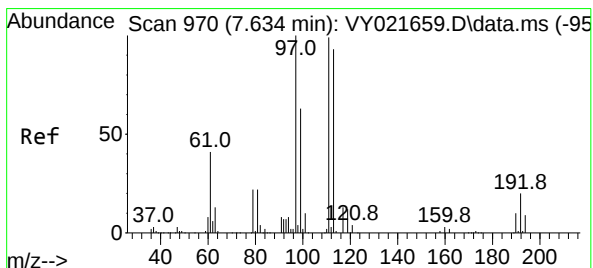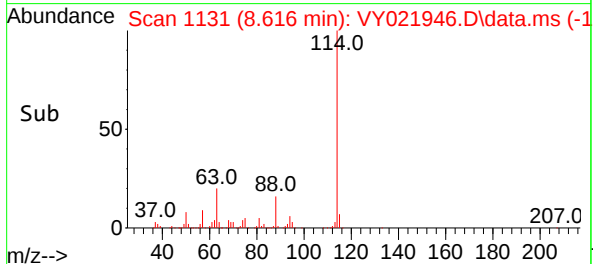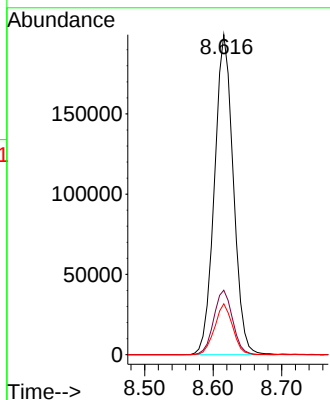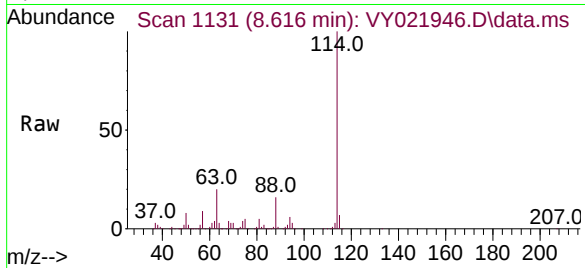

#35
Dibromofluoromethane
Concen: 53.368 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21

Tgt Ion:113 Resp: 131285
Ion Ratio Lower Upper
113 100
111 102.0 82.6 123.8
192 19.8 16.2 24.4

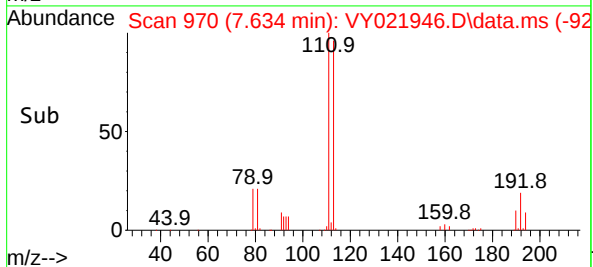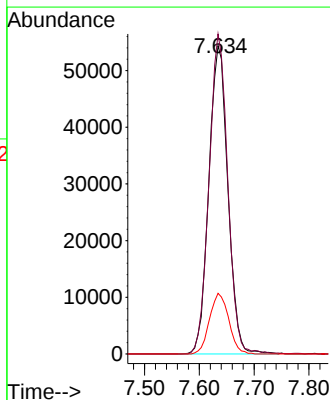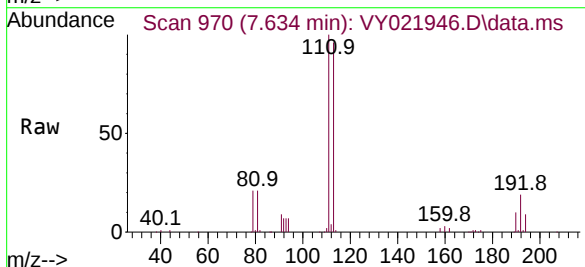

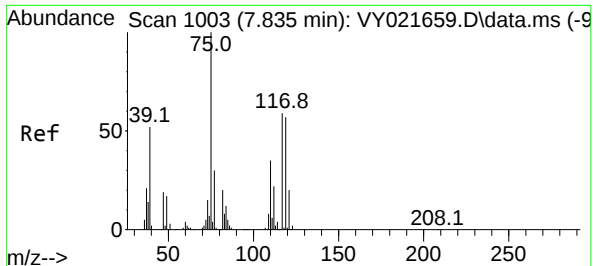

#36

1,1-Dichloropropene

Concen: 4.416 ug/l

RT: 7.707 min Scan# 982

Delta R.T. -0.128 min

Lab File: VY021946.D

Acq: 21 Apr 2025 14:21

Instrument :

MSVOA_Y

ClientSampleId :

PL-714-VOC-13





Tgt Ion: 75 Resp: 16547

Ion Ratio Lower Upper

75 100

110 10.1 17.0 50.9#

77 0.0 24.8 37.2#

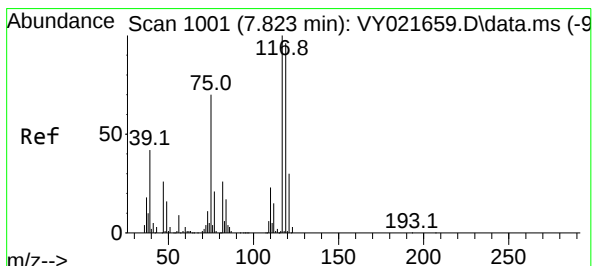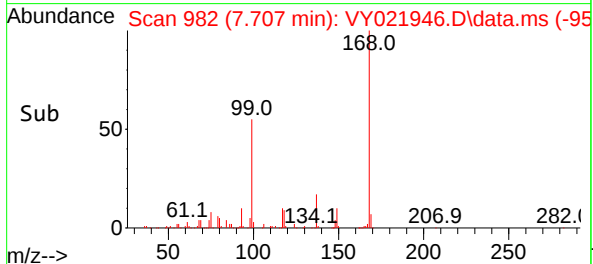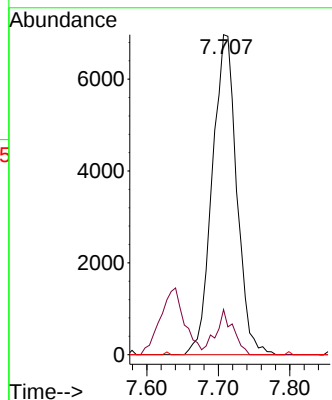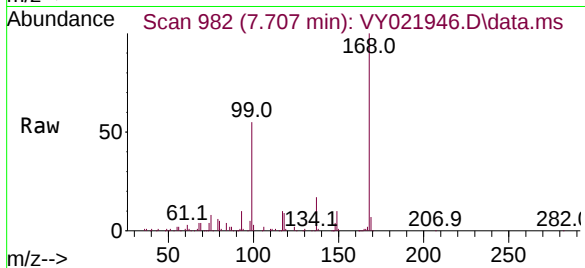

#38

Carbon Tetrachloride

Concen: 4.752 ug/l

RT: 7.707 min Scan# 982

Delta R.T. -0.116 min

Lab File: VY021946.D

Acq: 21 Apr 2025 14:21




Tgt Ion: 117 Resp: 20395


Ion Ratio Lower Upper

117 100

119 5.8 76.2 114.4#

121 0.0 24.2 36.4#


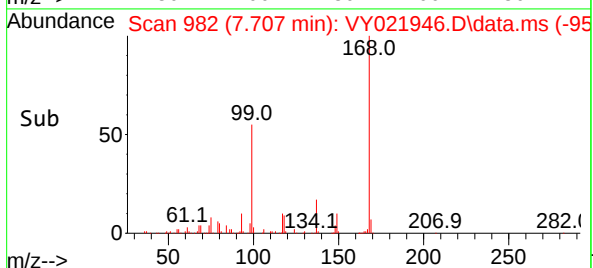
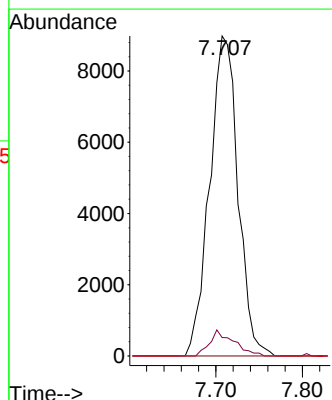
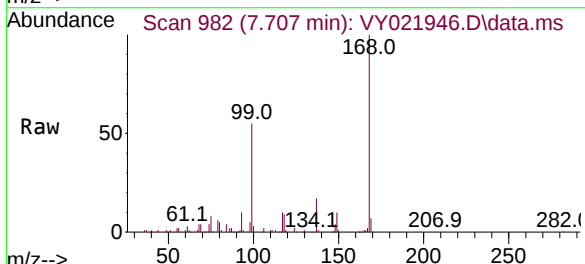


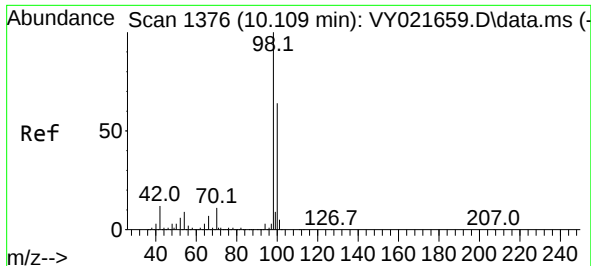

#50
Toluene-d8
Concen: 49.952 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-13


Tgt Ion: 98 Resp: 467477
Ion Ratio Lower Upper
98 100
100 63.8 52.1 78.1

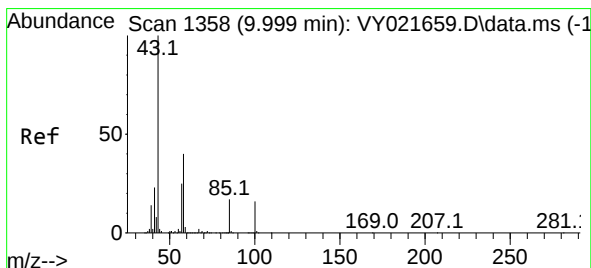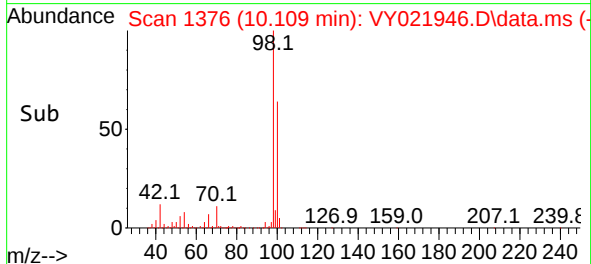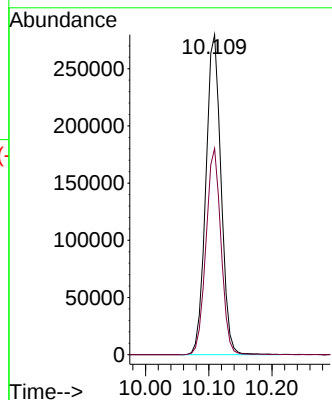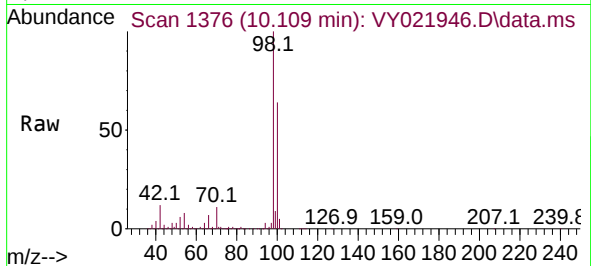

#51
4-Methyl-2-Pentanone
Concen: 1.182 ug/l
RT: 10.115 min Scan# 1377
Delta R.T. 0.116 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21

Tgt Ion: 43 Resp: 2062
Ion Ratio Lower Upper
43 100
58 194.3 31.5 47.3#


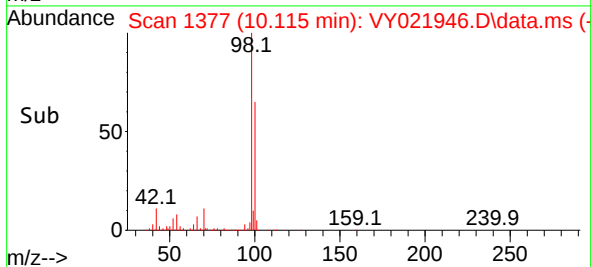
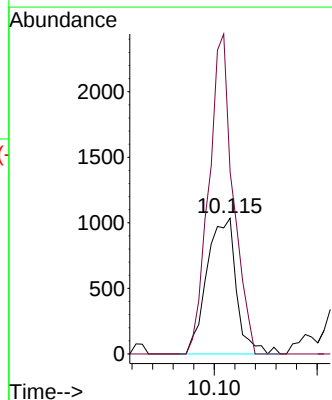
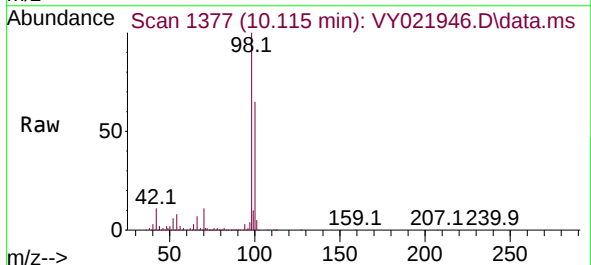


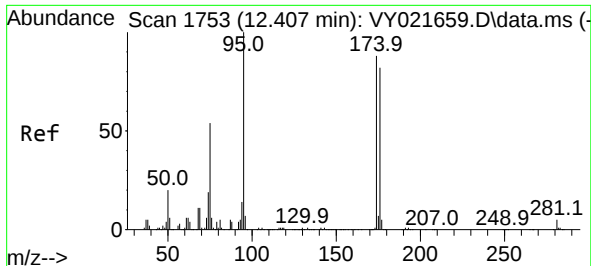

#62
4-Bromofluorobenzene
Concen: 41.884 ug/l
RT: 12.408 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-13


Tgt Ion: 95 Resp: 132582
Ion Ratio Lower Upper
95 100
174 84.7 0.0 170.8
176 81.3 0.0 162.0

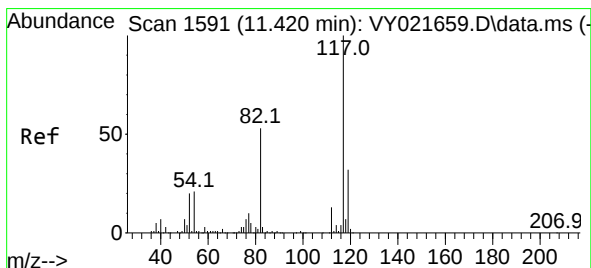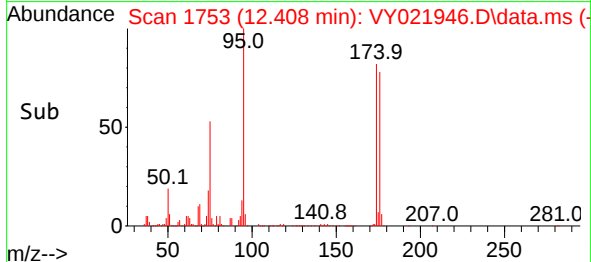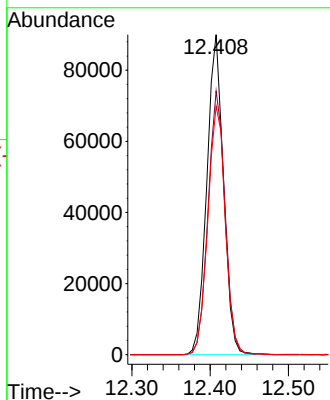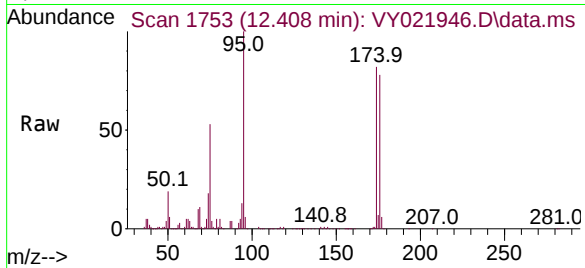

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 1590
Delta R.T. -0.006 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21

Tgt Ion: 117 Resp: 337671
Ion Ratio Lower Upper
117 100
82 56.8 42.8 64.2
119 31.3 25.7 38.5


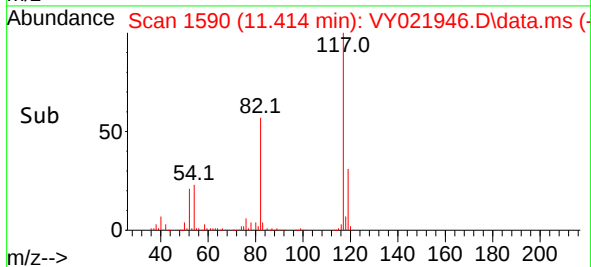
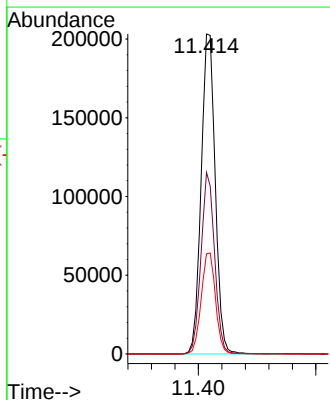
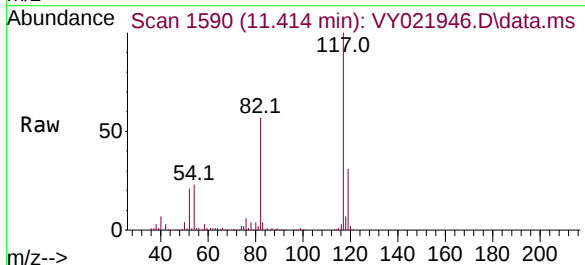


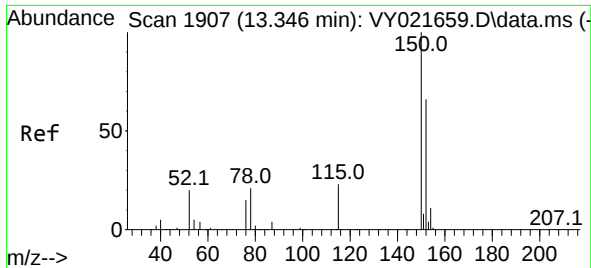

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 1907
 Delta R.T. 0.000 min
 Lab File: VY021946.D
 Acq: 21 Apr 2025 14:21




Instrument :
 MSVOA_Y
 ClientSampleId :
 PL-714-VOC-13


Tgt Ion:152 Resp: 129799
 Ion Ratio Lower Upper
 152 100
 115 58.8 28.8 86.5
 150 159.3 0.0 348.4

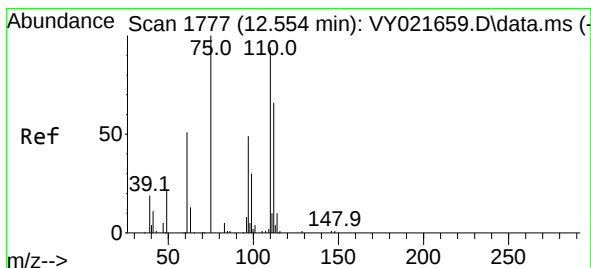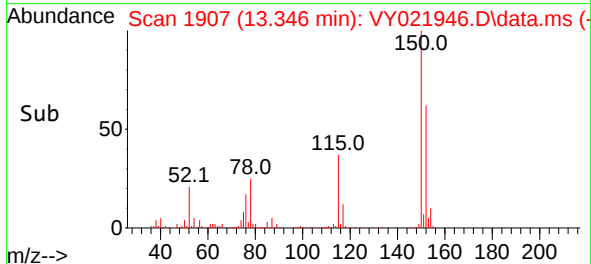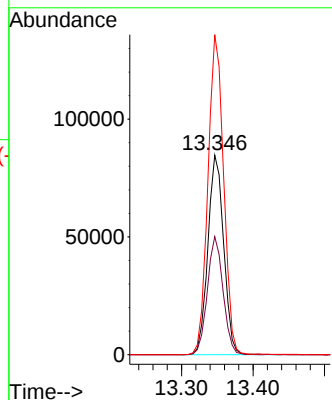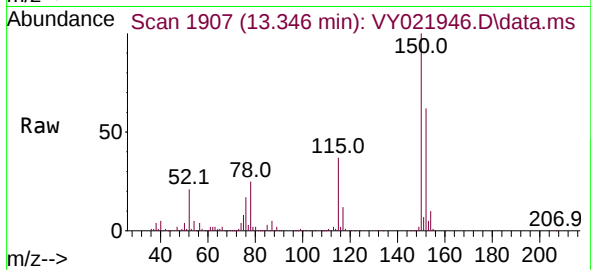

#76
 1,2,3-Trichloropropane
 Concen: 54.275 ug/l
 RT: 12.408 min Scan# 1753
 Delta R.T. -0.146 min
 Lab File: VY021946.D
 Acq: 21 Apr 2025 14:21

Tgt Ion: 75 Resp: 69833
 Ion Ratio Lower Upper
 75 100
 77 1.3 0.0 0.0#

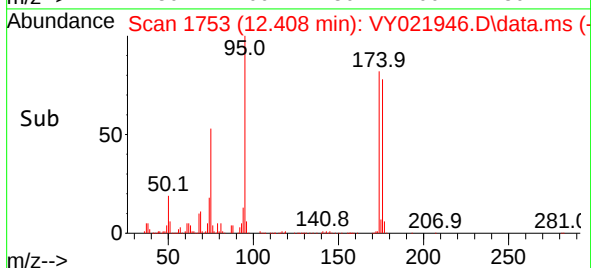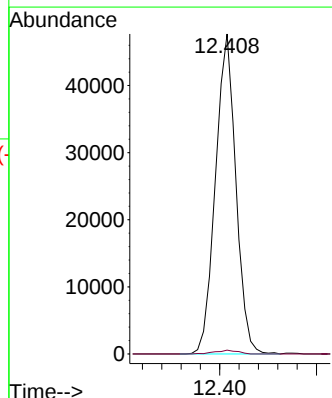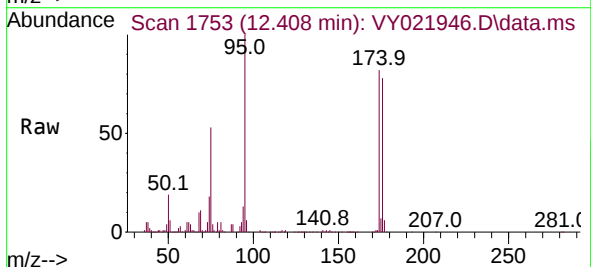

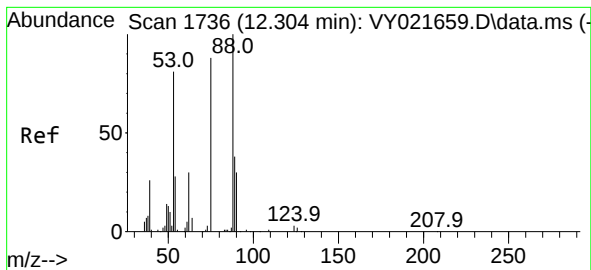

#81
 trans-1,4-Dichloro-2-butene
 Concen: 125.060 ug/l
 RT: 12.408 min Scan# 11
 Delta R.T. 0.104 min
 Lab File: VY021946.D
 Acq: 21 Apr 2025 14:21

Instrument :
 MSVOA_Y
 ClientSampleId :
 PL-714-VOC-13

Tgt Ion: 75 Resp: 69833
 Ion Ratio Lower Upper
 75 100
 53 0.3 76.1 114.1#
 89 0.0 36.2 54.4#

