

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042125\
 Data File : VY021946.D
 Acq On : 21 Apr 2025 14:21
 Operator : SY/MD
 Sample : Q1842-32
 Misc : 5.27g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 PL-714-VOC-13

Quant Time: Apr 22 02:45:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 28 02:30:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	200754	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	379227	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	337671	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	129799	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	119295	54.845	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	109.700%
35) Dibromofluoromethane	7.634	113	131285	53.368	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	106.740%
50) Toluene-d8	10.109	98	467477	49.952	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.900%
62) 4-Bromofluorobenzene	12.408	95	132582	41.884	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	83.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042125\
Data File : VY021946.D
Acq On : 21 Apr 2025 14:21
Operator : SY/MD
Sample : Q1842-32
Misc : 5.27g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-13

Quant Time: Apr 22 02:45:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 28 02:30:29 2025
Response via : Initial Calibration




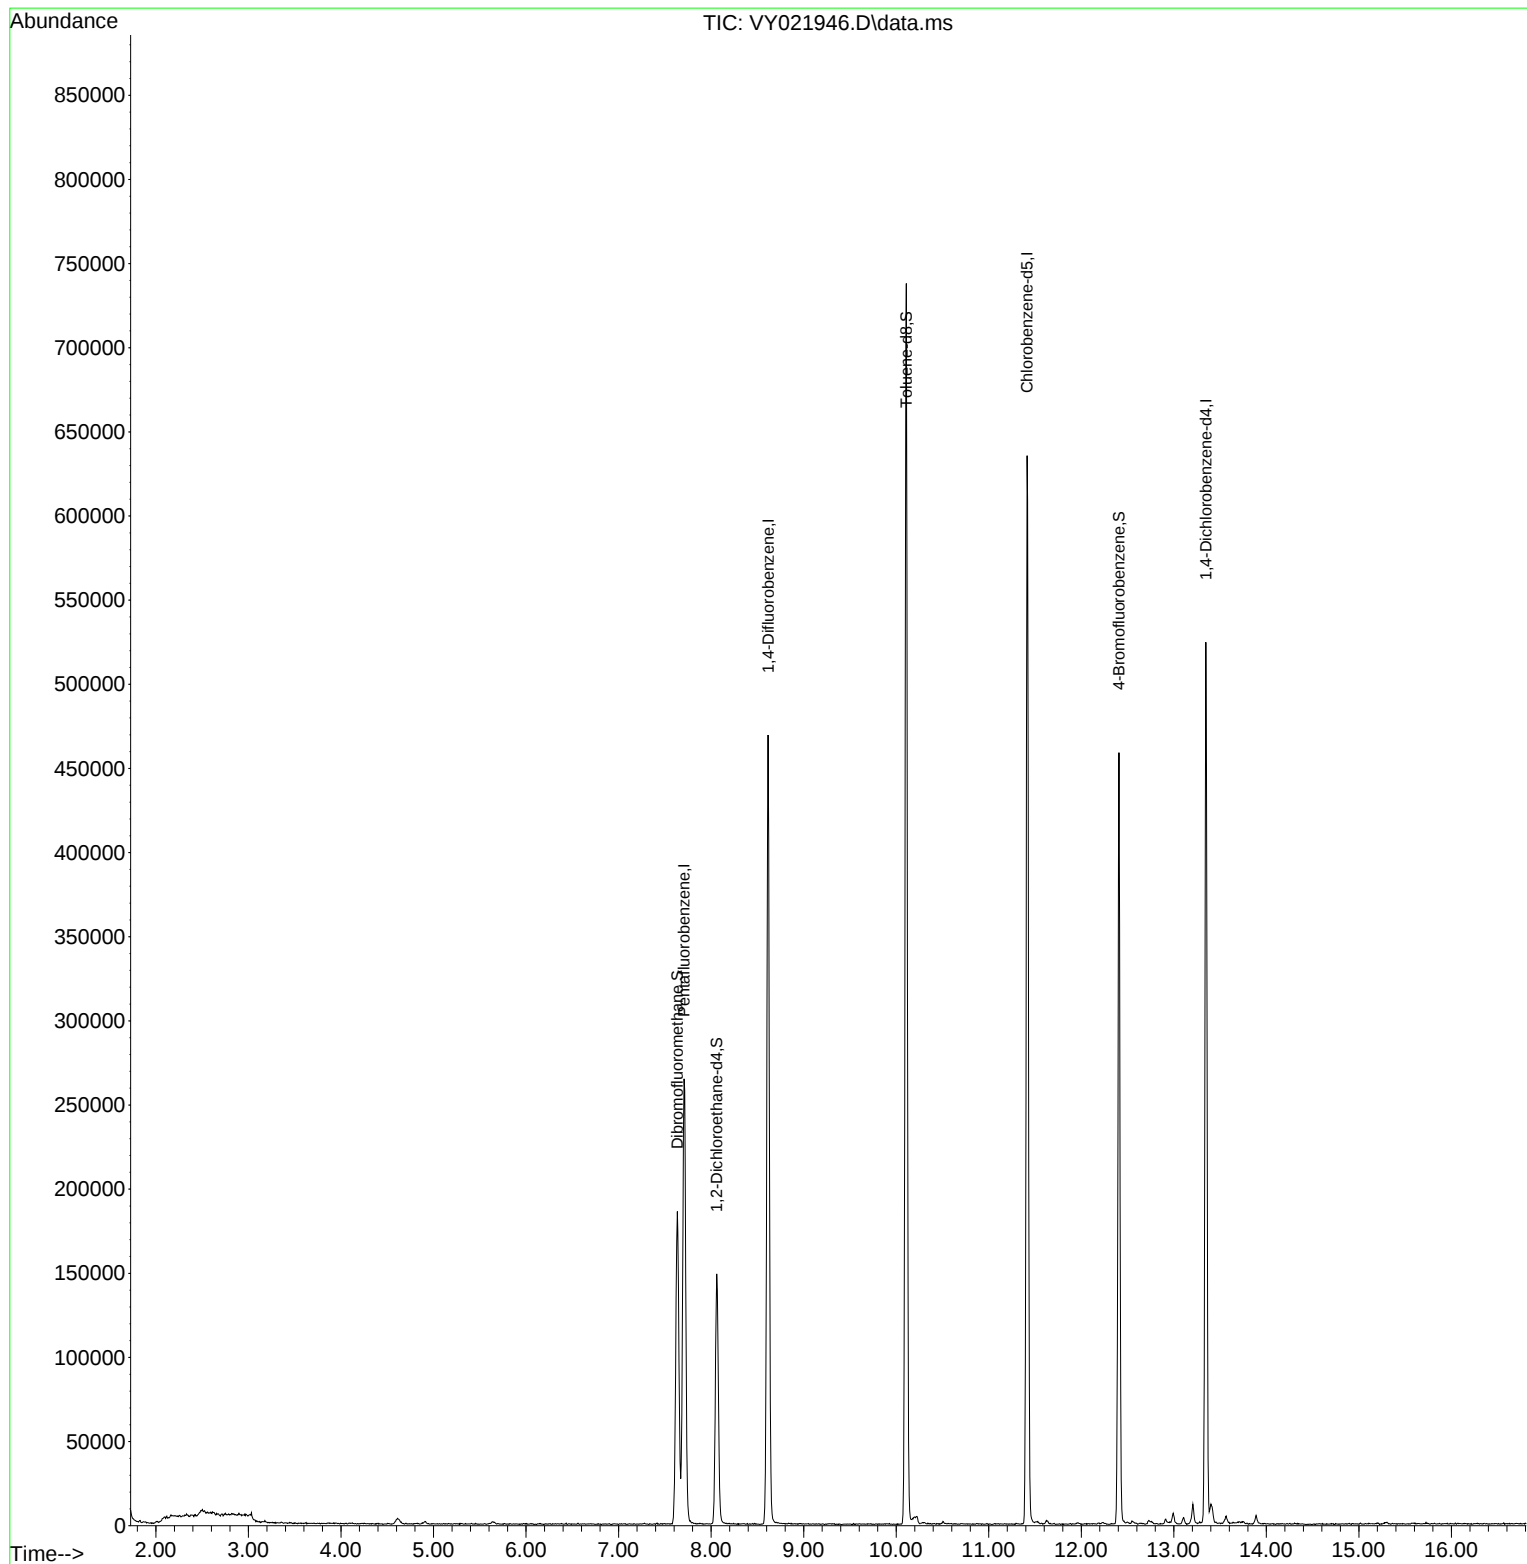


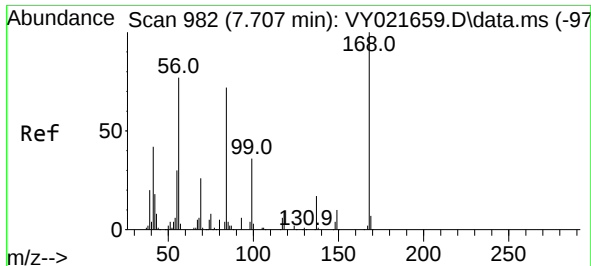

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-13


Tgt Ion:168 Resp: 200754
Ion Ratio Lower Upper
168 100
99 54.6 46.7 70.1

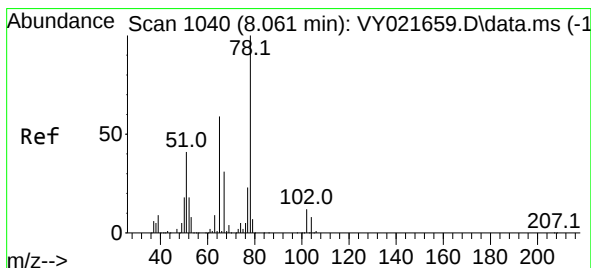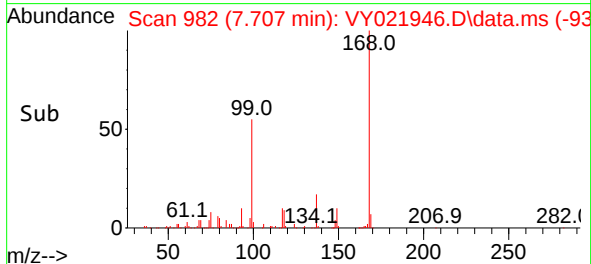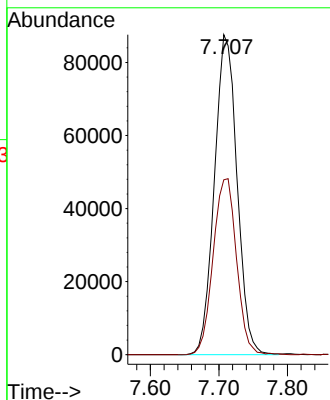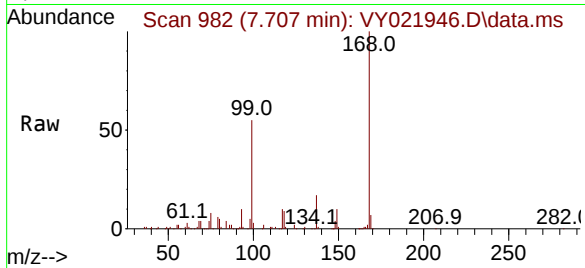

#33
1,2-Dichloroethane-d4
Concen: 54.845 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21

Tgt Ion: 65 Resp: 119295
Ion Ratio Lower Upper
65 100
67 52.9 0.0 104.6

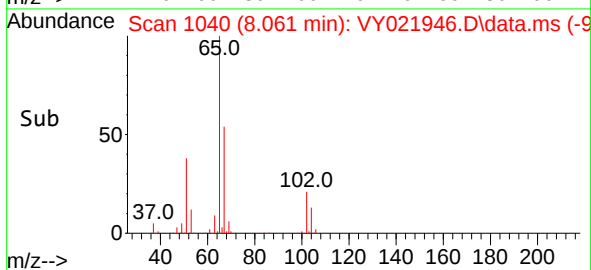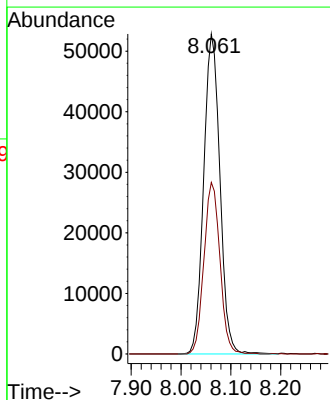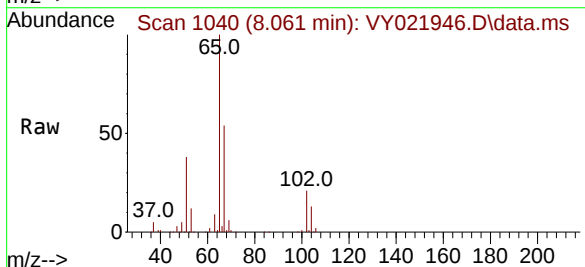

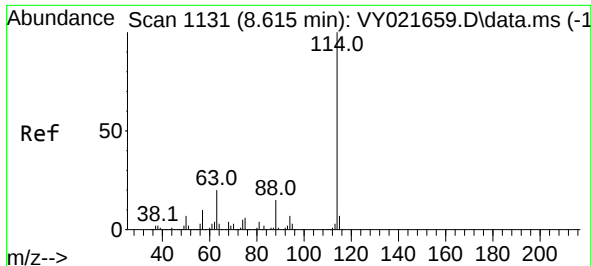

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY021946.D

Acq: 21 Apr 2025 14:21

Instrument :

MSVOA_Y

ClientSampleId :

PL-714-VOC-13





Tgt Ion:114 Resp: 379227

Ion Ratio Lower Upper

114 100

63 20.2 0.0 40.2

88 15.9 0.0 29.8

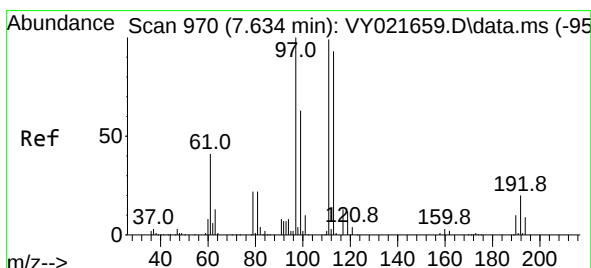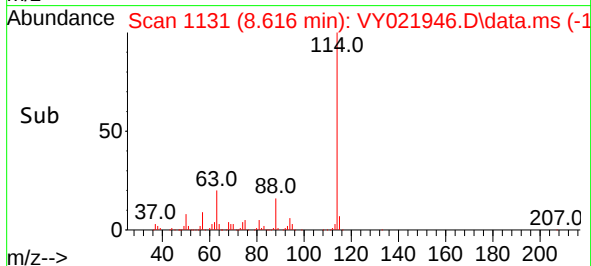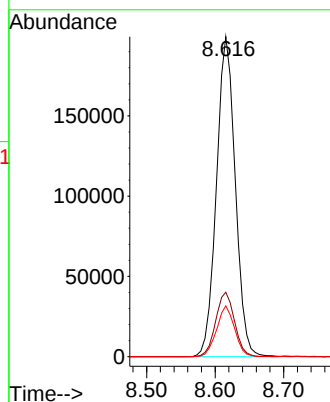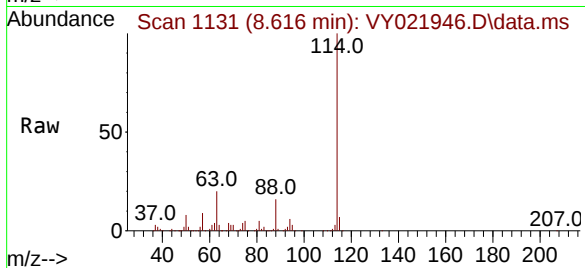

#35

Dibromofluoromethane

Concen: 53.368 ug/l

RT: 7.634 min Scan# 970

Delta R.T. 0.000 min

Lab File: VY021946.D

Acq: 21 Apr 2025 14:21




Tgt Ion:113 Resp: 131285


Ion Ratio Lower Upper

113 100

111 102.0 82.6 123.8

192 19.8 16.2 24.4

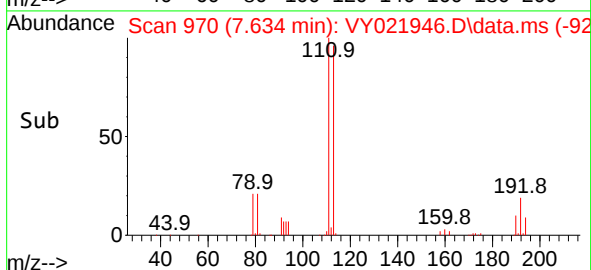
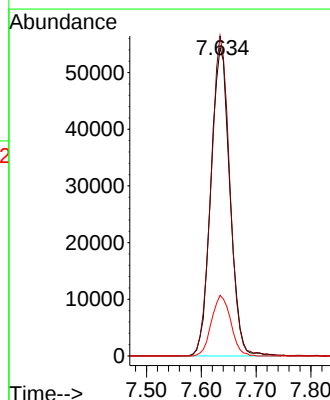
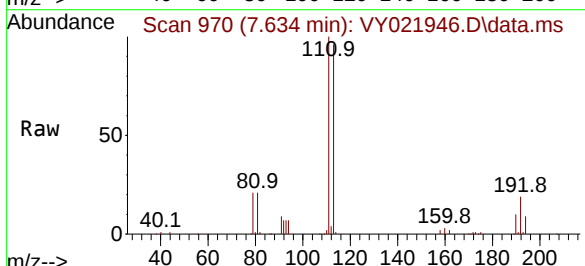


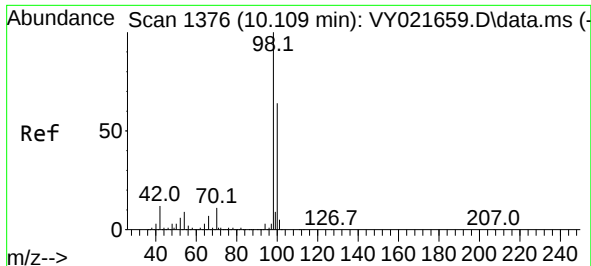

#50
Toluene-d8
Concen: 49.952 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21




Instrument :
MSVOA_Y
ClientSampleId :
PL-714-VOC-13


Tgt Ion: 98 Resp: 467477
Ion Ratio Lower Upper
98 100
100 63.8 52.1 78.1

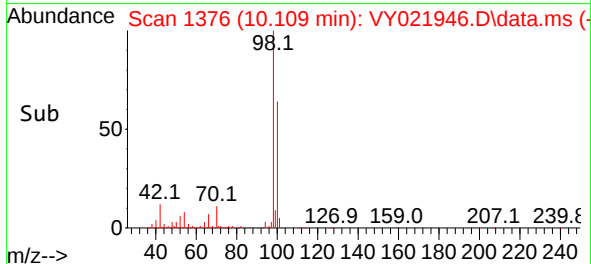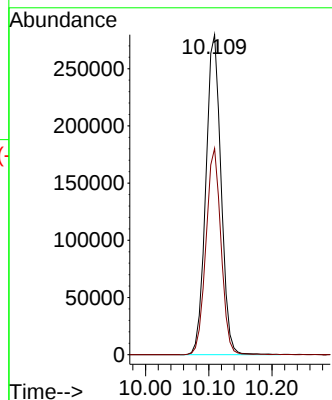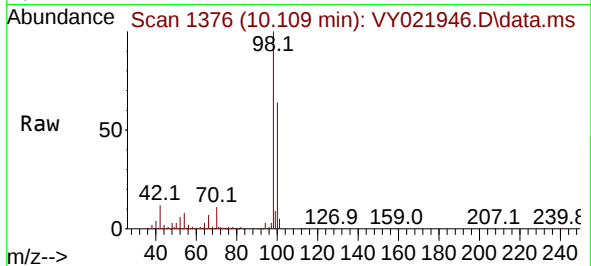

#62
4-Bromofluorobenzene
Concen: 41.884 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY021946.D
Acq: 21 Apr 2025 14:21

Tgt Ion: 95 Resp: 132582
Ion Ratio Lower Upper
95 100
174 84.7 0.0 170.8
176 81.3 0.0 162.0

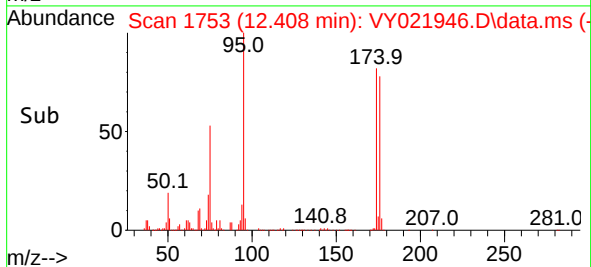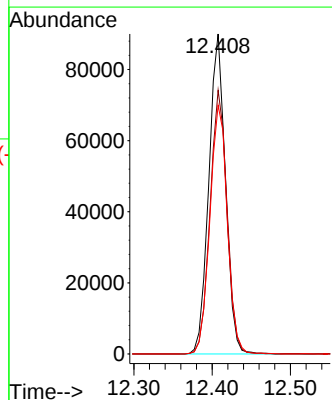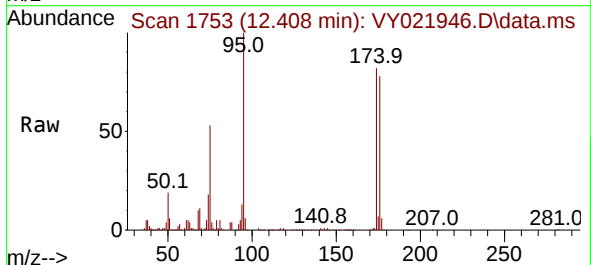

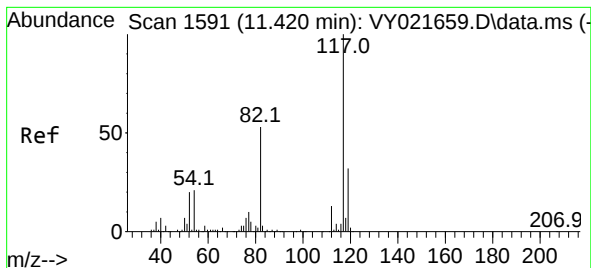

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY021946.D

Acq: 21 Apr 2025 14:21

Instrument :

MSVOA_Y

ClientSampleId :

PL-714-VOC-13





Tgt Ion:117 Resp: 337671

Ion Ratio Lower Upper

117 100

82 56.8 42.8 64.2

119 31.3 25.7 38.5

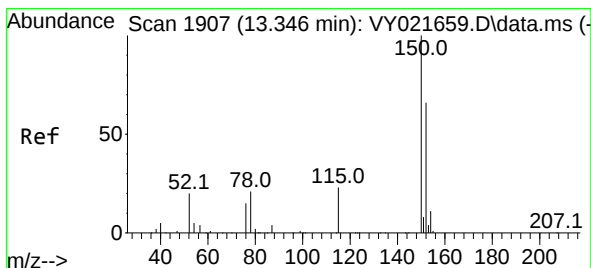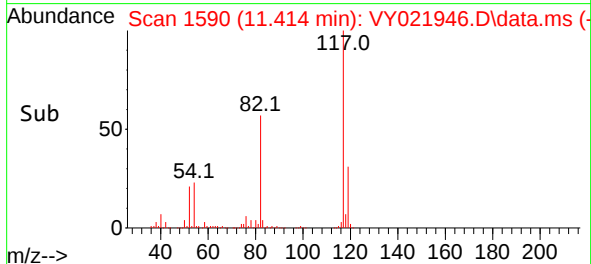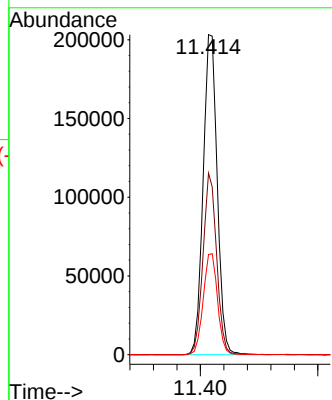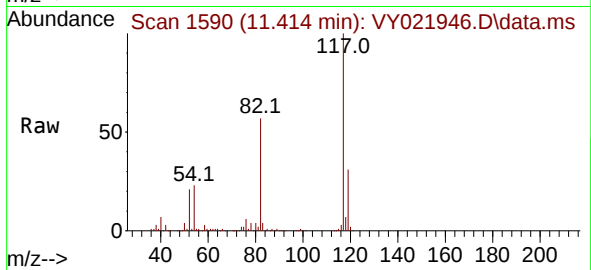

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY021946.D

Acq: 21 Apr 2025 14:21

Tgt Ion:152 Resp: 129799

Ion Ratio Lower Upper

152 100

115 58.8 28.8 86.5

150 159.3 0.0 348.4

