
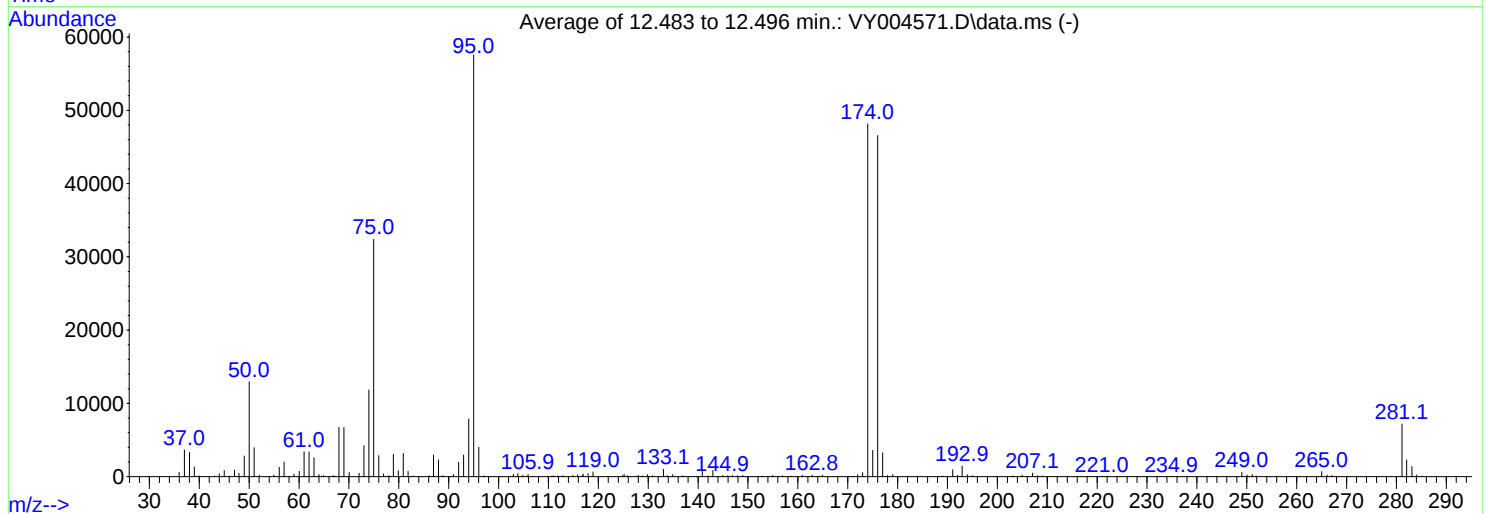


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042221\
Data File : VY004571.D
Acq On : 22 Apr 2021 09:08
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041221S.M
Title : SW846 8260
Last Update : Tue Apr 13 03:38:02 2021

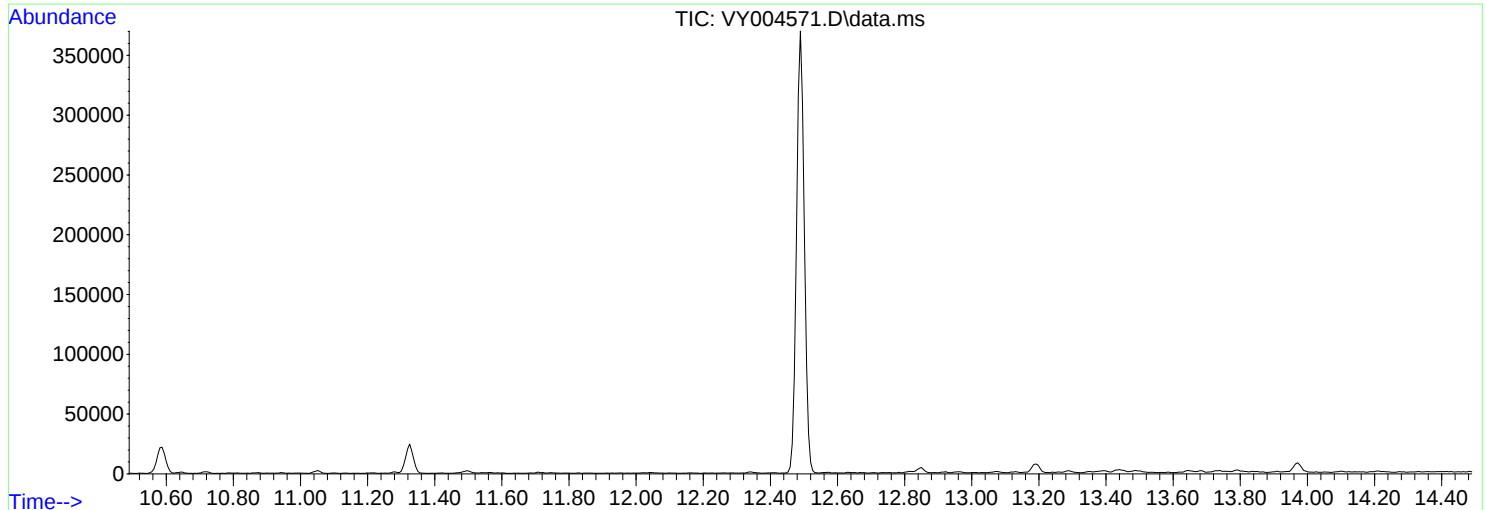

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	12962	PASS
75	95	30	60	56.3	32394	PASS
95	95	100	100	100.0	57573	PASS
96	95	5	9	7.0	4010	PASS
173	174	0.00	2	1.2	556	PASS
174	95	50	100	83.6	48152	PASS
175	174	5	9	7.4	3579	PASS
176	174	95	101	96.7	46568	PASS
177	176	5	9	7.0	3248	PASS