

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042222\
 Data File : VY008463.D
 Acq On : 22 Apr 2022 14:37
 Operator : KP/MD
 Sample : N2523-03
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SU-04-042122

Quant Time: Apr 23 01:52:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042122S.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 21 14:28:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	0.000	168	0	0.000	ug/l	-7.79
34) 1,4-Difluorobenzene	8.691	114	248	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	42	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ug/l	-13.43

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.000	65	0	0.000	ug/l	
Spiked Amount	50.000	Range	50 - 163	Recovery	=	0.000%#
35) Dibromofluoromethane	0.000	113	0	0.000	ug/l	
Spiked Amount	50.000	Range	54 - 147	Recovery	=	0.000%#
50) Toluene-d8	10.179	98	197	31.714	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	63.420%
62) 4-Bromofluorobenzene	0.000	95	0	0.000	ug/l	
Spiked Amount	50.000	Range	25 - 144	Recovery	=	0.000%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042222\
Data File : VY008463.D
Acq On : 22 Apr 2022 14:37
Operator : KP/MD
Sample : N2523-03
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SU-04-042122

Quant Time: Apr 23 01:52:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042122S.M
Quant Title : SW846 8260
QLast Update : Thu Apr 21 14:28:40 2022
Response via : Initial Calibration

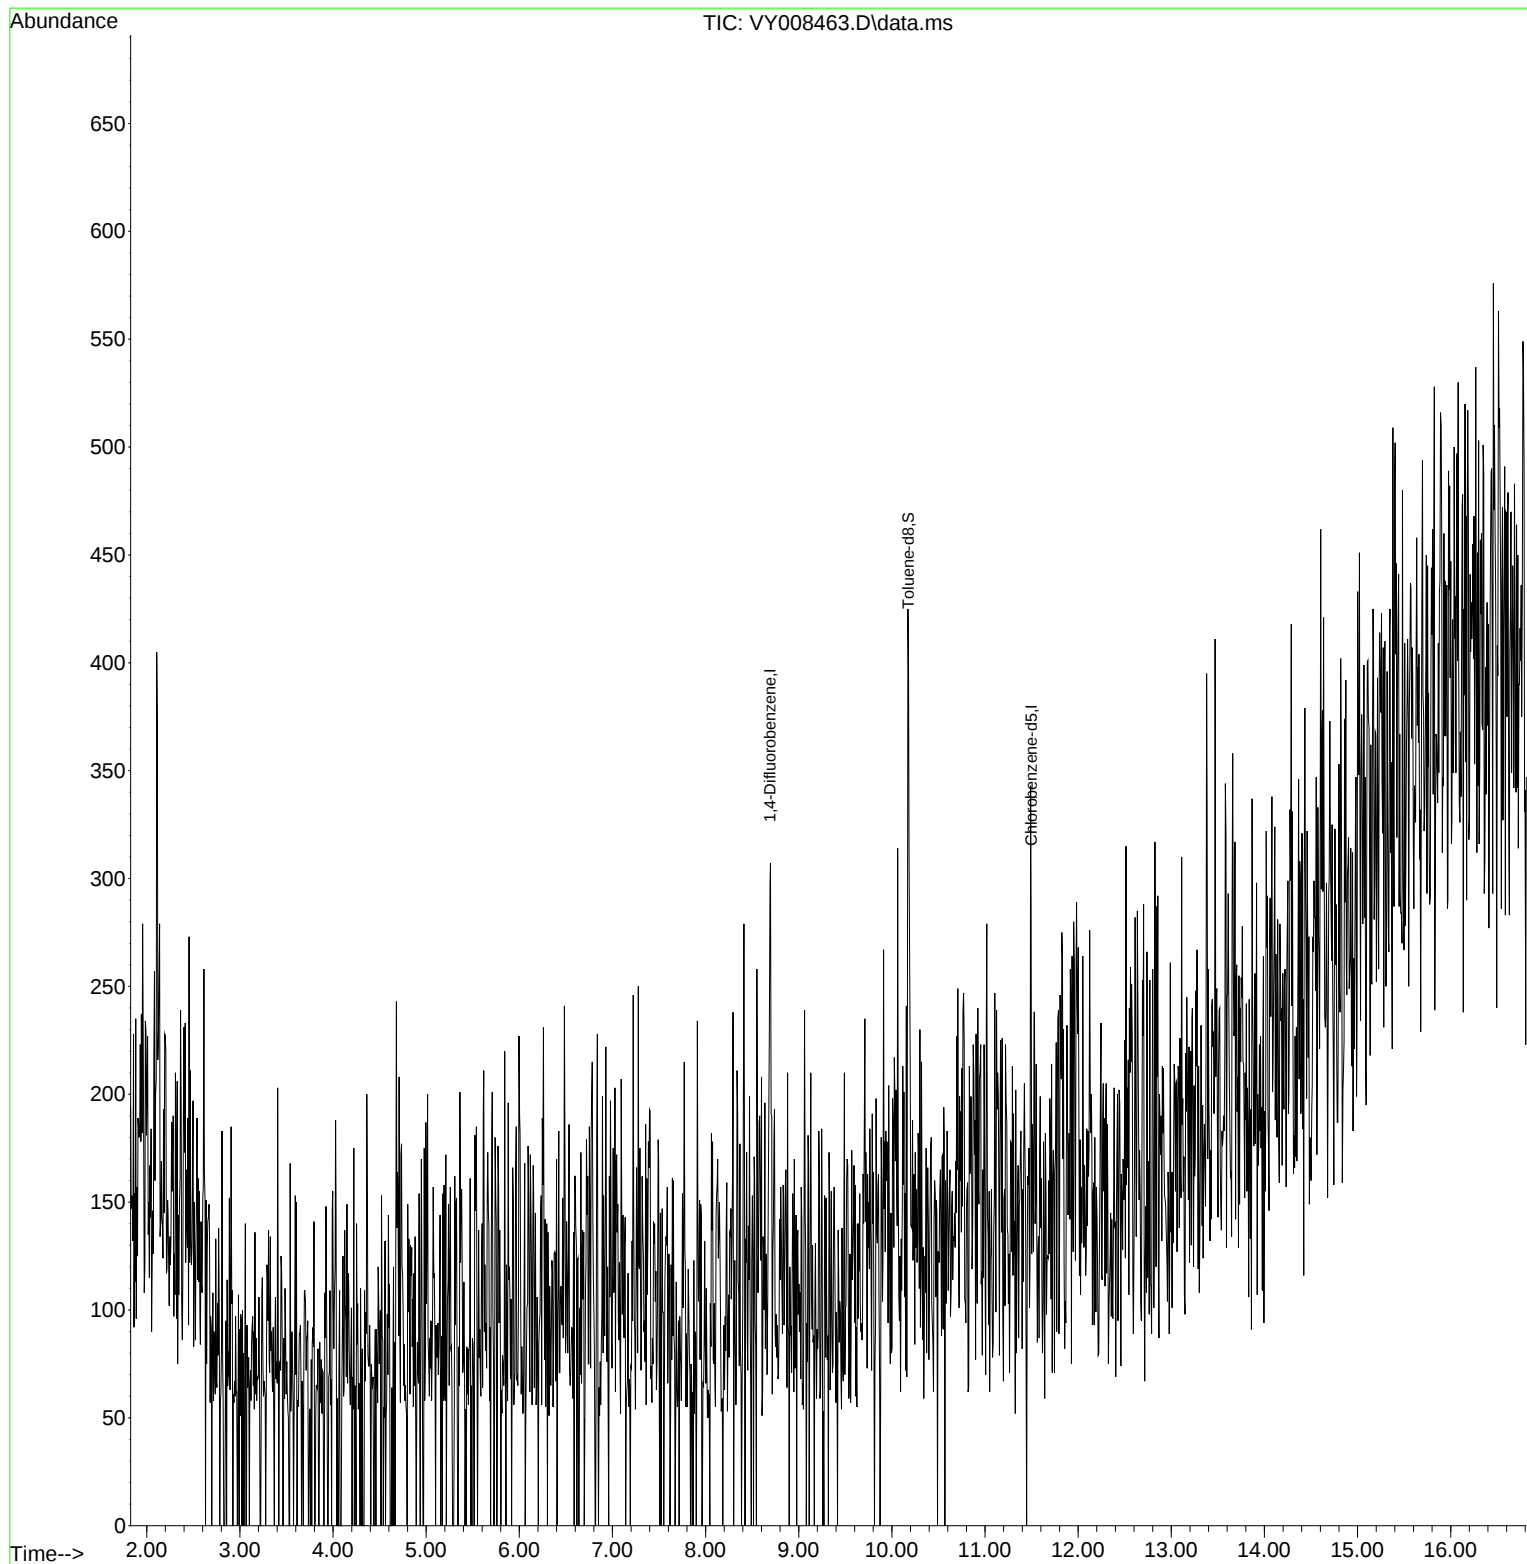


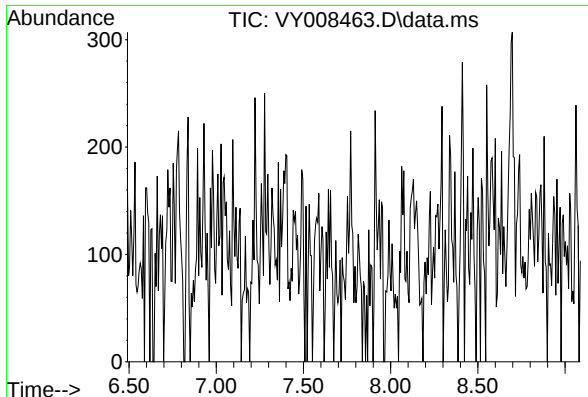


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 7.79 min

Lab File: VY008463.D
Acq: 22 Apr 2022 14:37

Instrument :
MSVOA_Y
ClientSampleId :
SU-04-042122


Tgt Ion: 168
Sig Exp Ratio
168 100
99 58.6

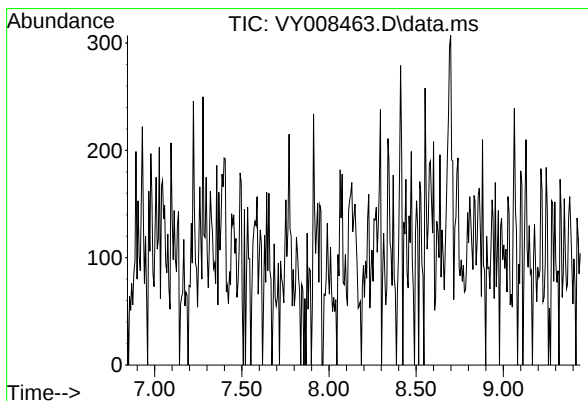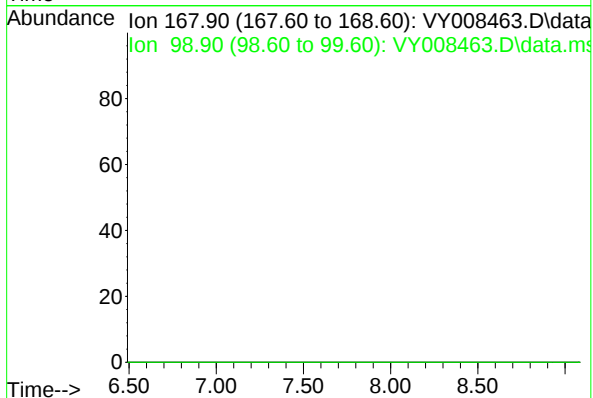


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 8.14 min

Lab File: VY008463.D
Acq: 22 Apr 2022 14:37

Tgt Ion: 65
Sig Exp Ratio
65 100
67 49.7

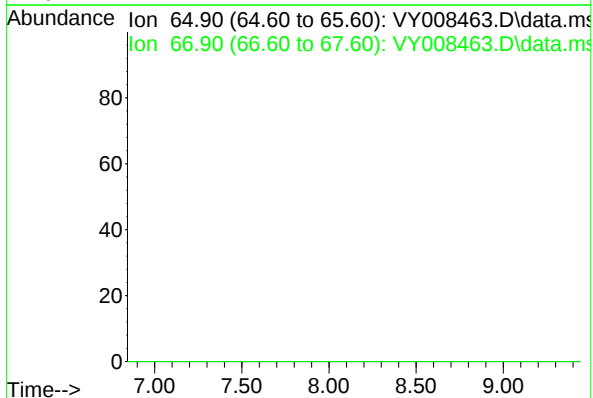

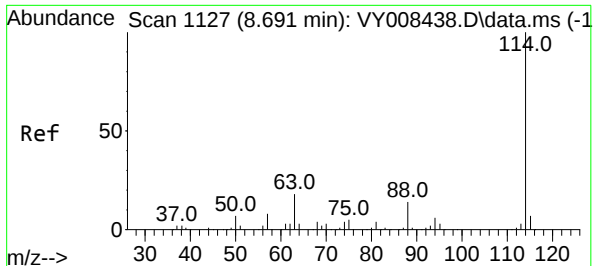

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY008463.D

Acq: 22 Apr 2022 14:37

Instrument :

MSVOA_Y

ClientSampleId :

SU-04-042122





Tgt Ion:114 Resp: 248

Ion Ratio Lower Upper

114 100

63 0.0 0.0 43.2

88 0.0 0.0 31.8

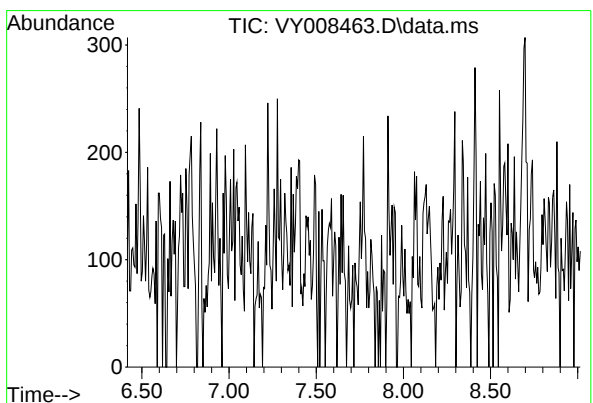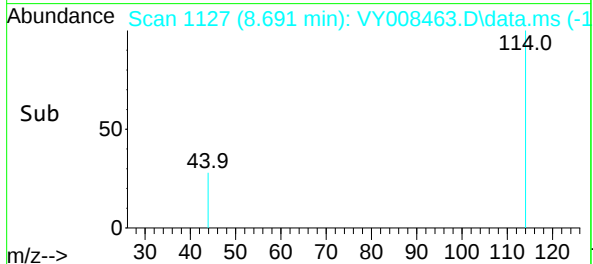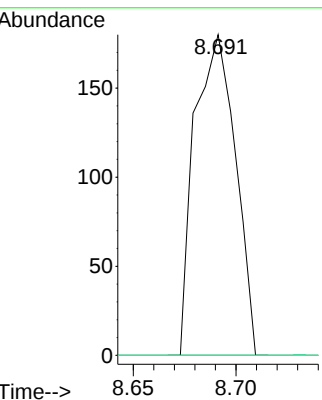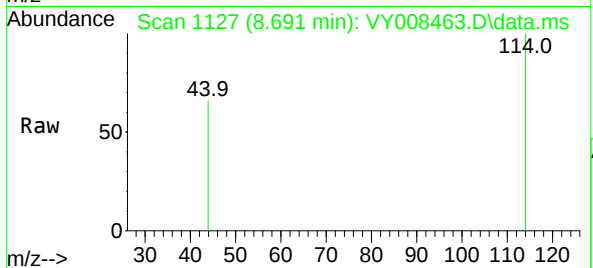

#35

Dibromofluoromethane

Concen: 0.000 ug/l

Expected RT: 7.72 min

Lab File: VY008463.D

Acq: 22 Apr 2022 14:37


Tgt Ion: 113


Sig Exp Ratio

113 100

111 103.3

192 22.0




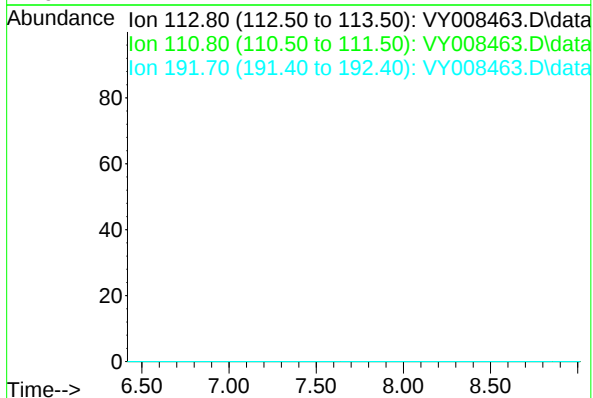


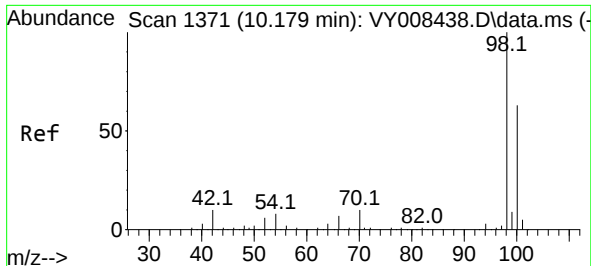

#50
Toluene-d8
Concen: 31.714 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY008463.D
Acq: 22 Apr 2022 14:37

Instrument :
MSVOA_Y
ClientSampleId :
SU-04-042122


Tgt Ion: 98 Resp: 197
Ion Ratio Lower Upper
98 100
100 19.3 50.2 75.2#

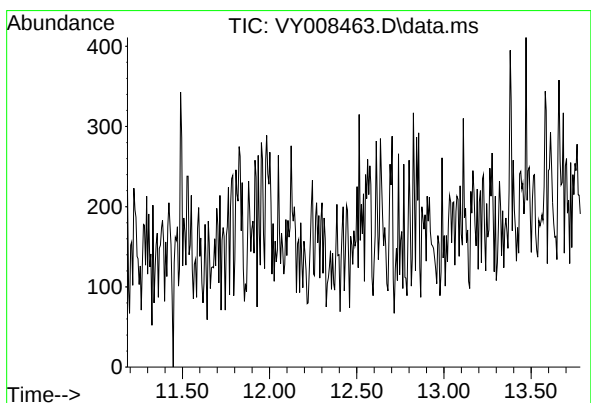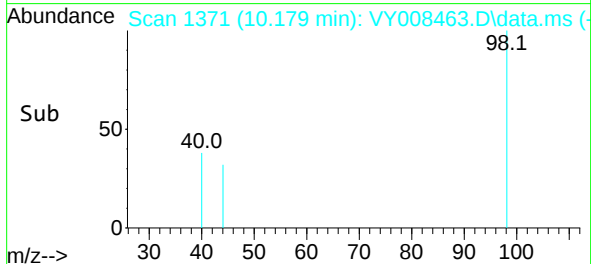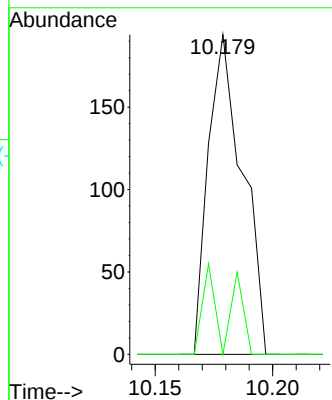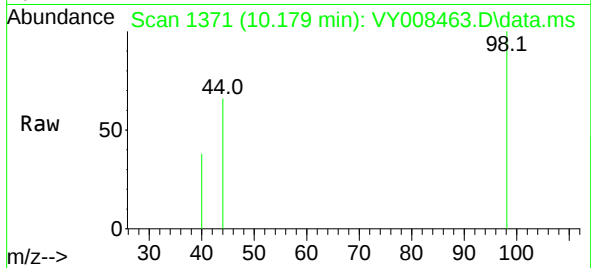


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.48 min

Lab File: VY008463.D
Acq: 22 Apr 2022 14:37


Tgt Ion: 95
Sig Exp Ratio
95 100
174 88.5
176 87.9

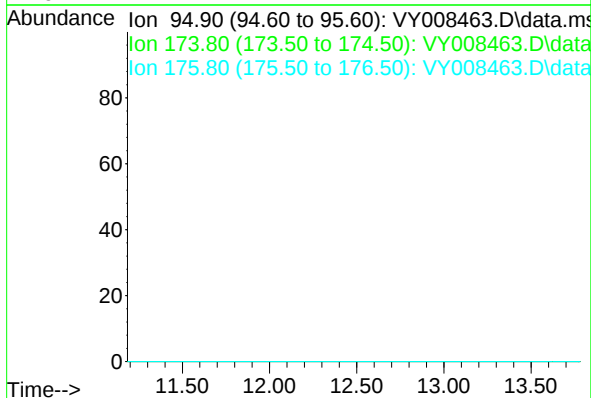



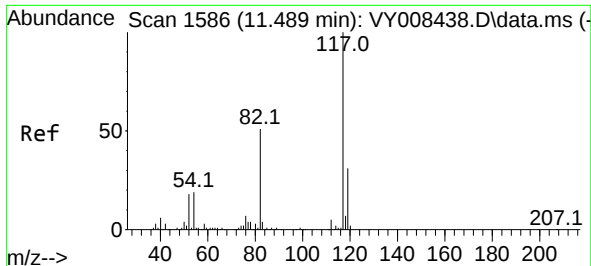


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 11
Delta R.T. 0.007 min
Lab File: VY008463.D
Acq: 22 Apr 2022 14:37

Instrument :
MSVOA_Y
ClientSampleId :
SU-04-042122

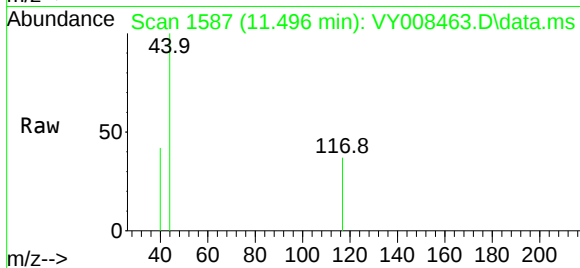

Tgt Ion:117 Resp: 42
Ion Ratio Lower Upper
117 100
82 0.0 43.0 64.4#
119 0.0 25.4 38.0#

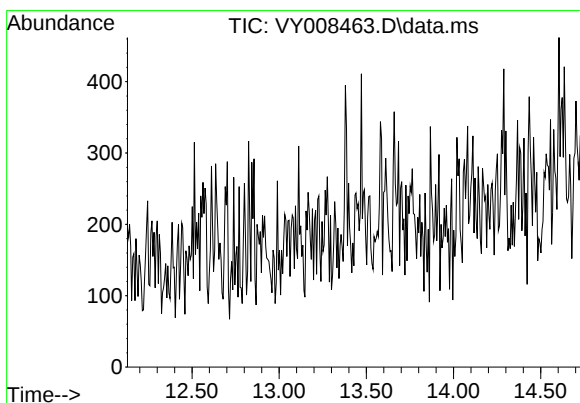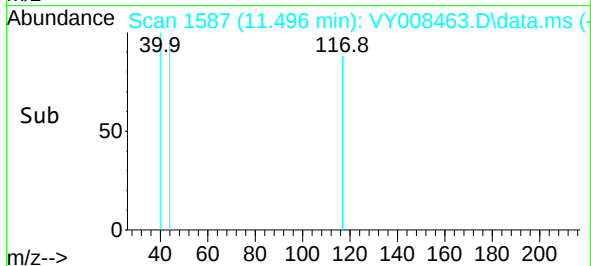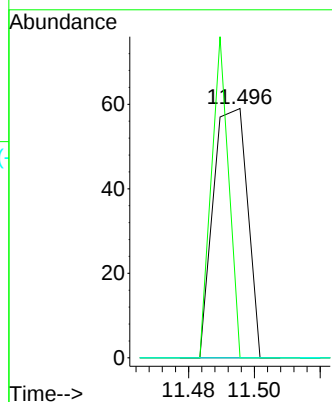

#72
1,4-Dichlorobenzene-d4
Concen: 0.000 ug/l
Expected RT: 13.43 min

Lab File: VY008463.D
Acq: 22 Apr 2022 14:37

Tgt Ion: 152
Sig Exp Ratio
152 100
115 56.5
150 173.8

