

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042325\
 Data File : VY021974.D
 Acq On : 23 Apr 2025 16:13
 Operator : SY/MD
 Sample : Q1852-01
 Misc : 5.45g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ETGI-354

Quant Time: Apr 24 03:46:52 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	317664	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	606820	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	519582	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	187426	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	150743	51.374	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 102.740%	
35) Dibromofluoromethane	7.634	113	197428	49.246	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 98.500%	
50) Toluene-d8	10.109	98	716691	47.420	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 94.840%	
62) 4-Bromofluorobenzene	12.408	95	192056	37.747	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 75.500%	
Target Compounds						
					Qvalue	
16) Acetone	3.873	43	366	Below Cal	#	41
31) Cyclohexane	7.701	56	5982	1.233	ug/l #	5
36) 1,1-Dichloropropene	7.707	75	23768	4.414	ug/l #	42
38) Carbon Tetrachloride	7.707	117	32112	4.990	ug/l #	17
51) 4-Methyl-2-Pentanone	10.103	43	2379	1.222	ug/l #	1
76) 1,2,3-Trichloropropane	12.408	75	93534	58.262	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.408	75	93534	140.304	ug/l #	16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 24 03:46:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY021974.D
Acq: 23 Apr 2025 16:13




Instrument :
MSVOA_Y
ClientSampleId :
ETGI-354


Tgt Ion:168 Resp: 317664
Ion Ratio Lower Upper
168 100
99 52.9 43.1 64.7

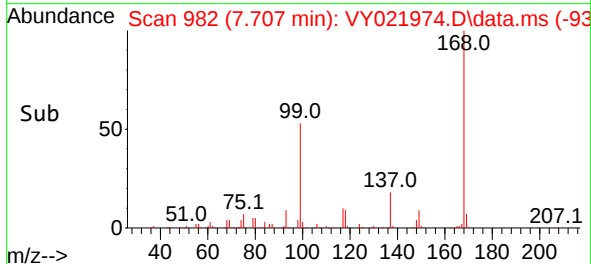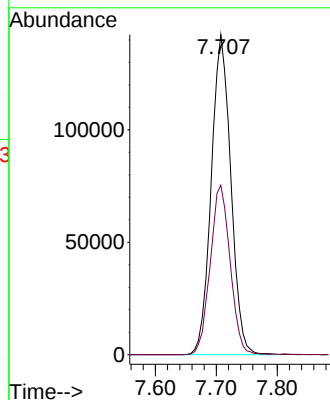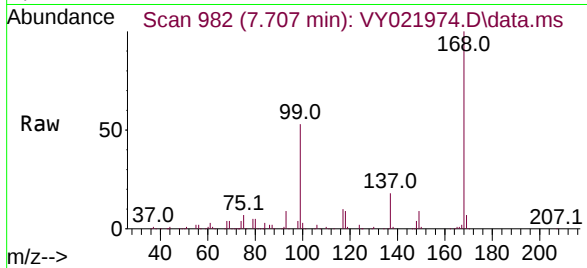

#16
Acetone
Concen: Below Cal
RT: 3.873 min Scan# 353
Delta R.T. -0.006 min
Lab File: VY021974.D
Acq: 23 Apr 2025 16:13

Tgt Ion: 43 Resp: 366
Ion Ratio Lower Upper
43 100
58 0.0 27.0 40.4#



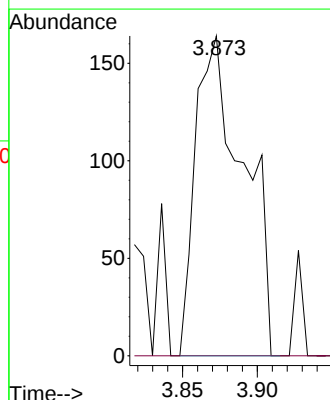
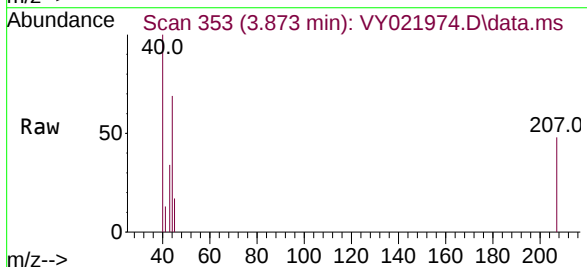


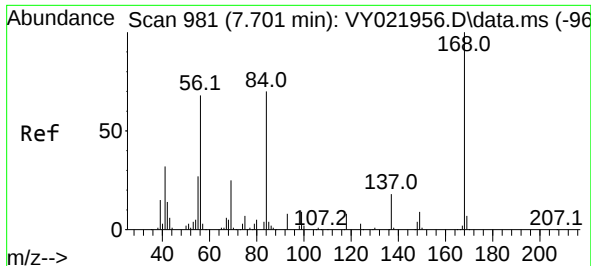

#31
Cyclohexane
Concen: 1.233 ug/l
RT: 7.701 min Scan# 981
Delta R.T. -0.000 min
Lab File: VY021974.D
Acq: 23 Apr 2025 16:13




Instrument :
MSVOA_Y
ClientSampleId :
ETGI-354


Tgt Ion: 56 Resp: 5982
Ion Ratio Lower Upper
56 100
69 179.4 29.4 44.2#
84 146.1 82.2 123.4#

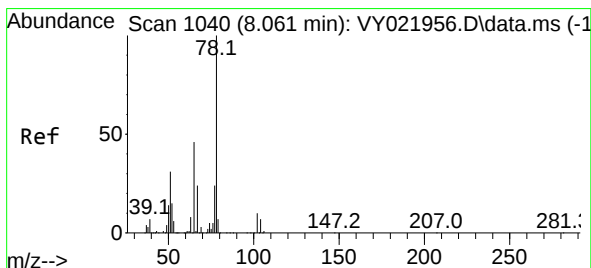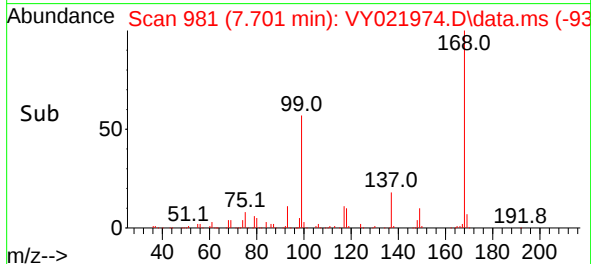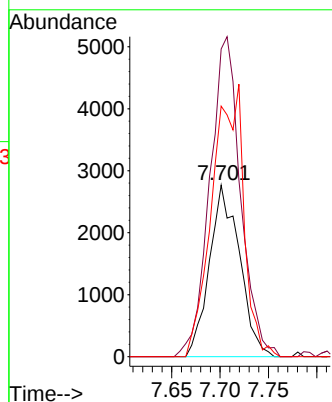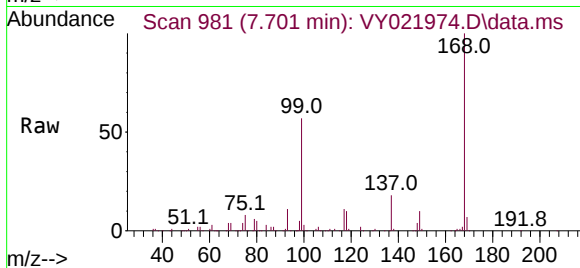

#33
1,2-Dichloroethane-d4
Concen: 51.374 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY021974.D
Acq: 23 Apr 2025 16:13

Tgt Ion: 65 Resp: 150743
Ion Ratio Lower Upper
65 100
67 52.1 0.0 105.8


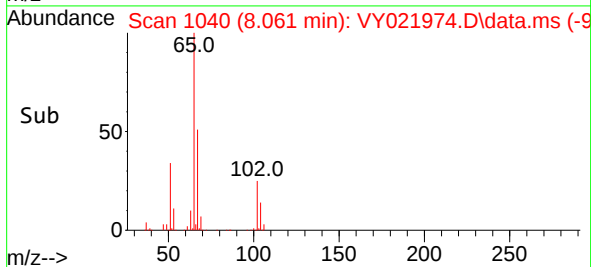
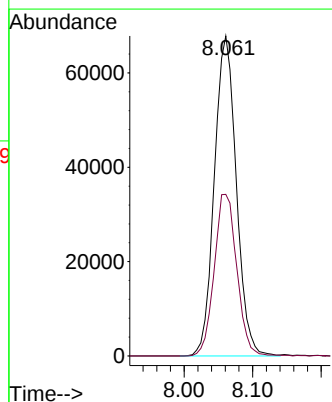
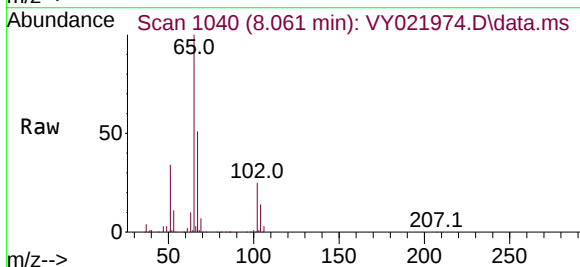


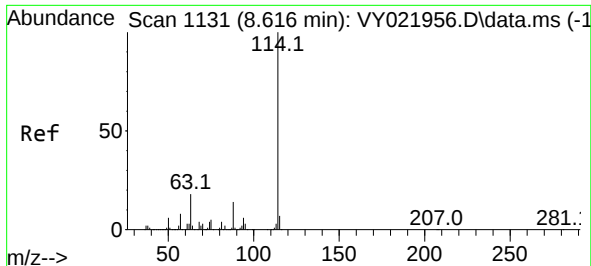

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VY021974.D
Acq: 23 Apr 2025 16:13




Instrument :
MSVOA_Y
ClientSampleId :
ETGI-354


Tgt Ion:114 Resp: 606820
Ion Ratio Lower Upper
114 100
63 18.0 0.0 35.4
88 14.6 0.0 28.2

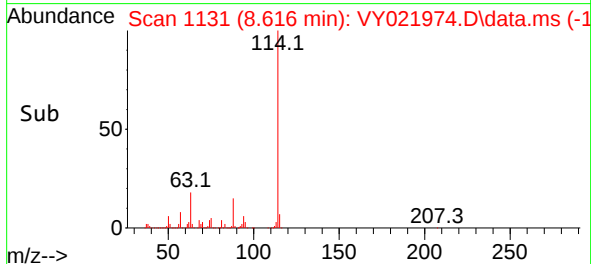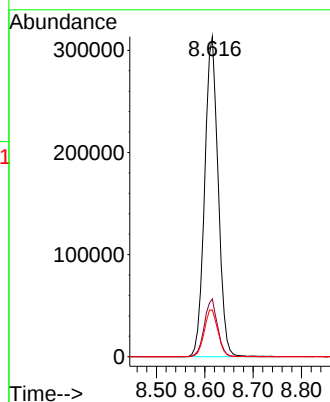

#35
Dibromofluoromethane
Concen: 49.246 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.000 min
Lab File: VY021974.D
Acq: 23 Apr 2025 16:13

Tgt Ion:113 Resp: 197428
Ion Ratio Lower Upper
113 100
111 101.3 81.8 122.8
192 19.4 15.6 23.4

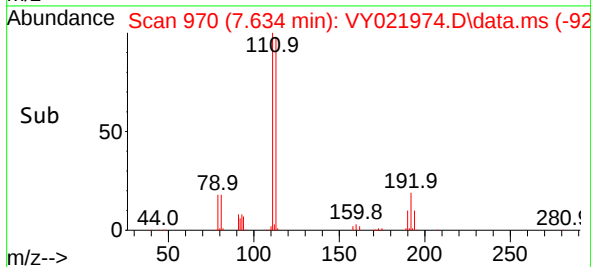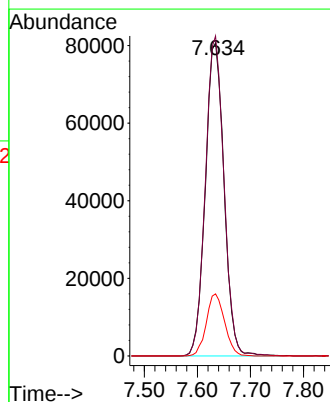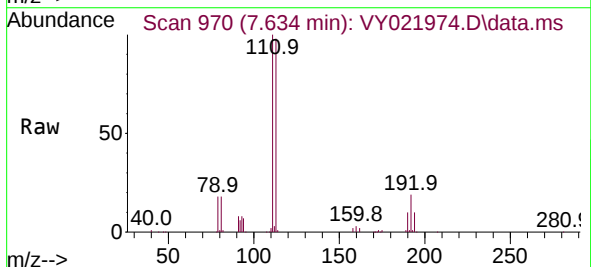

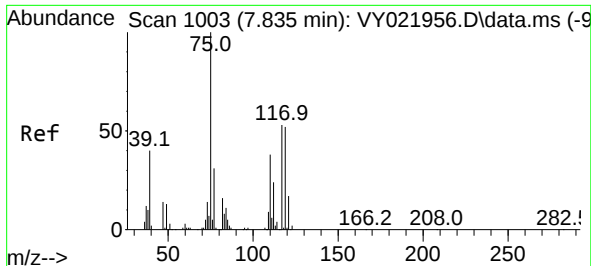

#36

1,1-Dichloropropene

Concen: 4.414 ug/l

RT: 7.707 min Scan# 982

Delta R.T. -0.128 min

Lab File: VY021974.D

Acq: 23 Apr 2025 16:13

Instrument :

MSVOA_Y

ClientSampleId :

ETGI-354





Tgt Ion: 75 Resp: 23768

Ion Ratio Lower Upper

75 100

110 3.0 19.1 57.3#

77 0.1 25.5 38.3#

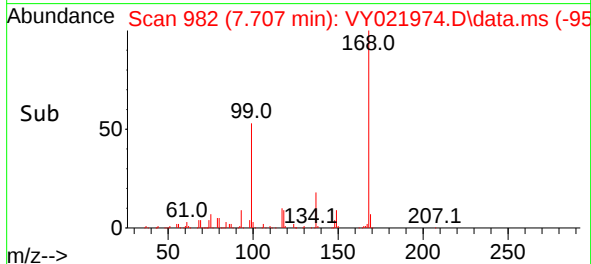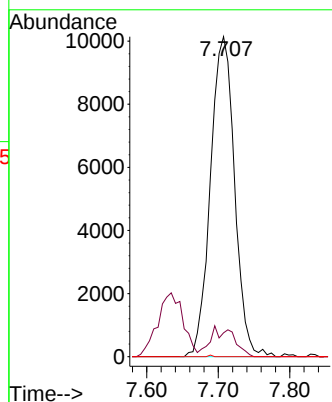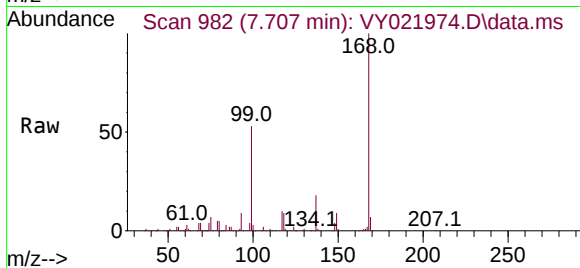

#38

Carbon Tetrachloride

Concen: 4.990 ug/l

RT: 7.707 min Scan# 982

Delta R.T. -0.110 min

Lab File: VY021974.D

Acq: 23 Apr 2025 16:13




Tgt Ion: 117 Resp: 32112


Ion Ratio Lower Upper

117 100

119 5.5 76.2 114.4#

121 0.0 24.0 36.0#


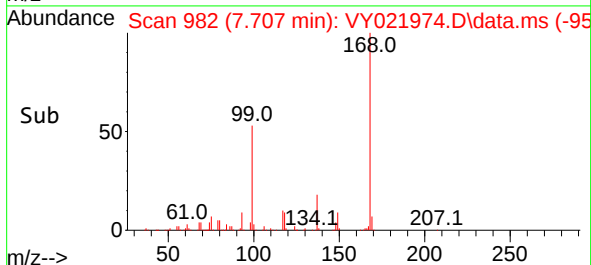
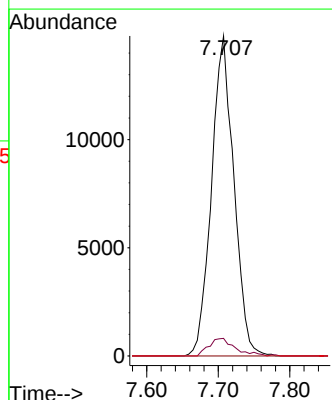
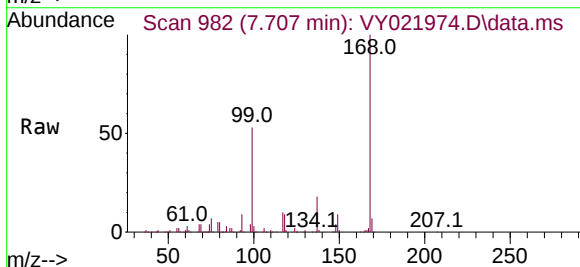


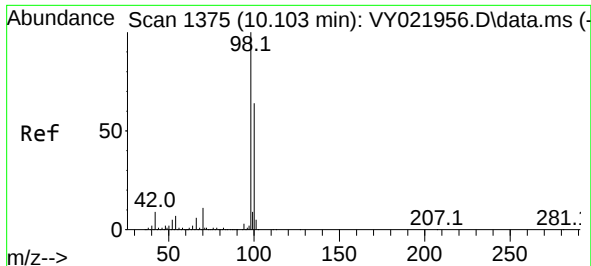

#50
Toluene-d8
Concen: 47.420 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.006 min
Lab File: VY021974.D
Acq: 23 Apr 2025 16:13




Instrument :
MSVOA_Y
ClientSampleId :
ETGI-354


Tgt Ion: 98 Resp: 716691
Ion Ratio Lower Upper
98 100
100 64.1 51.6 77.4

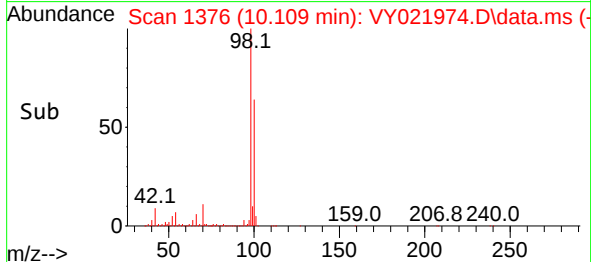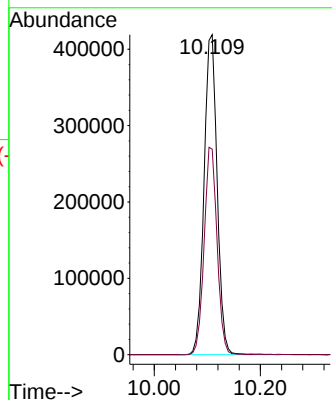

#51
4-Methyl-2-Pentanone
Concen: 1.222 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. 0.104 min
Lab File: VY021974.D
Acq: 23 Apr 2025 16:13

Tgt Ion: 43 Resp: 2379
Ion Ratio Lower Upper
43 100
58 216.4 36.6 55.0#


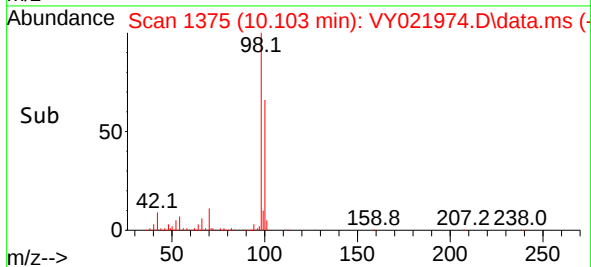
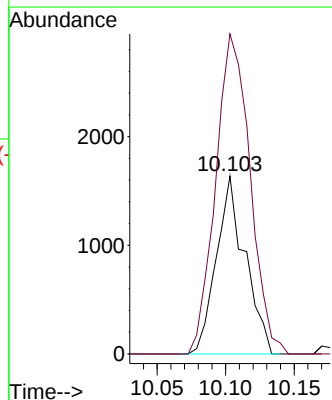
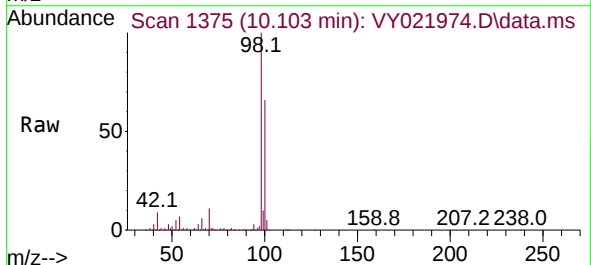




#62
4-Bromofluorobenzene
Concen: 37.747 ug/l
RT: 12.408 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY021974.D
Acq: 23 Apr 2025 16:13




Instrument :
MSVOA_Y
ClientSampleId :
ETGI-354


Tgt Ion: 95 Resp: 192056
Ion Ratio Lower Upper
95 100
174 88.1 0.0 179.0
176 84.7 0.0 171.8

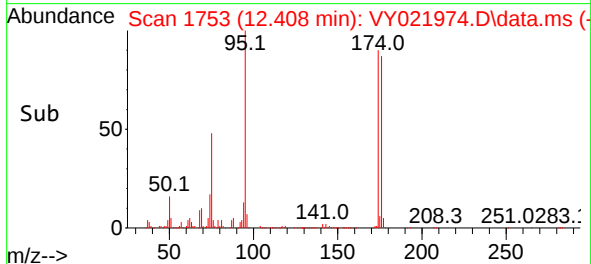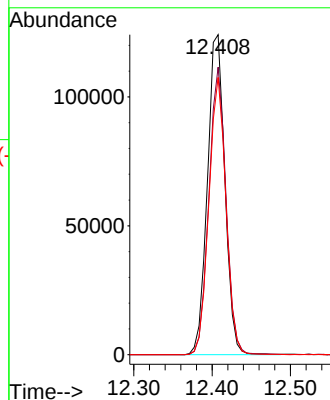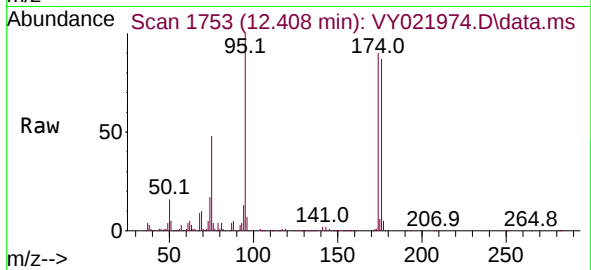

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 1590
Delta R.T. -0.000 min
Lab File: VY021974.D
Acq: 23 Apr 2025 16:13

Tgt Ion: 117 Resp: 519582
Ion Ratio Lower Upper
117 100
82 53.9 42.1 63.1
119 32.3 25.7 38.5


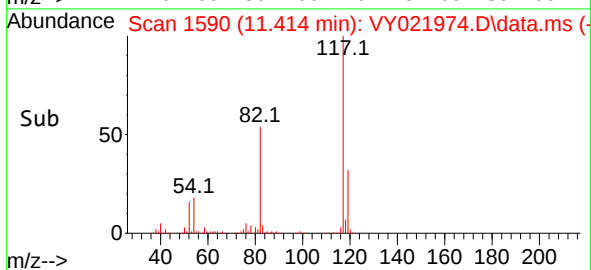
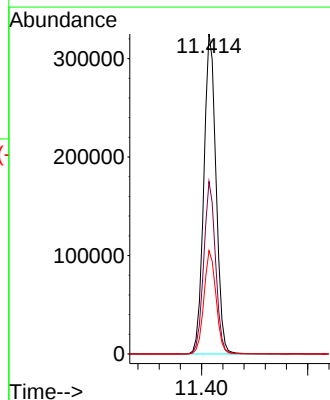
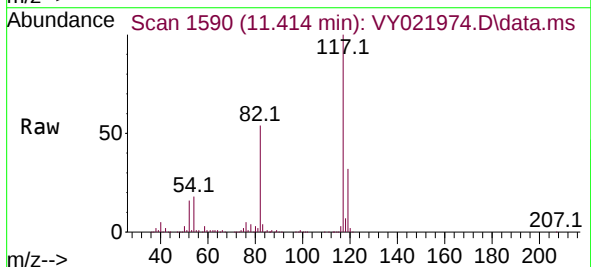




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 1907
 Delta R.T. -0.000 min
 Lab File: VY021974.D
 Acq: 23 Apr 2025 16:13




Instrument :
 MSVOA_Y
 ClientSampleId :
 ETGI-354


Tgt Ion:152 Resp: 187426
 Ion Ratio Lower Upper
 152 100
 115 56.4 28.0 84.0
 150 156.8 0.0 345.6

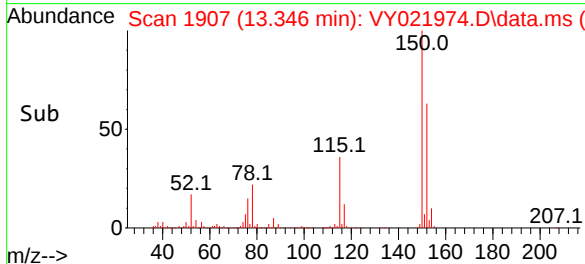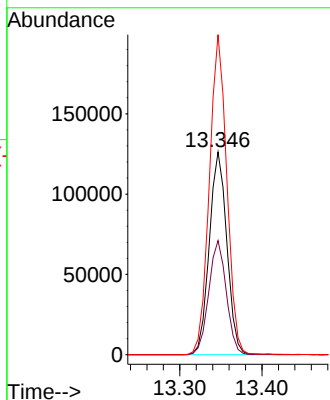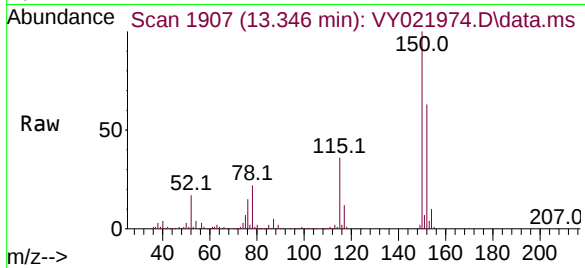

#76
 1,2,3-Trichloropropane
 Concen: 58.262 ug/l
 RT: 12.408 min Scan# 1753
 Delta R.T. -0.146 min
 Lab File: VY021974.D
 Acq: 23 Apr 2025 16:13

Tgt Ion: 75 Resp: 93534
 Ion Ratio Lower Upper
 75 100
 77 1.5 0.0 0.0#

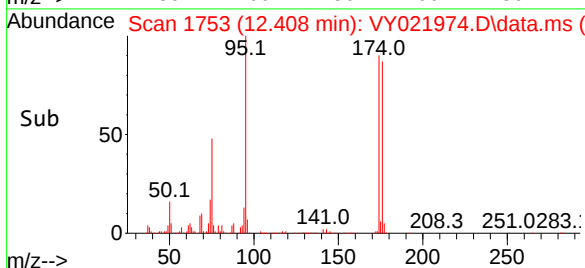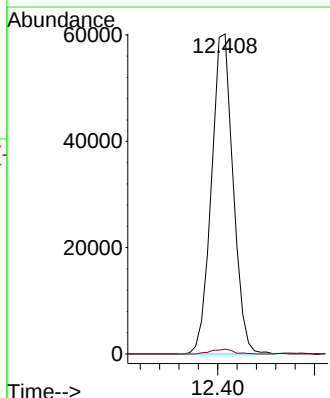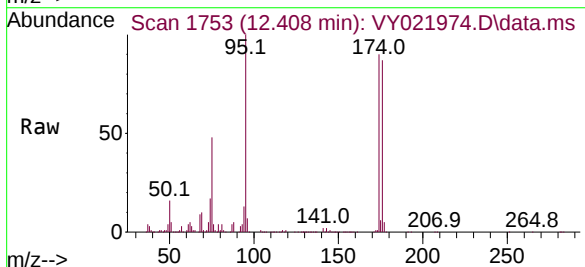

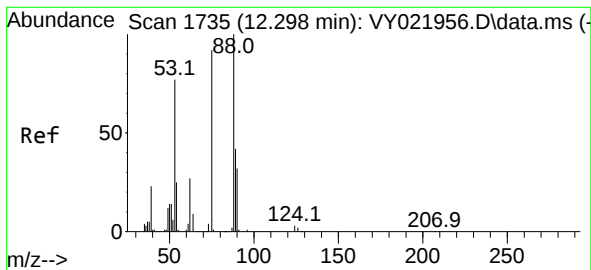

#81
 trans-1,4-Dichloro-2-butene
 Concen: 140.304 ug/l
 RT: 12.408 min Scan# 11
 Delta R.T. 0.110 min
 Lab File: VY021974.D
 Acq: 23 Apr 2025 16:13

Instrument :
 MSVOA_Y
 ClientSampleId :
 ETGI-354

Tgt Ion: 75 Resp: 93534
 Ion Ratio Lower Upper
 75 100
 53 0.1 66.0 99.0#
 89 0.0 37.2 55.8#

