

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042325\
 Data File : VY021979.D
 Acq On : 23 Apr 2025 18:11
 Operator : SY/MD
 Sample : Q1858-02
 Misc : 4.53g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 COMP-2

Quant Time: Apr 24 03:47:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	317972	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	595656	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	514825	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	191838	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	152225	51.829	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.660%
35) Dibromofluoromethane	7.634	113	196146	49.844	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.680%
50) Toluene-d8	10.103	98	712492	48.025	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.060%
62) 4-Bromofluorobenzene	12.408	95	195322	39.109	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	78.220%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042325\
Data File : VY021979.D
Acq On : 23 Apr 2025 18:11
Operator : SY/MD
Sample : Q1858-02
Misc : 4.53g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
COMP-2

Quant Time: Apr 24 03:47:40 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration




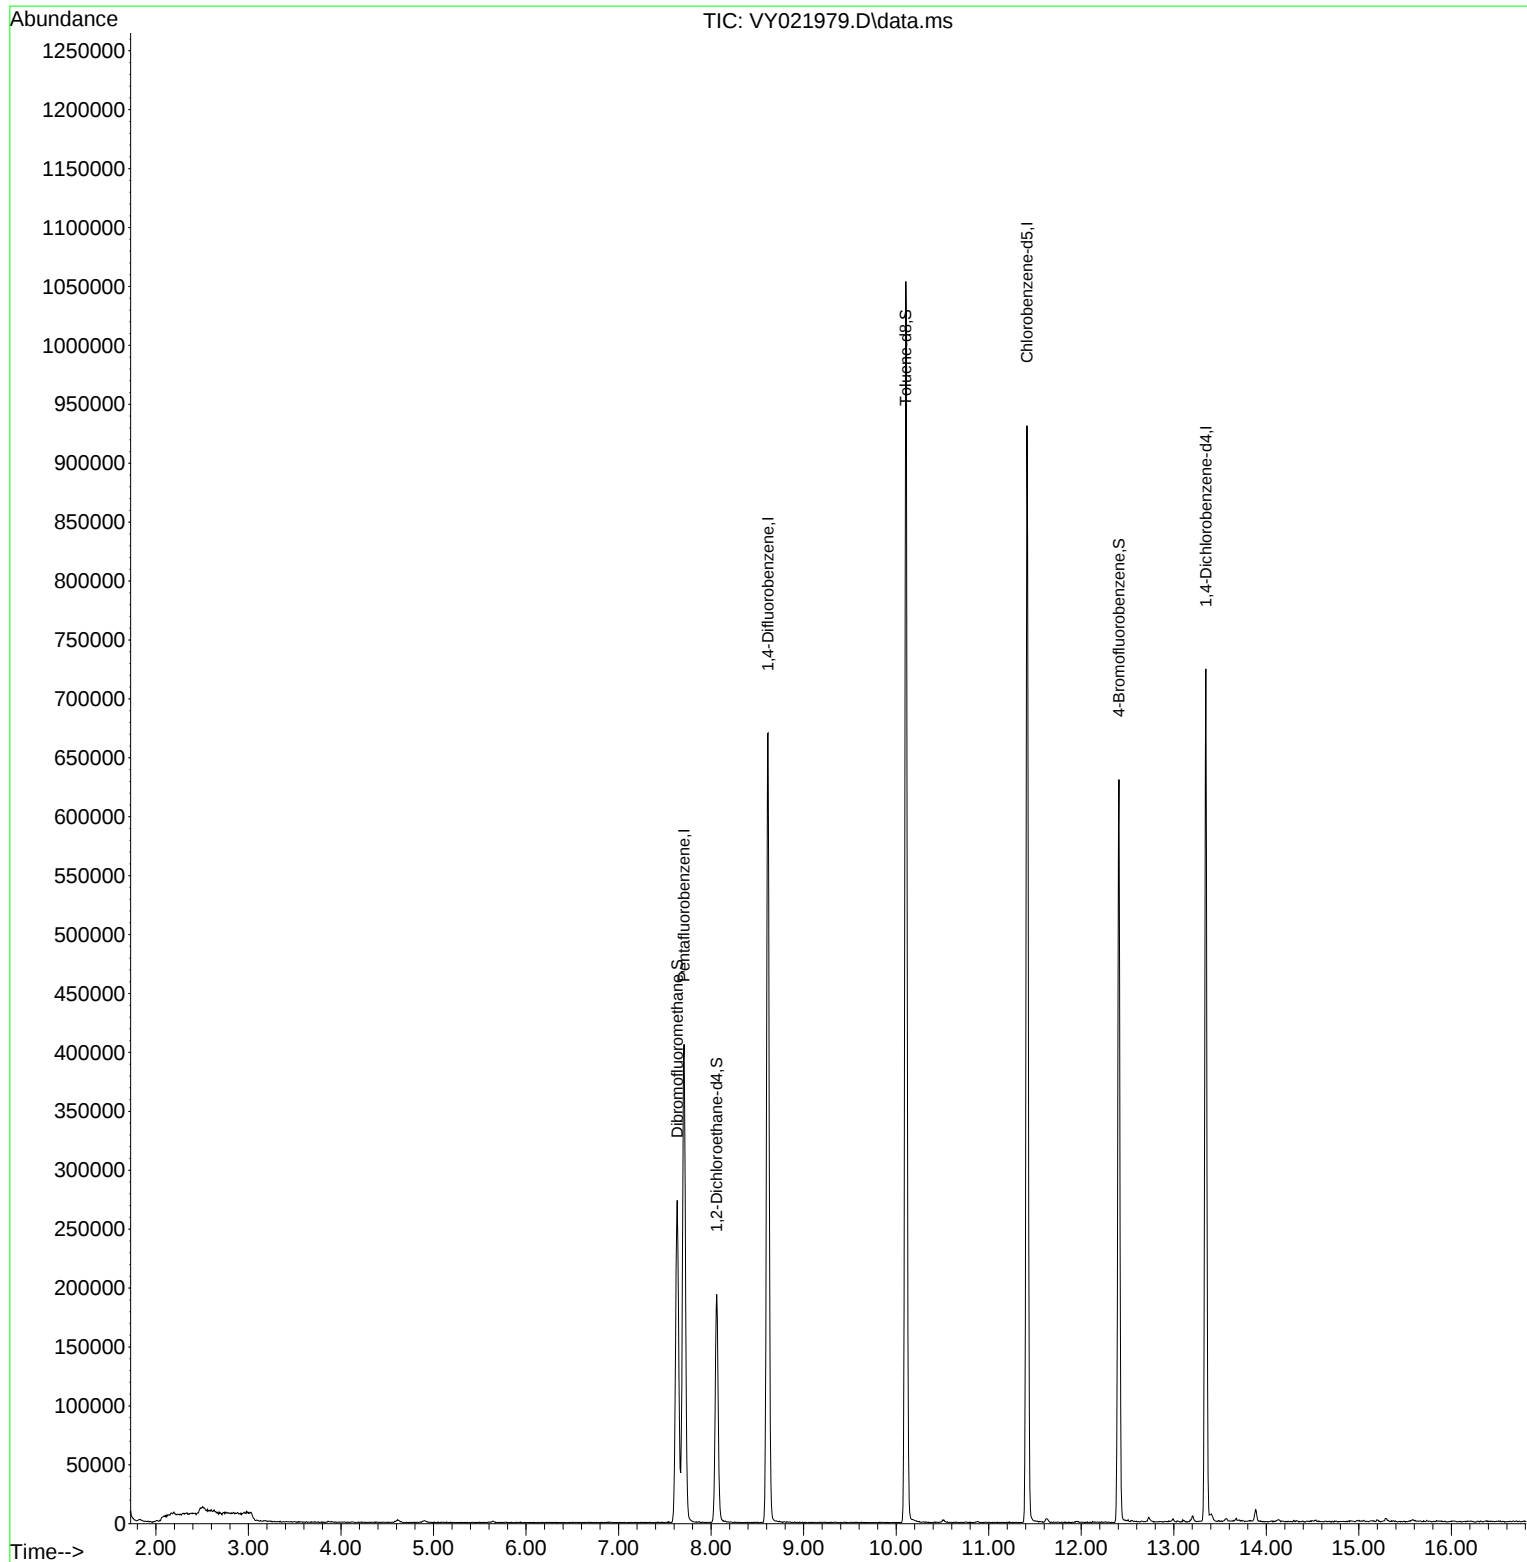




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY021979.D
Acq: 23 Apr 2025 18:11




Instrument :
MSVOA_Y
ClientSampleId :
COMP-2

Tgt Ion:168 Resp: 317972
Ion Ratio Lower Upper
168 100
99 53.1 43.1 64.7

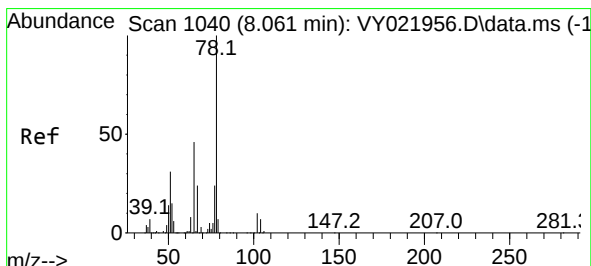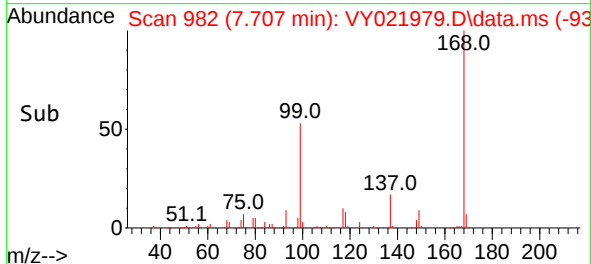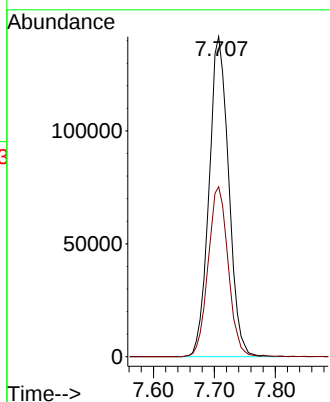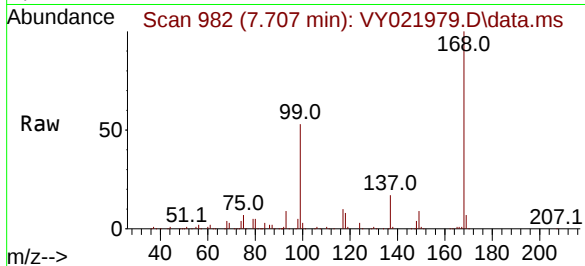

#33
1,2-Dichloroethane-d4
Concen: 51.829 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY021979.D
Acq: 23 Apr 2025 18:11

Tgt Ion: 65 Resp: 152225
Ion Ratio Lower Upper
65 100
67 53.4 0.0 105.8


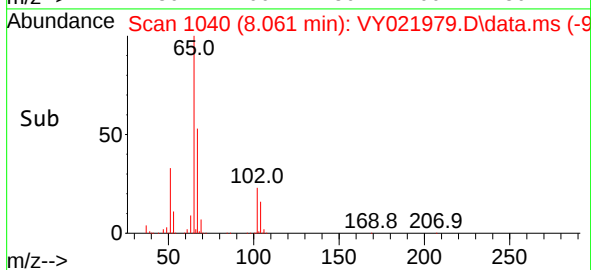
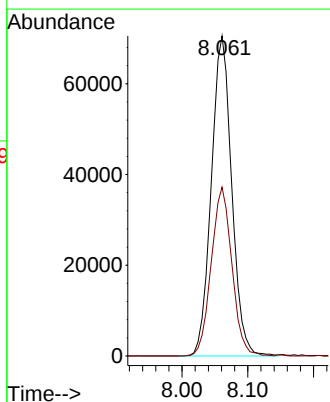
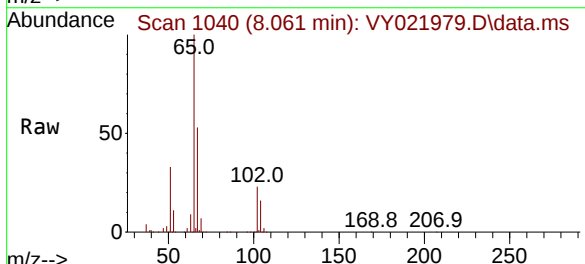




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VY021979.D
Acq: 23 Apr 2025 18:11




Instrument :
MSVOA_Y
ClientSampleId :
COMP-2

Tgt Ion:114 Resp: 595656
Ion Ratio Lower Upper
114 100
63 17.5 0.0 35.4
88 14.3 0.0 28.2

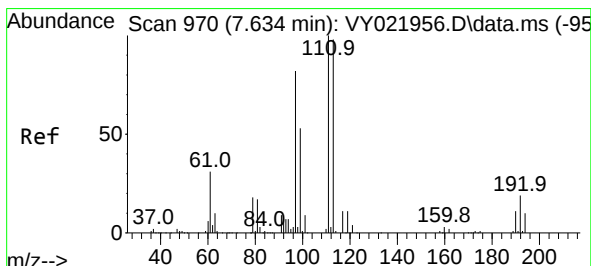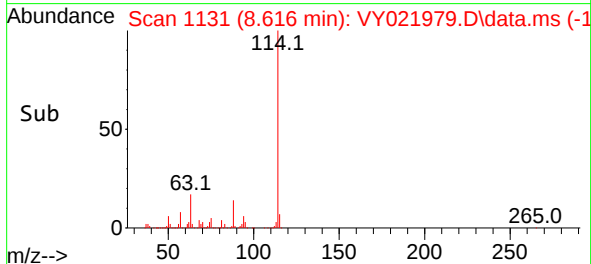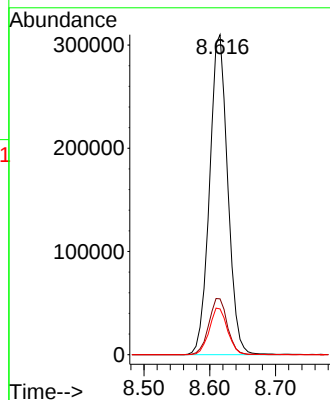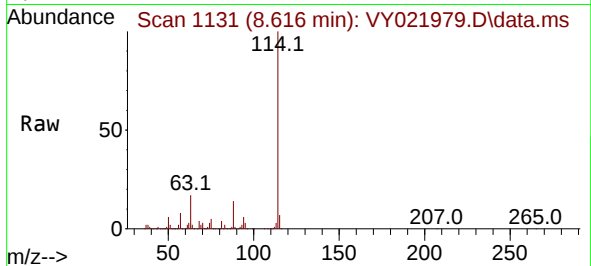

#35
Dibromofluoromethane
Concen: 49.844 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.000 min
Lab File: VY021979.D
Acq: 23 Apr 2025 18:11

Tgt Ion:113 Resp: 196146
Ion Ratio Lower Upper
113 100
111 102.4 81.8 122.8
192 20.0 15.6 23.4

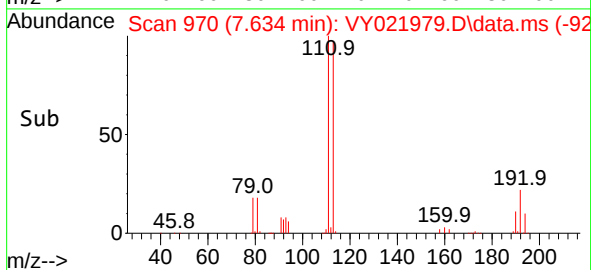
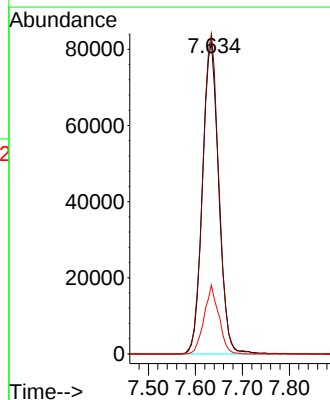
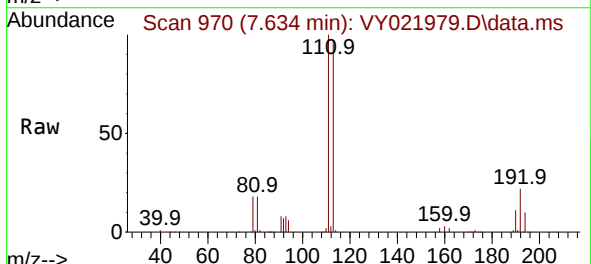




#50
Toluene-d8
Concen: 48.025 ug/l
RT: 10.103 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY021979.D
Acq: 23 Apr 2025 18:11




Instrument :
MSVOA_Y
ClientSampleId :
COMP-2


Tgt Ion: 98 Resp: 712492
Ion Ratio Lower Upper
98 100
100 64.5 51.6 77.4

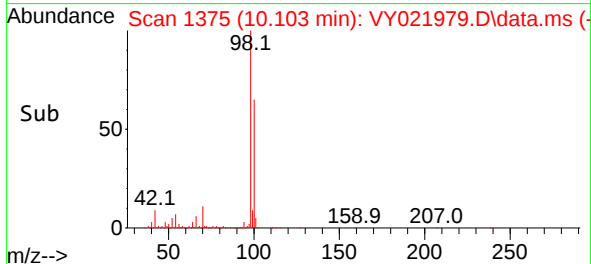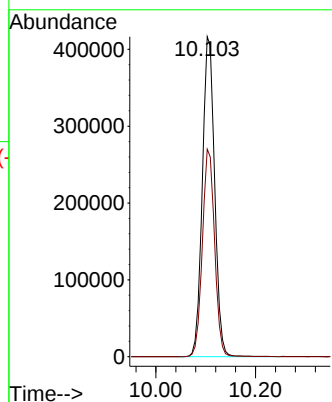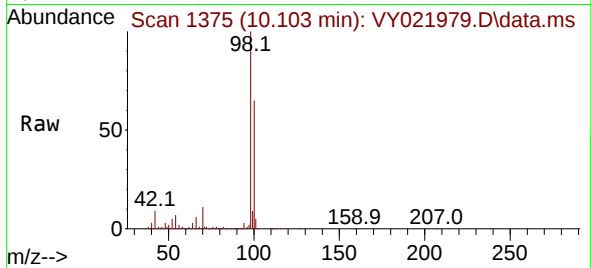

#62
4-Bromofluorobenzene
Concen: 39.109 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY021979.D
Acq: 23 Apr 2025 18:11

Tgt Ion: 95 Resp: 195322
Ion Ratio Lower Upper
95 100
174 87.7 0.0 179.0
176 84.1 0.0 171.8

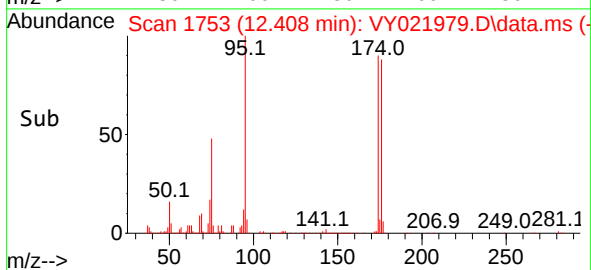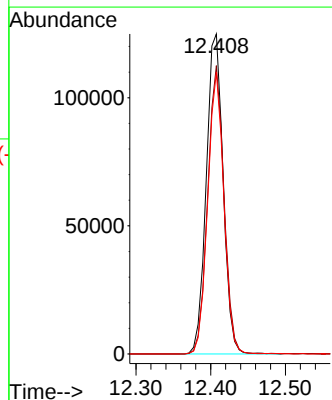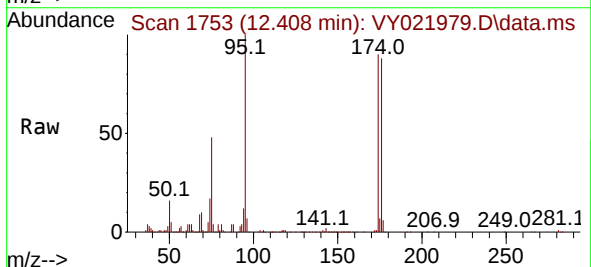

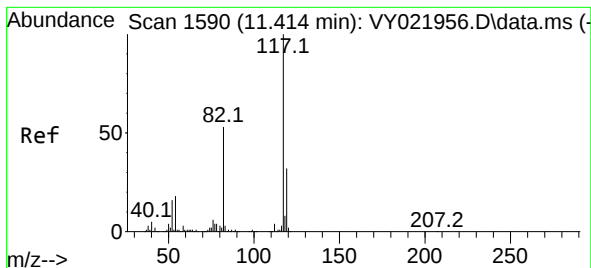

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY021979.D

Acq: 23 Apr 2025 18:11

Instrument :

MSVOA_Y

ClientSampleId :

COMP-2





Tgt Ion:117 Resp: 514825

Ion Ratio Lower Upper

117 100

82 52.0 42.1 63.1

119 32.1 25.7 38.5

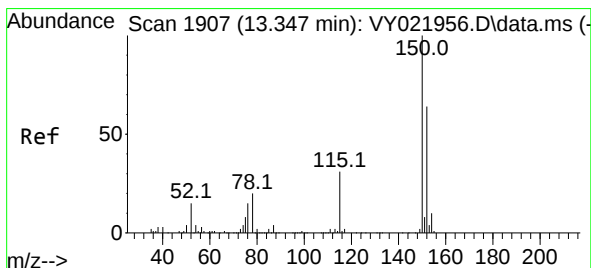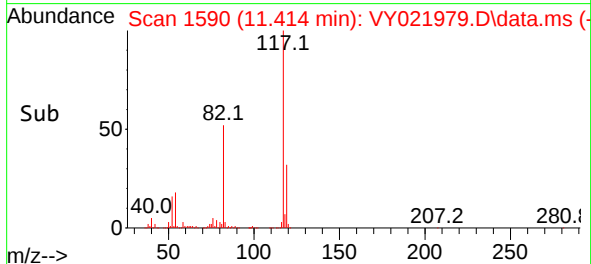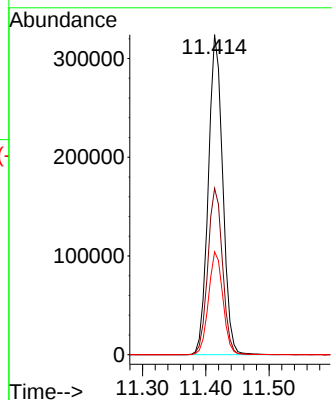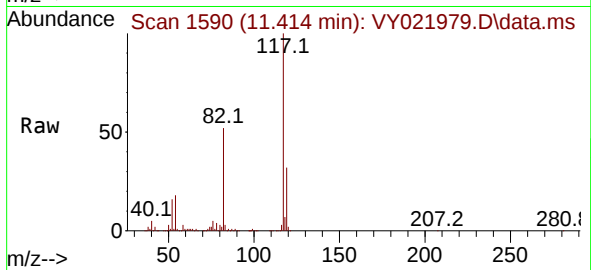

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VY021979.D

Acq: 23 Apr 2025 18:11

Tgt Ion:152 Resp: 191838

Ion Ratio Lower Upper

152 100

115 55.9 28.0 84.0

150 156.2 0.0 345.6

