
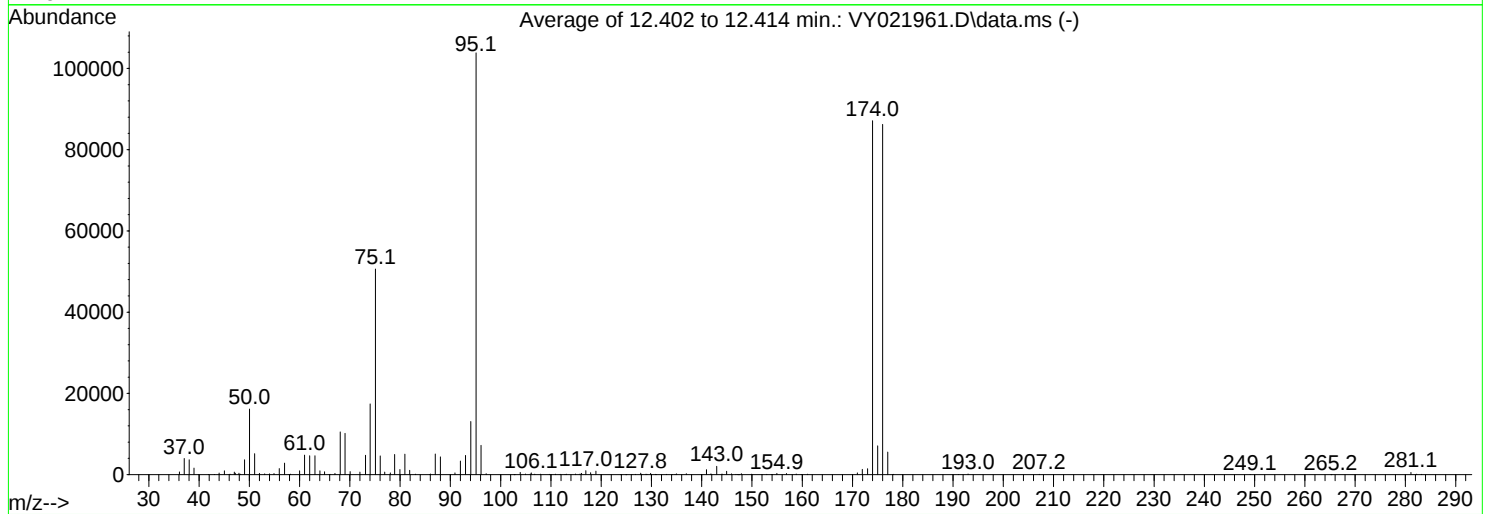


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042325\
Data File : VY021961.D
Acq On : 23 Apr 2025 09:27
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Title : SW846 8260
Last Update : Wed Apr 23 02:30:30 2025

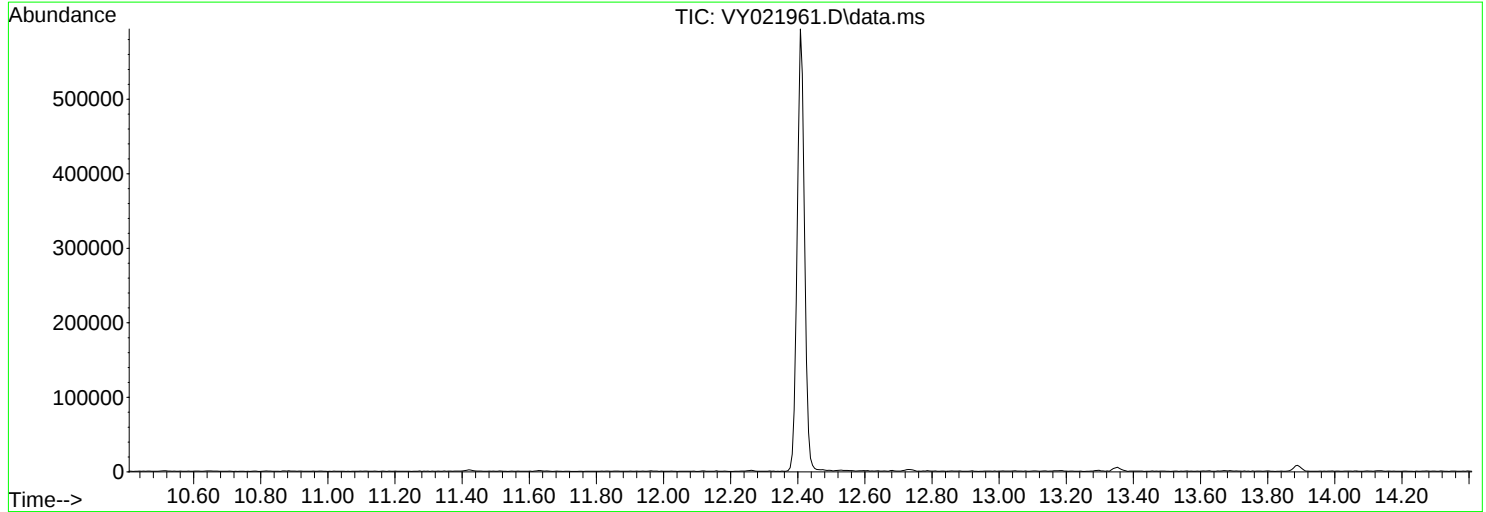

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	16153	PASS
75	95	30	60	48.7	50608	PASS
95	95	100	100	100.0	103837	PASS
96	95	5	9	6.9	7204	PASS
173	174	0.00	2	1.7	1445	PASS
174	95	50	100	83.9	87128	PASS
175	174	5	9	8.1	7073	PASS
176	174	95	101	99.0	86221	PASS
177	176	5	9	6.4	5550	PASS