

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042423\
 Data File : VY013426.D
 Acq On : 25 Apr 2023 04:14
 Operator : KP/MD
 Sample : 02389-22
 Misc : 3.93g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SPB-6WC-23-04-17

Quant Time: Apr 25 07:15:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	193487	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	317055	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	293547	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	123375	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	127377	60.054	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 120.100%	
35) Dibromofluoromethane	7.716	113	111048	55.687	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 111.380%	
50) Toluene-d8	10.179	98	384659	54.224	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 108.440%	
62) 4-Bromofluorobenzene	12.477	95	128030	53.534	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 107.060%	
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	4.966	59	1462	6.754	ug/l #	96
13) Acrolein	3.716	56	185	Below Cal	#	78
16) Acetone	3.954	43	64759	77.529	ug/l	97
17) Carbon Disulfide	4.192	76	10702	1.638	ug/l #	88
20) Methylene Chloride	4.716	84	34316	5.994	ug/l	90
25) 2-Butanone	6.990	43	24139	22.787	ug/l	90
26) 2,2-Dichloropropane	6.972	77	15129	4.320	ug/l #	52
31) Cyclohexane	7.789	56	4428	1.166	ug/l #	26
36) 1,1-Dichloropropene	7.789	75	14459	4.369	ug/l #	48
37) Ethyl Acetate	6.990	43	24139	9.692	ug/l #	69
38) Carbon Tetrachloride	7.789	117	18605	5.364	ug/l #	15
49) 1,4-Dioxane	9.167	88	22	1.056	ug/l #	25
51) 4-Methyl-2-Pentanone	10.075	43	3337	1.425	ug/l	98
68) m/p-Xylenes	11.697	106	13379	3.134	ug/l	97
69) o-Xylene	12.026	106	49005	12.139	ug/l	97
73) Isopropylbenzene	12.331	105	52549	5.631	ug/l	100
76) 1,2,3-Trichloropropane	12.672	75	4046	2.432	ug/l #	100
78) n-propylbenzene	12.672	91	573529	49.898	ug/l	98
79) 2-Chlorotoluene	12.733	91	203514	31.707	ug/l #	39
80) 1,3,5-Trimethylbenzene	12.812	105	1042488	136.873	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.477	75	69005	84.835	ug/l #	13
82) 4-Chlorotoluene	12.812	91	118163	17.663	ug/l #	39
83) tert-Butylbenzene	13.117	119	423637	64.201	ug/l #	61
84) 1,2,4-Trimethylbenzene	13.117	105	3443941	465.084	ug/l	100
85) sec-Butylbenzene	13.117	105	3443941	347.755	ug/l #	56
86) p-Isopropyltoluene	13.312	119	77628	9.747	ug/l	97
89) n-Butylbenzene	13.696	91	90720	11.671	ug/l #	69
90) Hexachloroethane	13.971	117	27755	16.559	ug/l #	8
92) 1,2-Dibromo-3-Chloropr...	14.330	75	798	1.981	ug/l #	1
95) Naphthalene	15.233	128	11637	2.313	ug/l #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042423\
Data File : VY013426.D
Acq On : 25 Apr 2023 04:14
Operator : KP/MD
Sample : 02389-22
Misc : 3.93g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17

Quant Time: Apr 25 07:15:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




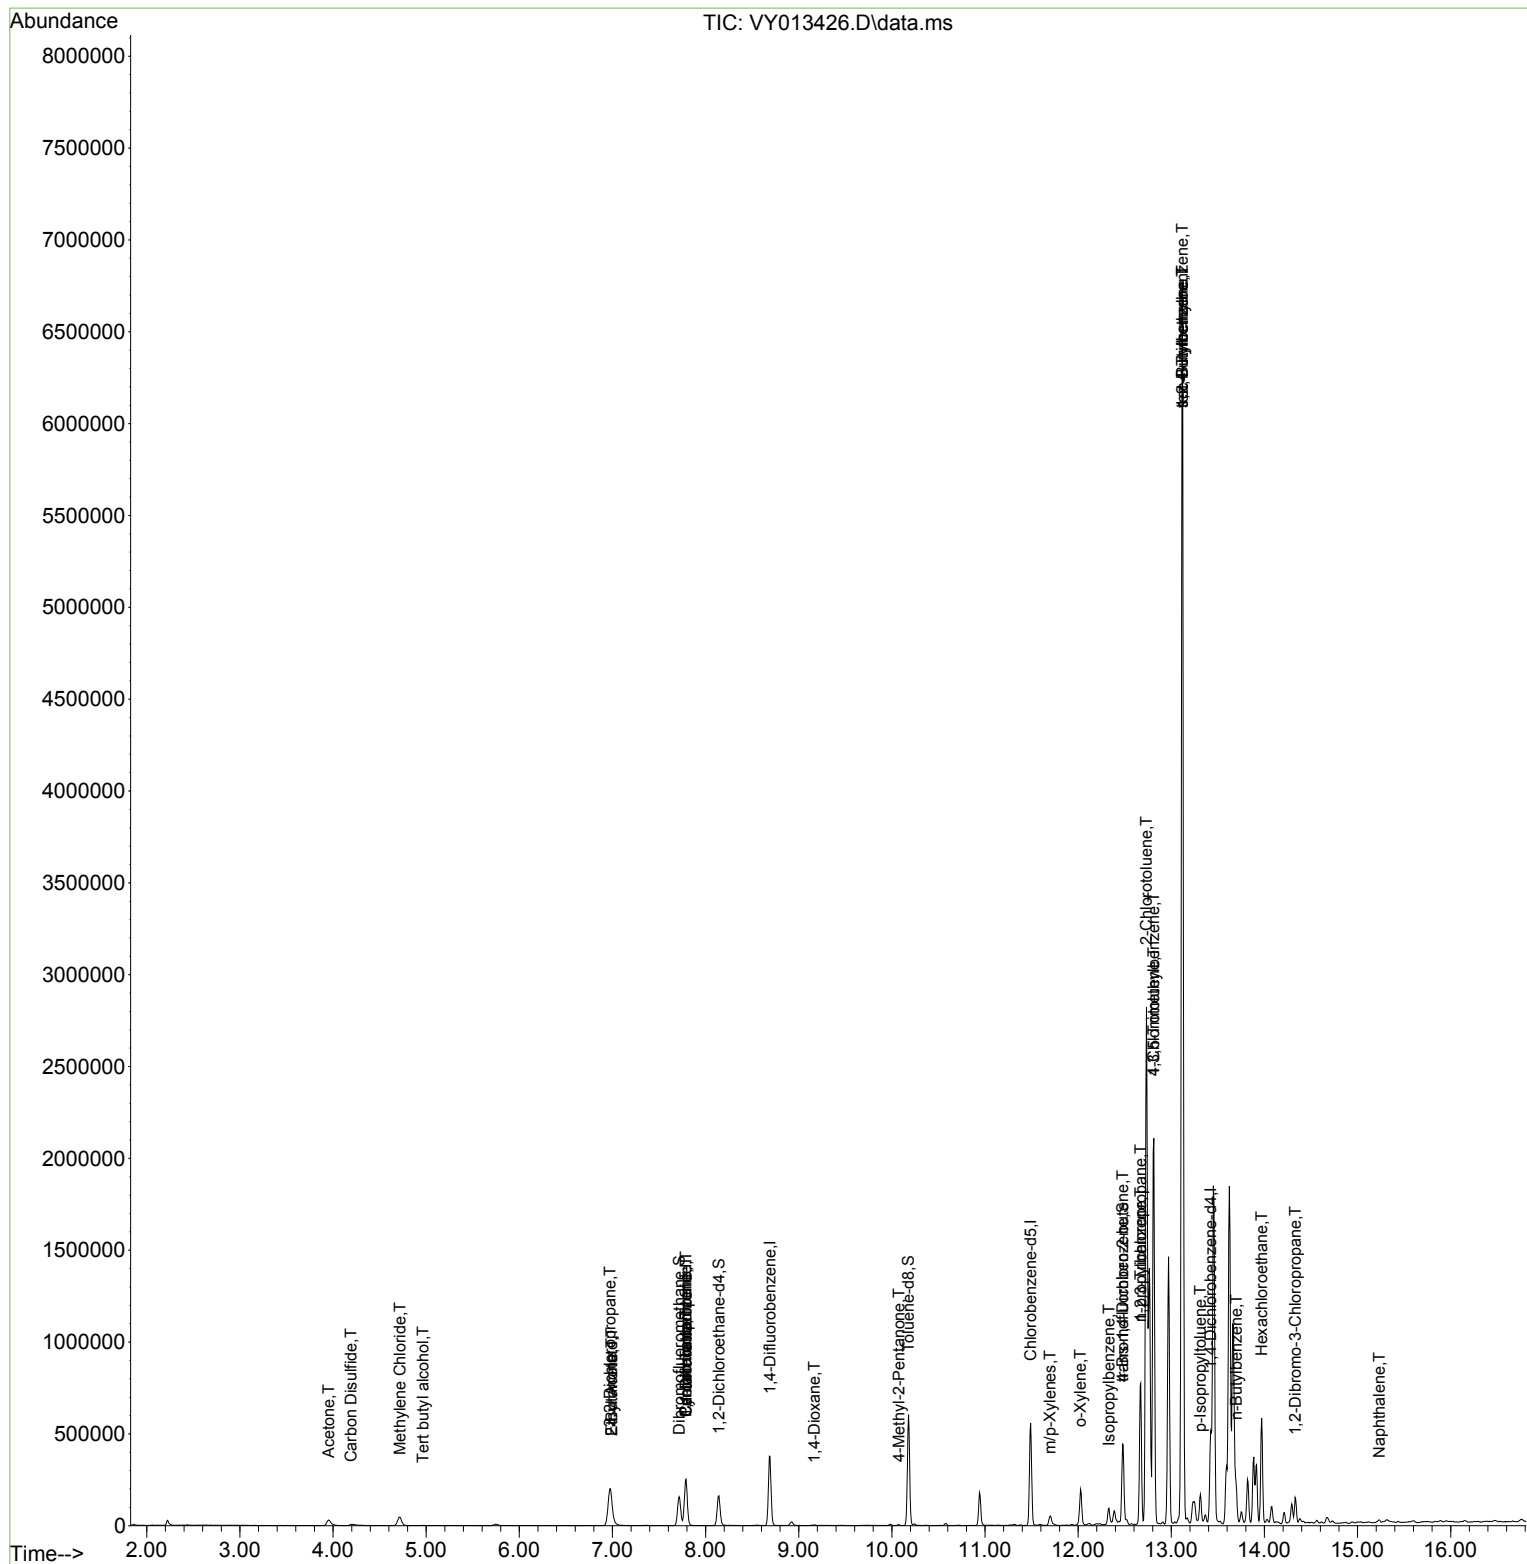


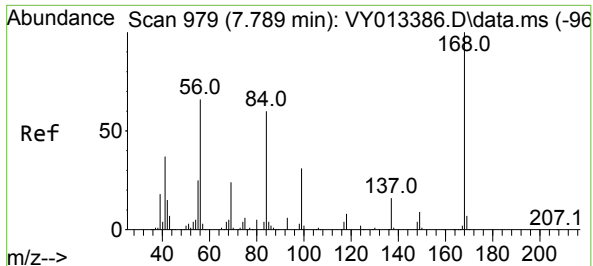

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion:168 Resp: 193487
Ion Ratio Lower Upper
168 100
99 49.8 41.8 62.6

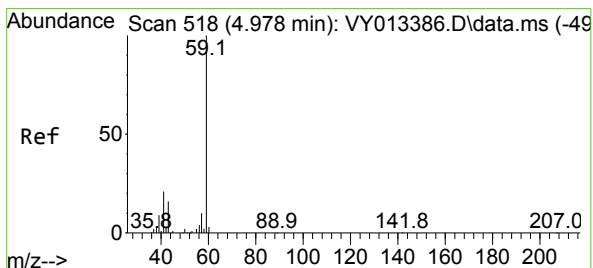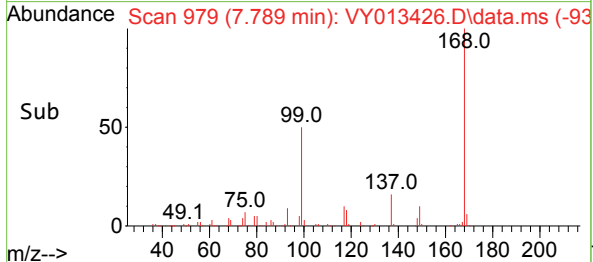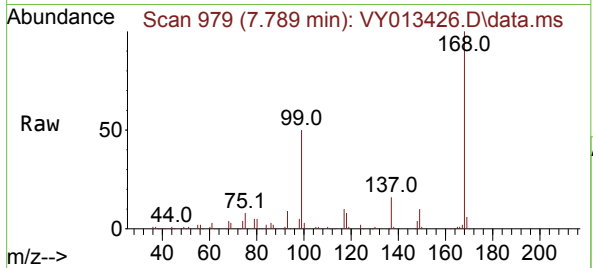

#11
Tert butyl alcohol
Concen: 6.754 ug/l
RT: 4.966 min Scan# 516
Delta R.T. -0.012 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 59 Resp: 1462
Ion Ratio Lower Upper
59 100
57 5.1 3.0 4.4#


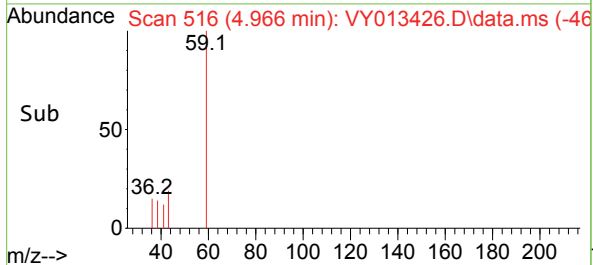

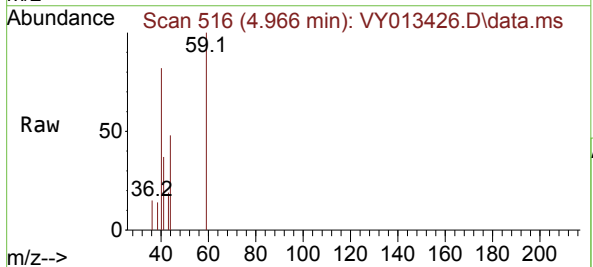


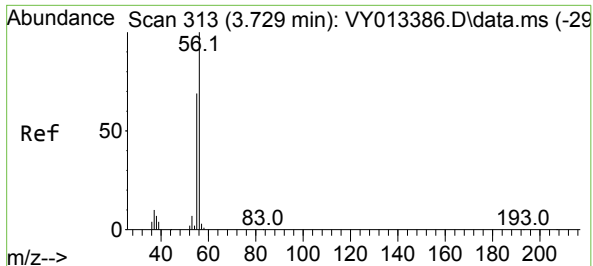

#13
Acrolein
Concen: Below Cal
RT: 3.716 min Scan# 311
Delta R.T. -0.013 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion: 56 Resp: 185
Ion Ratio Lower Upper
56 100
55 49.7 54.1 81.1#

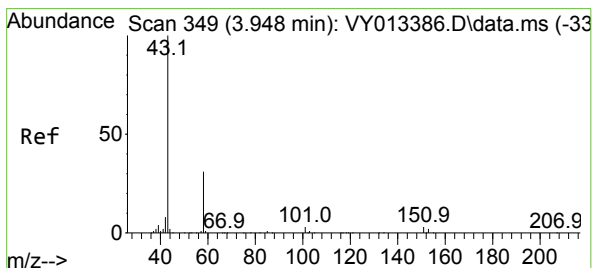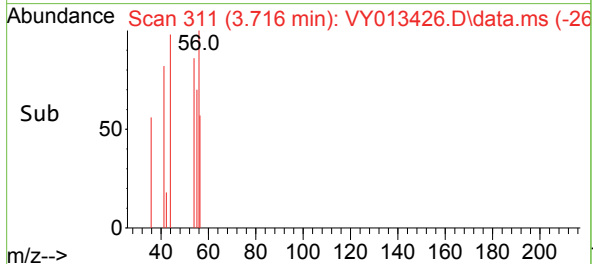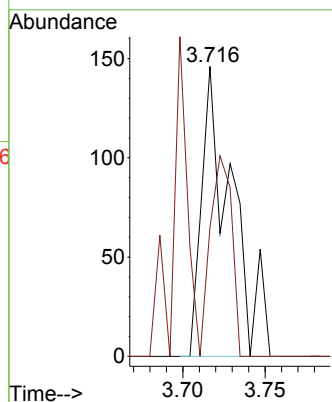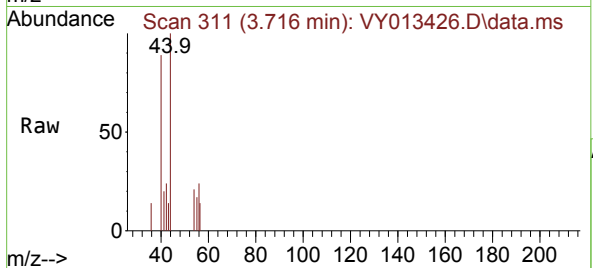

#16
Acetone
Concen: 77.529 ug/l
RT: 3.954 min Scan# 350
Delta R.T. 0.006 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 43 Resp: 64759
Ion Ratio Lower Upper
43 100
58 30.1 25.4 38.0


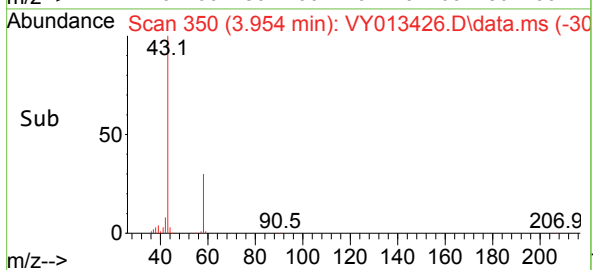
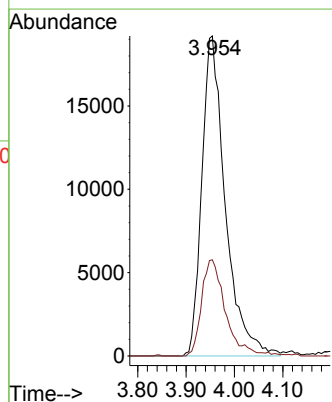
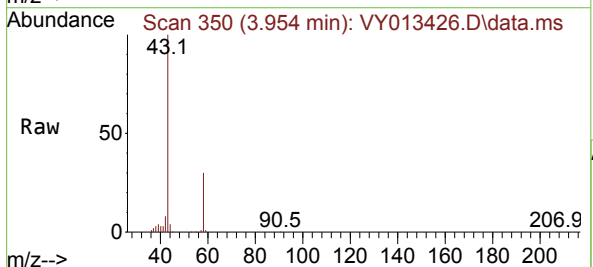




#17
Carbon Disulfide
Concen: 1.638 ug/l
RT: 4.192 min Scan# 389
Delta R.T. 0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion: 76 Resp: 10702
Ion Ratio Lower Upper
76 100
78 13.4 7.2 10.8#

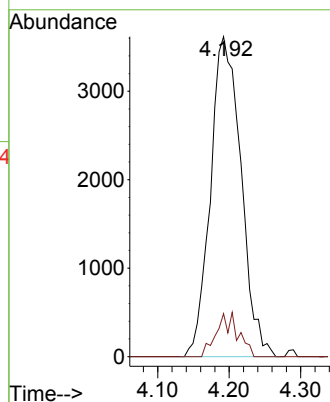

#20
Methylene Chloride
Concen: 5.994 ug/l
RT: 4.716 min Scan# 475
Delta R.T. 0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 84 Resp: 34316
Ion Ratio Lower Upper
84 100
49 125.1 88.0 132.0
51 39.0 27.4 41.0
86 66.2 50.4 75.6



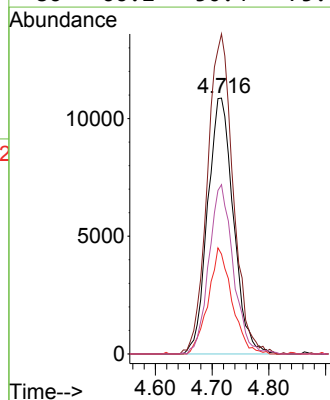
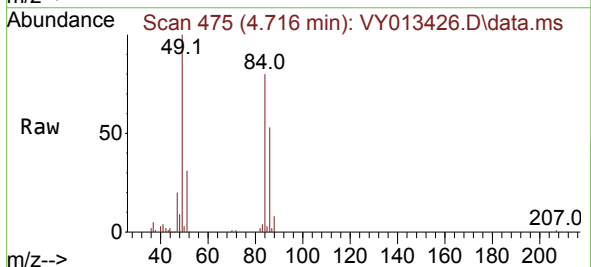


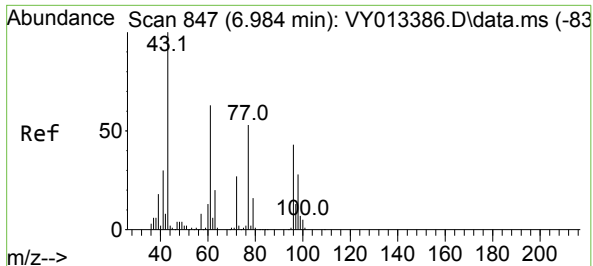

#25
2-Butanone
Concen: 22.787 ug/l
RT: 6.990 min Scan# 847
Delta R.T. 0.006 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion: 43 Resp: 24139
Ion Ratio Lower Upper
43 100
72 22.0 21.9 32.9

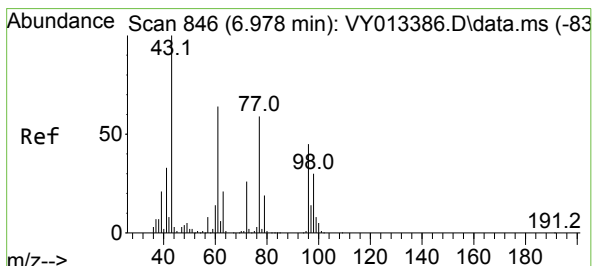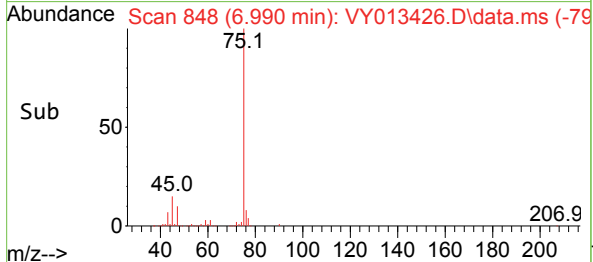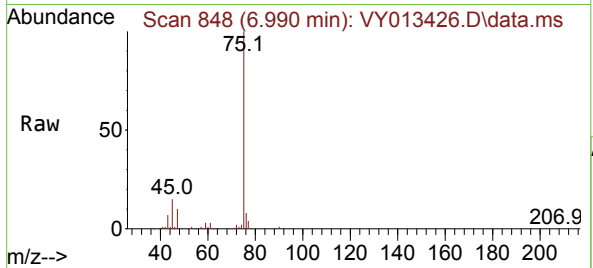

#26
2,2-Dichloropropane
Concen: 4.320 ug/l
RT: 6.972 min Scan# 845
Delta R.T. -0.006 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 77 Resp: 15129
Ion Ratio Lower Upper
77 100
97 0.0 11.8 35.4#


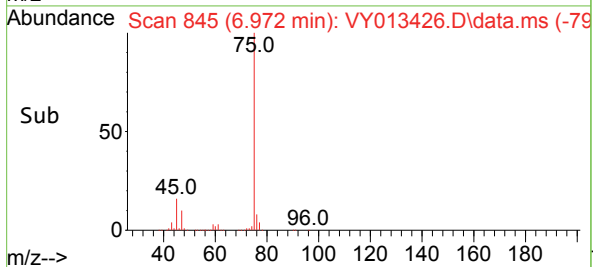

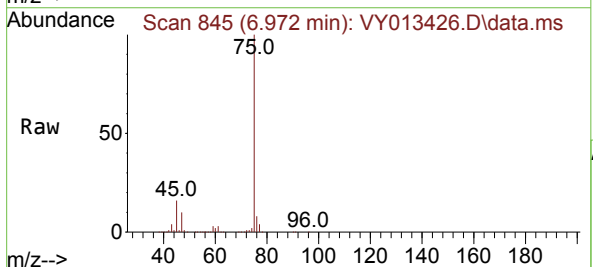


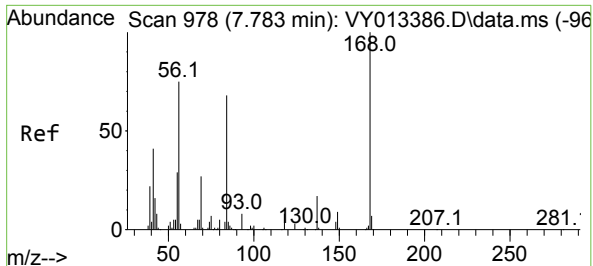

#31
Cyclohexane
Concen: 1.166 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion: 56 Resp: 4428
Ion Ratio Lower Upper
56 100
69 149.7 29.2 43.8#
84 117.0 73.0 109.6#

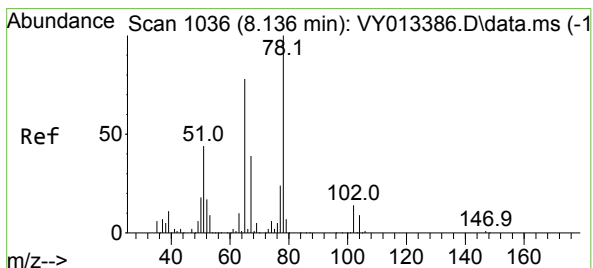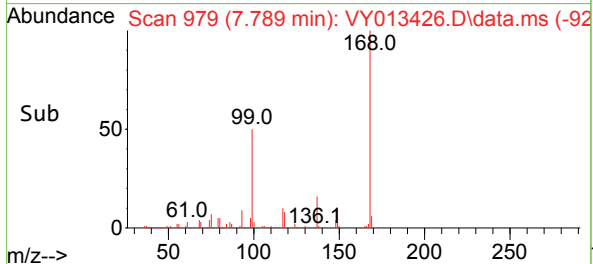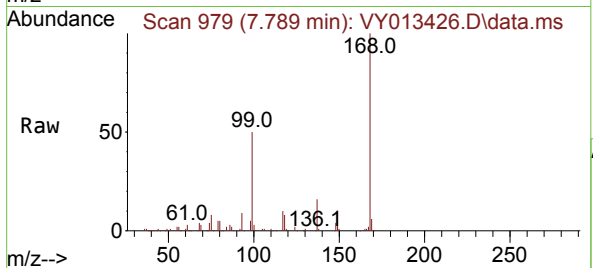

#33
1,2-Dichloroethane-d4
Concen: 60.054 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.007 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 65 Resp: 127377
Ion Ratio Lower Upper
65 100
67 52.0 0.0 103.4


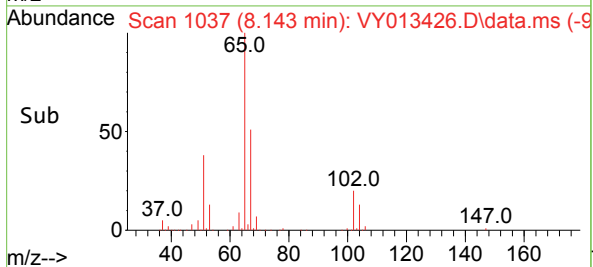

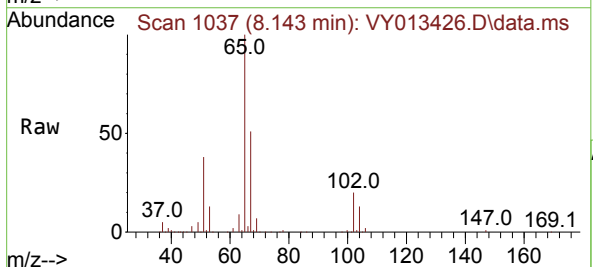




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion:	114	Resp:	317055
Ion	Ratio	Lower	Upper
114	100		
63	20.3	0.0	36.6
88	15.1	0.0	28.8

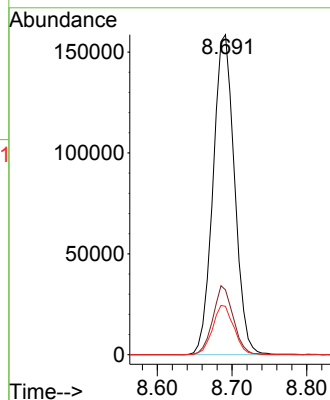

#35
Dibromofluoromethane
Concen: 55.687 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14


Tgt Ion:	113	Resp:	111048
Ion	Ratio	Lower	Upper
113	100		
111	101.8	82.2	123.2
192	19.7	16.7	25.1

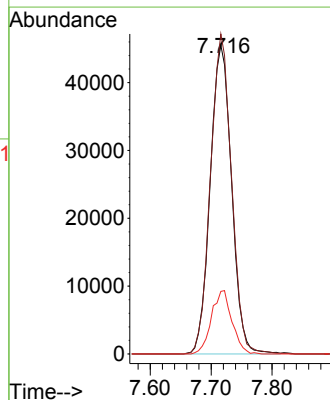






#36
1,1-Dichloropropene
Concen: 4.369 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.128 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17







Tgt Ion: 75 Resp: 14459
Ion Ratio Lower Upper
75 100
110 8.3 18.7 56.1#
77 0.0 24.6 37.0#

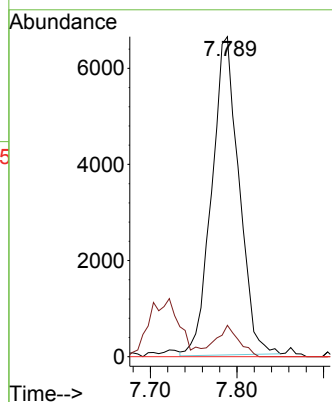

#37
Ethyl Acetate
Concen: 9.692 ug/l
RT: 6.990 min Scan# 848
Delta R.T. -0.079 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 43 Resp: 24139
Ion Ratio Lower Upper
43 100
61 0.0 11.4 17.0#
70 0.5 7.9 11.9#









#38
Carbon Tetrachloride
Concen: 5.364 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.110 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion:117 Resp: 18605
Ion Ratio Lower Upper
117 100
119 5.3 79.0 118.6#
121 0.0 26.6 40.0#

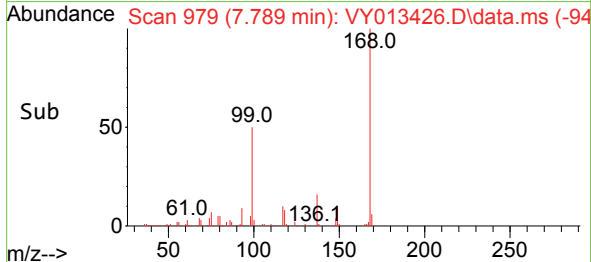

#49
1,4-Dioxane
Concen: 1.056 ug/l
RT: 9.167 min Scan# 1205
Delta R.T. -0.140 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 88 Resp: 22
Ion Ratio Lower Upper
88 100
43 0.0 16.8 25.2#
58 0.0 54.3 81.5#


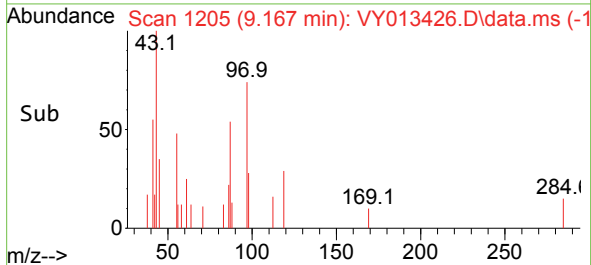

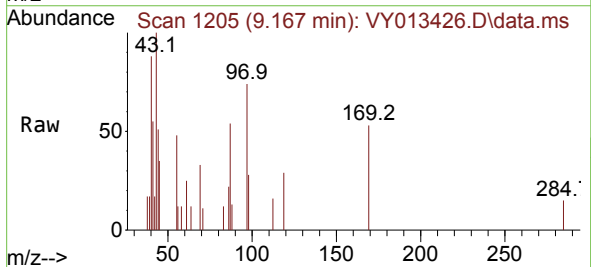


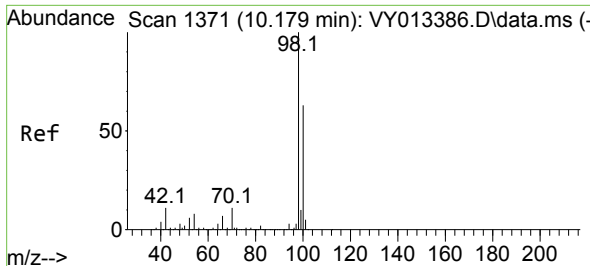

#50
Toluene-d8
Concen: 54.224 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion: 98 Resp: 384659
Ion Ratio Lower Upper
98 100
100 62.8 50.5 75.7

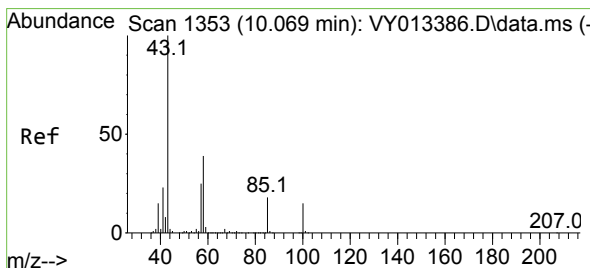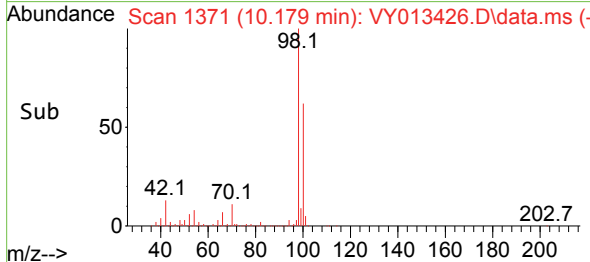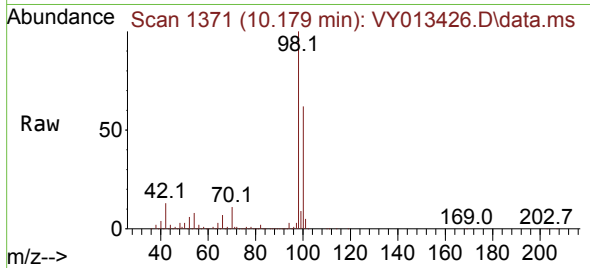

#51
4-Methyl-2-Pentanone
Concen: 1.425 ug/l
RT: 10.075 min Scan# 1354
Delta R.T. 0.006 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 43 Resp: 3337
Ion Ratio Lower Upper
43 100
58 36.9 30.6 46.0


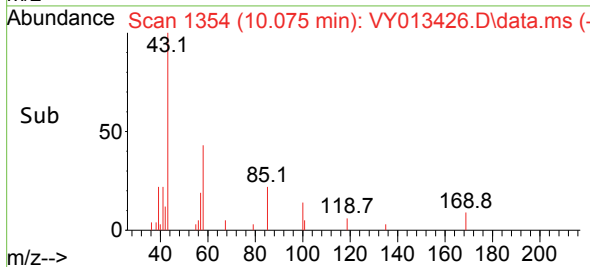

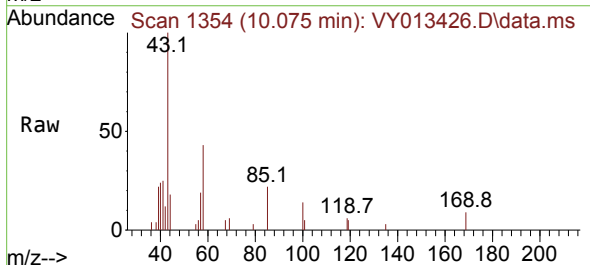




#62
4-Bromofluorobenzene
Concen: 53.534 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion: 95 Resp: 128030
Ion Ratio Lower Upper
95 100
174 88.0 0.0 182.0
176 85.4 0.0 175.4

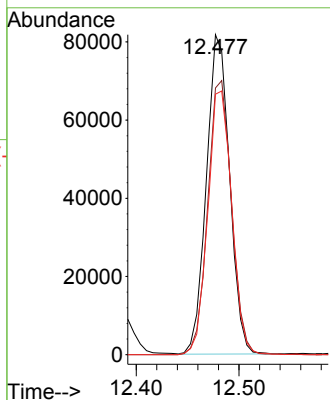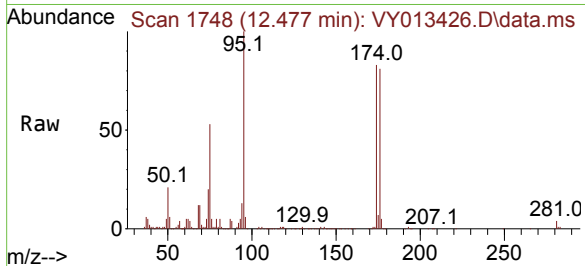

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. 0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 117 Resp: 293547
Ion Ratio Lower Upper
117 100
82 55.6 43.0 64.6
119 31.7 25.5 38.3


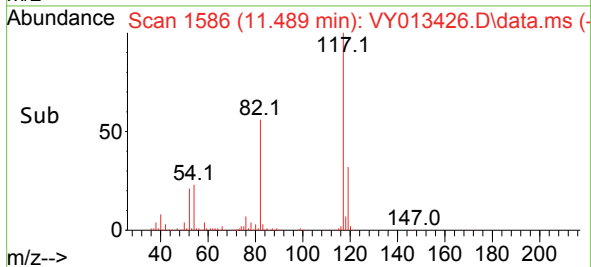
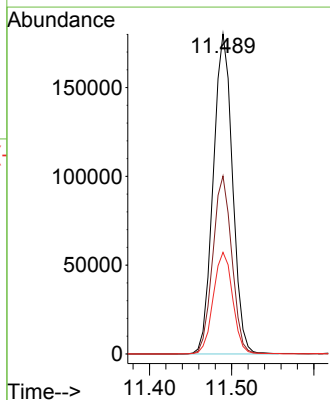
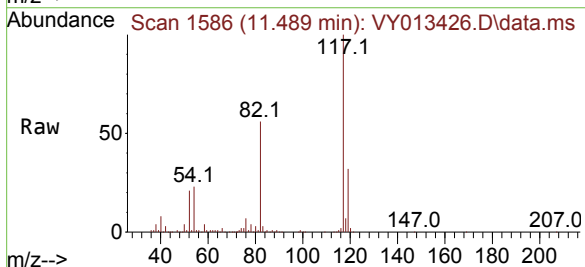




#68
m/p-Xylenes
Concen: 3.134 ug/l
RT: 11.697 min Scan# 1620
Delta R.T. -0.006 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion:106 Resp: 13379
Ion Ratio Lower Upper
106 100
91 196.9 160.9 241.3

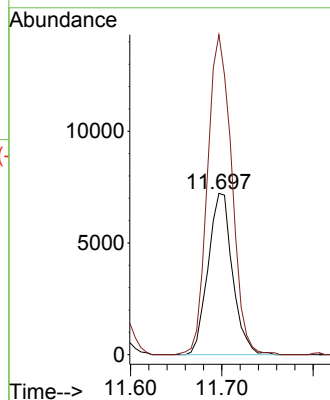

#69
o-Xylene
Concen: 12.139 ug/l
RT: 12.026 min Scan# 1674
Delta R.T. -0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion:106 Resp: 49005
Ion Ratio Lower Upper
106 100
91 216.0 105.5 316.4



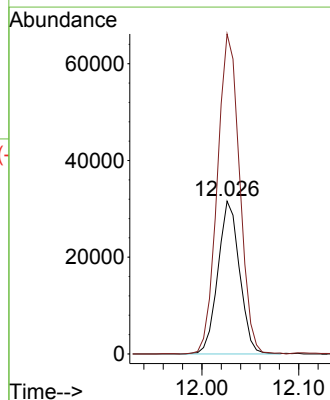
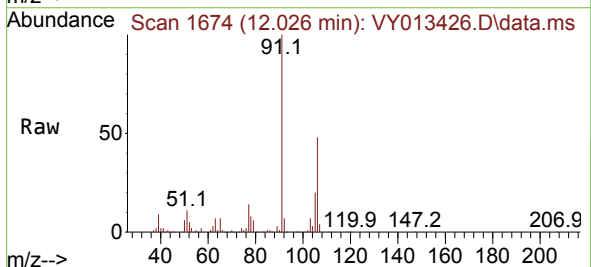




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion:152 Resp: 123375
Ion Ratio Lower Upper
152 100
115 58.7 28.1 84.2
150 158.9 0.0 352.0

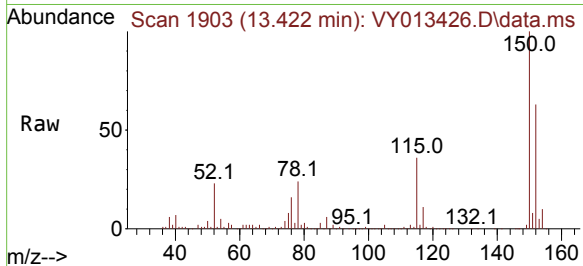

#73
Isopropylbenzene
Concen: 5.631 ug/l
RT: 12.331 min Scan# 1724
Delta R.T. -0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion:105 Resp: 52549
Ion Ratio Lower Upper
105 100
120 27.1 13.7 41.0

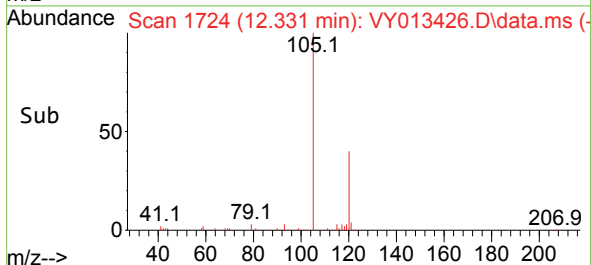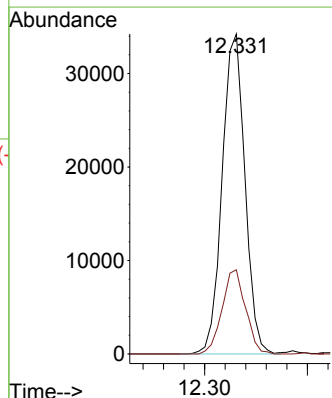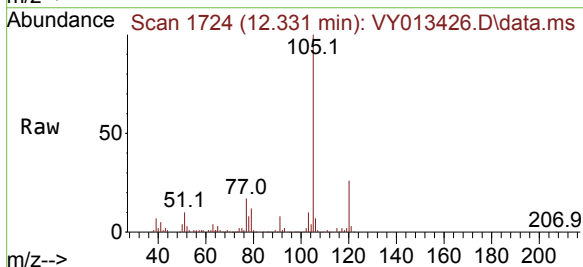



#76

1,2,3-Trichloropropane

Concen: 2.432 ug/l

RT: 12.672 min Scan# 1780

Delta R.T. 0.043 min

Lab File: VY013426.D

Acq: 25 Apr 2023 04:14

Instrument :

MSVOA_Y

ClientSampleId :





SPB-6WC-23-04-17

Tgt Ion: 75 Resp: 4046

Ion Ratio Lower Upper

75 100

77 578.3 0.0 0.0#

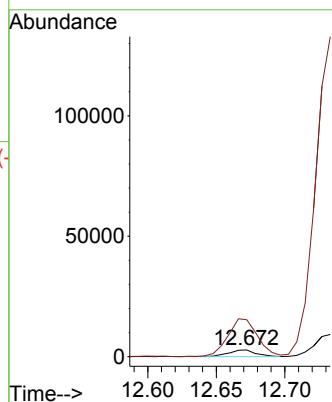

#78

n-propylbenzene

Concen: 49.898 ug/l

RT: 12.672 min Scan# 1780

Delta R.T. 0.000 min

Lab File: VY013426.D




Acq: 25 Apr 2023 04:14


Tgt Ion: 91 Resp: 573529

Ion Ratio Lower Upper

91 100

120 22.8 11.9 35.9



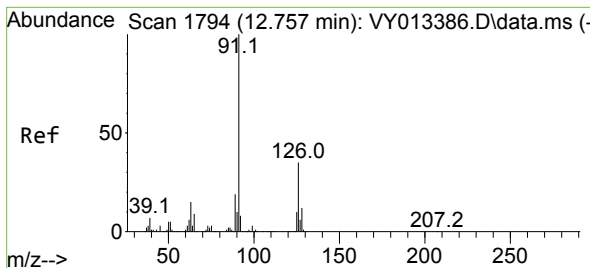

#79

2-Chlorotoluene

Concen: 31.707 ug/l

RT: 12.733 min Scan# 1790

Delta R.T. -0.024 min

Lab File: VY013426.D

Acq: 25 Apr 2023 04:14

Instrument :

MSVOA_Y

ClientSampleId :





SPB-6WC-23-04-17

Tgt Ion: 91 Resp: 203514

Ion Ratio Lower Upper

91 100

126 0.0 17.8 53.4#

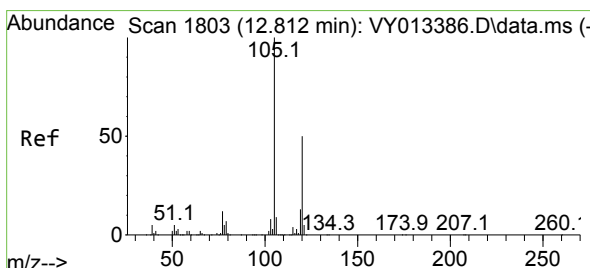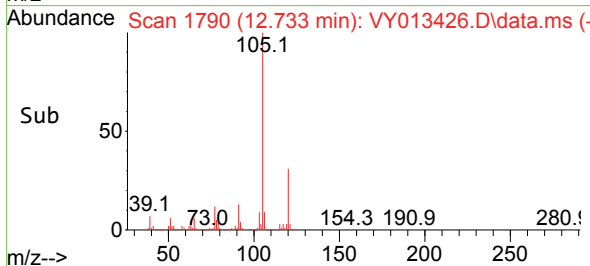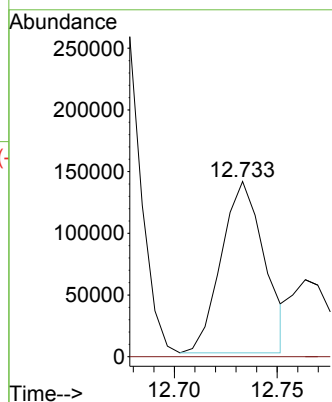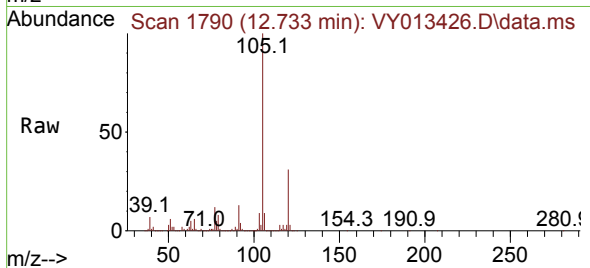

#80

1,3,5-Trimethylbenzene

Concen: 136.873 ug/l

RT: 12.812 min Scan# 1803

Delta R.T. 0.000 min

Lab File: VY013426.D




Acq: 25 Apr 2023 04:14


Tgt Ion:105 Resp: 1042488

Ion Ratio Lower Upper

105 100

120 48.0 24.7 74.1


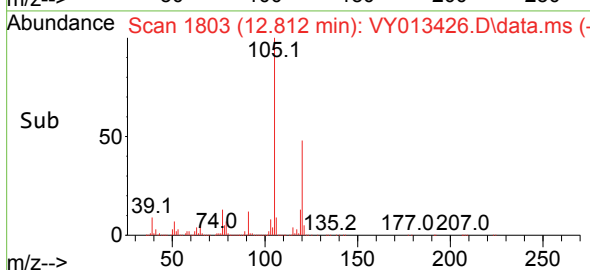

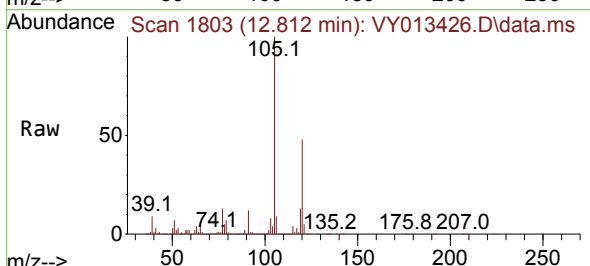




#81
trans-1,4-Dichloro-2-butene
Concen: 84.835 ug/l
RT: 12.477 min Scan# 11
Delta R.T. 0.098 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion: 75 Resp: 69005
Ion Ratio Lower Upper
75 100
53 0.2 73.2 109.8#
89 0.0 38.0 57.0#



#82
4-Chlorotoluene
Concen: 17.663 ug/l
RT: 12.812 min Scan# 1803
Delta R.T. -0.043 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 91 Resp: 118163
Ion Ratio Lower Upper
91 100
126 0.0 17.9 53.8#





#83

tert-Butylbenzene

Concen: 64.201 ug/l

RT: 13.117 min Scan# 1853

Delta R.T. 0.043 min

Lab File: VY013426.D

Acq: 25 Apr 2023 04:14

Instrument :

MSVOA_Y

ClientSampleId :

SPB-6WC-23-04-17





Tgt Ion:119 Resp: 423637

Ion Ratio Lower Upper

119 100

91 91.5 32.2 96.6

134 0.0 13.0 38.9#

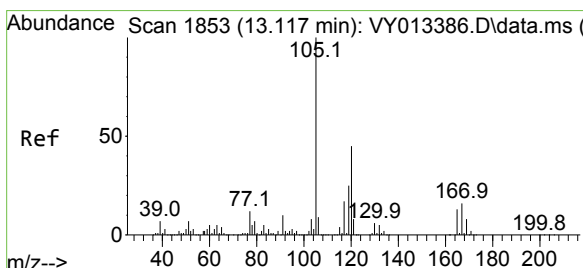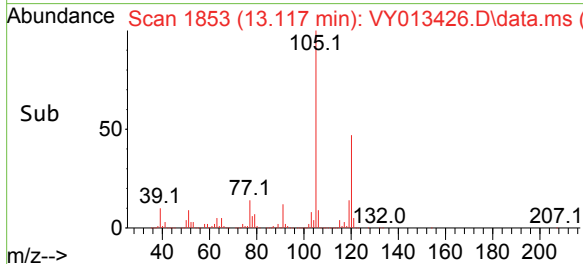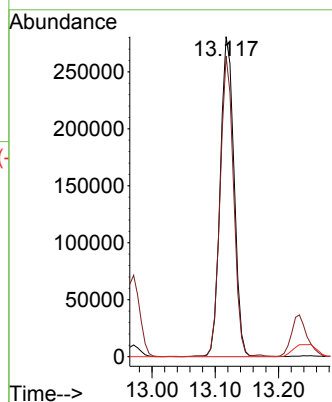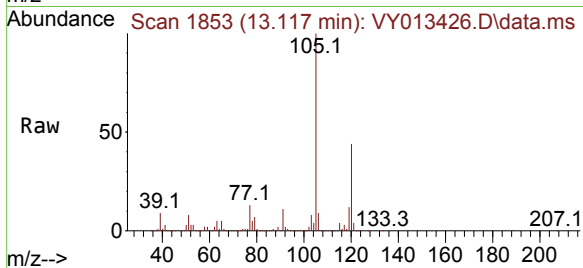

#84

1,2,4-Trimethylbenzene

Concen: 465.084 ug/l

RT: 13.117 min Scan# 1853

Delta R.T. 0.000 min

Lab File: VY013426.D




Acq: 25 Apr 2023 04:14


Tgt Ion:105 Resp: 3443941

Ion Ratio Lower Upper

105 100

120 44.9 22.3 66.9

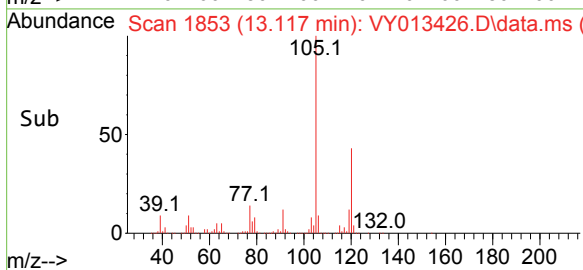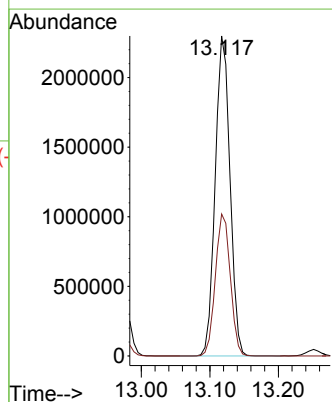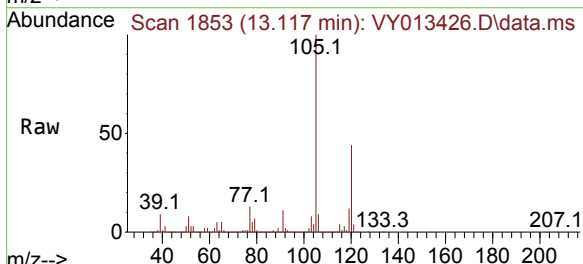

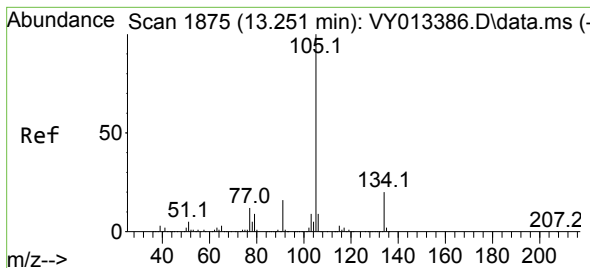

#85

sec-Butylbenzene

Concen: 347.755 ug/l

RT: 13.117 min Scan# 1853

Delta R.T. -0.134 min

Lab File: VY013426.D

Acq: 25 Apr 2023 04:14

Instrument :

MSVOA_Y

ClientSampleId :





SPB-6WC-23-04-17

Tgt Ion:105 Resp: 3443941

Ion Ratio Lower Upper

105 100

134 0.0 10.3 30.9#

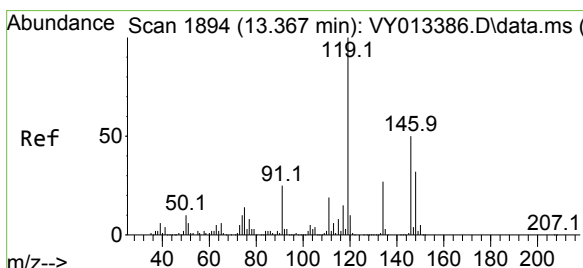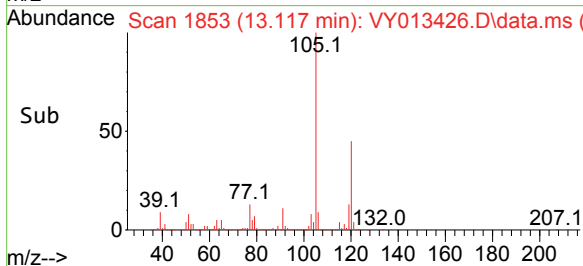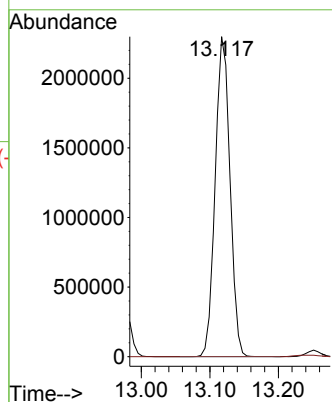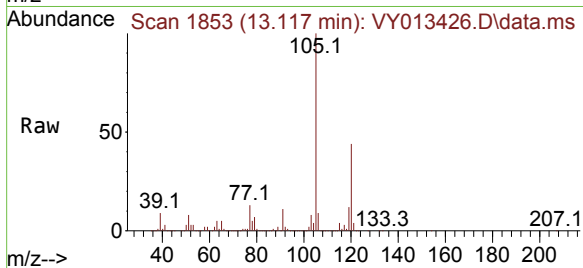

#86

p-Isopropyltoluene

Concen: 9.747 ug/l

RT: 13.312 min Scan# 1885

Delta R.T. -0.055 min

Lab File: VY013426.D

Acq: 25 Apr 2023 04:14




Tgt Ion:119 Resp: 77628


Ion Ratio Lower Upper

119 100

134 29.3 13.4 40.2

91 25.1 12.1 36.3


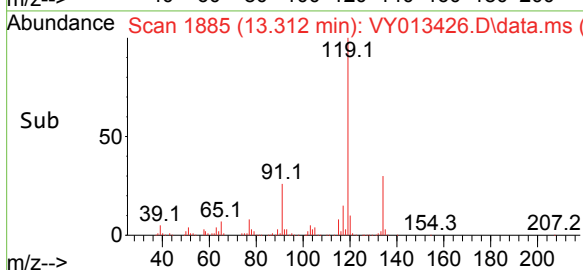

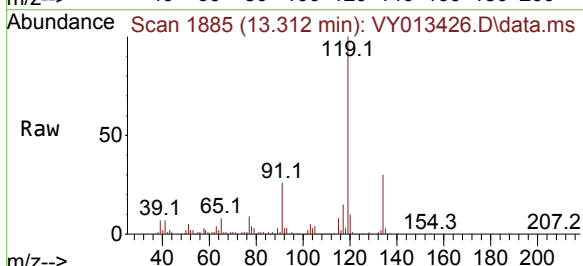




#89
n-Butylbenzene
Concen: 11.671 ug/l
RT: 13.696 min Scan# 1948
Delta R.T. 0.000 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14




Instrument :
MSVOA_Y
ClientSampleId :
SPB-6WC-23-04-17


Tgt Ion: 91 Resp: 90720
Ion Ratio Lower Upper
91 100
92 65.8 25.8 77.3
134 0.0 13.5 40.4#



#90
Hexachloroethane
Concen: 16.559 ug/l
RT: 13.971 min Scan# 1993
Delta R.T. 0.013 min
Lab File: VY013426.D
Acq: 25 Apr 2023 04:14

Tgt Ion: 117 Resp: 27755
Ion Ratio Lower Upper
117 100
201 0.0 41.6 124.8#




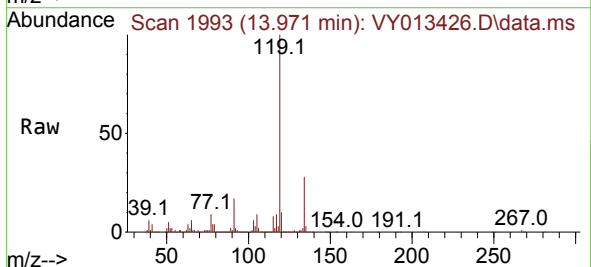




#92
 1,2-Dibromo-3-Chloropropane
 Concen: 1.981 ug/l
 RT: 14.330 min Scan# 2052
 Delta R.T. -0.025 min
 Lab File: VY013426.D
 Acq: 25 Apr 2023 04:14

Instrument :
 MSVOA_Y
 ClientSampleId :
 SPB-6WC-23-04-17

Tgt Ion: 75 Resp: 798
 Ion Ratio Lower Upper
 75 100
 155 2.4 44.6 134.0#
 157 0.0 57.6 172.7#

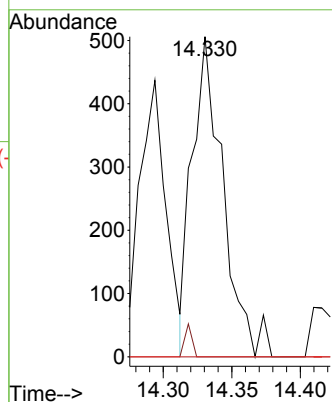

#95
 Naphthalene
 Concen: 2.313 ug/l
 RT: 15.233 min Scan# 2200
 Delta R.T. -0.000 min
 Lab File: VY013426.D
 Acq: 25 Apr 2023 04:14

Tgt Ion: 128 Resp: 11637
 Ion Ratio Lower Upper
 128 100
 127 16.4 10.7 16.1#
 129 11.3 8.8 13.2

