

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042423\
 Data File : VY013432.D
 Acq On : 25 Apr 2023 06:35
 Operator : KP/MD
 Sample : 02423-14
 Misc : 3.43g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SPE-2WC-23-04-18

Quant Time: Apr 25 07:17:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	161342	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	276330	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	246359	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	97326	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	110259	62.340	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	124.680%
35) Dibromofluoromethane	7.716	113	96235	55.371	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.740%
50) Toluene-d8	10.179	98	333526	53.945	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	107.880%
62) 4-Bromofluorobenzene	12.483	95	93550	44.882	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	89.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042423\
Data File : VY013432.D
Acq On : 25 Apr 2023 06:35
Operator : KP/MD
Sample : 02423-14
Misc : 3.43g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SPE-2WC-23-04-18

Quant Time: Apr 25 07:17:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




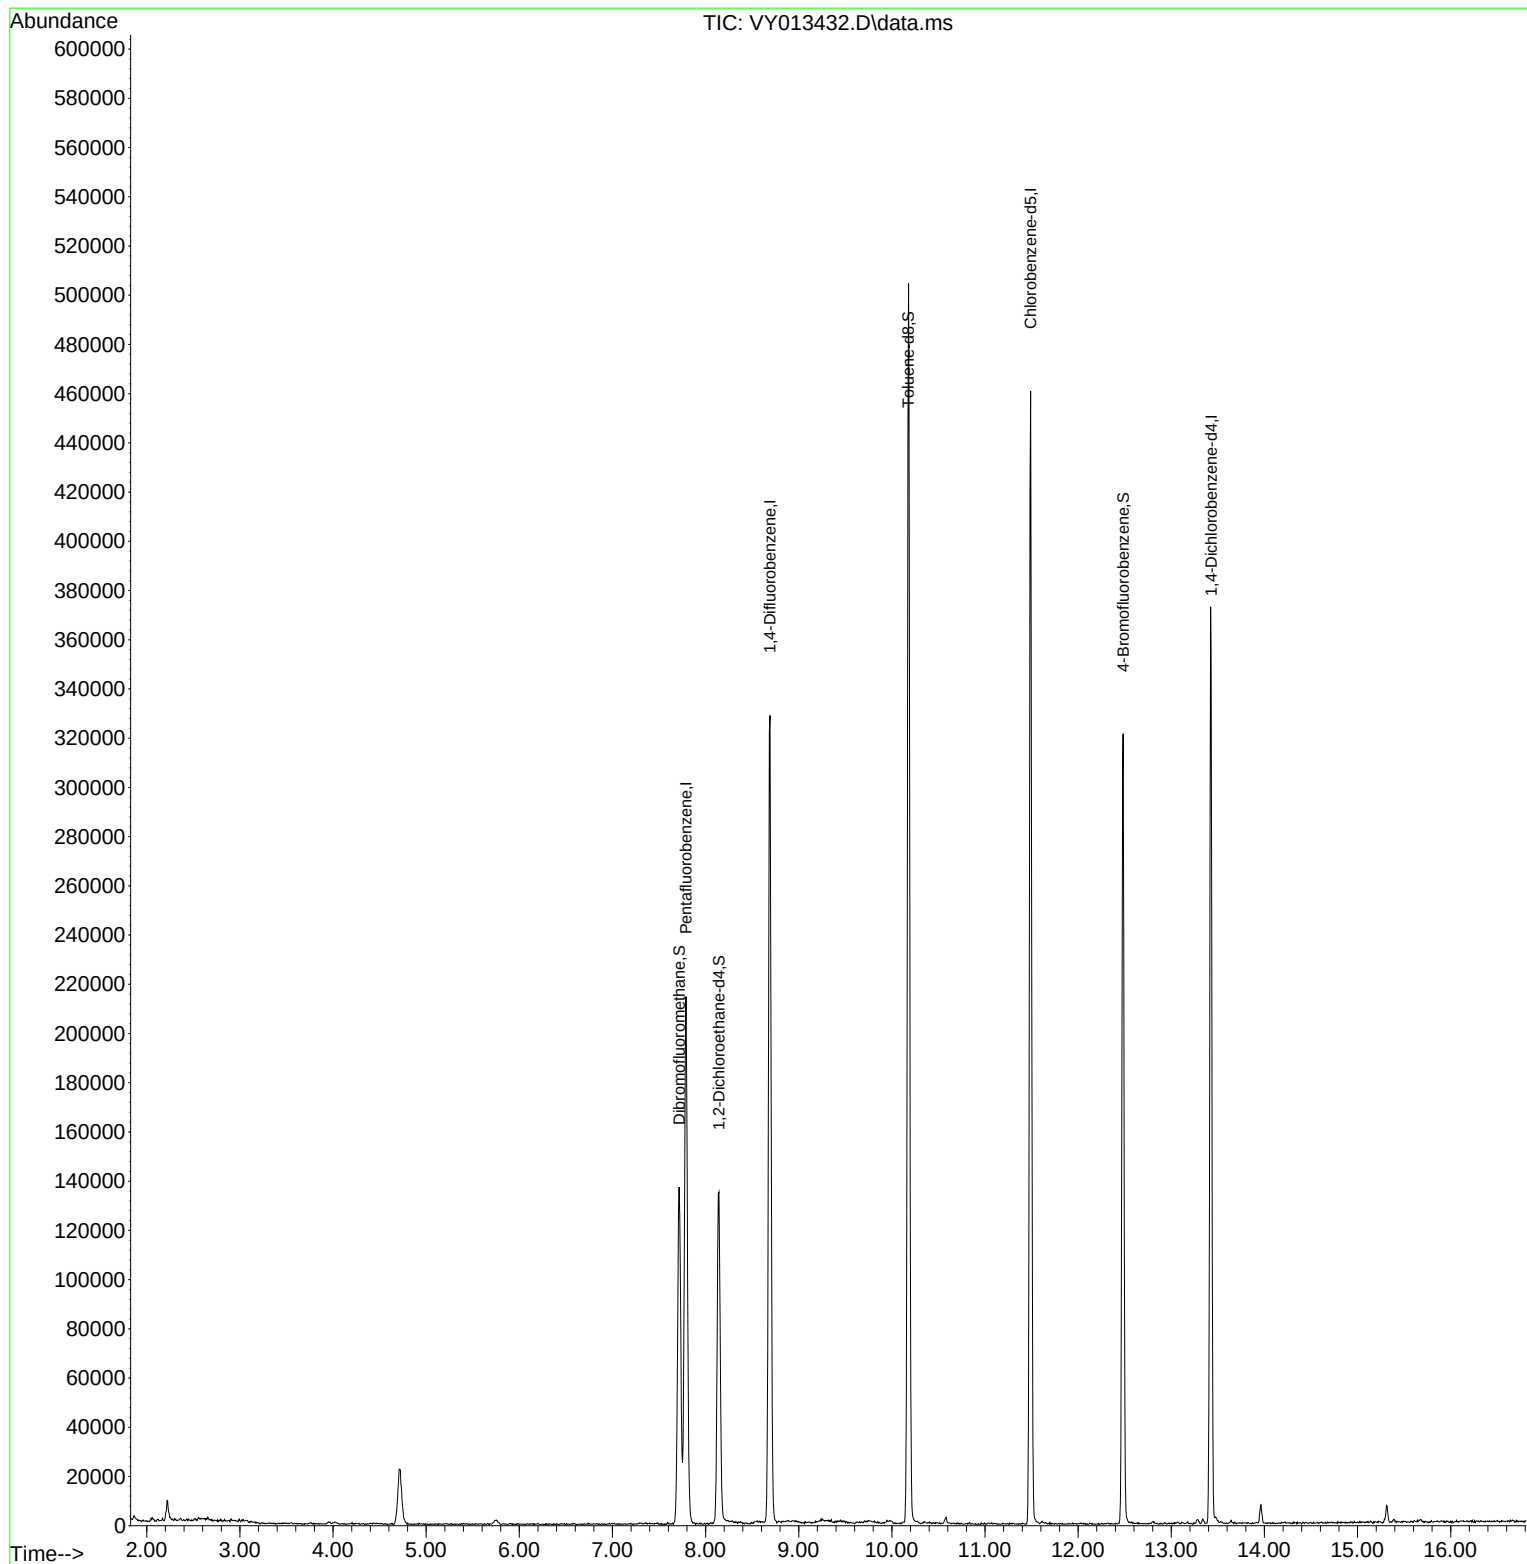


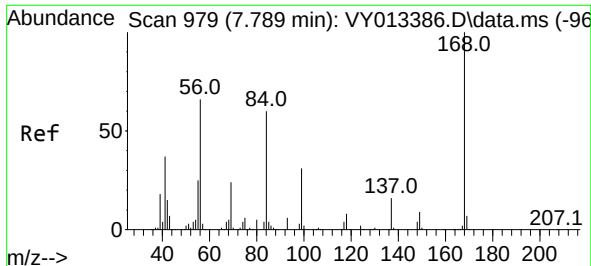

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY013432.D
Acq: 25 Apr 2023 06:35




Instrument :
MSVOA_Y
ClientSampleId :
SPE-2WC-23-04-18


Tgt Ion:168 Resp: 161342
Ion Ratio Lower Upper
168 100
99 52.8 41.8 62.6

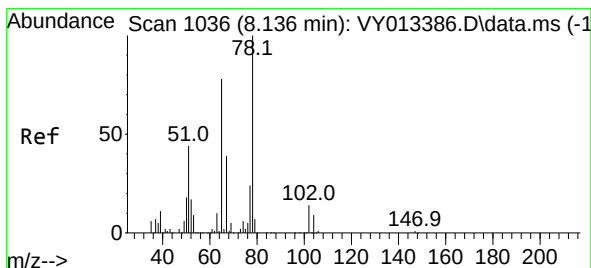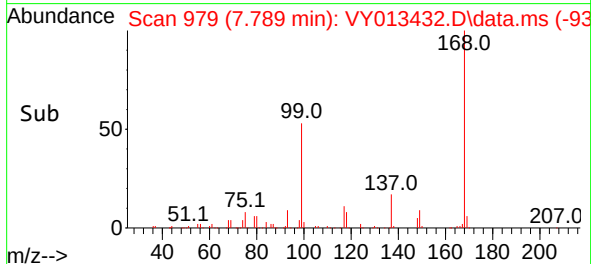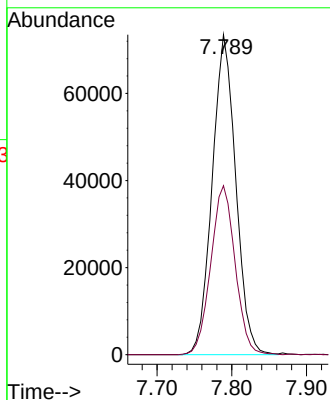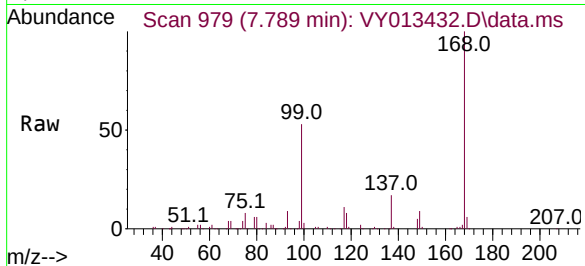

#33
1,2-Dichloroethane-d4
Concen: 62.340 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VY013432.D
Acq: 25 Apr 2023 06:35

Tgt Ion: 65 Resp: 110259
Ion Ratio Lower Upper
65 100
67 51.4 0.0 103.4

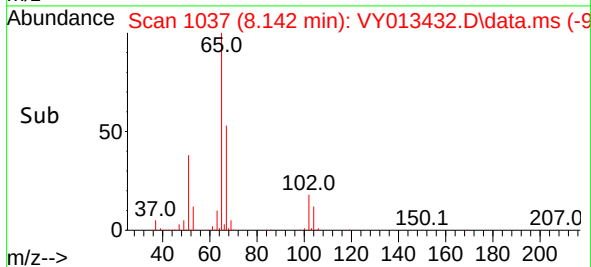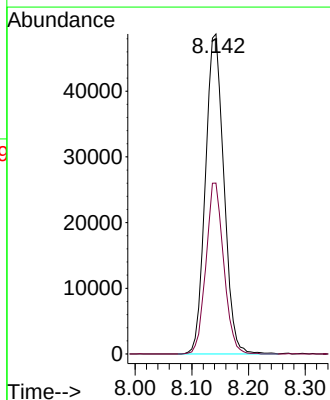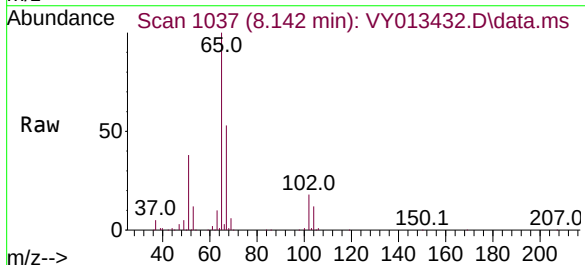

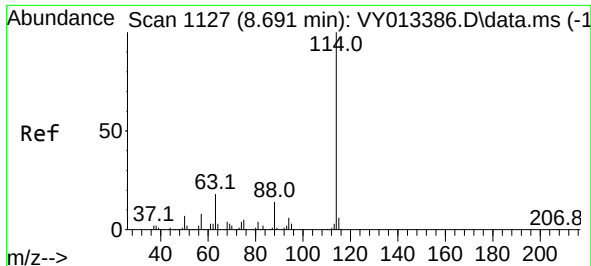

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY013432.D

Acq: 25 Apr 2023 06:35

Instrument :

MSVOA_Y

ClientSampleId :

SPE-2WC-23-04-18





Tgt Ion:114 Resp: 276330

Ion Ratio Lower Upper

114 100

63 19.4 0.0 36.6

88 14.0 0.0 28.8

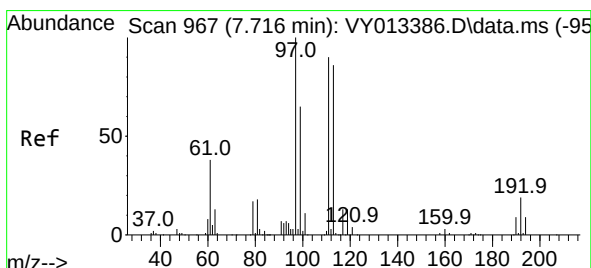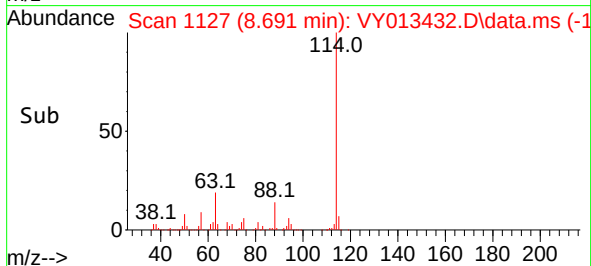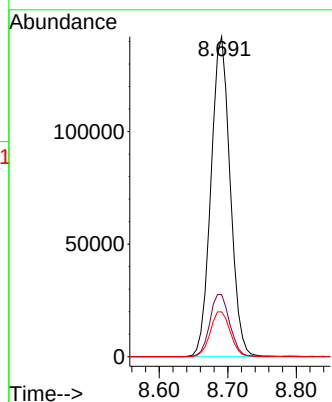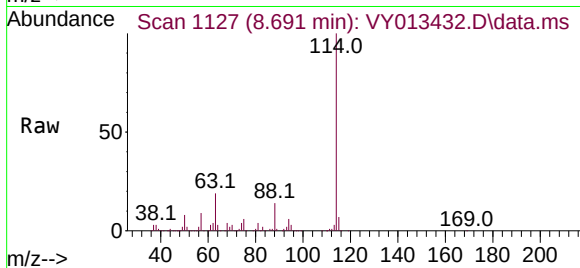

#35

Dibromofluoromethane

Concen: 55.371 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY013432.D

Acq: 25 Apr 2023 06:35




Tgt Ion:113 Resp: 96235


Ion Ratio Lower Upper

113 100

111 100.8 82.2 123.2

192 19.8 16.7 25.1


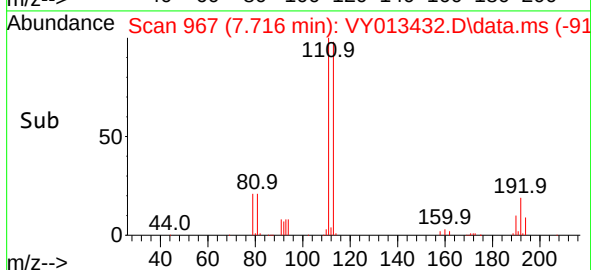
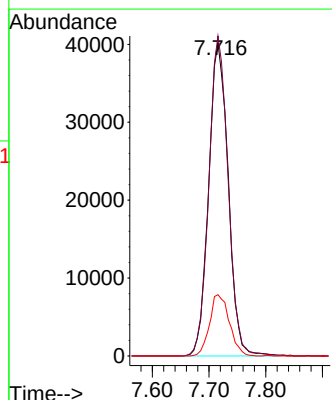
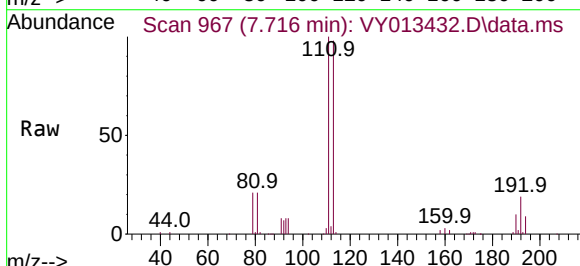


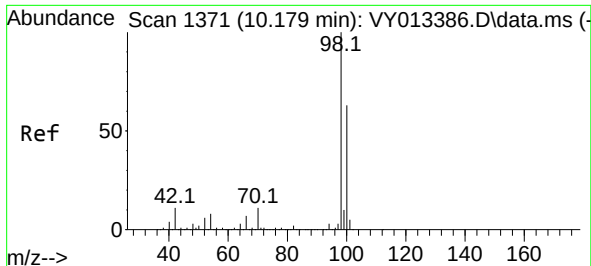

#50
Toluene-d8
Concen: 53.945 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY013432.D
Acq: 25 Apr 2023 06:35




Instrument :
MSVOA_Y
ClientSampleId :
SPE-2WC-23-04-18


Tgt Ion: 98 Resp: 333526
Ion Ratio Lower Upper
98 100
100 61.1 50.5 75.7

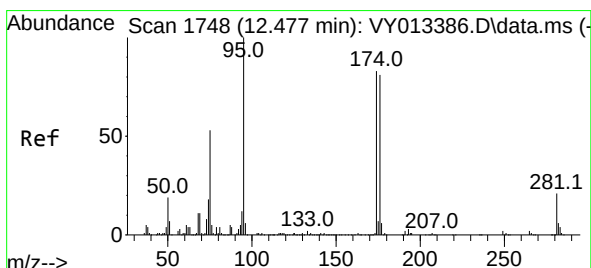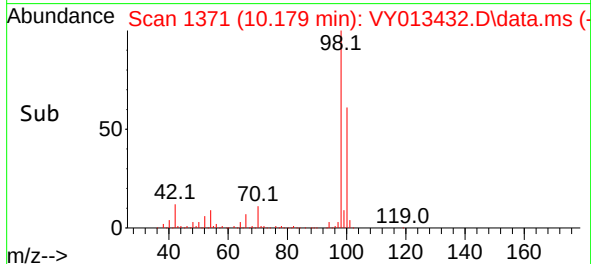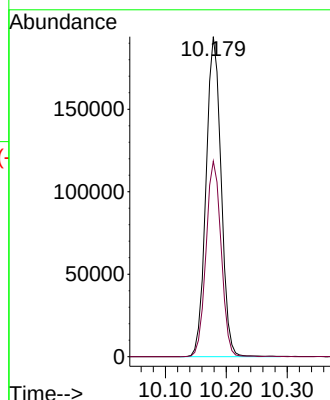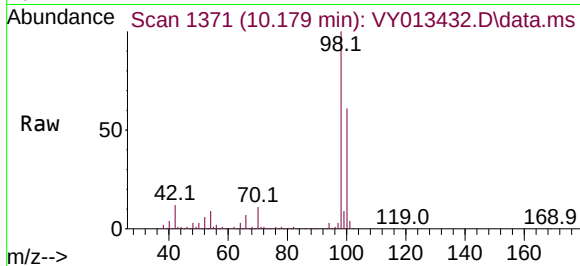

#62
4-Bromofluorobenzene
Concen: 44.882 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY013432.D
Acq: 25 Apr 2023 06:35

Tgt Ion: 95 Resp: 93550
Ion Ratio Lower Upper
95 100
174 90.2 0.0 182.0
176 84.8 0.0 175.4


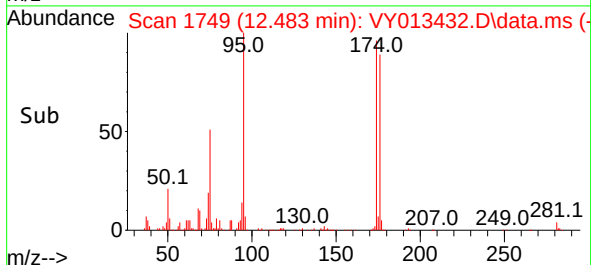
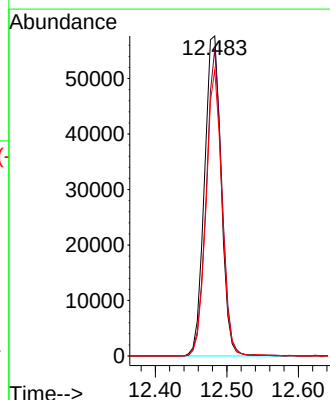
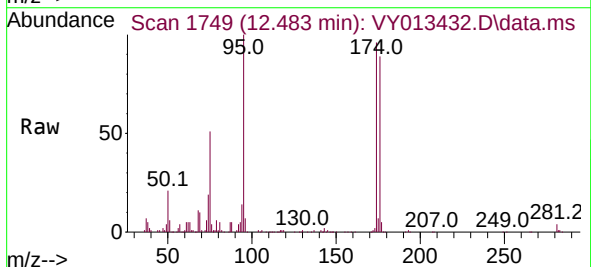


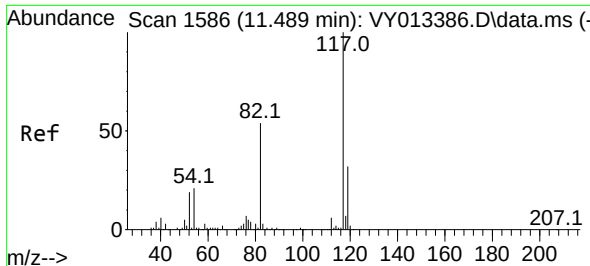

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY013432.D
Acq: 25 Apr 2023 06:35

Instrument :
MSVOA_Y
ClientSampleId :
SPE-2WC-23-04-18

Tgt Ion:117 Resp: 246359
Ion Ratio Lower Upper
117 100
82 53.7 43.0 64.6
119 32.8 25.5 38.3

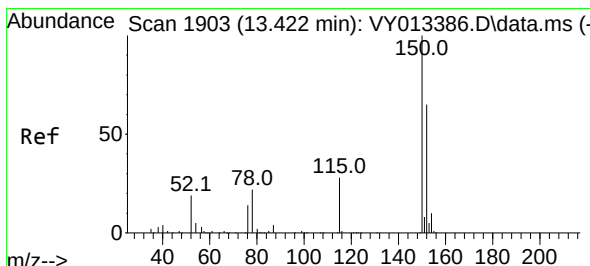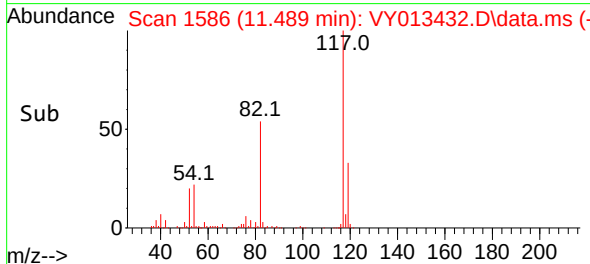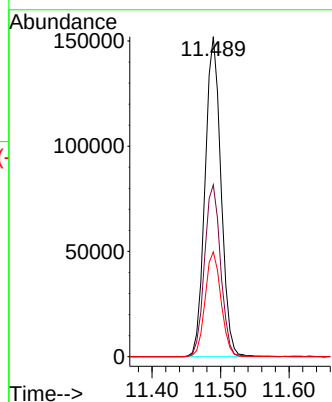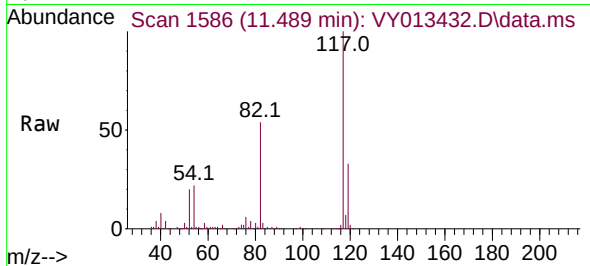

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY013432.D
Acq: 25 Apr 2023 06:35

Tgt Ion:152 Resp: 97326
Ion Ratio Lower Upper
152 100
115 54.4 28.1 84.2
150 156.6 0.0 352.0

