
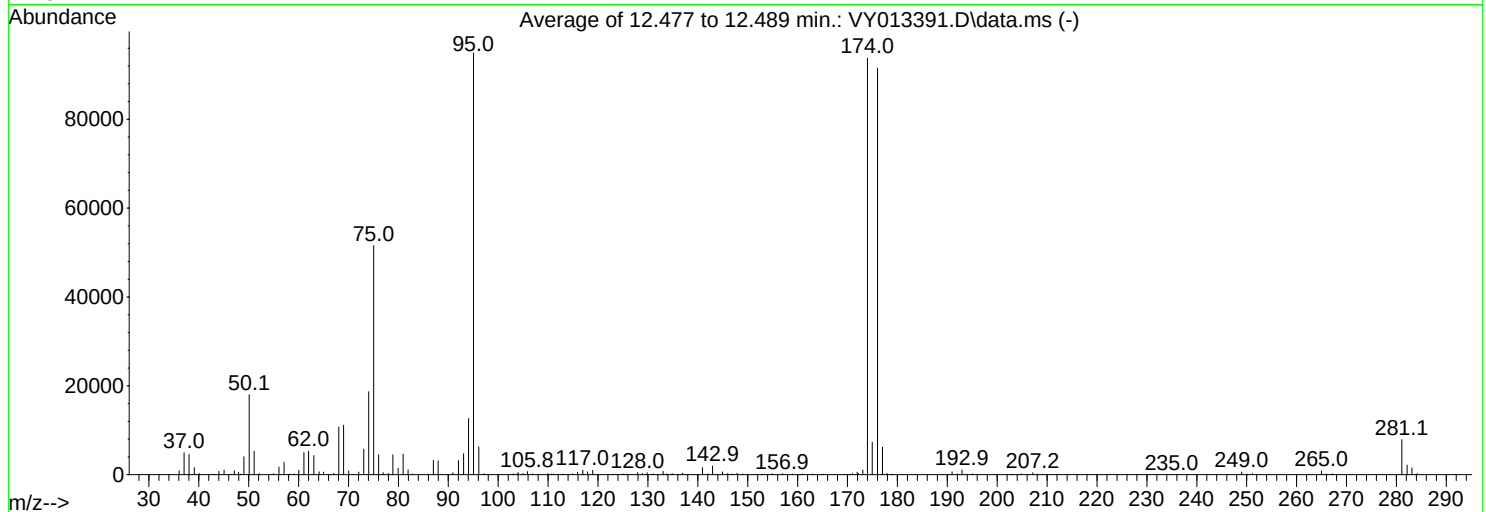


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042423\
Data File : VY013391.D
Acq On : 24 Apr 2023 09:12
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Title : SW846 8260
Last Update : Tue Apr 25 02:39:58 2023

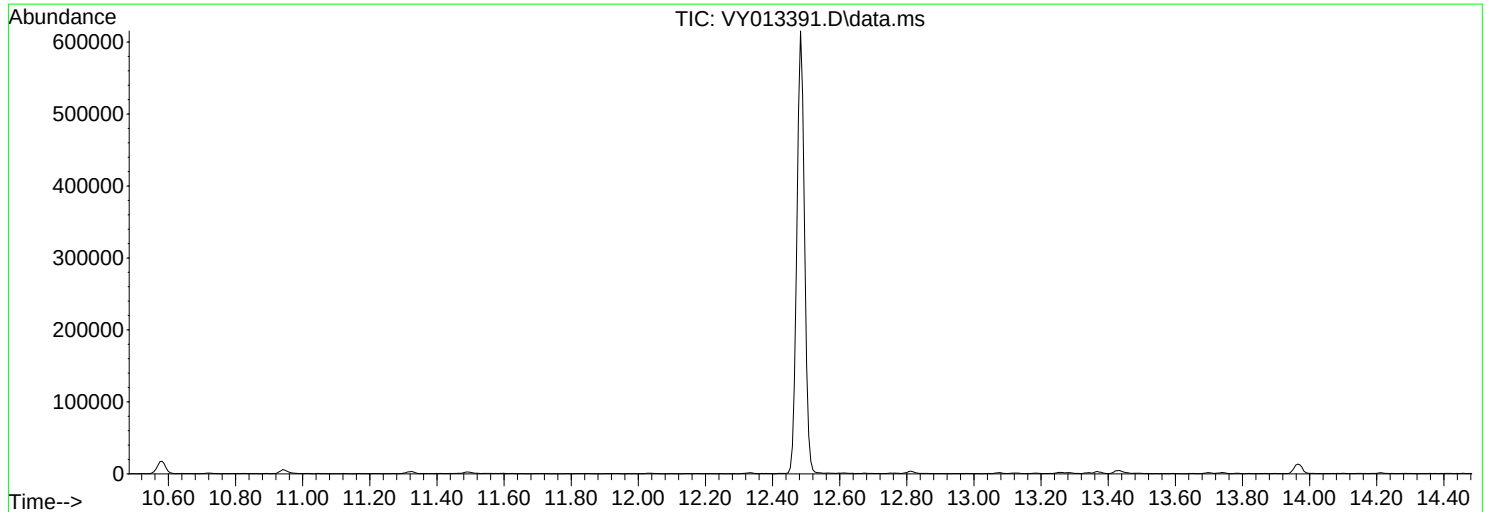

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	18028	PASS
75	95	30	60	54.3	51584	PASS
95	95	100	100	100.0	94965	PASS
96	95	5	9	6.6	6283	PASS
173	174	0.00	2	1.1	1057	PASS
174	95	50	100	98.7	93768	PASS
175	174	5	9	7.8	7328	PASS
176	174	95	101	97.6	91544	PASS
177	176	5	9	6.7	6171	PASS