
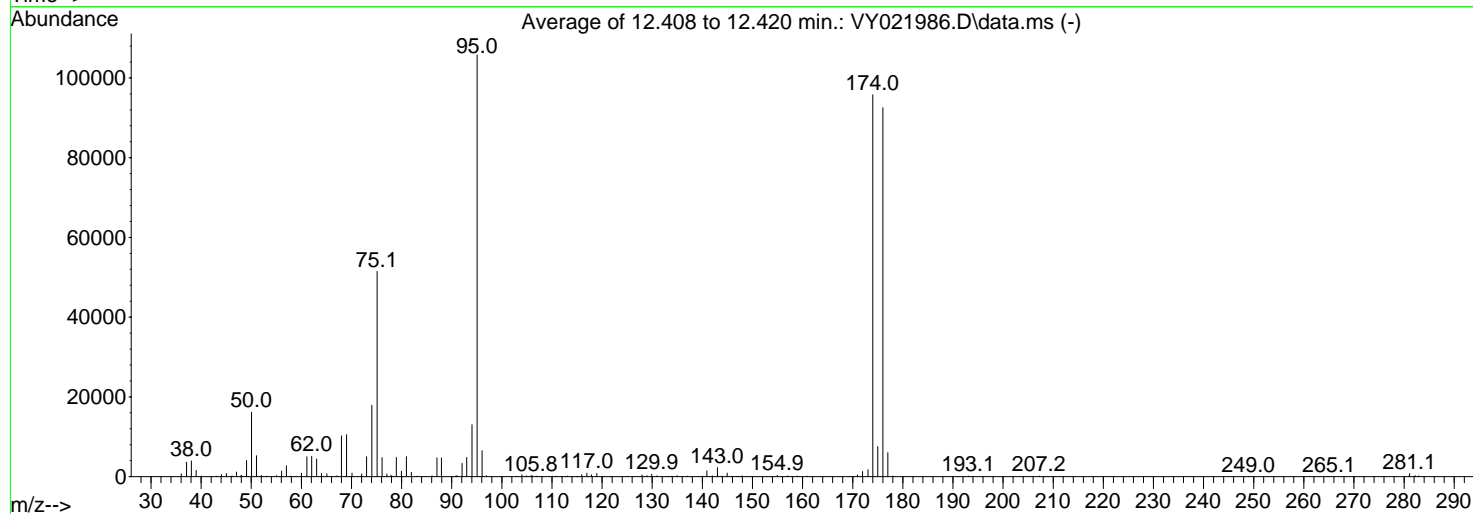


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042425\
 Data File : VY021986.D
 Acq On : 24 Apr 2025 07:59
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Title : SW846 8260
 Last Update : Wed Apr 23 02:30:30 2025

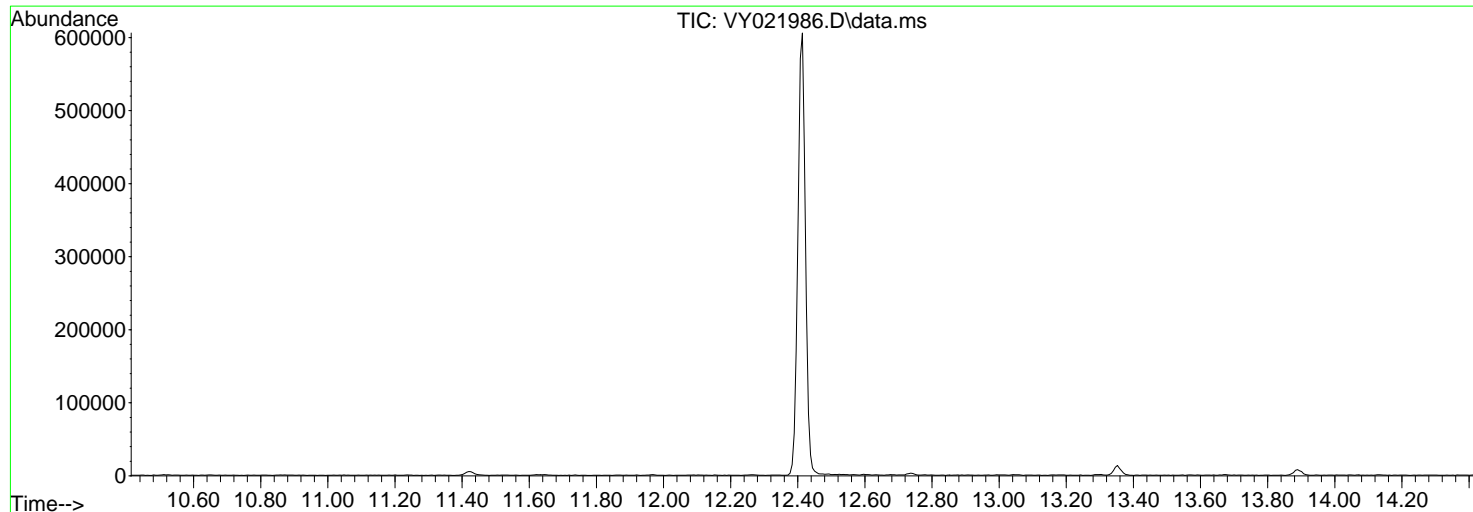

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	16187	PASS
75	95	30	60	48.7	51488	PASS
95	95	100	100	100.0	105800	PASS
96	95	5	9	6.2	6529	PASS
173	174	0.00	2	1.8	1733	PASS
174	95	50	100	90.5	95800	PASS
175	174	5	9	7.9	7547	PASS
176	174	95	101	96.6	92531	PASS
177	176	5	9	6.5	6039	PASS