

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042522\
 Data File : VY008474.D
 Acq On : 25 Apr 2022 12:10
 Operator : KP/MD
 Sample : N2523-03
 Misc : 4.99g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SU-04-042122

Quant Time: Apr 26 01:54:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042122S.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 21 14:28:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	44675	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	78507	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	72554	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	29762	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	24564	46.730	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	93.460%
35) Dibromofluoromethane	7.716	113	24733	48.815	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.620%
50) Toluene-d8	10.179	98	93337	46.389	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	92.780%
62) 4-Bromofluorobenzene	12.483	95	27972	40.999	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	82.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042522\
Data File : VY008474.D
Acq On : 25 Apr 2022 12:10
Operator : KP/MD
Sample : N2523-03
Misc : 4.99g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SU-04-042122

Quant Time: Apr 26 01:54:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042122S.M
Quant Title : SW846 8260
QLast Update : Thu Apr 21 14:28:40 2022
Response via : Initial Calibration




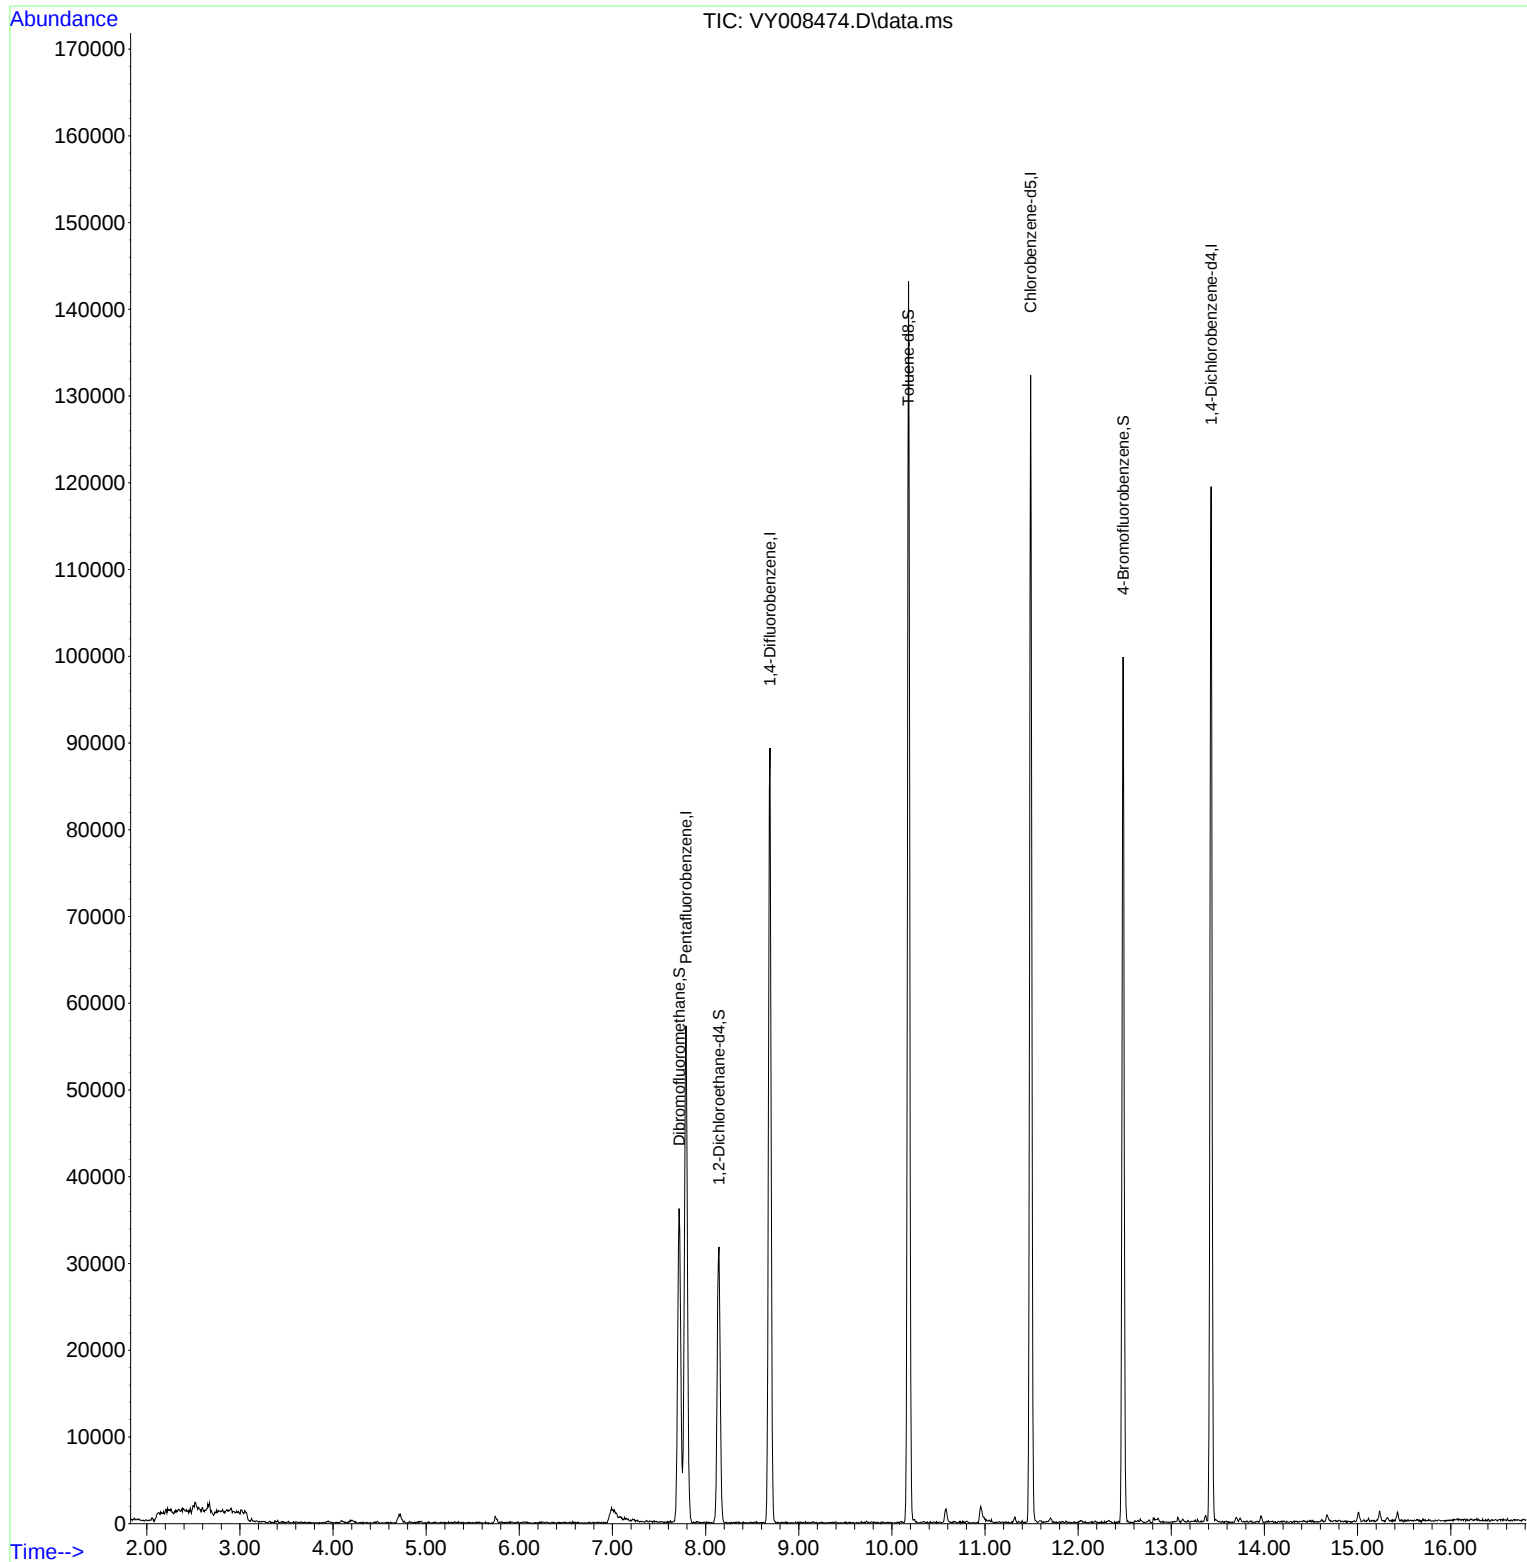


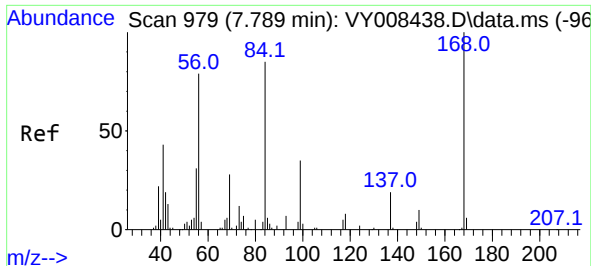

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008474.D
Acq: 25 Apr 2022 12:10




Instrument :
MSVOA_Y
ClientSampleId :
SU-04-042122


Tgt Ion:168 Resp: 44675
Ion Ratio Lower Upper
168 100
99 51.9 46.9 70.3

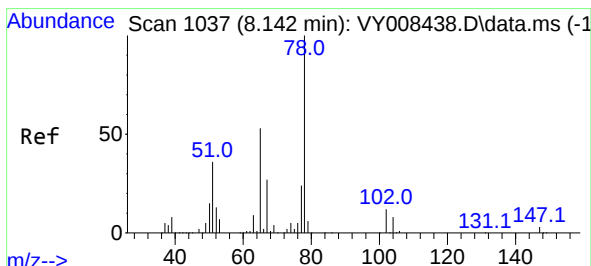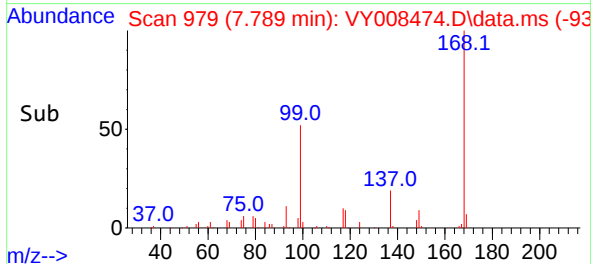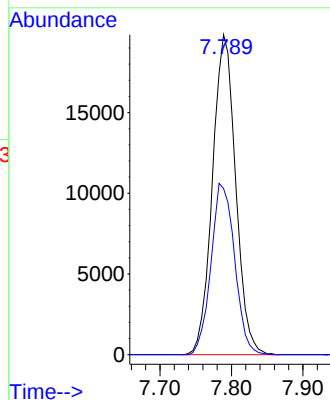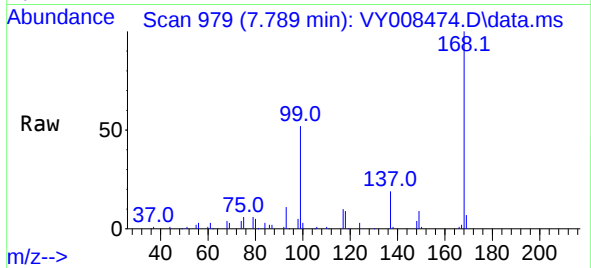

#33
1,2-Dichloroethane-d4
Concen: 46.730 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VY008474.D
Acq: 25 Apr 2022 12:10

Tgt Ion: 65 Resp: 24564
Ion Ratio Lower Upper
65 100
67 52.5 0.0 99.4

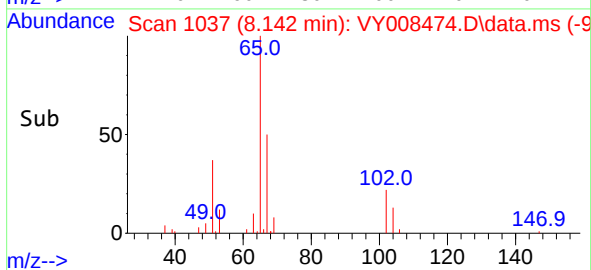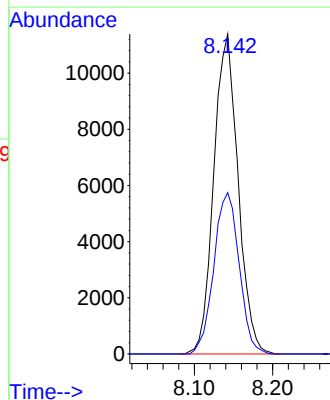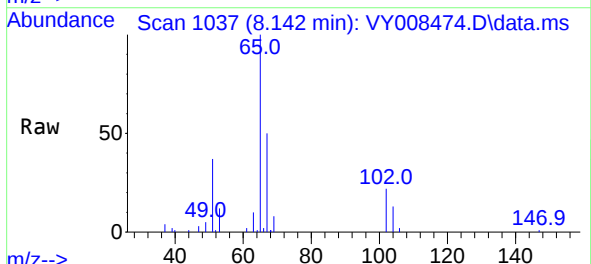

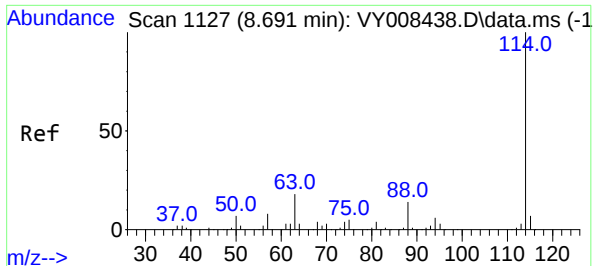

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY008474.D

Acq: 25 Apr 2022 12:10

Instrument :

MSVOA_Y

ClientSampleId :

SU-04-042122





Tgt Ion:114 Resp: 78507

Ion Ratio Lower Upper

114 100

63 18.4 0.0 43.2

88 13.7 0.0 31.8

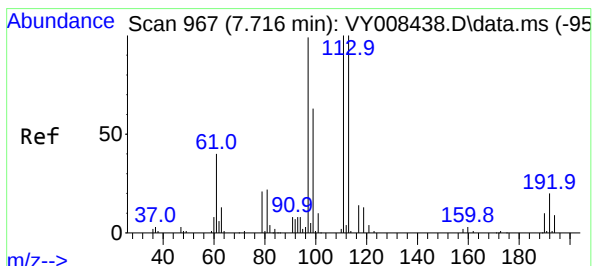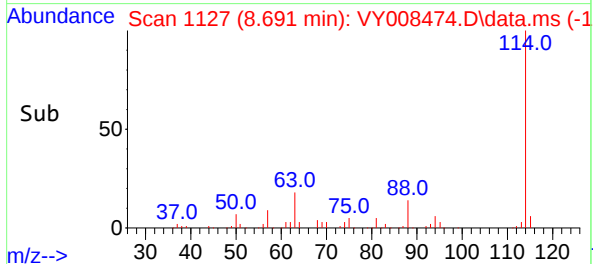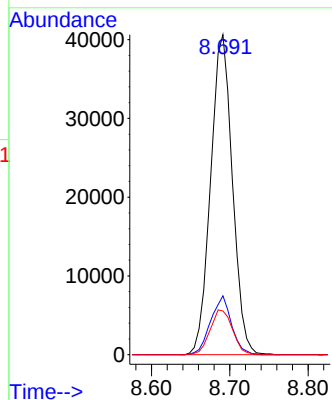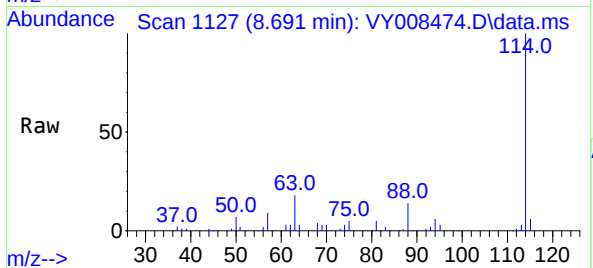

#35

Dibromofluoromethane

Concen: 48.815 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY008474.D

Acq: 25 Apr 2022 12:10




Tgt Ion:113 Resp: 24733


Ion Ratio Lower Upper

113 100

111 104.2 82.6 124.0

192 19.2 17.6 26.4


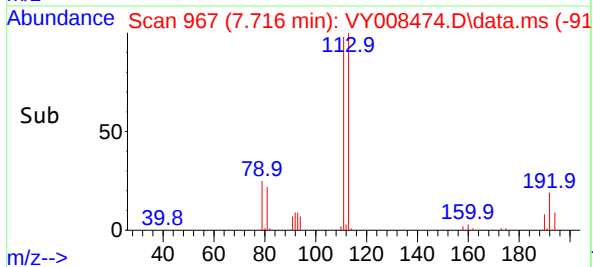
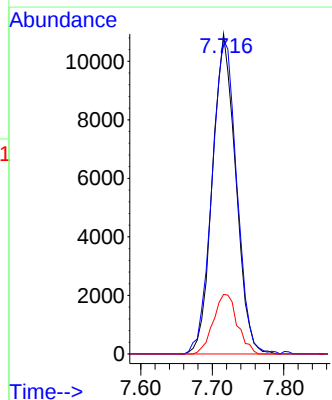
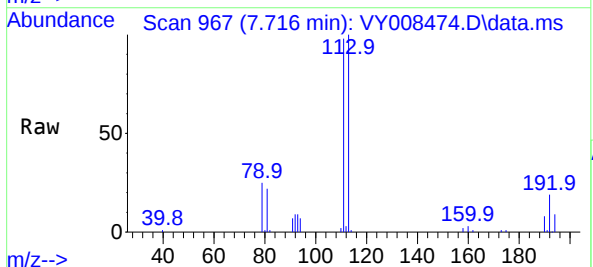


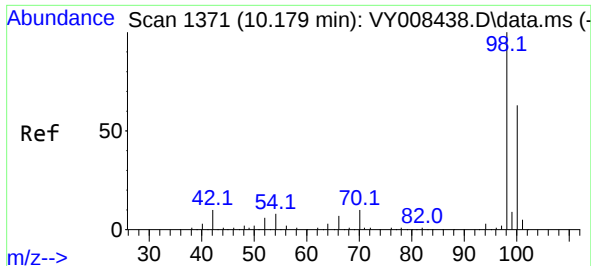

#50
Toluene-d8
Concen: 46.389 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY008474.D
Acq: 25 Apr 2022 12:10




Instrument :
MSVOA_Y
ClientSampleId :
SU-04-042122


Tgt Ion: 98 Resp: 93337
Ion Ratio Lower Upper
98 100
100 65.6 50.2 75.2

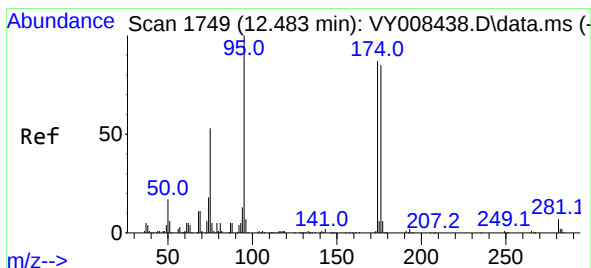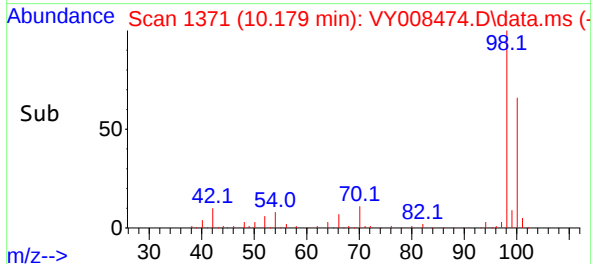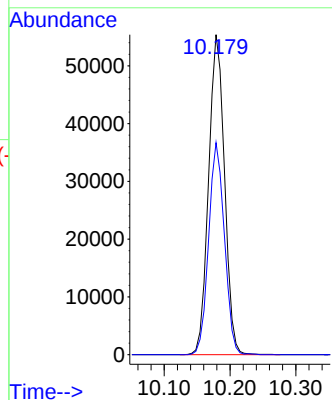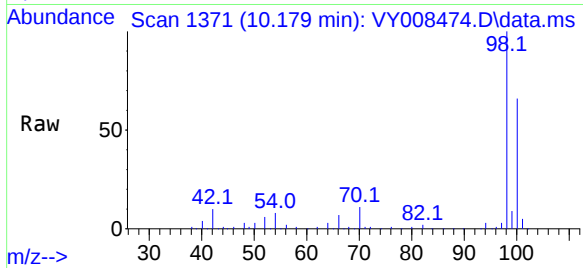

#62
4-Bromofluorobenzene
Concen: 40.999 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008474.D
Acq: 25 Apr 2022 12:10

Tgt Ion: 95 Resp: 27972
Ion Ratio Lower Upper
95 100
174 88.5 0.0 177.0
176 87.6 0.0 175.8


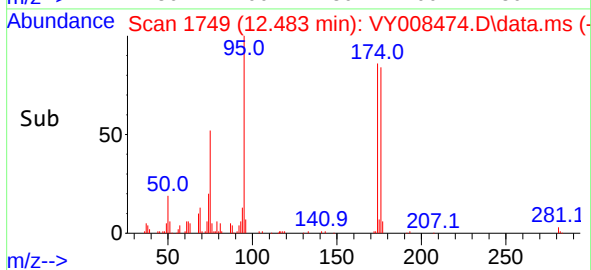
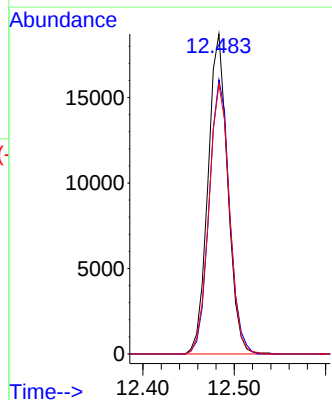
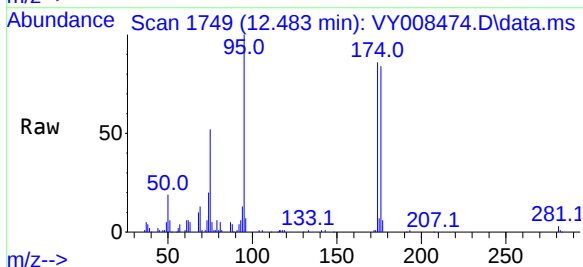


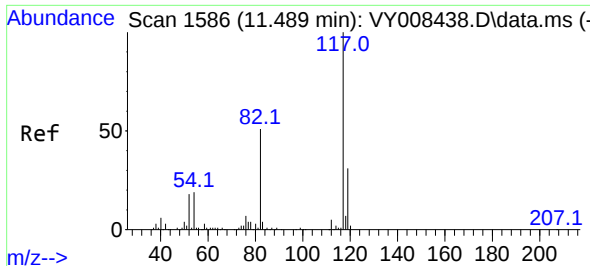

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY008474.D
Acq: 25 Apr 2022 12:10

Instrument :
MSVOA_Y
ClientSampleId :
SU-04-042122

Tgt Ion:	117	Resp:	72554
Ion Ratio	Lower	Upper	
117	100		
82	52.8	43.0	64.4
119	32.3	25.4	38.0

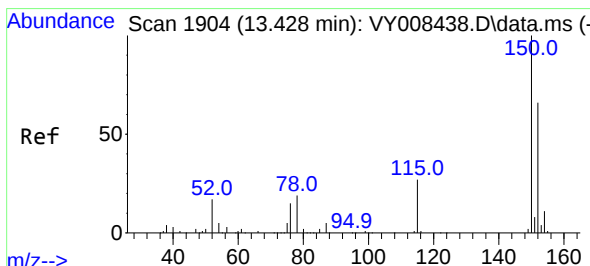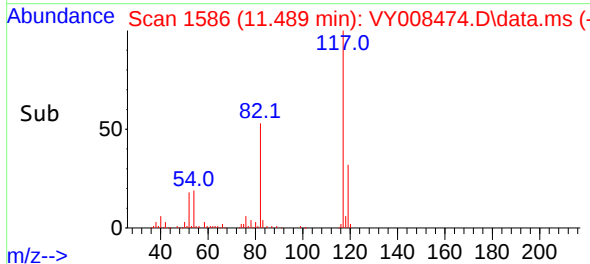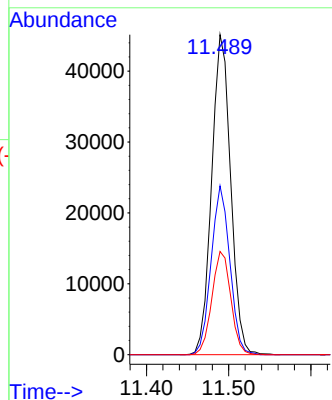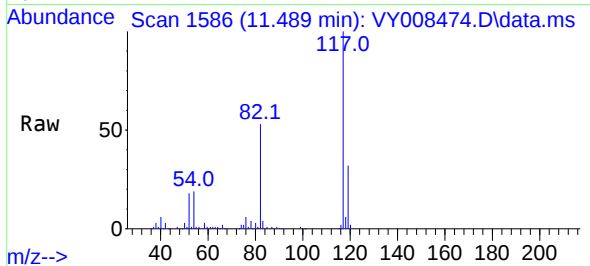

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008474.D
Acq: 25 Apr 2022 12:10

Tgt Ion:	152	Resp:	29762
Ion Ratio	Lower	Upper	
152	100		
115	56.9	28.2	84.7
150	159.5	0.0	347.6

