

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042525\
 Data File : VY022003.D
 Acq On : 25 Apr 2025 12:41
 Operator : SY/MD
 Sample : Q1869-03
 Misc : 5.75g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 MH-F-VOC

Quant Time: Apr 25 22:55:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	302222	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	578395	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	516695	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	207068	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	150865	54.043	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	108.080%
35) Dibromofluoromethane	7.634	113	194319	50.853	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.700%
50) Toluene-d8	10.103	98	695812	48.301	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.600%
62) 4-Bromofluorobenzene	12.408	95	195676	40.349	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	80.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042525\
Data File : VY022003.D
Acq On : 25 Apr 2025 12:41
Operator : SY/MD
Sample : Q1869-03
Misc : 5.75g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
MH-F-VOC

Quant Time: Apr 25 22:55:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration




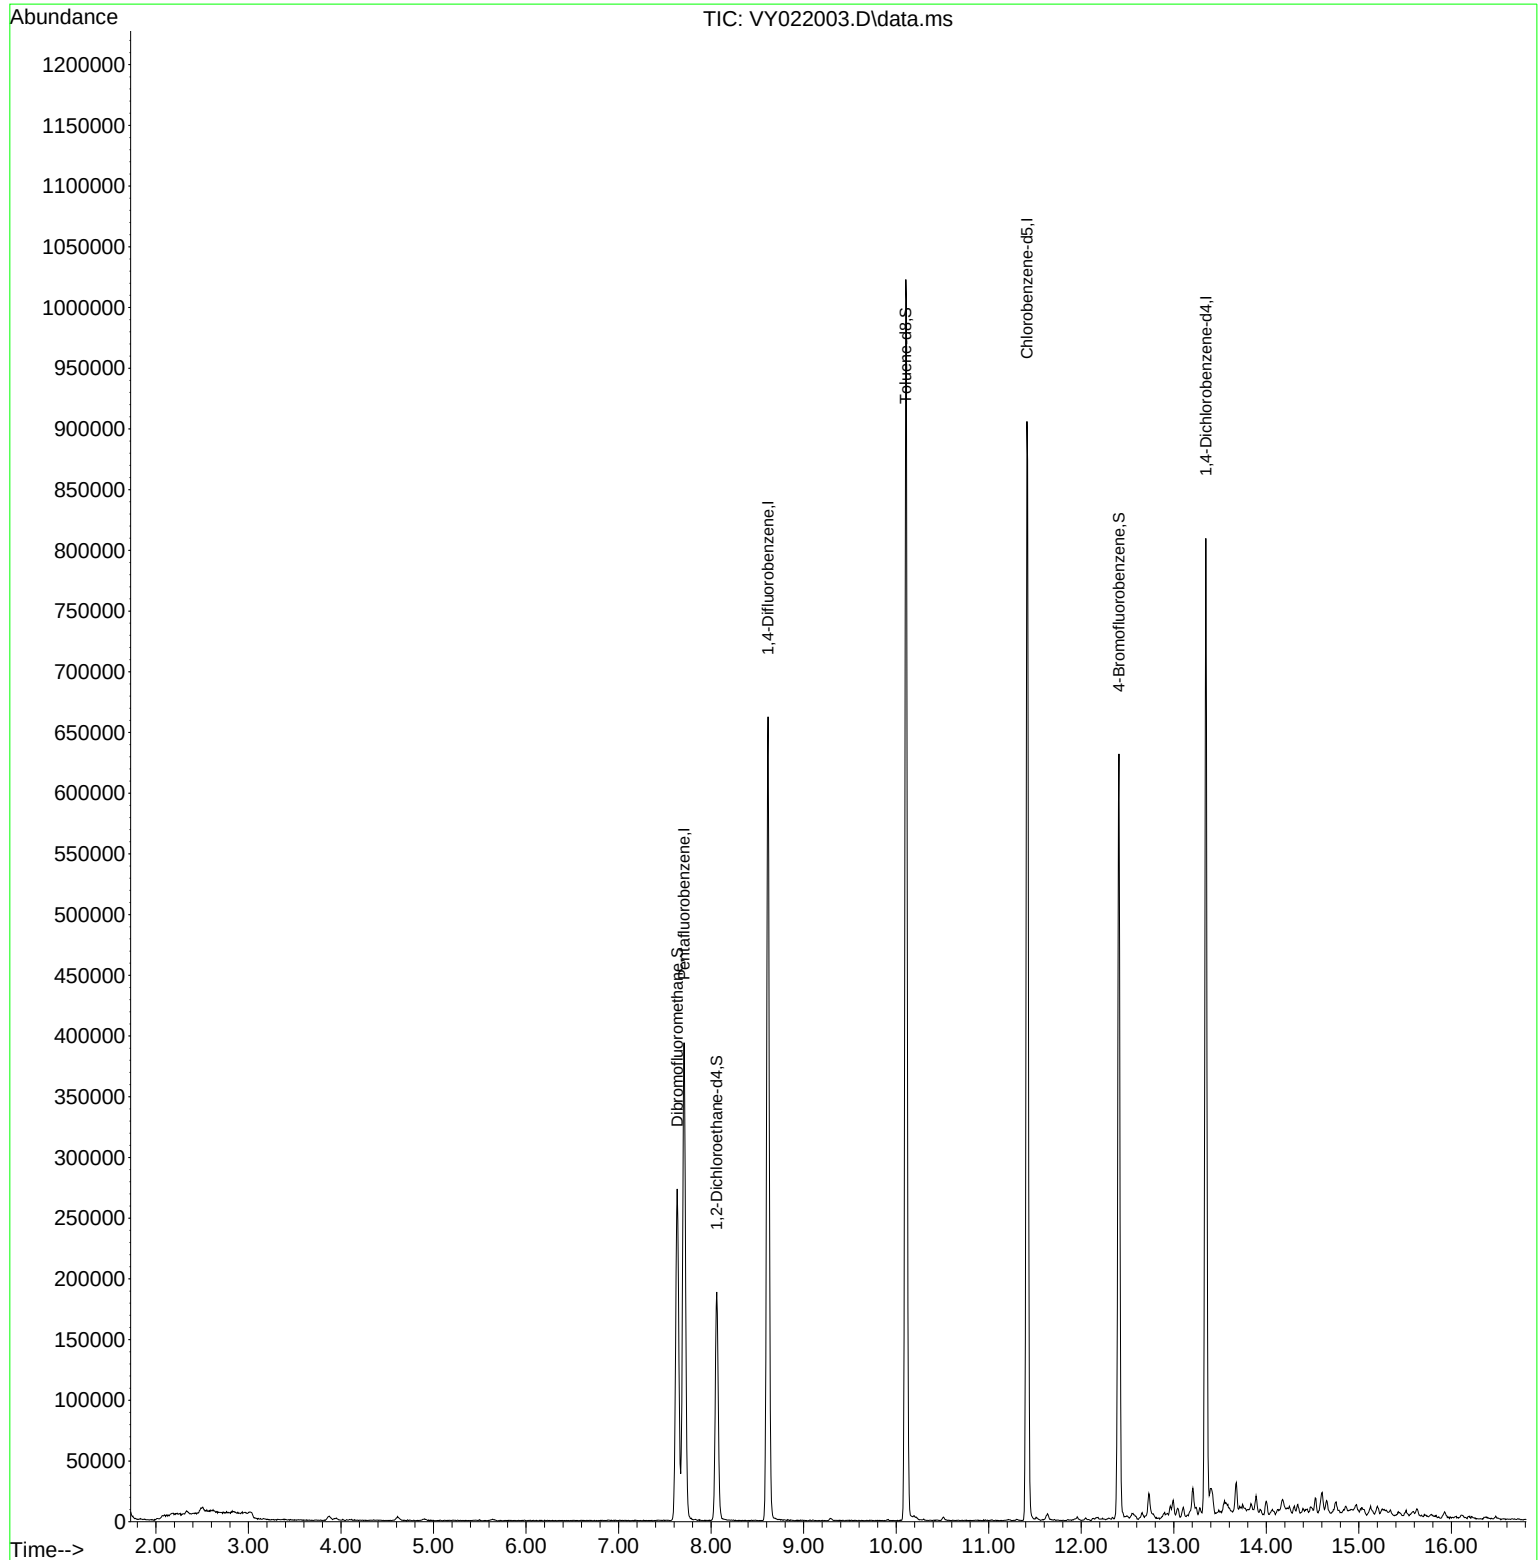


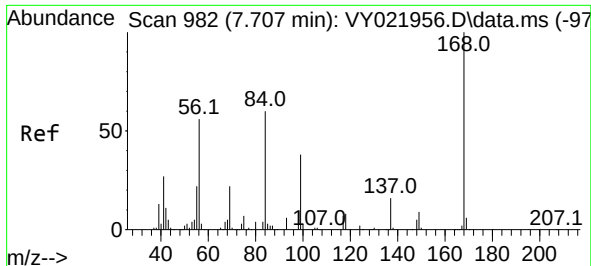

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY022003.D
Acq: 25 Apr 2025 12:41




Instrument :
MSVOA_Y
ClientSampleId :
MH-F-VOC


Tgt Ion:168 Resp: 302222
Ion Ratio Lower Upper
168 100
99 53.4 43.1 64.7

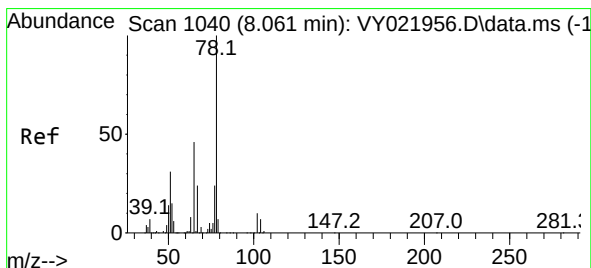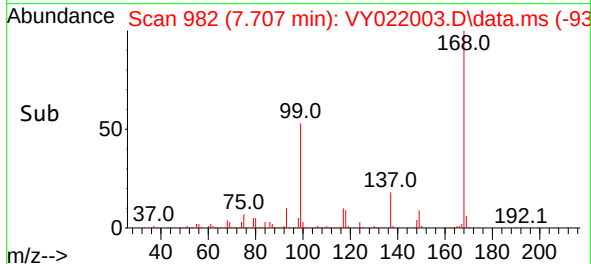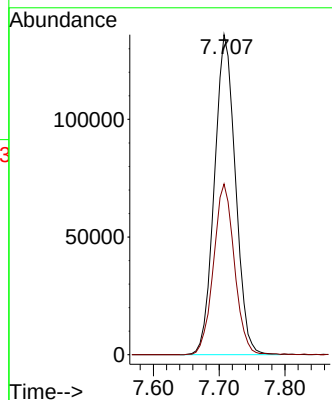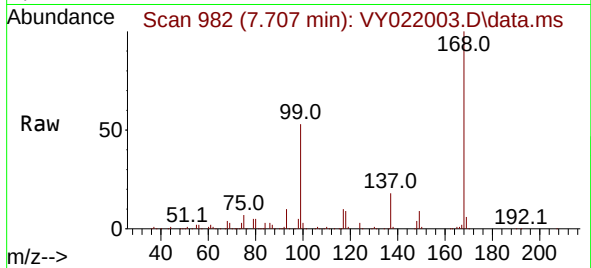

#33
1,2-Dichloroethane-d4
Concen: 54.043 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY022003.D
Acq: 25 Apr 2025 12:41

Tgt Ion: 65 Resp: 150865
Ion Ratio Lower Upper
65 100
67 52.5 0.0 105.8

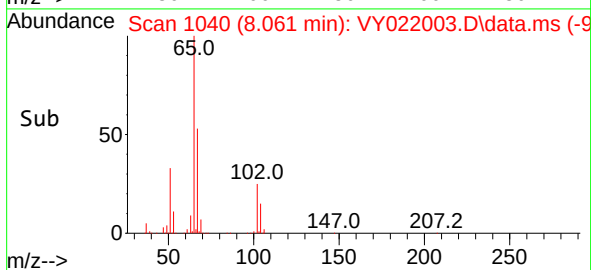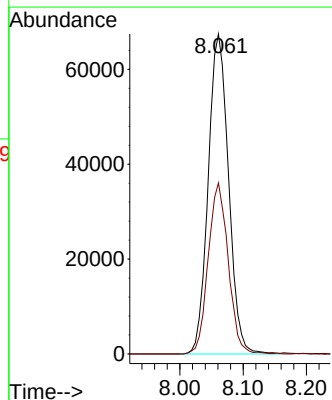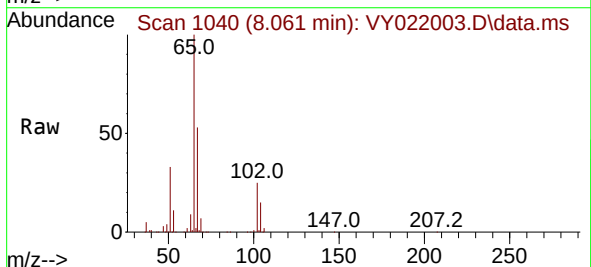

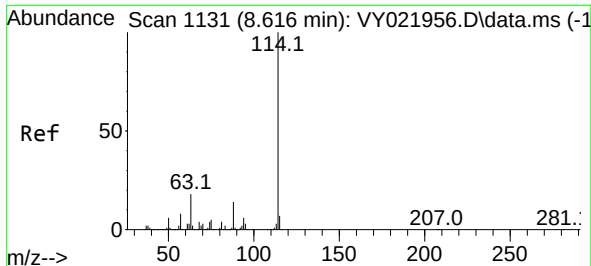

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY022003.D

Acq: 25 Apr 2025 12:41

Instrument :

MSVOA_Y

ClientSampleId :

MH-F-VOC





Tgt Ion:114 Resp: 578395

Ion Ratio Lower Upper

114 100

63 18.1 0.0 35.4

88 14.5 0.0 28.2

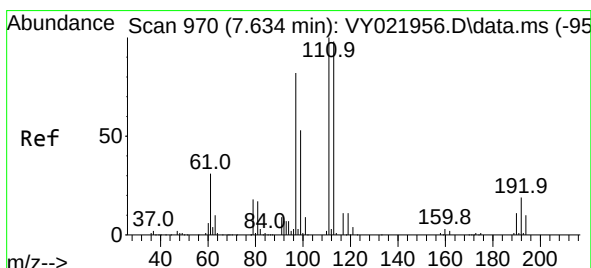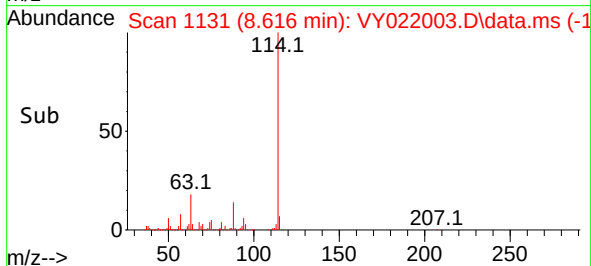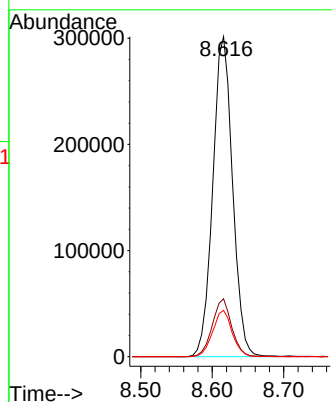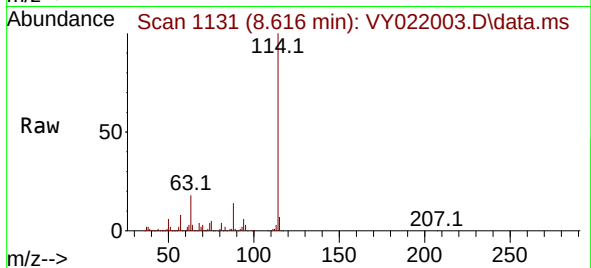

#35

Dibromofluoromethane

Concen: 50.853 ug/l

RT: 7.634 min Scan# 970

Delta R.T. 0.000 min

Lab File: VY022003.D

Acq: 25 Apr 2025 12:41




Tgt Ion:113 Resp: 194319


Ion Ratio Lower Upper

113 100

111 102.5 81.8 122.8

192 20.2 15.6 23.4


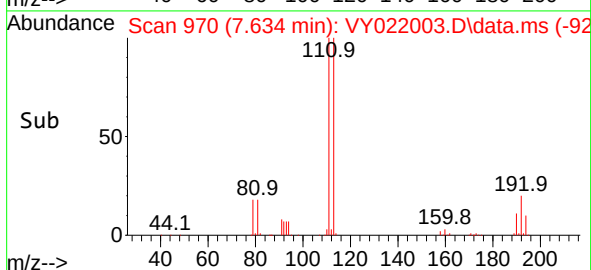
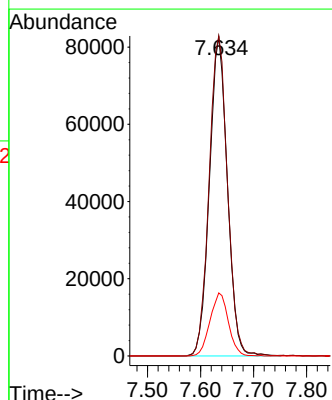
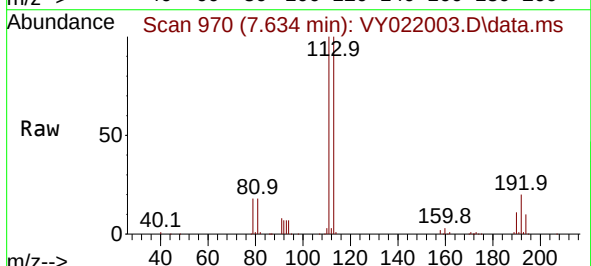


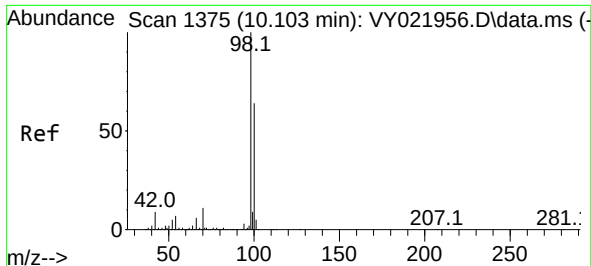

#50
Toluene-d8
Concen: 48.301 ug/l
RT: 10.103 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY022003.D
Acq: 25 Apr 2025 12:41




Instrument :
MSVOA_Y
ClientSampleId :
MH-F-VOC


Tgt Ion: 98 Resp: 695812
Ion Ratio Lower Upper
98 100
100 64.2 51.6 77.4

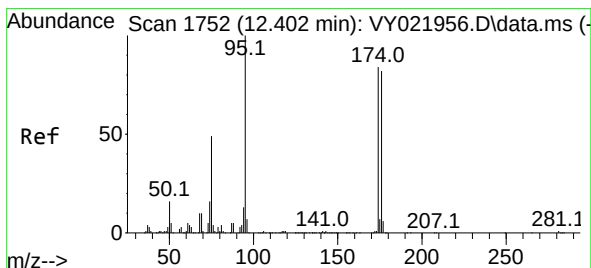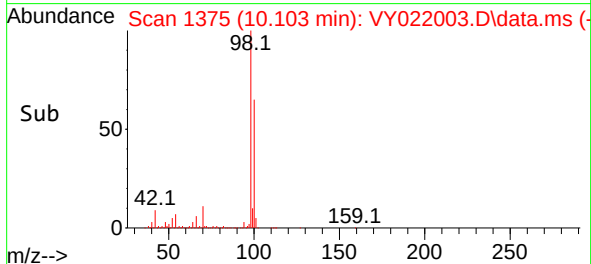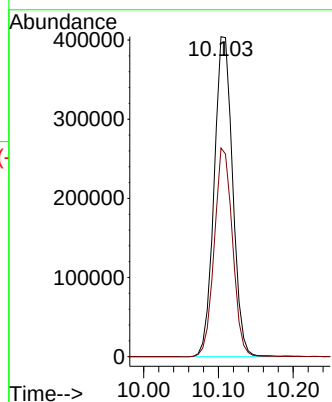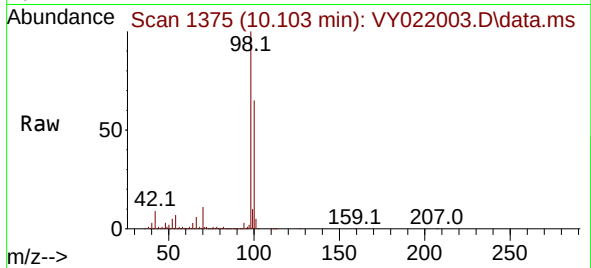

#62
4-Bromofluorobenzene
Concen: 40.349 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY022003.D
Acq: 25 Apr 2025 12:41

Tgt Ion: 95 Resp: 195676
Ion Ratio Lower Upper
95 100
174 88.0 0.0 179.0
176 83.9 0.0 171.8


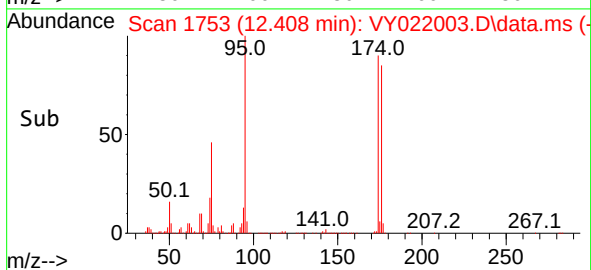
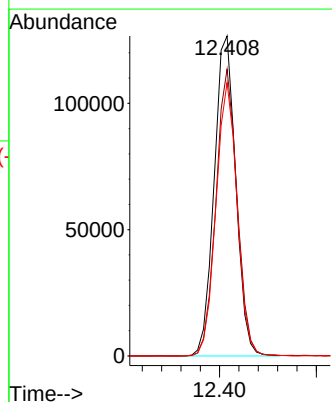
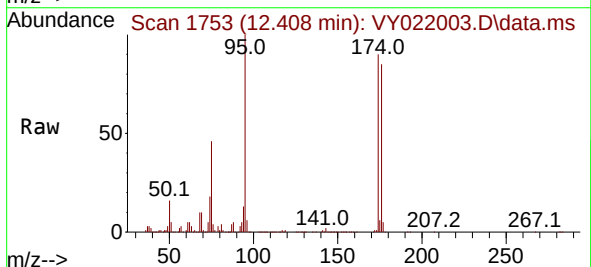


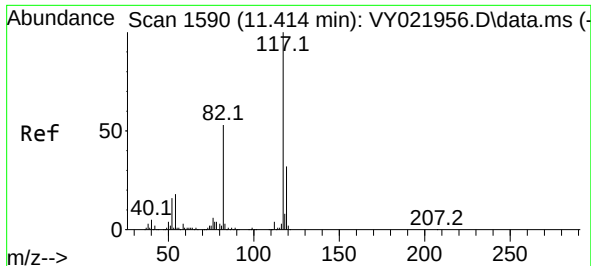

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY022003.D
Acq: 25 Apr 2025 12:41

Instrument :
MSVOA_Y
ClientSampleId :
MH-F-VOC

Tgt Ion:117 Resp: 516695
Ion Ratio Lower Upper
117 100
82 53.7 42.1 63.1
119 32.3 25.7 38.5

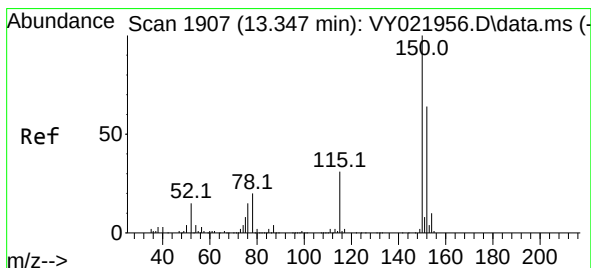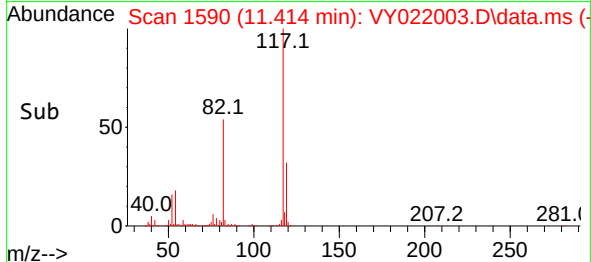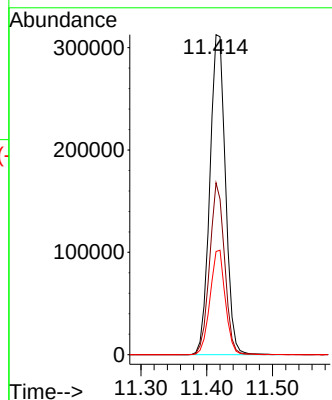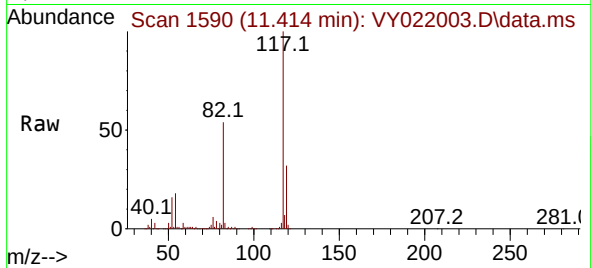

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.347 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY022003.D
Acq: 25 Apr 2025 12:41

Tgt Ion:152 Resp: 207068
Ion Ratio Lower Upper
152 100
115 57.5 28.0 84.0
150 158.7 0.0 345.6

