
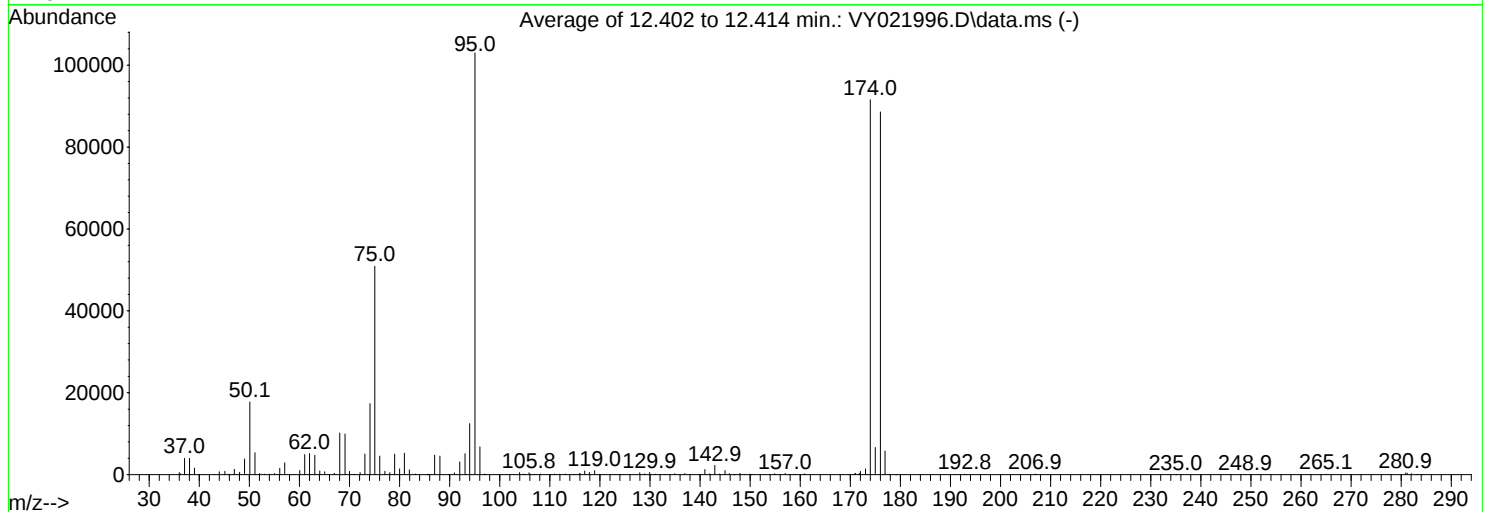


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042525\
Data File : VY021996.D
Acq On : 25 Apr 2025 09:00
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Title : SW846 8260
Last Update : Wed Apr 23 02:30:30 2025

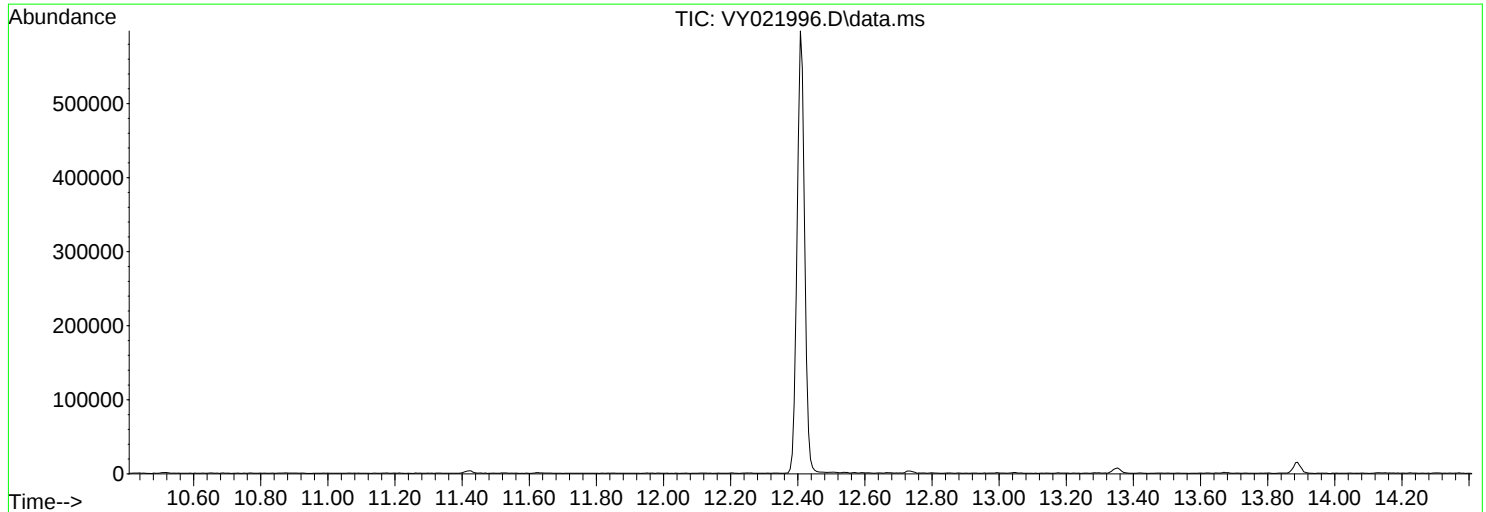

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	17746	PASS
75	95	30	60	49.4	50909	PASS
95	95	100	100	100.0	103013	PASS
96	95	5	9	6.6	6794	PASS
173	174	0.00	2	1.5	1413	PASS
174	95	50	100	88.9	91573	PASS
175	174	5	9	7.2	6628	PASS
176	174	95	101	96.7	88576	PASS
177	176	5	9	6.5	5795	PASS