

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042825\
 Data File : VY022036.D
 Acq On : 28 Apr 2025 17:02
 Operator : SY/MD
 Sample : Q1891-03
 Misc : 4.61g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 MH-C-VOC

Quant Time: Apr 29 03:55:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	299712	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	571993	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	533506	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	222901	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	155503	56.171	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	112.340%
35) Dibromofluoromethane	7.634	113	194111	51.367	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.740%
50) Toluene-d8	10.103	98	699839	49.124	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	98.240%
62) 4-Bromofluorobenzene	12.408	95	220033	45.879	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	91.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042825\
Data File : VY022036.D
Acq On : 28 Apr 2025 17:02
Operator : SY/MD
Sample : Q1891-03
Misc : 4.61g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
MH-C-VOC

Quant Time: Apr 29 03:55:17 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration




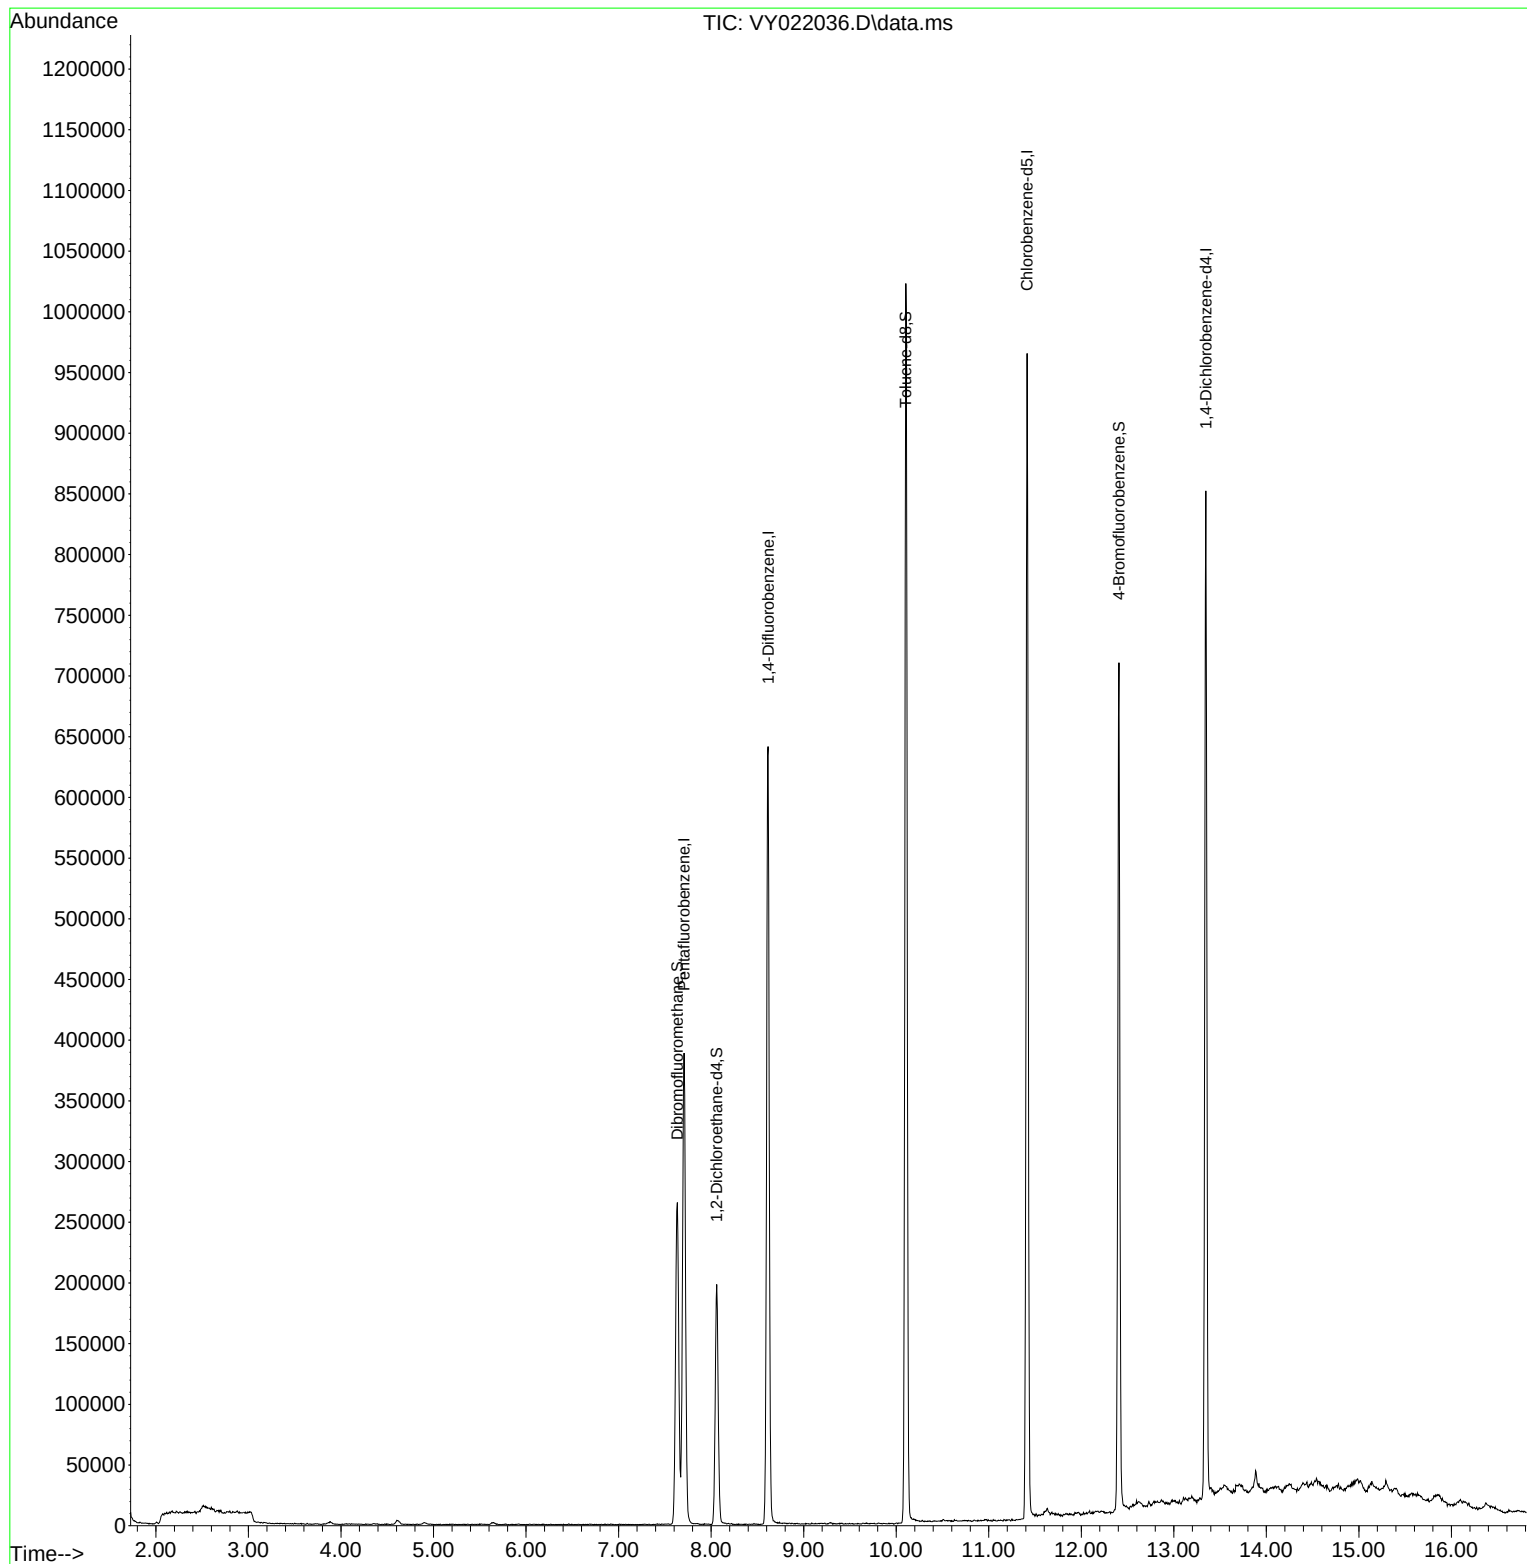


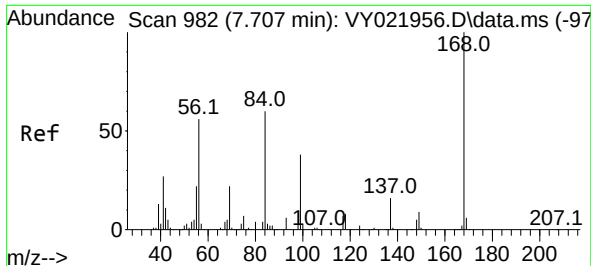

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY022036.D
Acq: 28 Apr 2025 17:02




Instrument :
MSVOA_Y
ClientSampleId :
MH-C-VOC


Tgt Ion:168 Resp: 299712
Ion Ratio Lower Upper
168 100
99 54.5 43.1 64.7

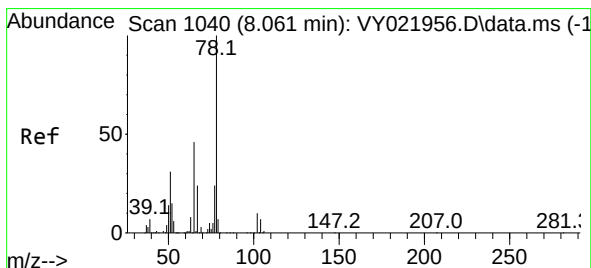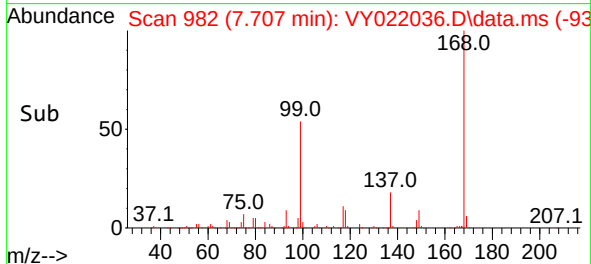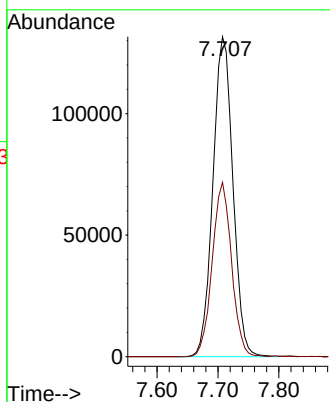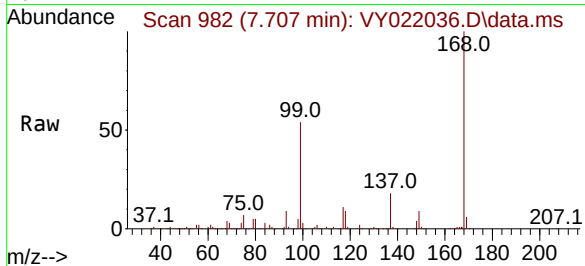

#33
1,2-Dichloroethane-d4
Concen: 56.171 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY022036.D
Acq: 28 Apr 2025 17:02

Tgt Ion: 65 Resp: 155503
Ion Ratio Lower Upper
65 100
67 52.4 0.0 105.8


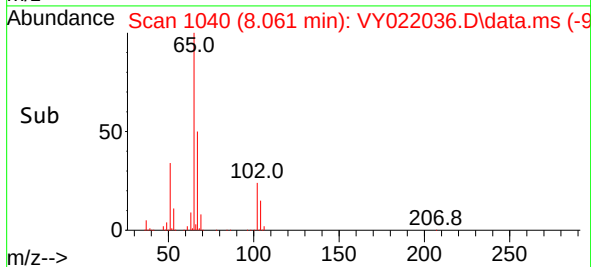
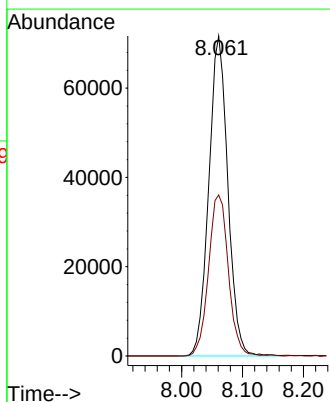
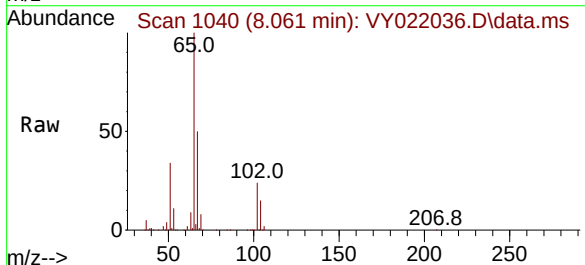


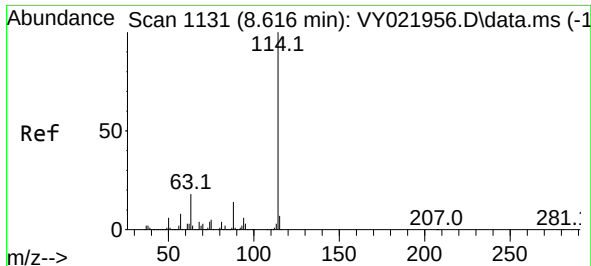

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY022036.D
Acq: 28 Apr 2025 17:02




Instrument :
MSVOA_Y
ClientSampleId :
MH-C-VOC


Tgt Ion:114 Resp: 571993
Ion Ratio Lower Upper
114 100
63 17.3 0.0 35.4
88 14.9 0.0 28.2

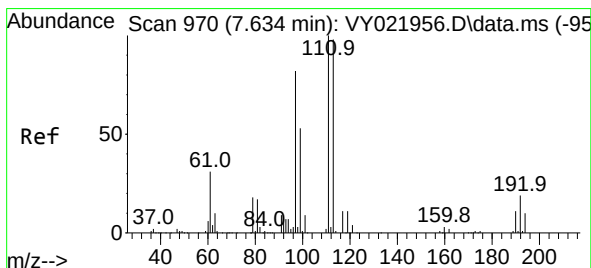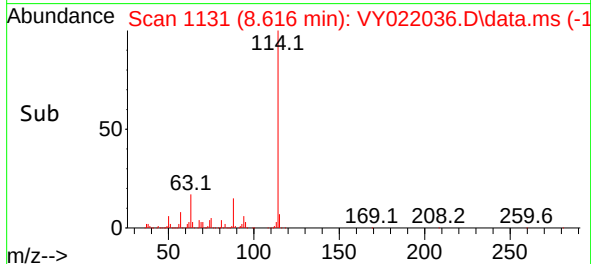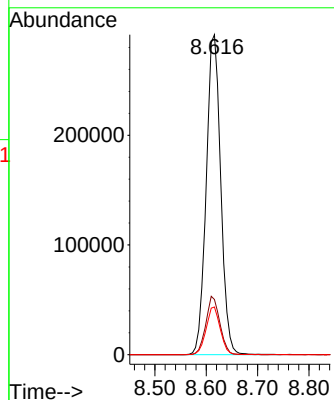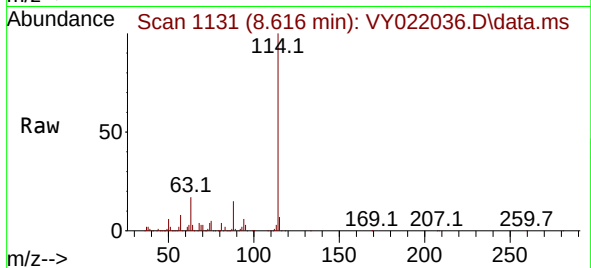

#35
Dibromofluoromethane
Concen: 51.367 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY022036.D
Acq: 28 Apr 2025 17:02

Tgt Ion:113 Resp: 194111
Ion Ratio Lower Upper
113 100
111 101.4 81.8 122.8
192 20.3 15.6 23.4


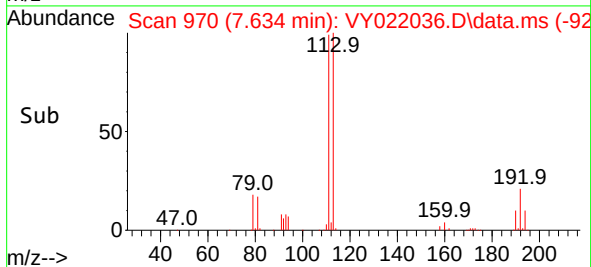
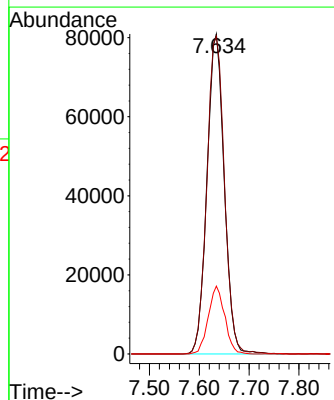
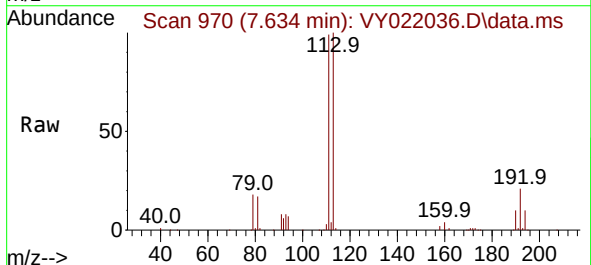


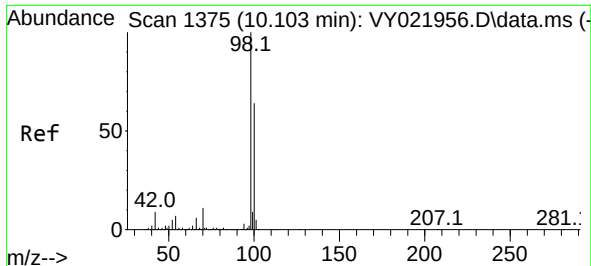

#50
Toluene-d8
Concen: 49.124 ug/l
RT: 10.103 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY022036.D
Acq: 28 Apr 2025 17:02




Instrument :
MSVOA_Y
ClientSampleId :
MH-C-VOC


Tgt Ion: 98 Resp: 699839
Ion Ratio Lower Upper
98 100
100 63.8 51.6 77.4

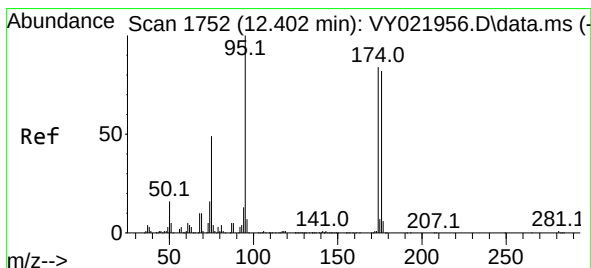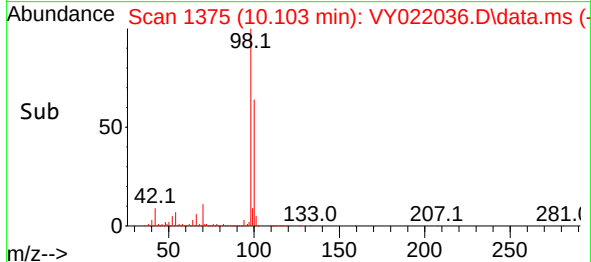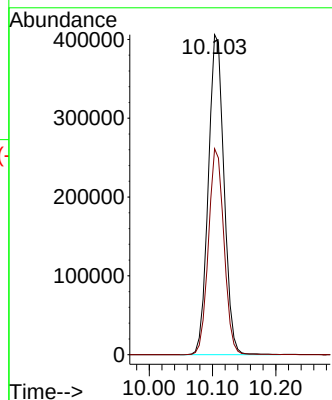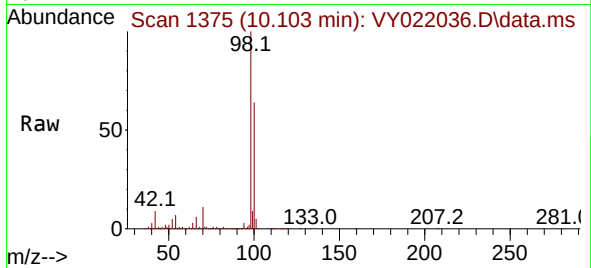

#62
4-Bromofluorobenzene
Concen: 45.879 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY022036.D
Acq: 28 Apr 2025 17:02

Tgt Ion: 95 Resp: 220033
Ion Ratio Lower Upper
95 100
174 89.3 0.0 179.0
176 84.3 0.0 171.8

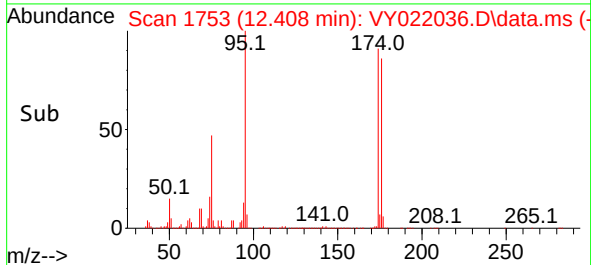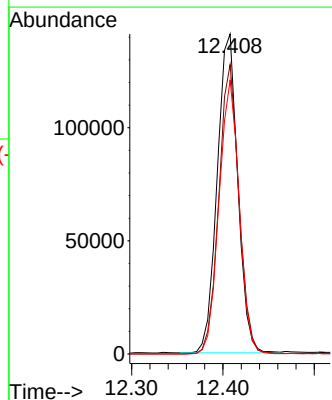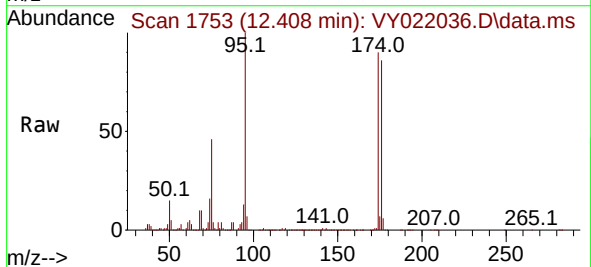

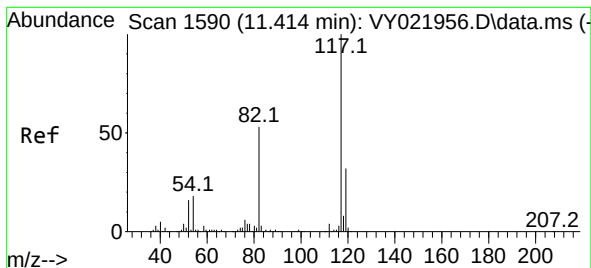

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 1590

Delta R.T. 0.000 min

Lab File: VY022036.D

Acq: 28 Apr 2025 17:02

Instrument :

MSVOA_Y

ClientSampleId :

MH-C-VOC





Tgt Ion:117 Resp: 533506

Ion Ratio Lower Upper

117 100

82 52.2 42.1 63.1

119 32.7 25.7 38.5

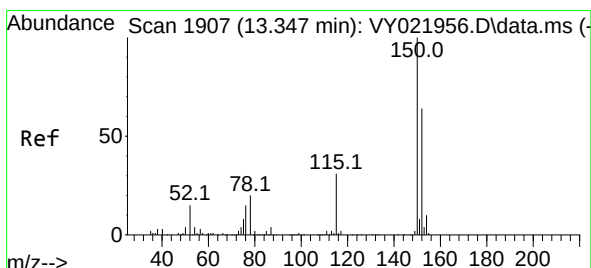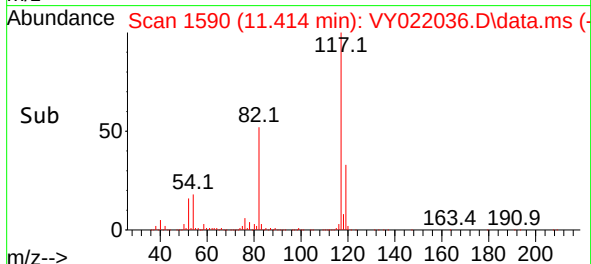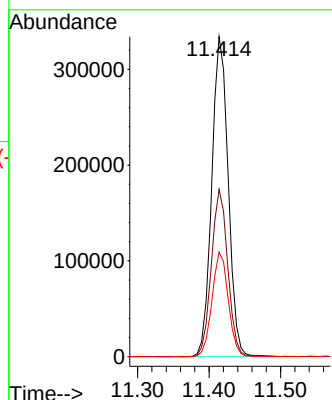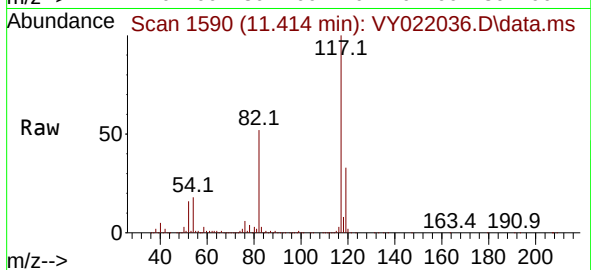

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY022036.D

Acq: 28 Apr 2025 17:02

Tgt Ion:152 Resp: 222901

Ion Ratio Lower Upper

152 100

115 57.1 28.0 84.0

150 157.1 0.0 345.6

