
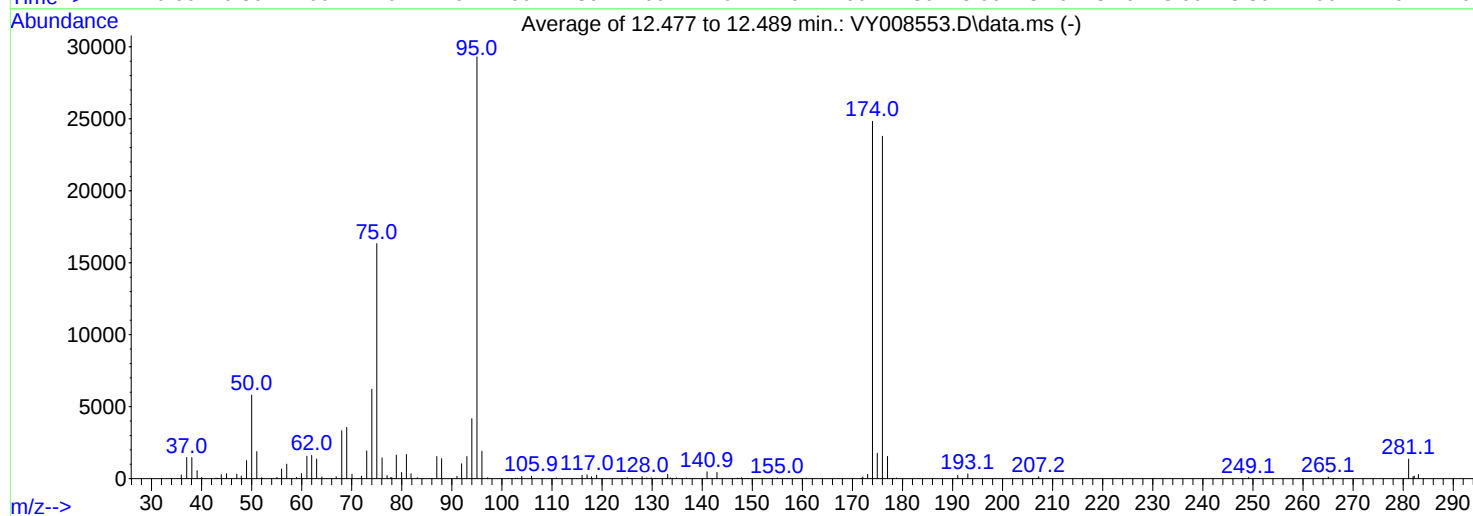


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042922\
 Data File : VY008553.D
 Acq On : 29 Apr 2022 08:42
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042122S.M
 Title : SW846 8260
 Last Update : Thu Apr 21 14:28:40 2022

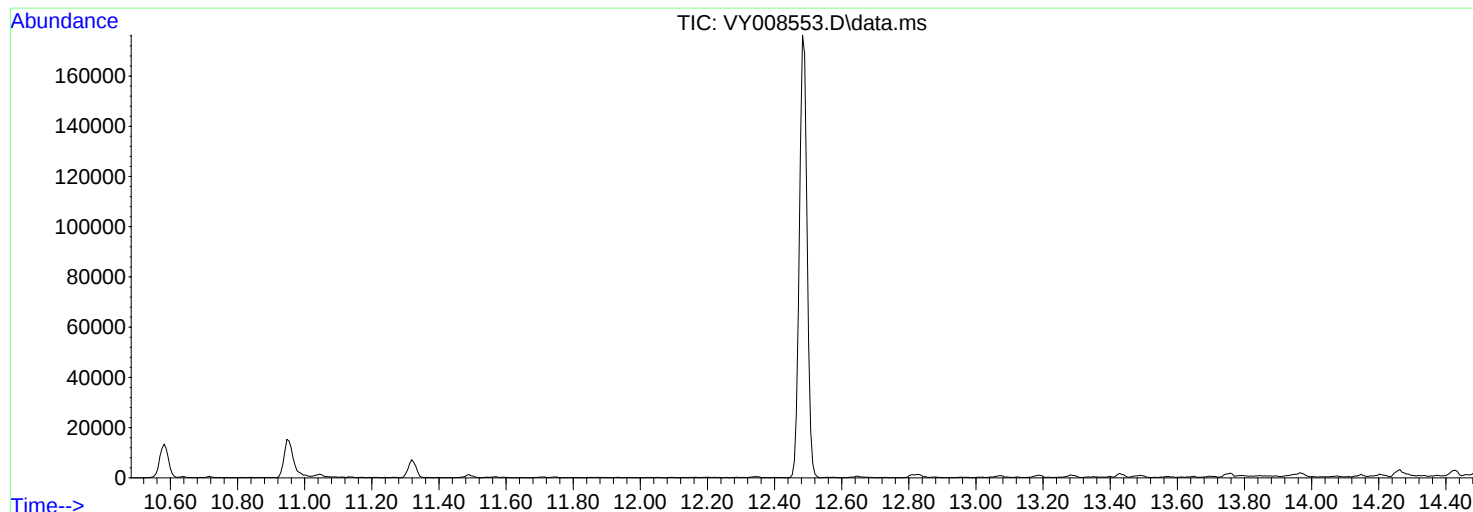

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	5805	PASS
75	95	30	60	55.7	16335	PASS
95	95	100	100	100.0	29304	PASS
96	95	5	9	6.5	1909	PASS
173	174	0.00	2	1.2	296	PASS
174	95	50	100	84.7	24824	PASS
175	174	5	9	7.1	1772	PASS
176	174	95	101	95.8	23784	PASS
177	176	5	9	6.5	1541	PASS