

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042925\
 Data File : VY022059.D
 Acq On : 29 Apr 2025 16:16
 Operator : SY/MD
 Sample : Q1906-15
 Misc : 5.65g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-7-VOC

Quant Time: Apr 30 01:34:52 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	300823	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	578128	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	513103	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	189515	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	149720	53.882	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 107.760%	
35) Dibromofluoromethane	7.634	113	195097	51.080	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 102.160%	
50) Toluene-d8	10.109	98	693883	48.189	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 96.380%	
62) 4-Bromofluorobenzene	12.407	95	190233	39.245	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 78.480%	
Target Compounds						
					Qvalue	
16) Acetone	3.878	43	310	Below Cal	#	78
31) Cyclohexane	7.707	56	5390	1.173	ug/l #	20
36) 1,1-Dichloropropene	7.707	75	22402	4.366	ug/l #	48
38) Carbon Tetrachloride	7.707	117	30003	4.894	ug/l #	16
51) 4-Methyl-2-Pentanone	10.103	43	2279	1.229	ug/l #	1
76) 1,2,3-Trichloropropane	12.407	75	90854	55.969	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.407	75	90854	134.782	ug/l #	16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 30 01:34:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration







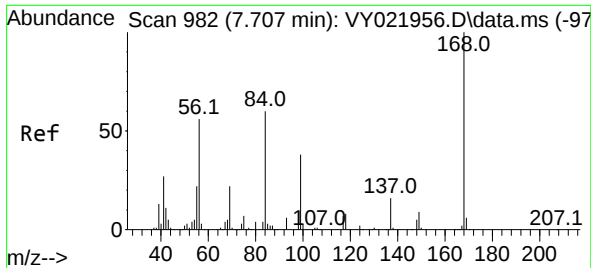

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY022059.D
Acq: 29 Apr 2025 16:16




Instrument :
MSVOA_Y
ClientSampleId :
WC-7-VOC


Tgt Ion:168 Resp: 300823
Ion Ratio Lower Upper
168 100
99 53.9 43.1 64.7

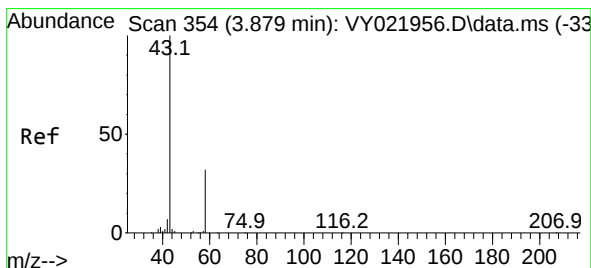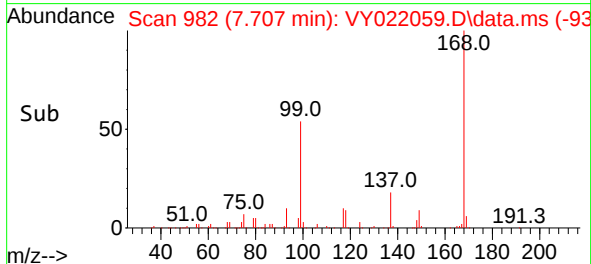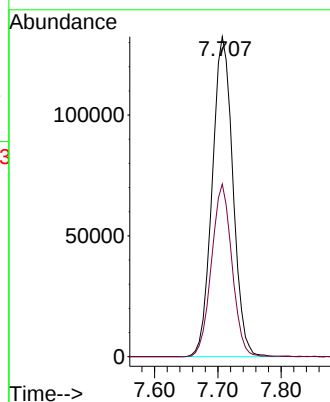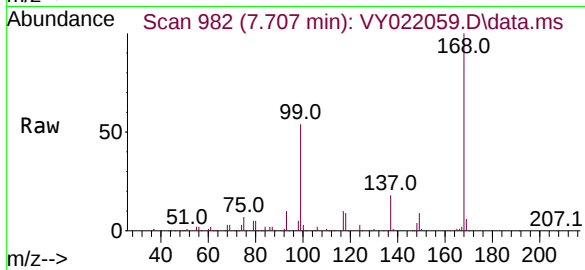

#16
Acetone
Concen: Below Cal
RT: 3.878 min Scan# 354
Delta R.T. -0.001 min
Lab File: VY022059.D
Acq: 29 Apr 2025 16:16

Tgt Ion: 43 Resp: 310
Ion Ratio Lower Upper
43 100
58 46.2 27.0 40.4#


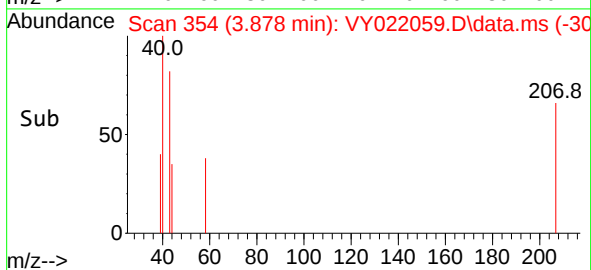
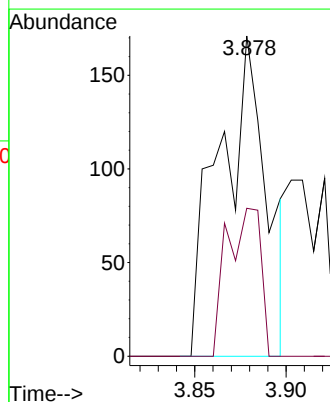
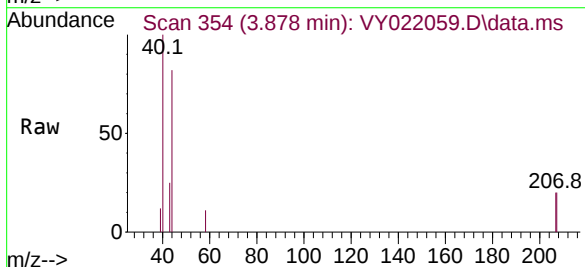


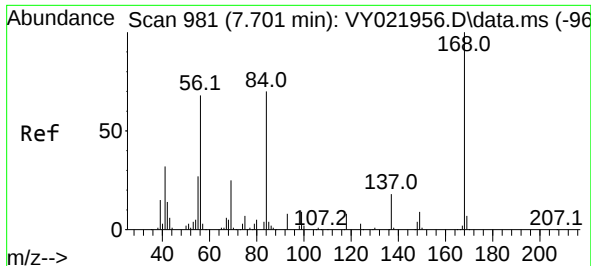

#31
Cyclohexane
Concen: 1.173 ug/l
RT: 7.707 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY022059.D
Acq: 29 Apr 2025 16:16




Instrument :
MSVOA_Y
ClientSampleId :
WC-7-VOC


Tgt Ion: 56 Resp: 5390
Ion Ratio Lower Upper
56 100
69 178.8 29.4 44.2#
84 125.8 82.2 123.4#

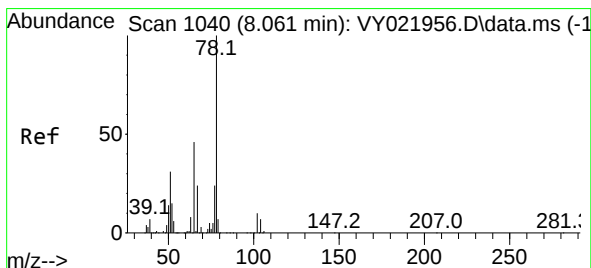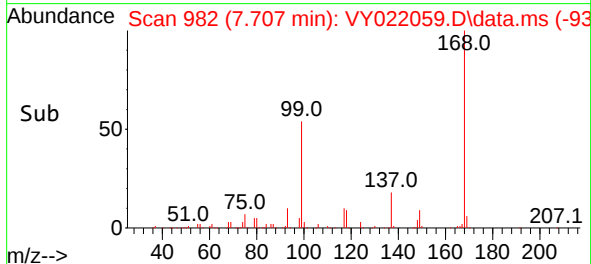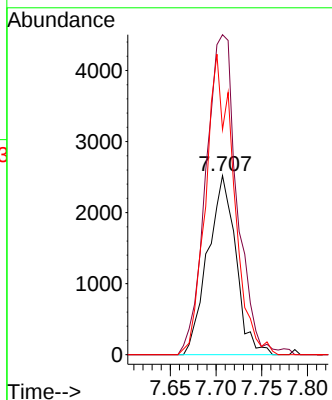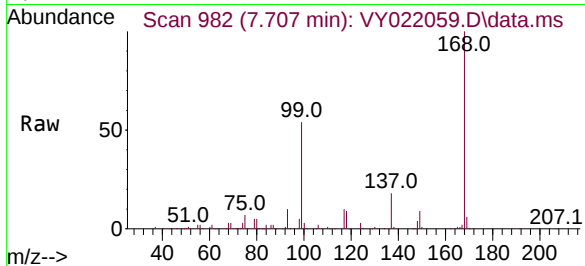

#33
1,2-Dichloroethane-d4
Concen: 53.882 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY022059.D
Acq: 29 Apr 2025 16:16

Tgt Ion: 65 Resp: 149720
Ion Ratio Lower Upper
65 100
67 53.7 0.0 105.8


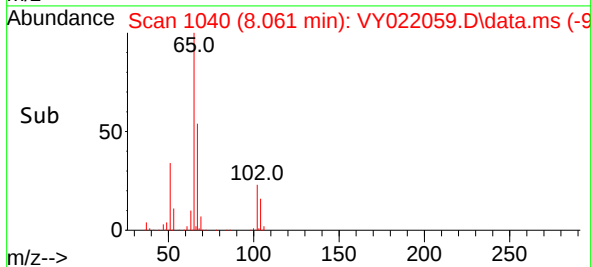
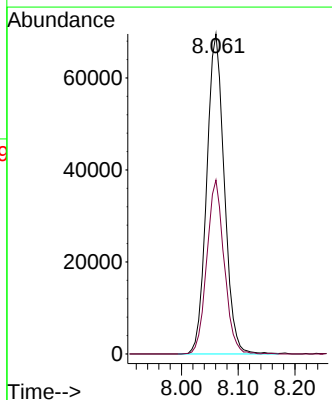
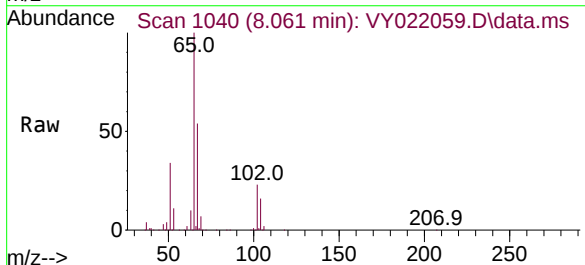


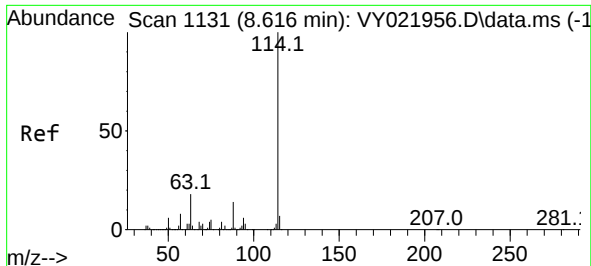

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.615 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VY022059.D
Acq: 29 Apr 2025 16:16




Instrument :
MSVOA_Y
ClientSampleId :
WC-7-VOC


Tgt Ion:114 Resp: 578128
Ion Ratio Lower Upper
114 100
63 17.0 0.0 35.4
88 14.1 0.0 28.2

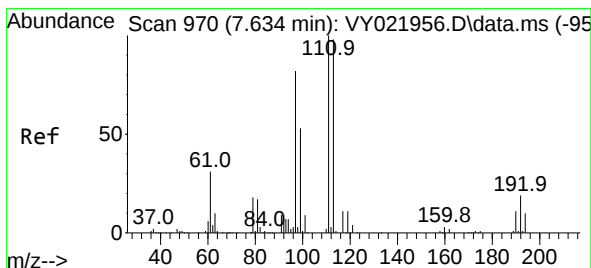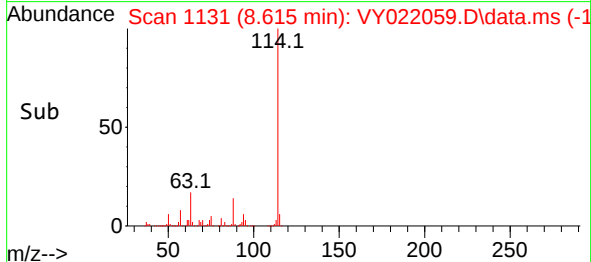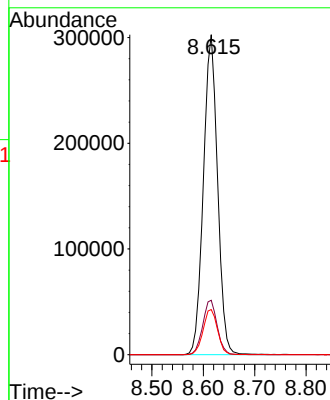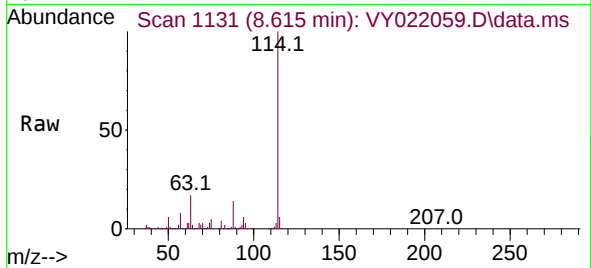

#35
Dibromofluoromethane
Concen: 51.080 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.000 min
Lab File: VY022059.D
Acq: 29 Apr 2025 16:16

Tgt Ion:113 Resp: 195097
Ion Ratio Lower Upper
113 100
111 100.2 81.8 122.8
192 19.5 15.6 23.4


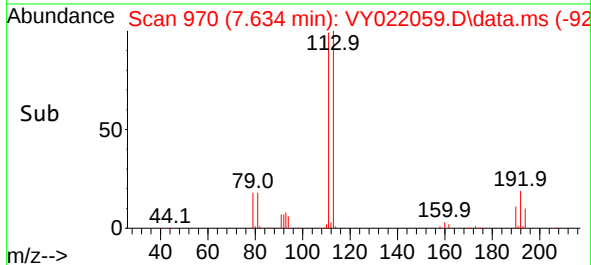
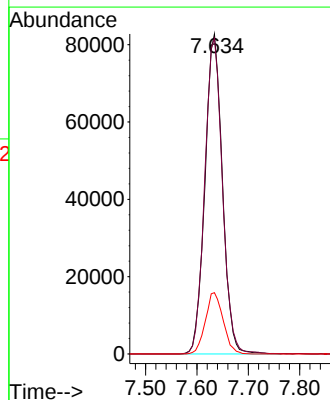
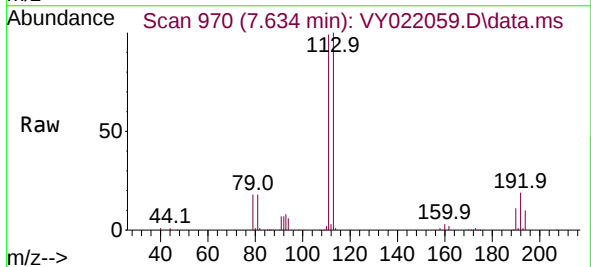


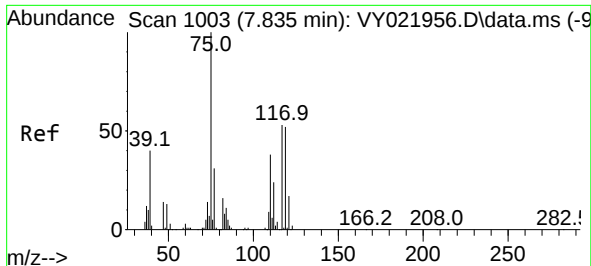

#36
 1,1-Dichloropropene
 Concen: 4.366 ug/l
 RT: 7.707 min Scan# 982
 Delta R.T. -0.128 min
 Lab File: VY022059.D
 Acq: 29 Apr 2025 16:16




Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-7-VOC


Tgt Ion: 75 Resp: 22402
 Ion Ratio Lower Upper
 75 100
 110 9.5 19.1 57.3#
 77 0.0 25.5 38.3#

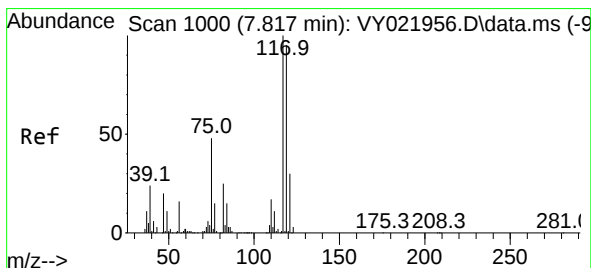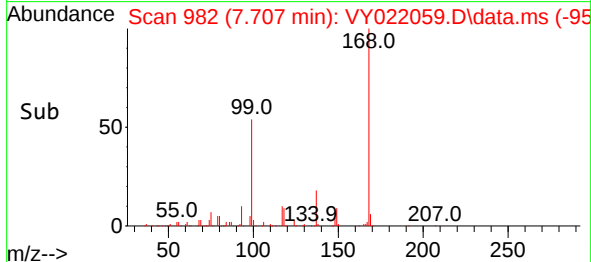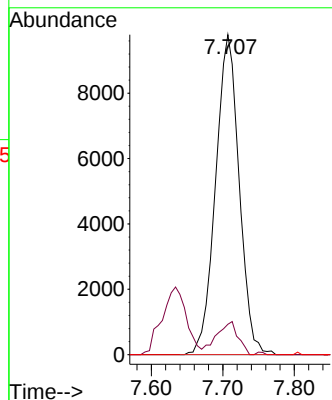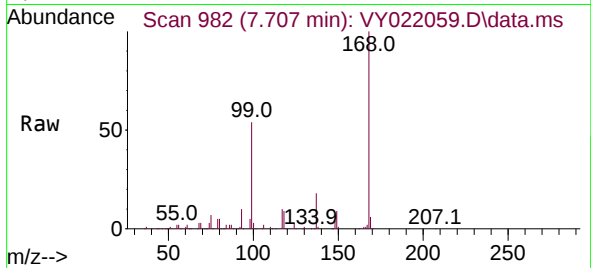

#38
 Carbon Tetrachloride
 Concen: 4.894 ug/l
 RT: 7.707 min Scan# 982
 Delta R.T. -0.110 min
 Lab File: VY022059.D
 Acq: 29 Apr 2025 16:16

Tgt Ion: 117 Resp: 30003
 Ion Ratio Lower Upper
 117 100
 119 5.0 76.2 114.4#
 121 0.0 24.0 36.0#


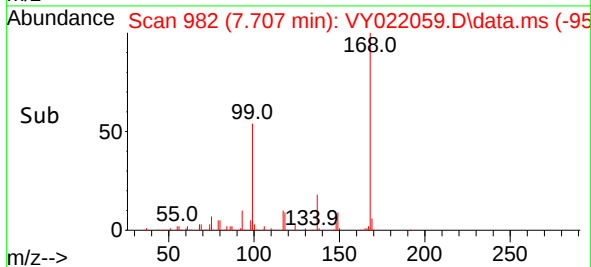
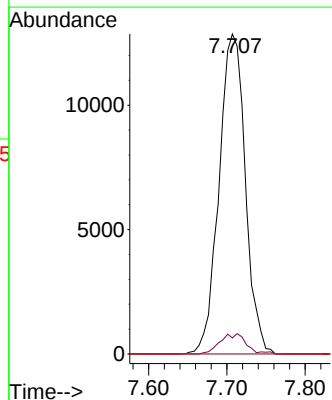
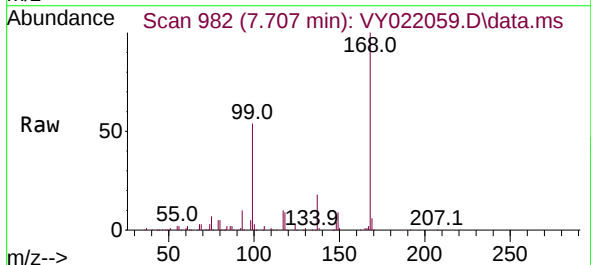


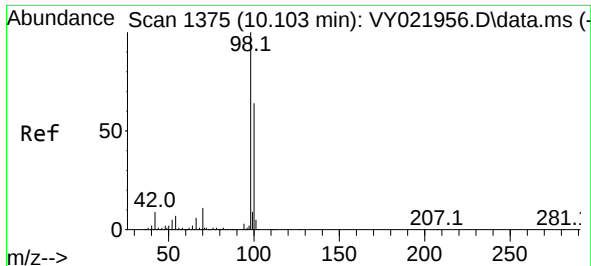

#50
Toluene-d8
Concen: 48.189 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY022059.D
Acq: 29 Apr 2025 16:16




Instrument :
MSVOA_Y
ClientSampleId :
WC-7-VOC


Tgt Ion: 98 Resp: 693883
Ion Ratio Lower Upper
98 100
100 63.9 51.6 77.4

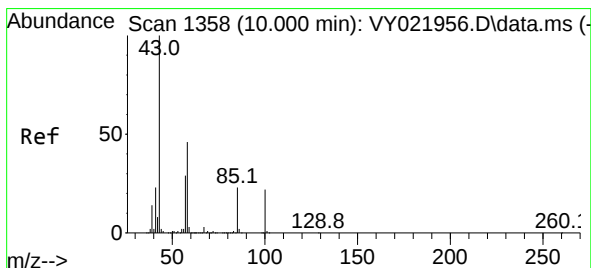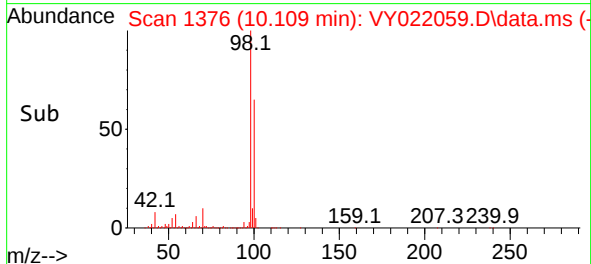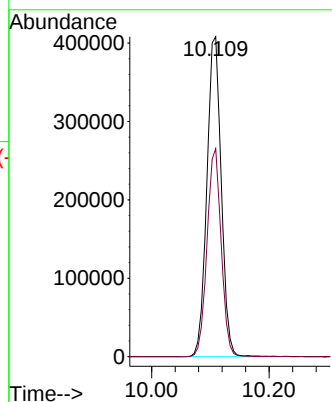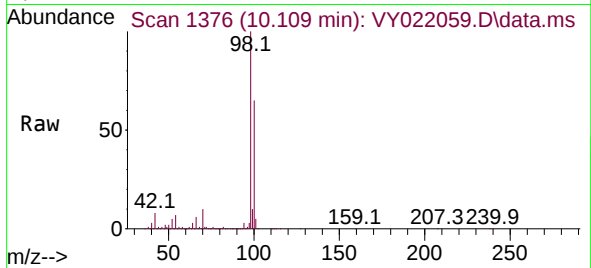

#51
4-Methyl-2-Pentanone
Concen: 1.229 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. 0.103 min
Lab File: VY022059.D
Acq: 29 Apr 2025 16:16

Tgt Ion: 43 Resp: 2279
Ion Ratio Lower Upper
43 100
58 212.4 36.6 55.0#


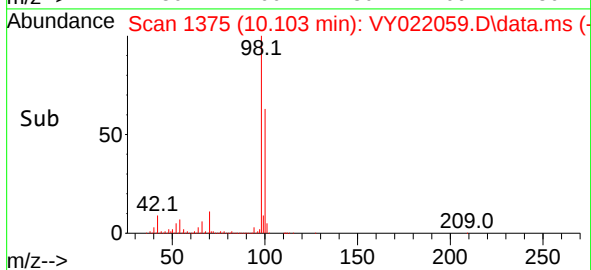
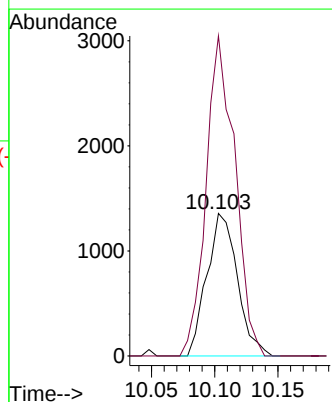
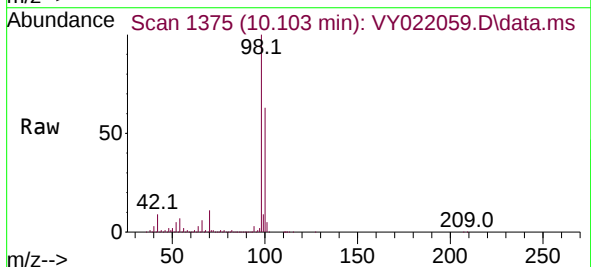


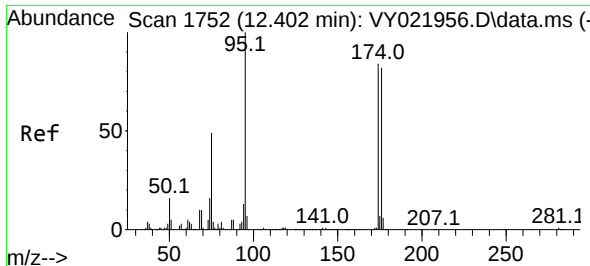

#62
4-Bromofluorobenzene
Concen: 39.245 ug/l
RT: 12.407 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY022059.D
Acq: 29 Apr 2025 16:16




Instrument :
MSVOA_Y
ClientSampleId :
WC-7-VOC


Tgt Ion: 95 Resp: 190233
Ion Ratio Lower Upper
95 100
174 88.8 0.0 179.0
176 84.9 0.0 171.8

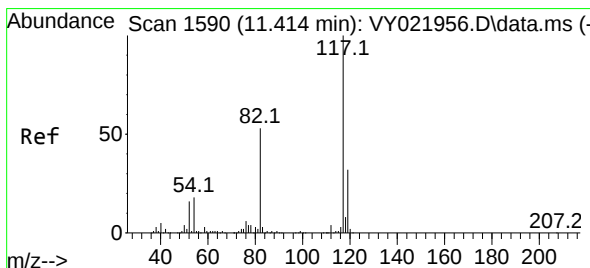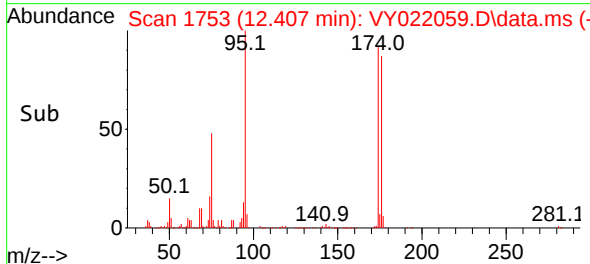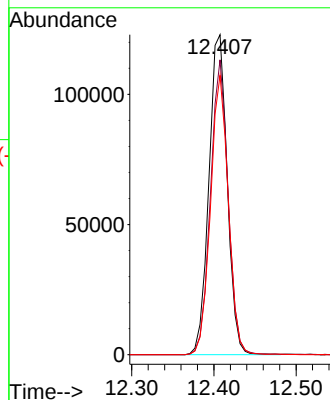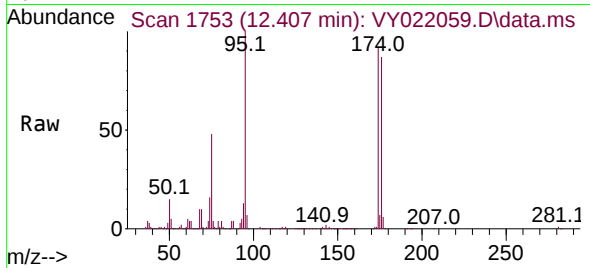

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 1590
Delta R.T. -0.000 min
Lab File: VY022059.D
Acq: 29 Apr 2025 16:16

Tgt Ion: 117 Resp: 513103
Ion Ratio Lower Upper
117 100
82 52.9 42.1 63.1
119 31.8 25.7 38.5


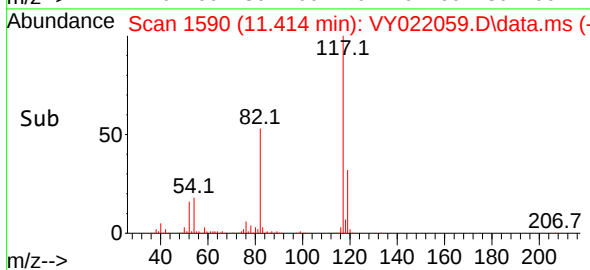
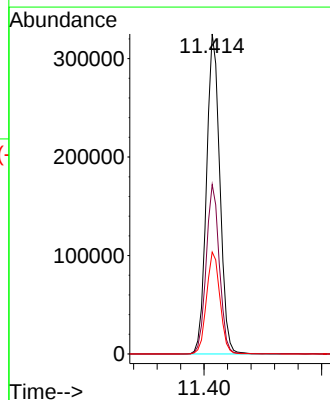
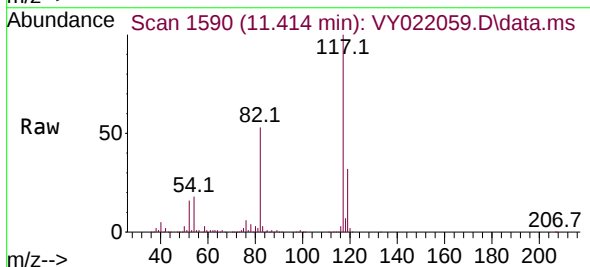


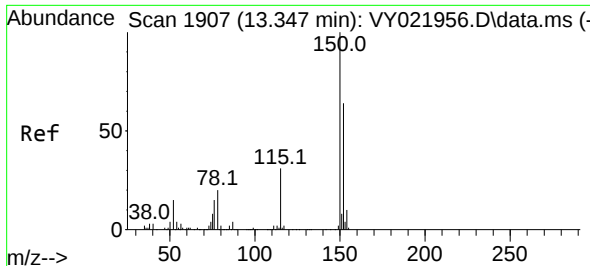

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 1907
 Delta R.T. -0.000 min
 Lab File: VY022059.D
 Acq: 29 Apr 2025 16:16




Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-7-VOC


Tgt Ion:152 Resp: 189515
 Ion Ratio Lower Upper
 152 100
 115 56.3 28.0 84.0
 150 157.1 0.0 345.6

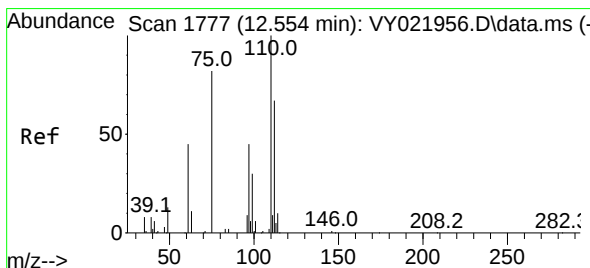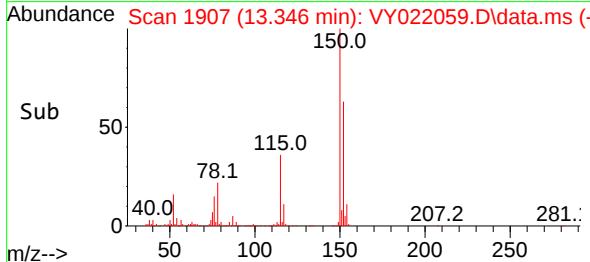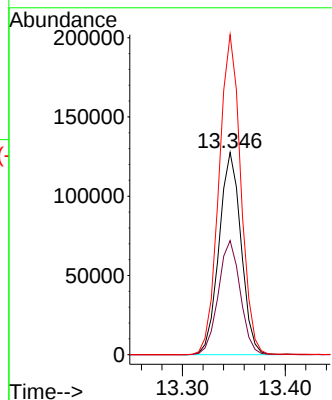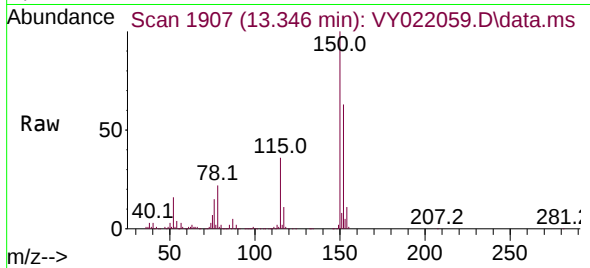

#76
 1,2,3-Trichloropropane
 Concen: 55.969 ug/l
 RT: 12.407 min Scan# 1753
 Delta R.T. -0.147 min
 Lab File: VY022059.D
 Acq: 29 Apr 2025 16:16

Tgt Ion: 75 Resp: 90854
 Ion Ratio Lower Upper
 75 100
 77 1.3 0.0 0.0#

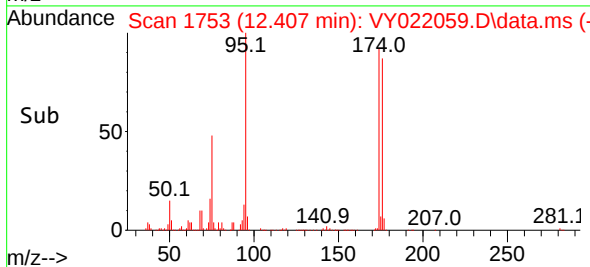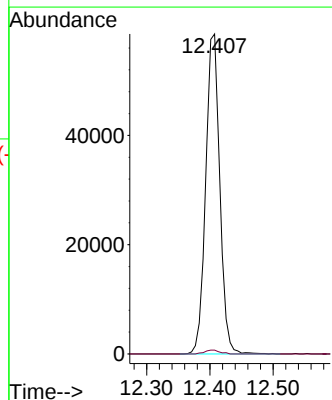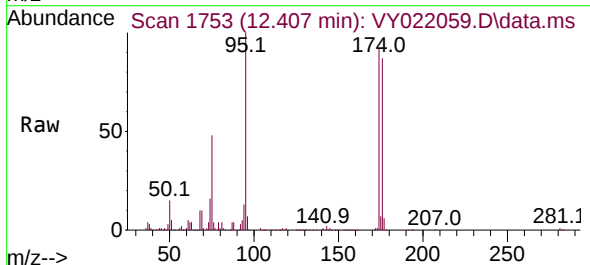

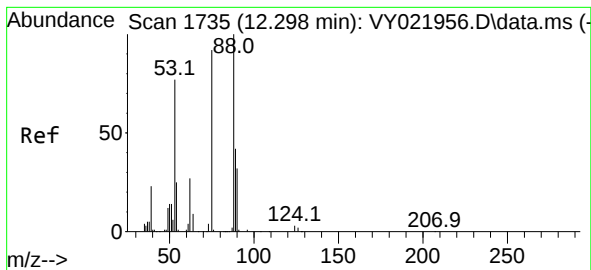

#81
 trans-1,4-Dichloro-2-butene
 Concen: 134.782 ug/l
 RT: 12.407 min Scan# 11
 Delta R.T. 0.109 min
 Lab File: VY022059.D
 Acq: 29 Apr 2025 16:16

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-7-VOC

Tgt Ion: 75 Resp: 90854
 Ion Ratio Lower Upper
 75 100
 53 0.2 66.0 99.0#
 89 0.1 37.2 55.8#

