

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042925\
 Data File : VY022057.D
 Acq On : 29 Apr 2025 15:30
 Operator : SY/MD
 Sample : Q1906-07
 Misc : 5.52g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-5-VOC

Quant Time: Apr 30 01:34:31 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	303348	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	573841	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	507934	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	188168	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	140874	50.277	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	100.560%
35) Dibromofluoromethane	7.634	113	189330	49.941	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.880%
50) Toluene-d8	10.109	98	685875	47.989	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	95.980%
62) 4-Bromofluorobenzene	12.408	95	183842	38.210	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	76.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042925\
Data File : VY022057.D
Acq On : 29 Apr 2025 15:30
Operator : SY/MD
Sample : Q1906-07
Misc : 5.52g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-5-VOC

Quant Time: Apr 30 01:34:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration



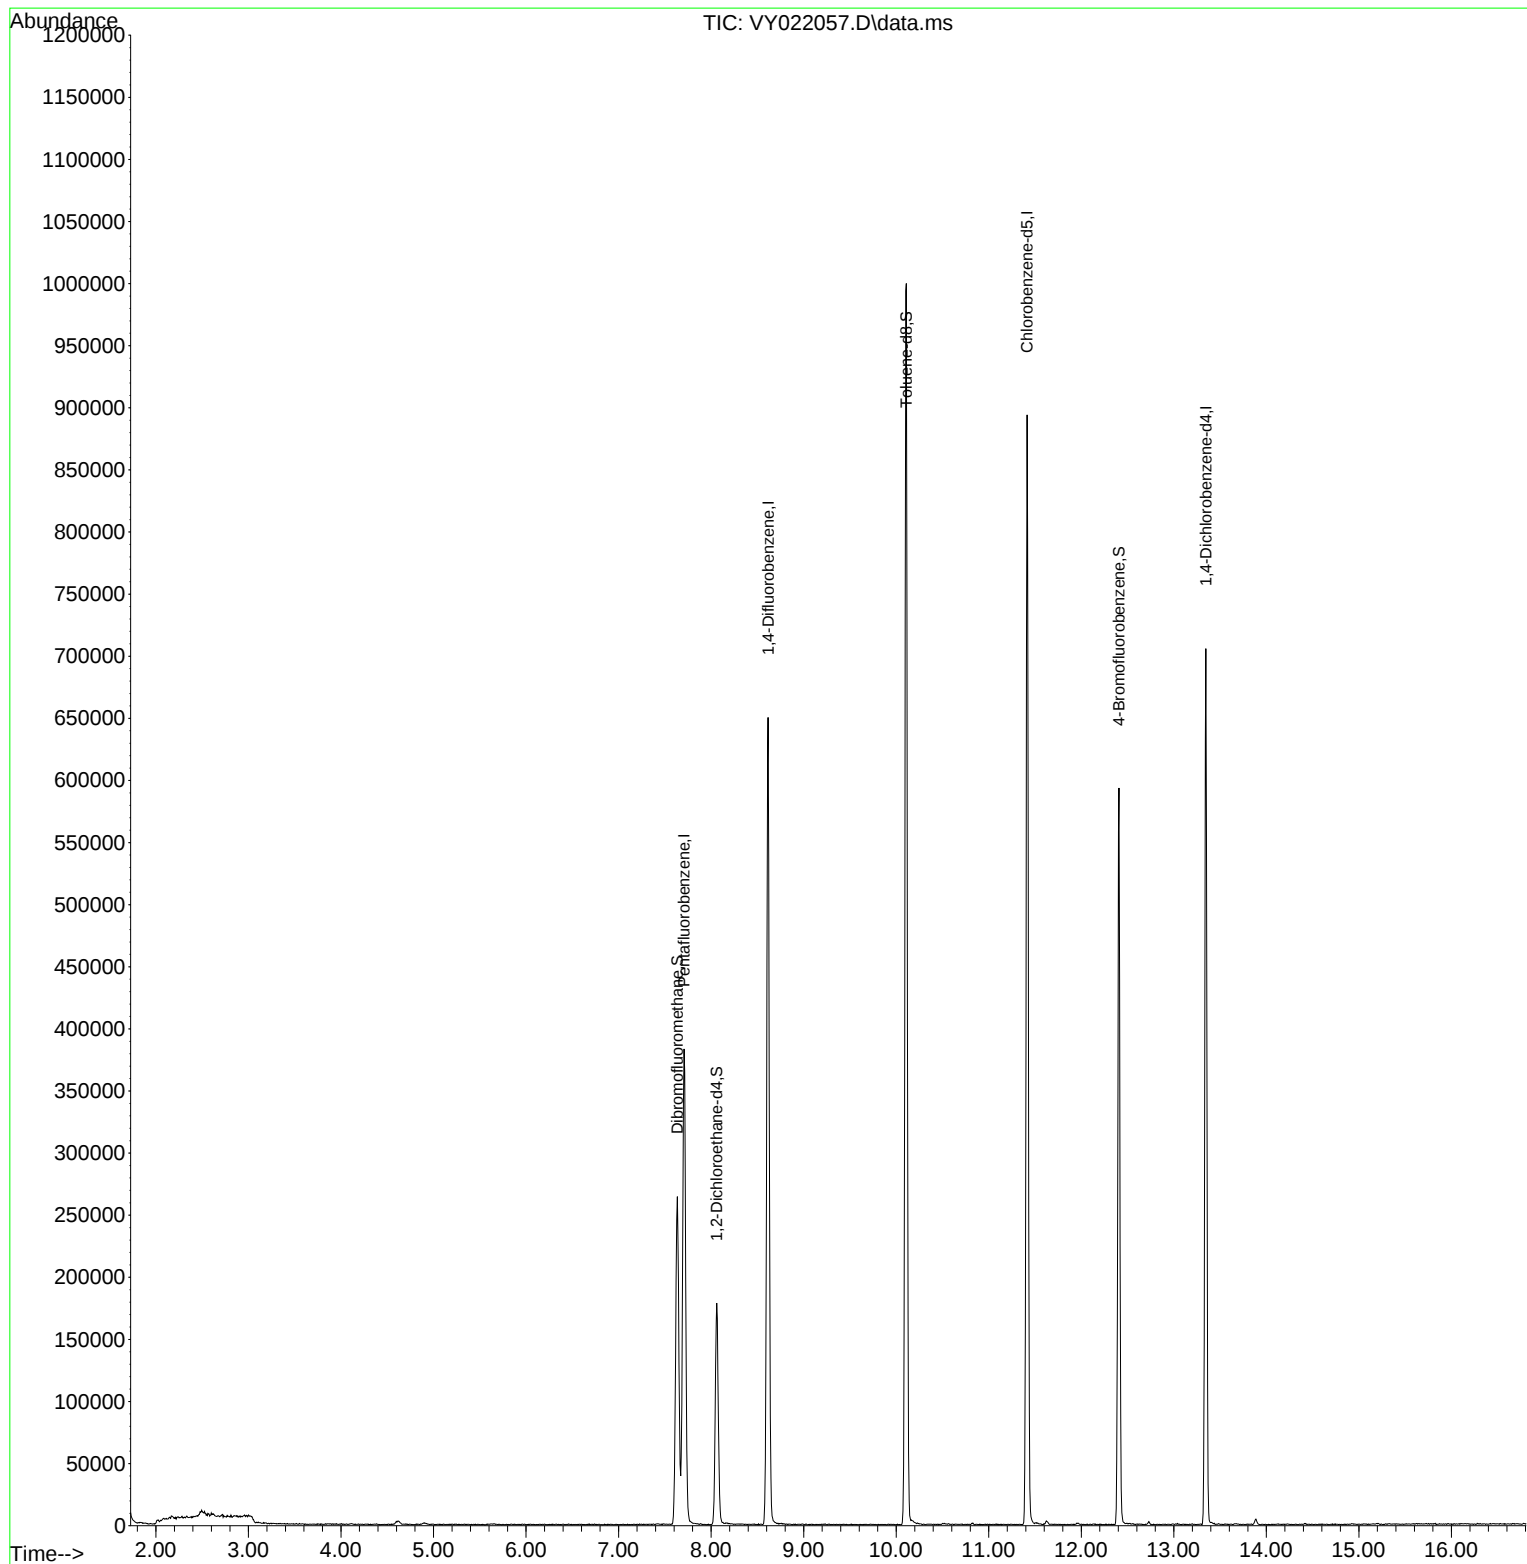


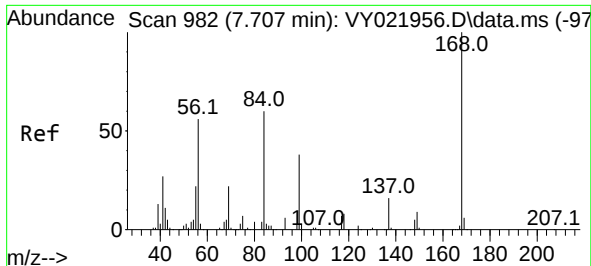

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY022057.D
Acq: 29 Apr 2025 15:30




Instrument :
MSVOA_Y
ClientSampleId :
WC-5-VOC

Tgt Ion:168 Resp: 303348
Ion Ratio Lower Upper
168 100
99 53.8 43.1 64.7

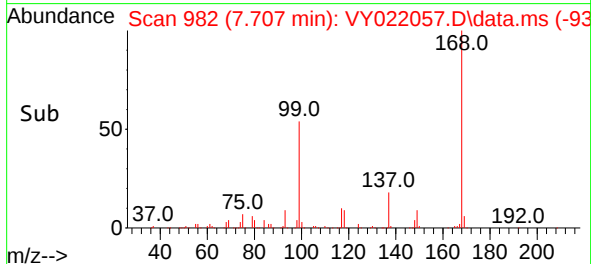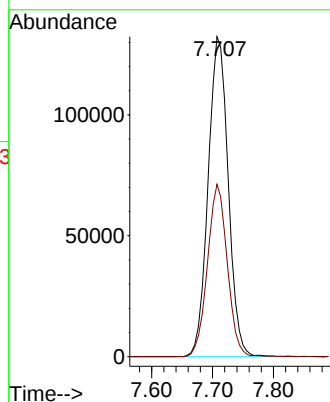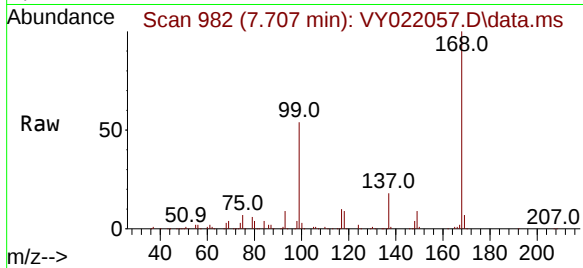

#33
1,2-Dichloroethane-d4
Concen: 50.277 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY022057.D
Acq: 29 Apr 2025 15:30

Tgt Ion: 65 Resp: 140874
Ion Ratio Lower Upper
65 100
67 53.4 0.0 105.8


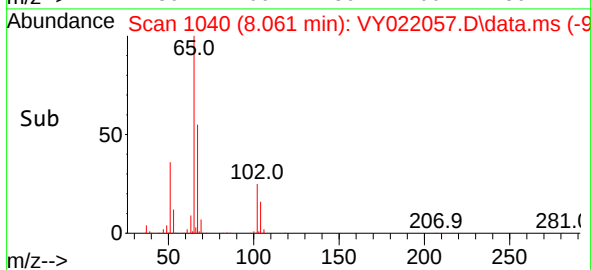
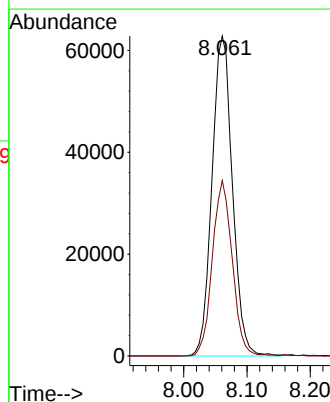
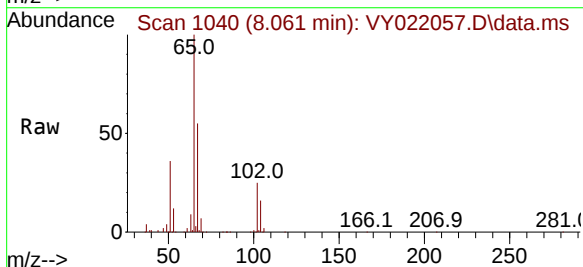




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY022057.D
Acq: 29 Apr 2025 15:30




Instrument :
MSVOA_Y
ClientSampleId :
WC-5-VOC

Tgt Ion:114 Resp: 573841
Ion Ratio Lower Upper
114 100
63 17.3 0.0 35.4
88 14.4 0.0 28.2

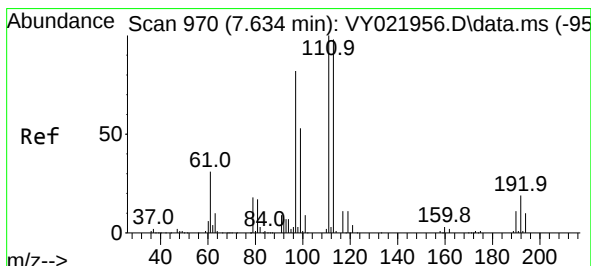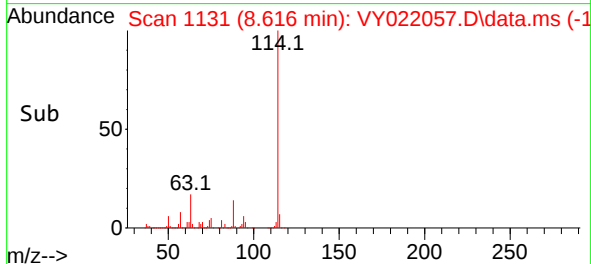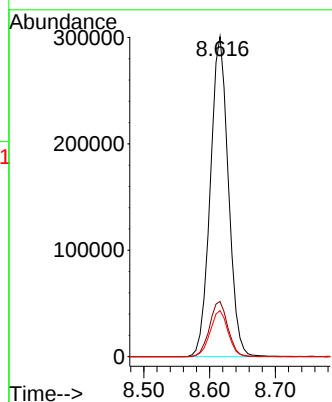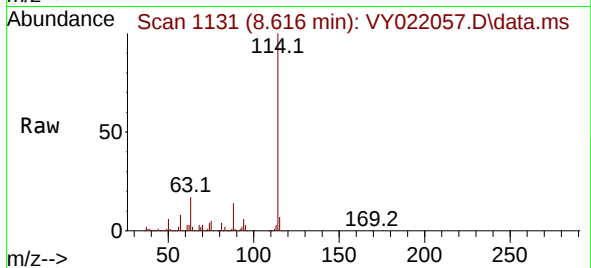

#35
Dibromofluoromethane
Concen: 49.941 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY022057.D
Acq: 29 Apr 2025 15:30

Tgt Ion:113 Resp: 189330
Ion Ratio Lower Upper
113 100
111 102.6 81.8 122.8
192 20.4 15.6 23.4

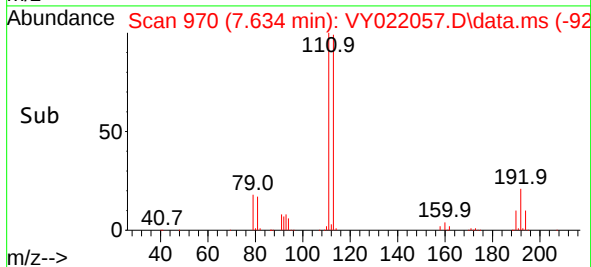
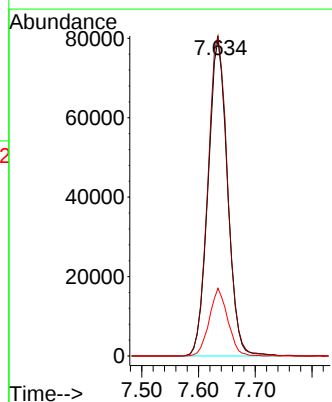
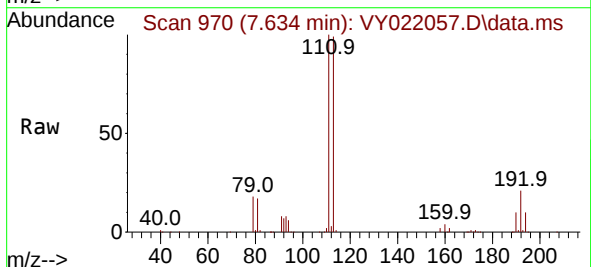




#50
Toluene-d8
Concen: 47.989 ug/l
RT: 10.109 min Scan# 1375
Delta R.T. 0.006 min
Lab File: VY022057.D
Acq: 29 Apr 2025 15:30




Instrument :
MSVOA_Y
ClientSampleId :
WC-5-VOC


Tgt Ion: 98 Resp: 685875
Ion Ratio Lower Upper
98 100
100 64.3 51.6 77.4

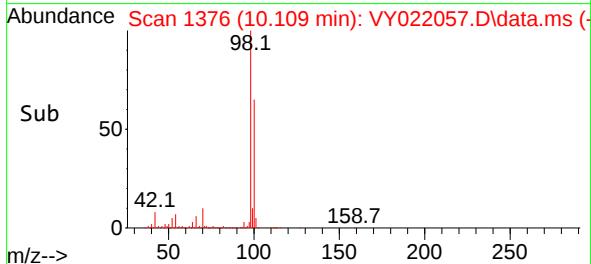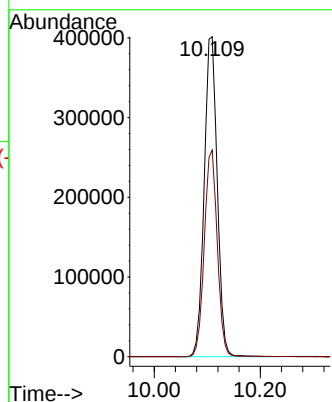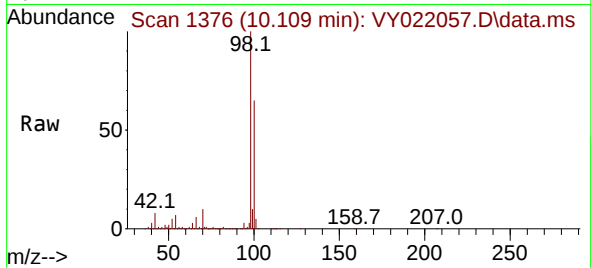

#62
4-Bromofluorobenzene
Concen: 38.210 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY022057.D
Acq: 29 Apr 2025 15:30

Tgt Ion: 95 Resp: 183842
Ion Ratio Lower Upper
95 100
174 89.9 0.0 179.0
176 85.7 0.0 171.8

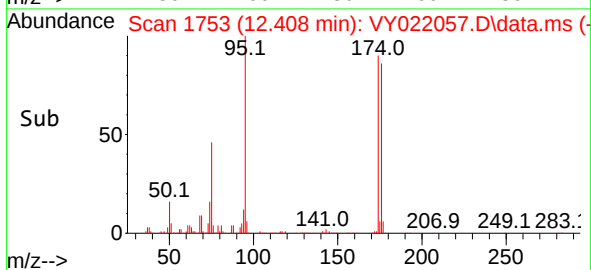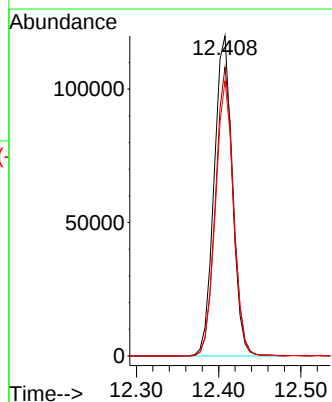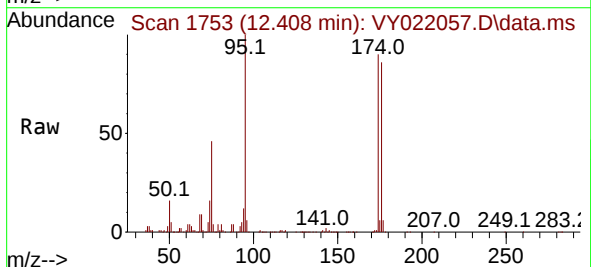

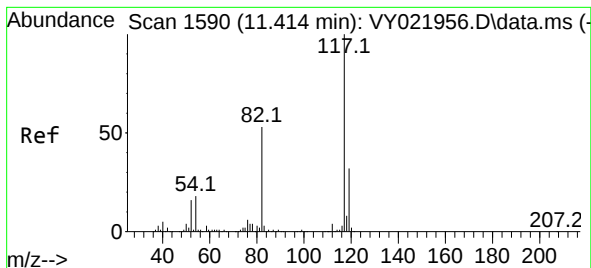

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY022057.D

Acq: 29 Apr 2025 15:30

Instrument :

MSVOA_Y

ClientSampleId :

WC-5-VOC





Tgt Ion:117 Resp: 507934

Ion Ratio Lower Upper

117 100

82 51.3 42.1 63.1

119 32.4 25.7 38.5

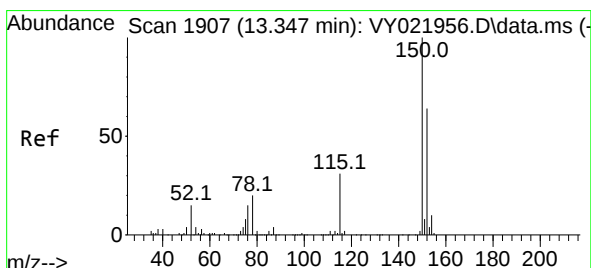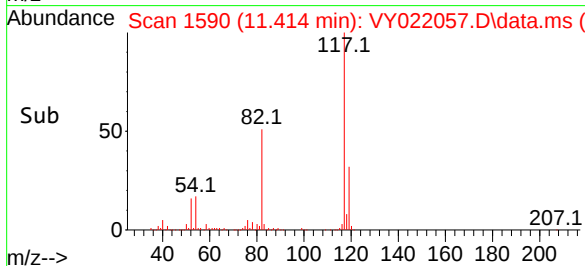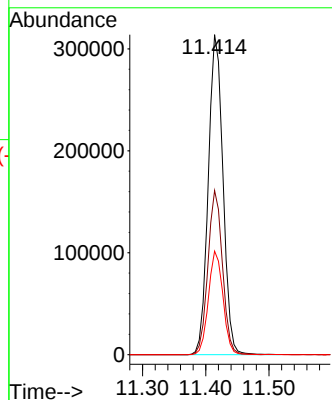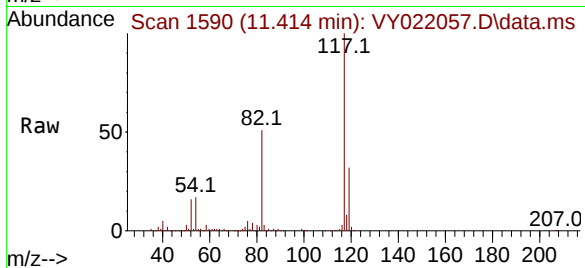

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY022057.D

Acq: 29 Apr 2025 15:30

Tgt Ion:152 Resp: 188168

Ion Ratio Lower Upper

152 100

115 55.6 28.0 84.0

150 155.7 0.0 345.6

