
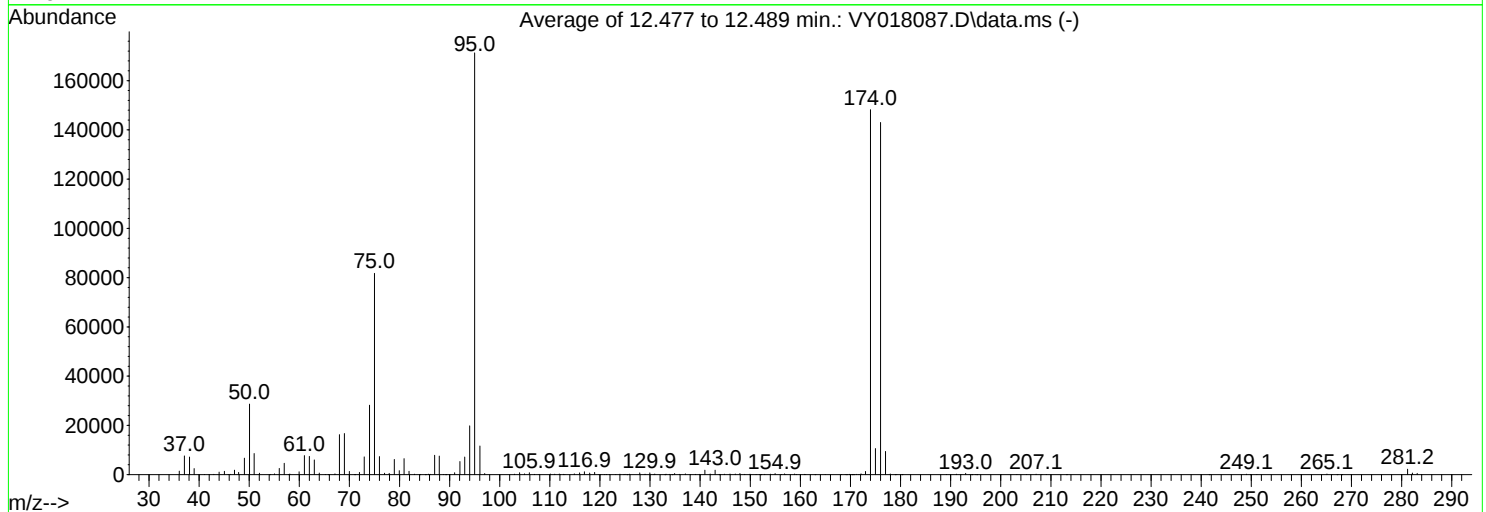


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050124\
Data File : VY018087.D
Acq On : 01 May 2024 08:28
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050124S.M
Title : SW846 8260
Last Update : Wed May 01 16:21:20 2024

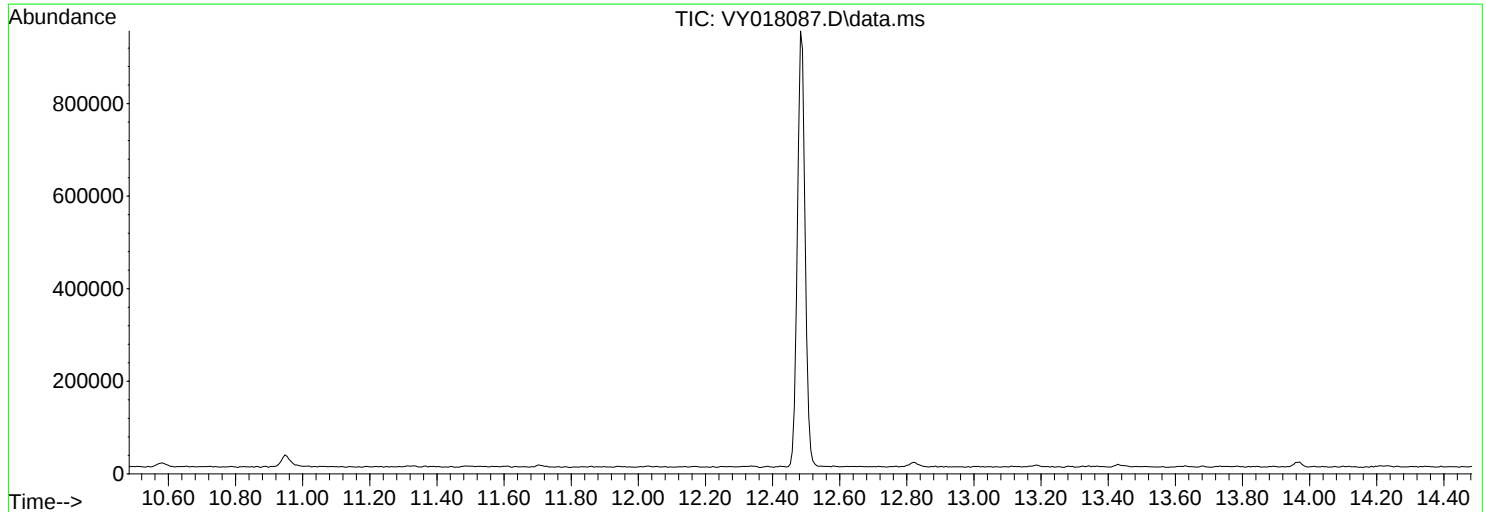

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	28659	PASS
75	95	30	60	47.7	81765	PASS
95	95	100	100	100.0	171295	PASS
96	95	5	9	6.8	11646	PASS
173	174	0.00	2	0.9	1307	PASS
174	95	50	100	86.5	148219	PASS
175	174	5	9	7.2	10616	PASS
176	174	95	101	96.5	143051	PASS
177	176	5	9	6.6	9405	PASS