

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050125\
 Data File : VY022101.D
 Acq On : 01 May 2025 12:41
 Operator : SY/MD
 Sample : Q1916-03
 Misc : 6.04g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-12-VOC

Quant Time: May 02 01:29:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	310146	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	581141	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	521540	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	198625	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	144212	50.340	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	100.680%
35) Dibromofluoromethane	7.634	113	196023	51.057	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.120%
50) Toluene-d8	10.109	98	693134	47.887	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	95.780%
62) 4-Bromofluorobenzene	12.408	95	191657	39.333	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	78.660%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050125\
Data File : VY022101.D
Acq On : 01 May 2025 12:41
Operator : SY/MD
Sample : Q1916-03
Misc : 6.04g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-12-VOC

Quant Time: May 02 01:29:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration




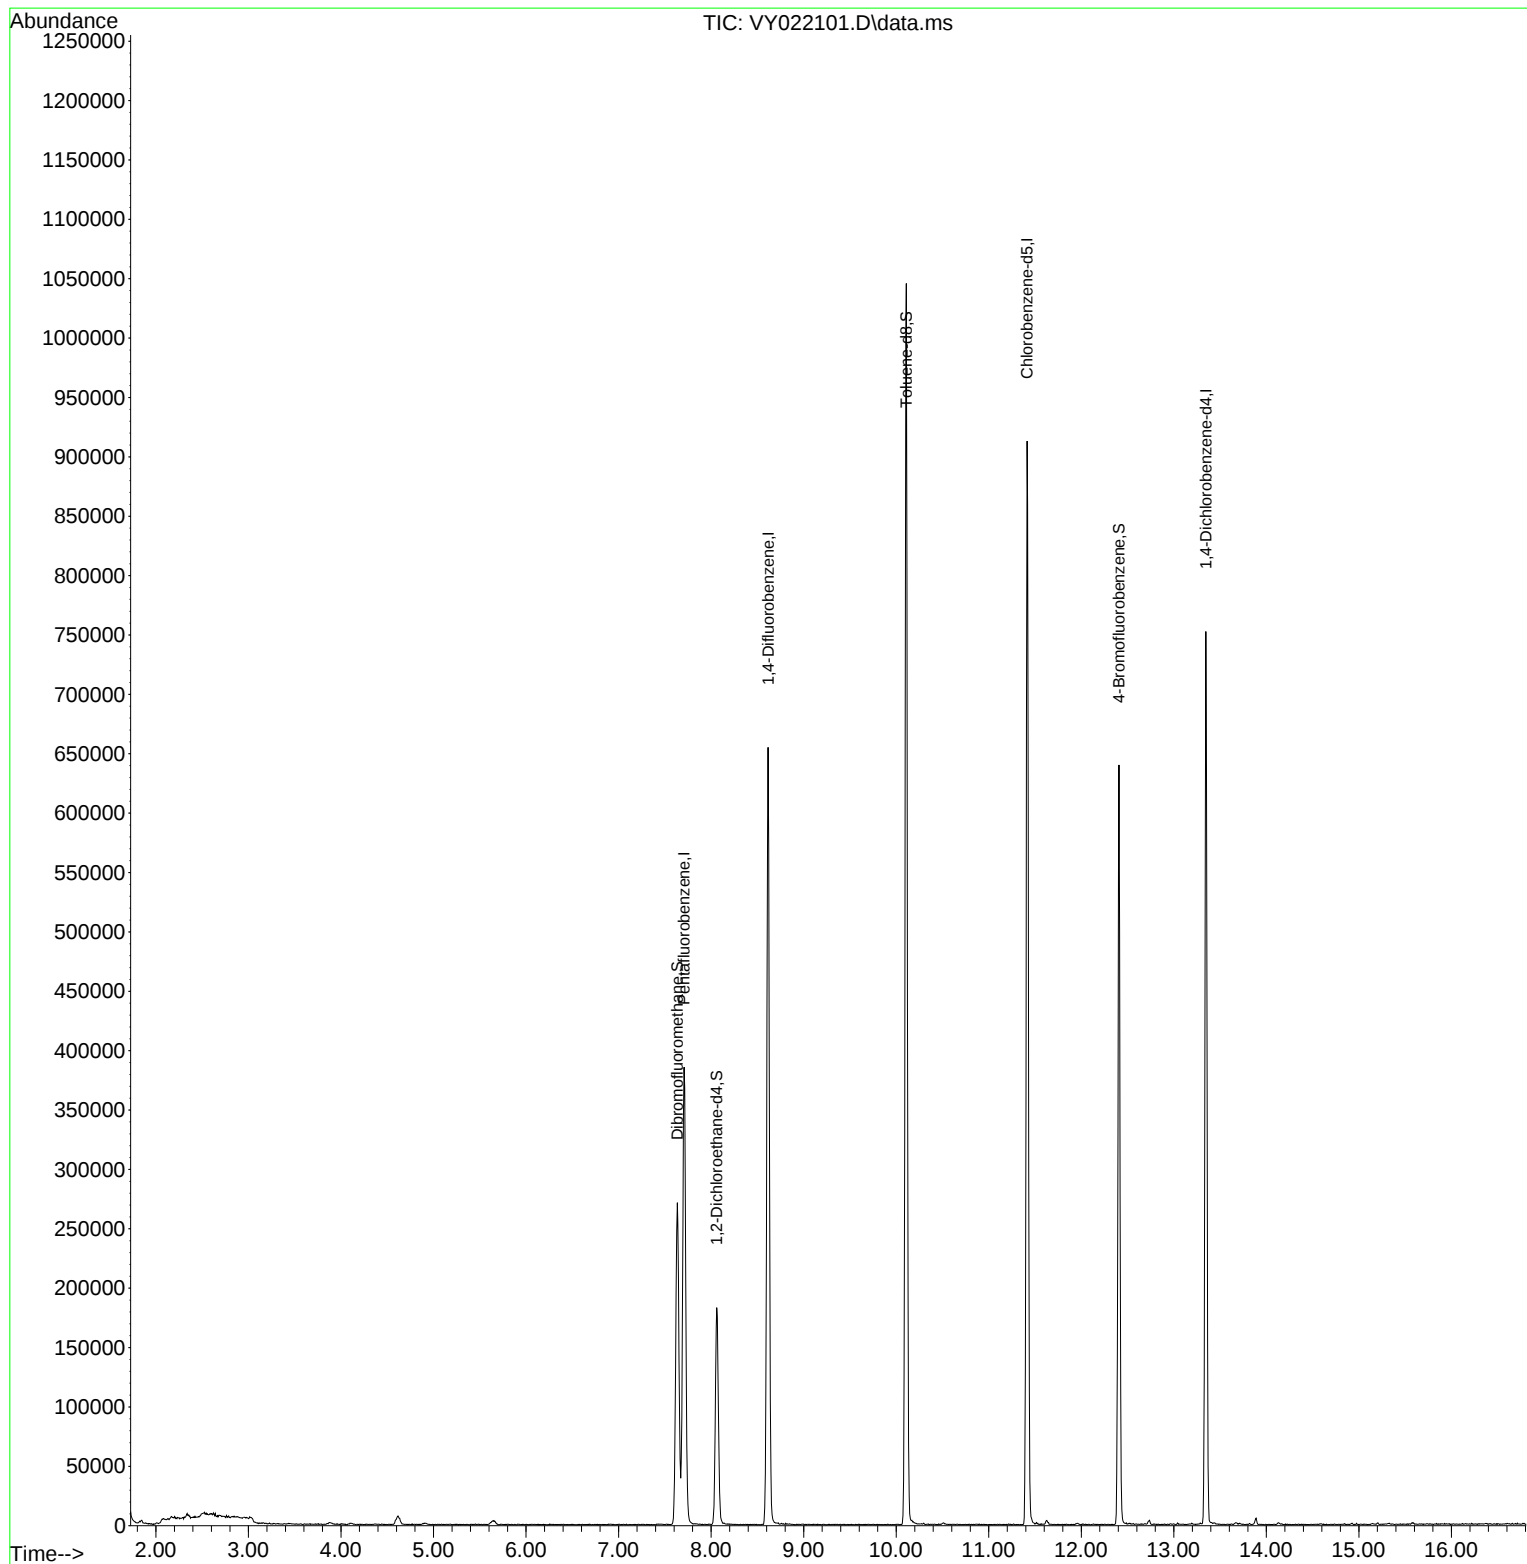


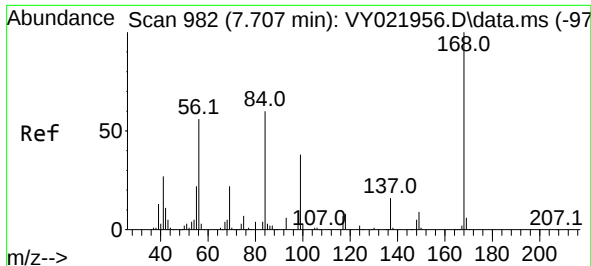

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY022101.D
Acq: 01 May 2025 12:41




Instrument :
MSVOA_Y
ClientSampleId :
WC-12-VOC


Tgt Ion:168 Resp: 310146
Ion Ratio Lower Upper
168 100
99 50.6 43.1 64.7

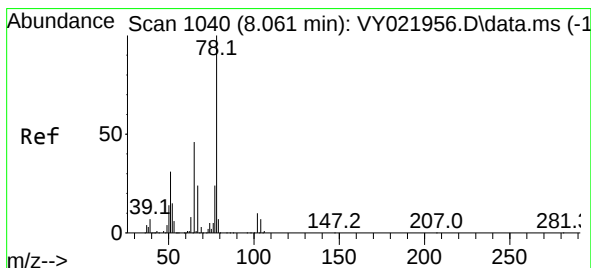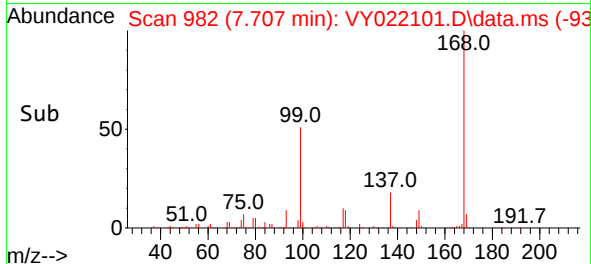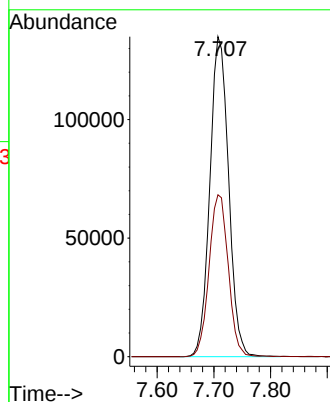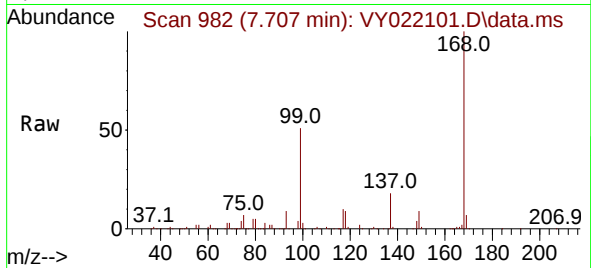

#33
1,2-Dichloroethane-d4
Concen: 50.340 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY022101.D
Acq: 01 May 2025 12:41

Tgt Ion: 65 Resp: 144212
Ion Ratio Lower Upper
65 100
67 54.4 0.0 105.8

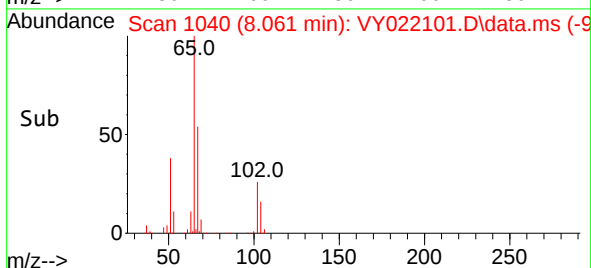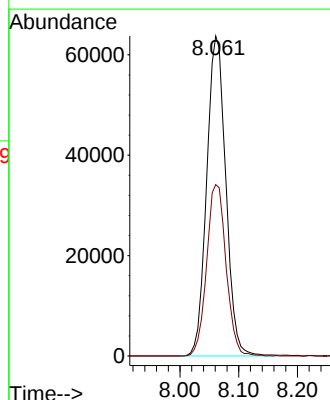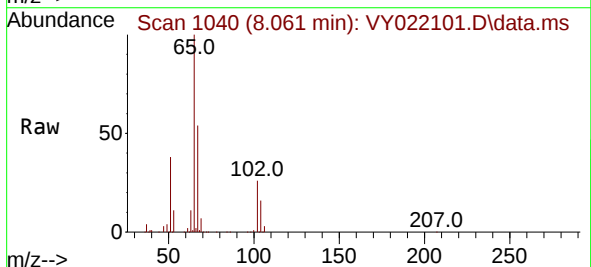

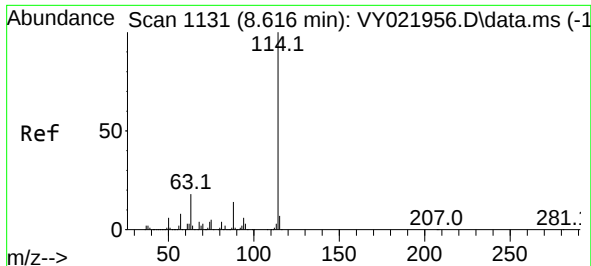

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VY022101.D

Acq: 01 May 2025 12:41

Instrument :

MSVOA_Y

ClientSampleId :

WC-12-VOC





Tgt Ion:114 Resp: 581141

Ion Ratio Lower Upper

114 100

63 17.4 0.0 35.4

88 15.0 0.0 28.2

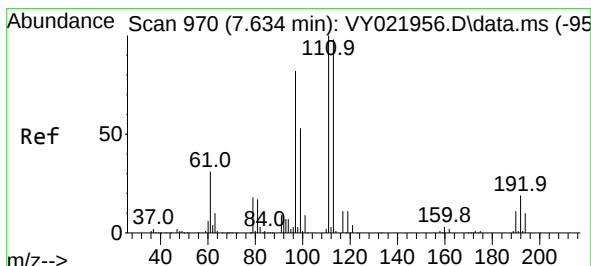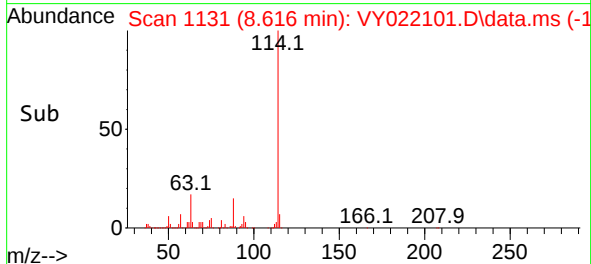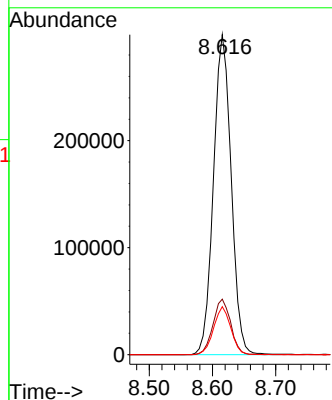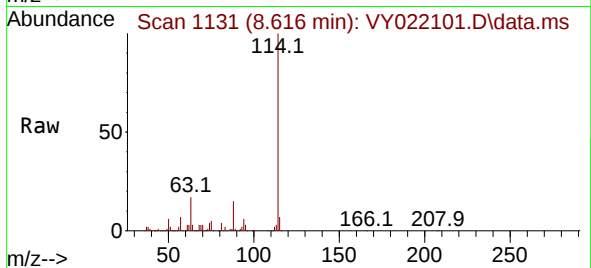

#35

Dibromofluoromethane

Concen: 51.057 ug/l

RT: 7.634 min Scan# 970

Delta R.T. -0.000 min

Lab File: VY022101.D

Acq: 01 May 2025 12:41




Tgt Ion:113 Resp: 196023


Ion Ratio Lower Upper

113 100

111 102.3 81.8 122.8

192 20.8 15.6 23.4


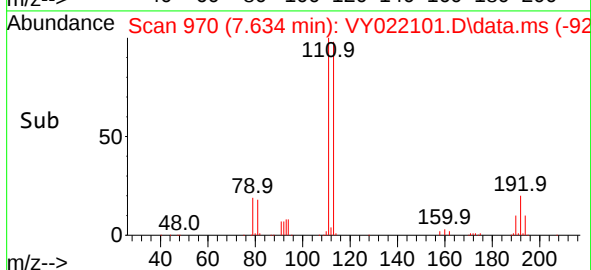
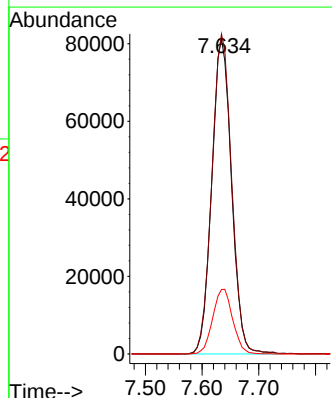
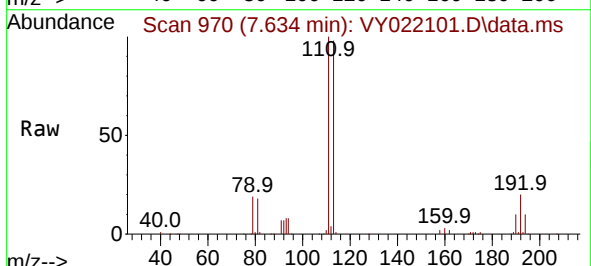


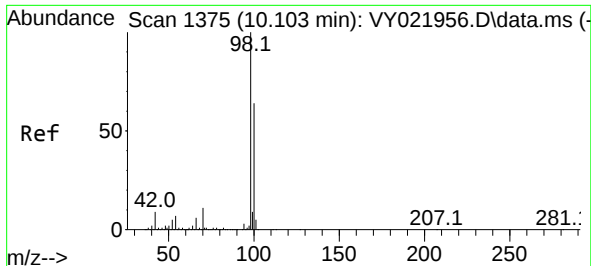

#50
Toluene-d8
Concen: 47.887 ug/l
RT: 10.109 min Scan# 1375
Delta R.T. 0.006 min
Lab File: VY022101.D
Acq: 01 May 2025 12:41




Instrument :
MSVOA_Y
ClientSampleId :
WC-12-VOC


Tgt Ion: 98 Resp: 693134
Ion Ratio Lower Upper
98 100
100 64.3 51.6 77.4

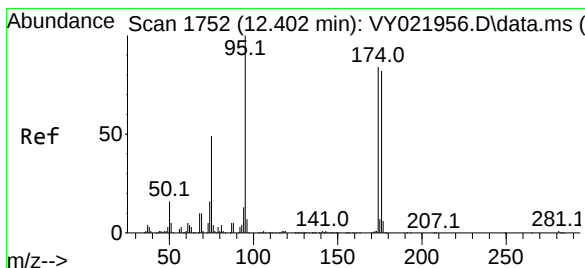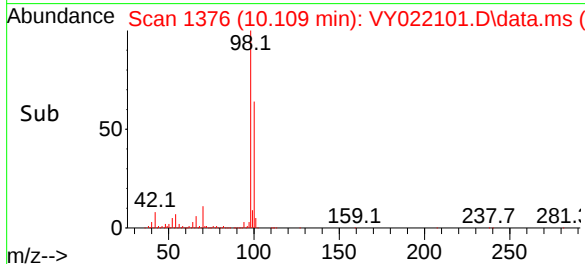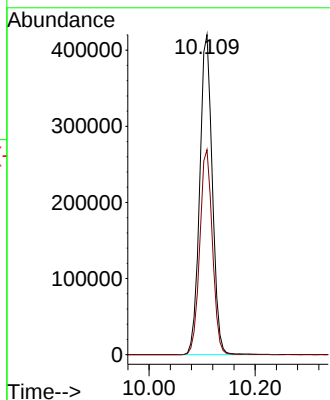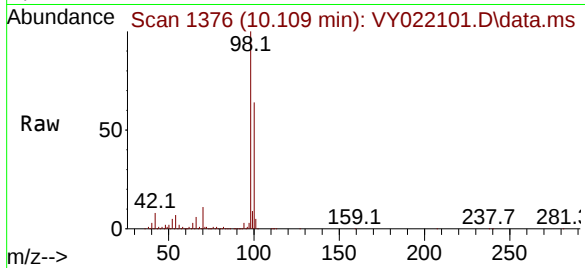

#62
4-Bromofluorobenzene
Concen: 39.333 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY022101.D
Acq: 01 May 2025 12:41

Tgt Ion: 95 Resp: 191657
Ion Ratio Lower Upper
95 100
174 90.4 0.0 179.0
176 86.9 0.0 171.8

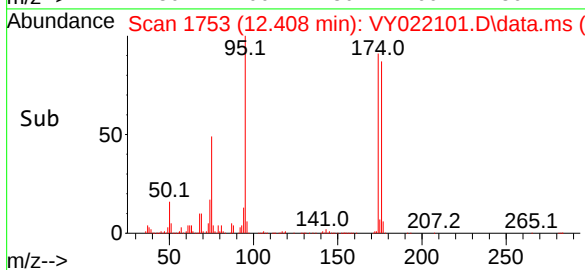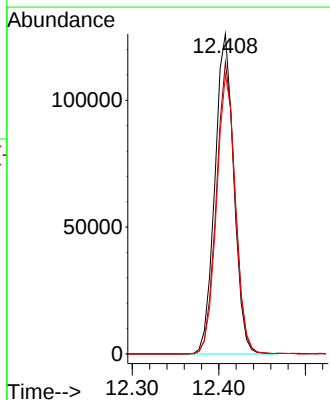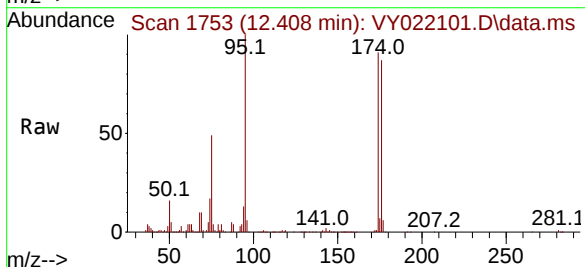

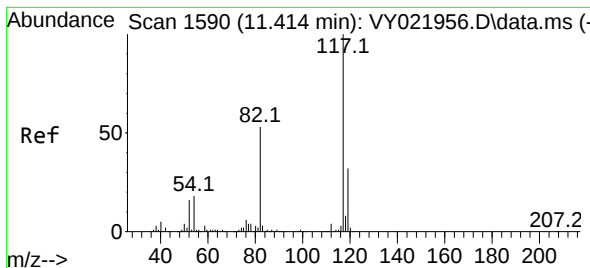

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY022101.D

Acq: 01 May 2025 12:41

Instrument :

MSVOA_Y

ClientSampleId :

WC-12-VOC





Tgt Ion:117 Resp: 521540

Ion Ratio Lower Upper

117 100

82 51.6 42.1 63.1

119 31.7 25.7 38.5

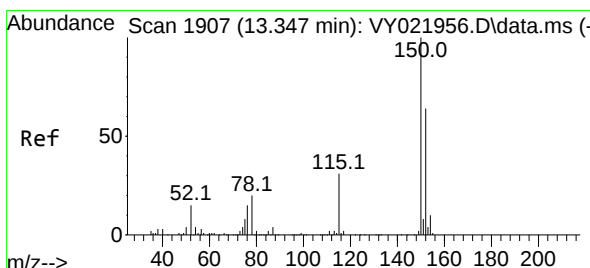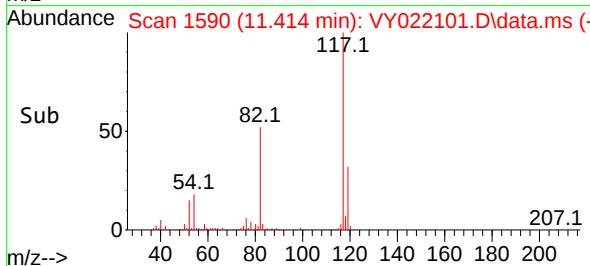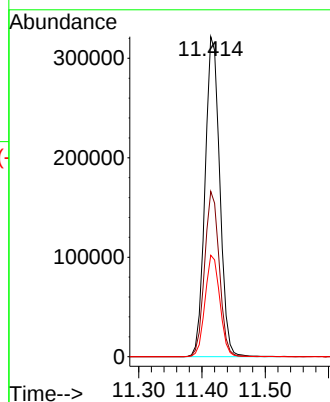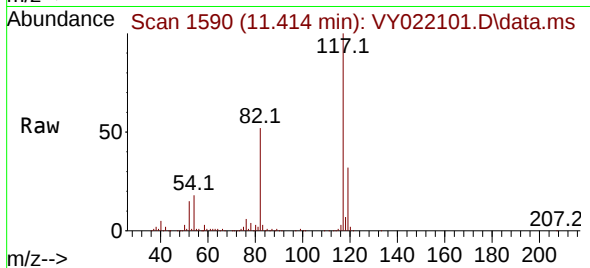

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VY022101.D

Acq: 01 May 2025 12:41

Tgt Ion:152 Resp: 198625

Ion Ratio Lower Upper

152 100

115 56.4 28.0 84.0

150 158.5 0.0 345.6

