

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050224\
 Data File : VY018116.D
 Acq On : 02 May 2024 14:54
 Operator : SY/MD
 Sample : P2323-01
 Misc : 3.16g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-1

Quant Time: May 02 23:04:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050124S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 01 16:21:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	295464	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	515516	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	452108	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	181207	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	119555	51.334	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	102.660%
35) Dibromofluoromethane	7.710	113	148229	50.035	ug/l	-0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.060%
50) Toluene-d8	10.179	98	566967	49.022	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	98.040%
62) 4-Bromofluorobenzene	12.477	95	177313	44.549	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	89.100%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050224\
Data File : VY018116.D
Acq On : 02 May 2024 14:54
Operator : SY/MD
Sample : P2323-01
Misc : 3.16g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-1

Quant Time: May 02 23:04:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050124S.M
Quant Title : SW846 8260
QLast Update : Wed May 01 16:21:20 2024
Response via : Initial Calibration




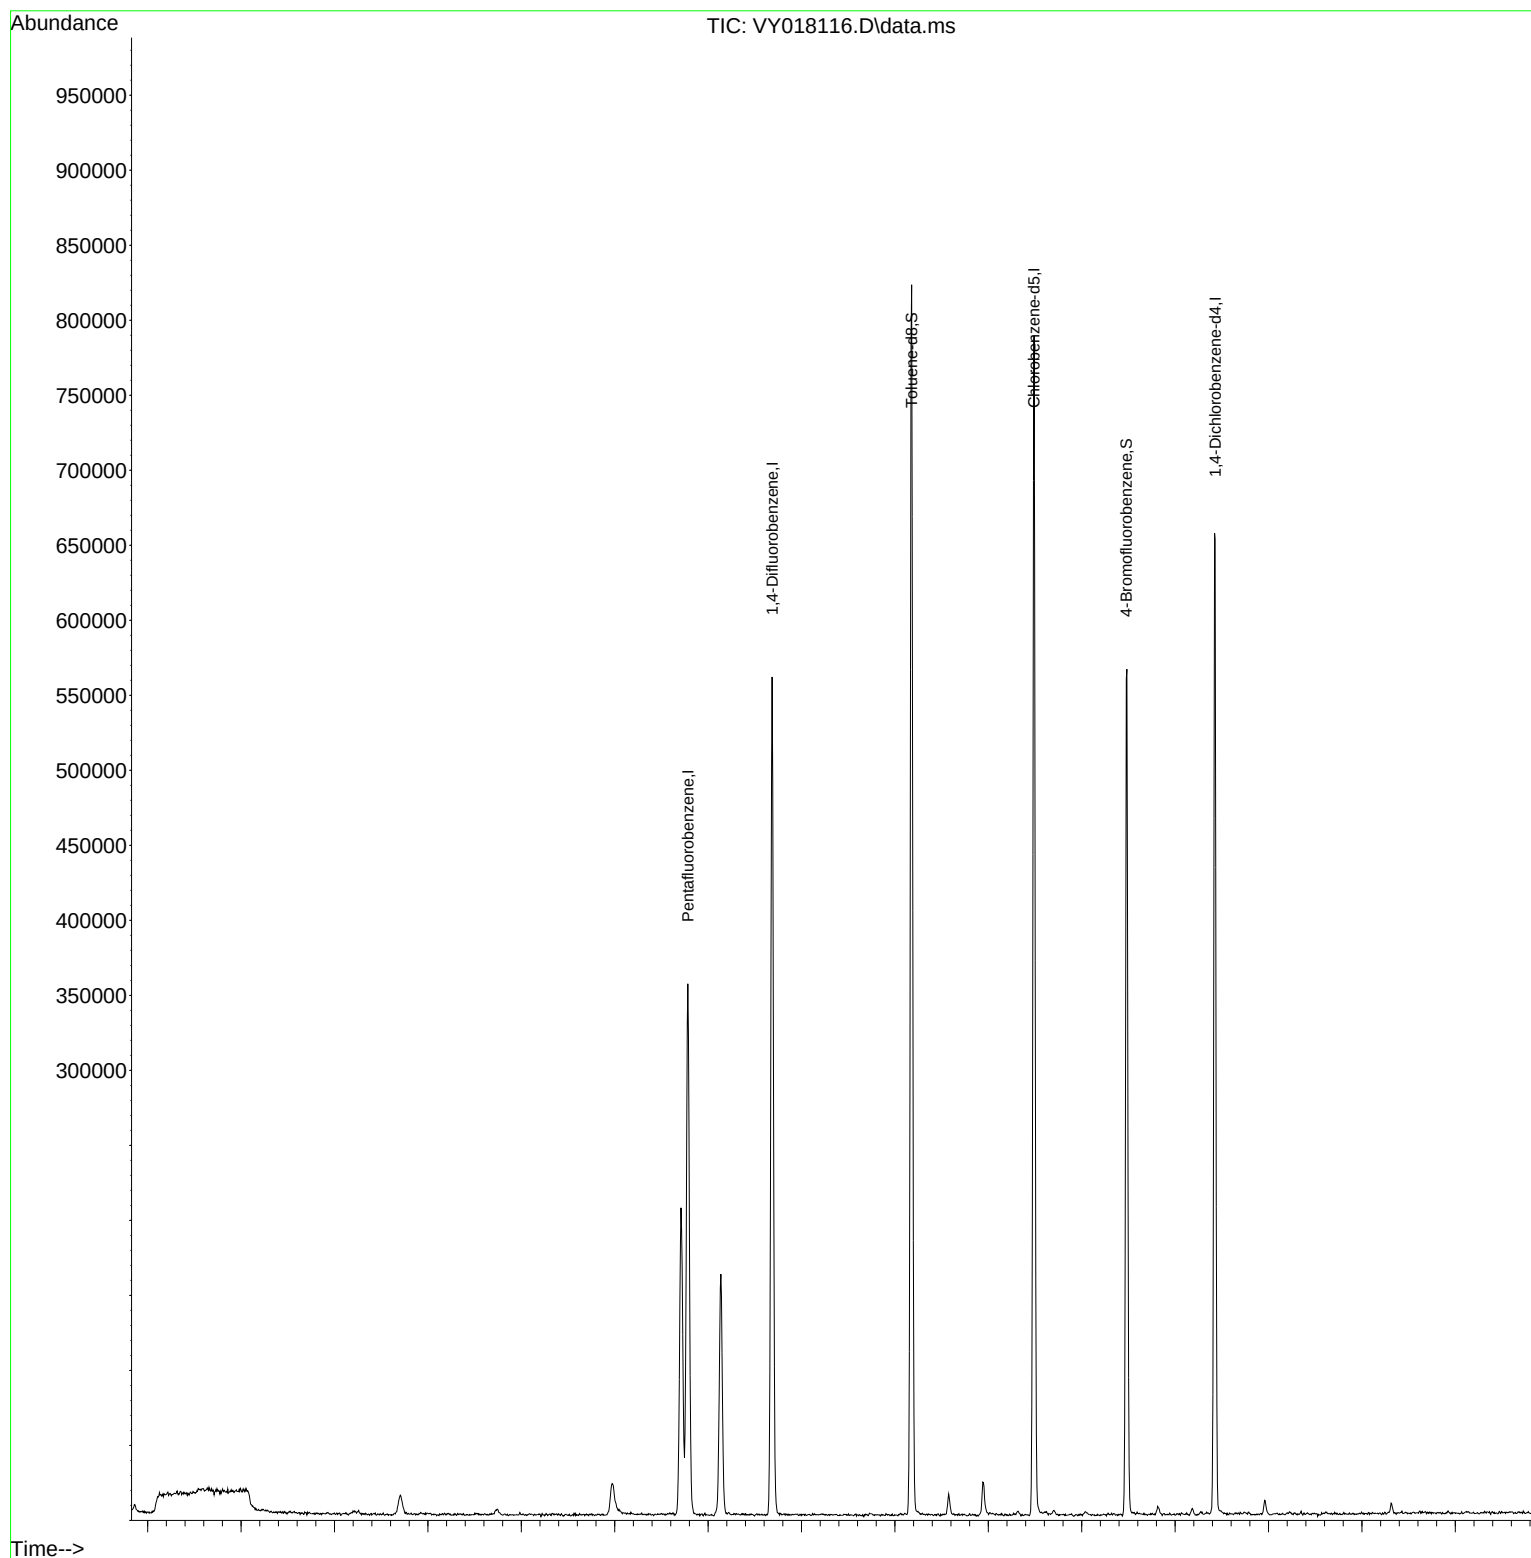


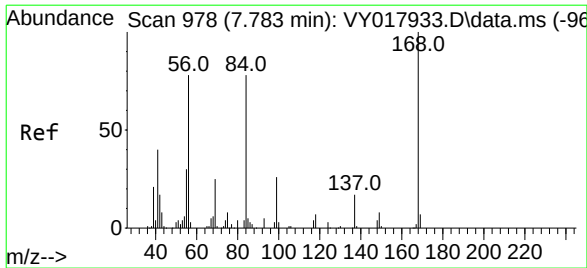

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 97
Delta R.T. -0.006 min
Lab File: VY018116.D
Acq: 02 May 2024 14:54




Instrument :
MSVOA_Y
ClientSampleId :
TP-1


Tgt Ion:168 Resp: 295464
Ion Ratio Lower Upper
168 100
99 49.2 39.1 58.7

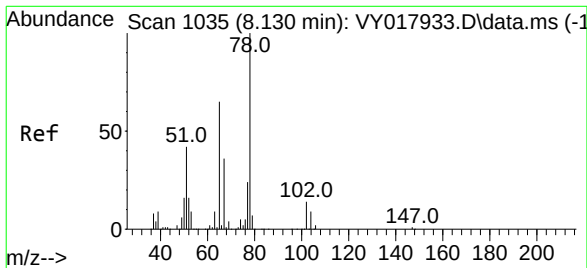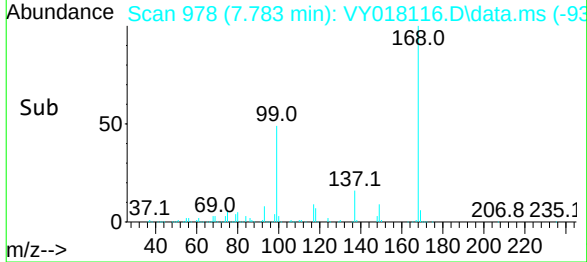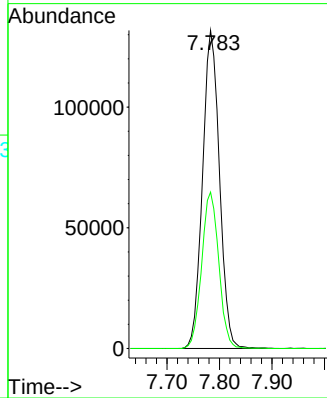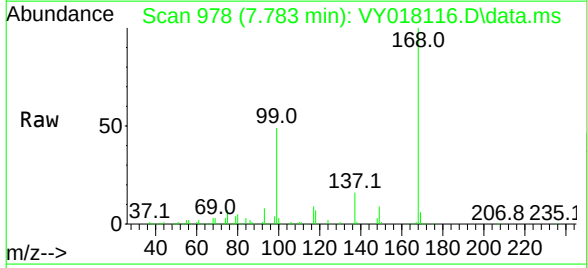

#33
1,2-Dichloroethane-d4
Concen: 51.334 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. -0.005 min
Lab File: VY018116.D
Acq: 02 May 2024 14:54

Tgt Ion: 65 Resp: 119555
Ion Ratio Lower Upper
65 100
67 54.9 0.0 109.6


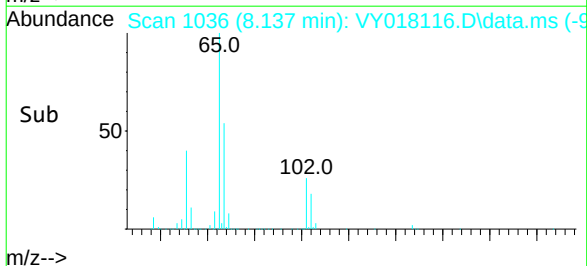
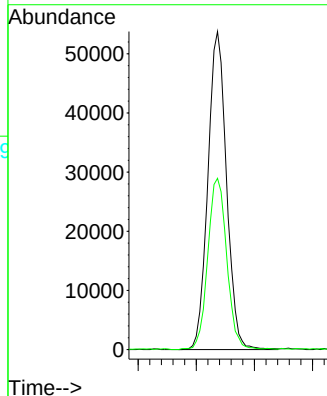
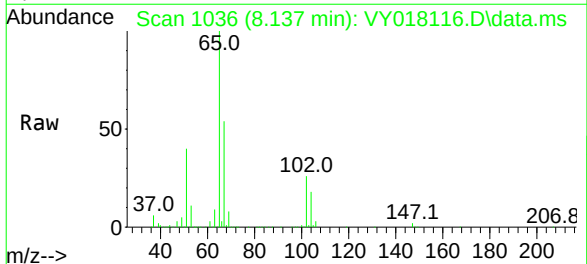


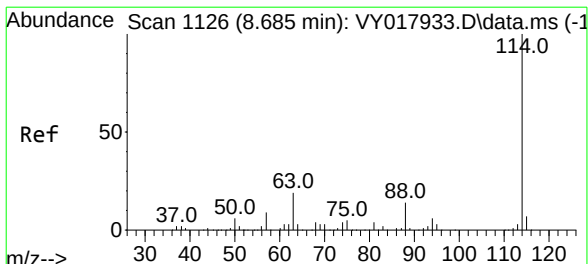

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.685 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: VY018116.D
 Acq: 02 May 2024 14:54




Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-1


Tgt Ion:	114	Resp:	515516
Ion	Ratio	Lower	Upper
114	100		
63	16.3	0.0	35.0
88	14.7	0.0	27.2

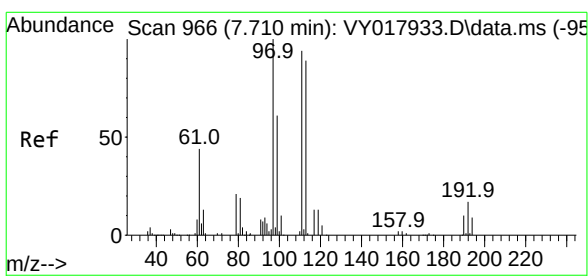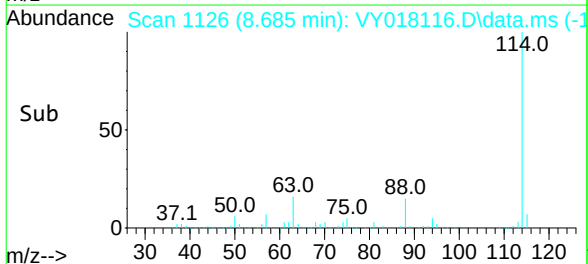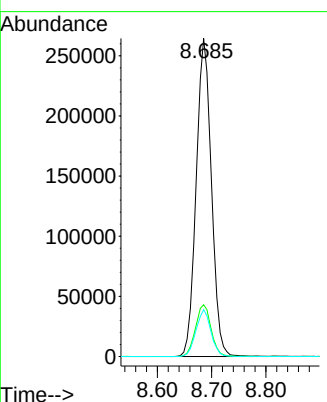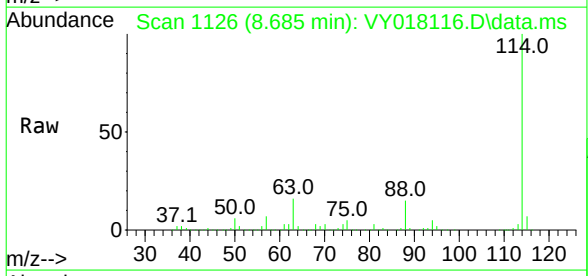

#35
 Dibromofluoromethane
 Concen: 50.035 ug/l
 RT: 7.710 min Scan# 966
 Delta R.T. -0.012 min
 Lab File: VY018116.D
 Acq: 02 May 2024 14:54

Tgt Ion:	113	Resp:	148229
Ion	Ratio	Lower	Upper
113	100		
111	102.7	82.2	123.4
192	20.9	15.9	23.9

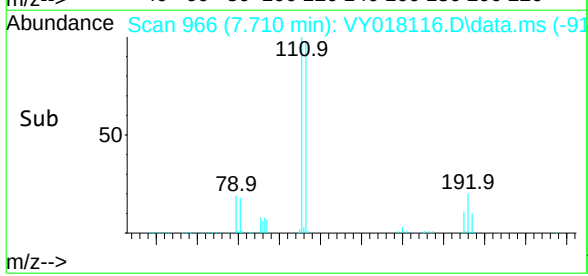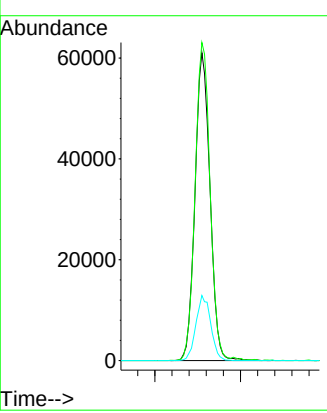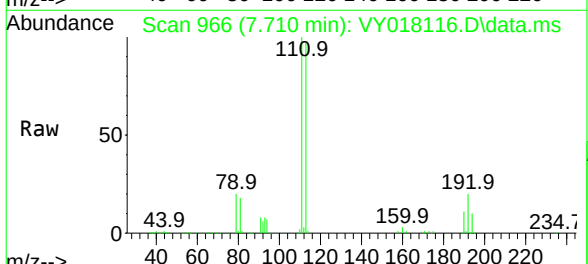

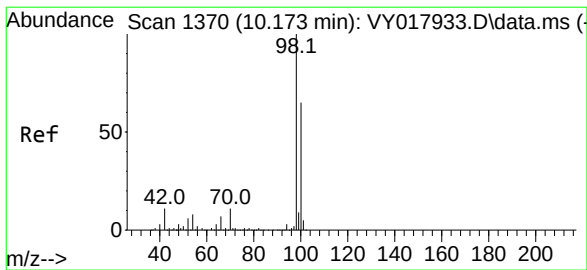

#50

Toluene-d8

Concen: 49.022 ug/l

RT: 10.179 min Scan# 1370

Delta R.T. -0.000 min

Lab File: VY018116.D

Acq: 02 May 2024 14:54

Instrument :

MSVOA_Y

ClientSampleId :





TP-1

Tgt Ion: 98 Resp: 566967

Ion Ratio Lower Upper

98 100

100 66.6 52.0 78.0

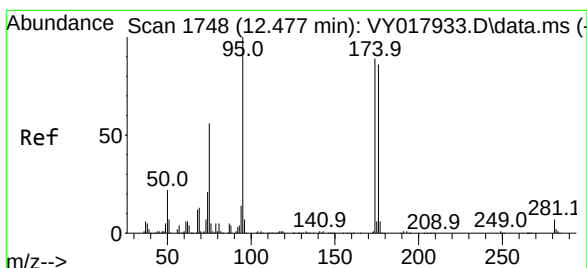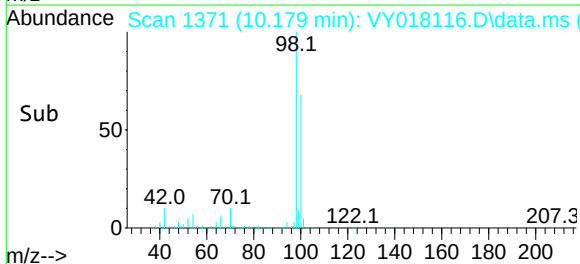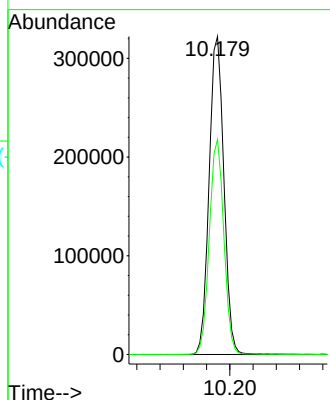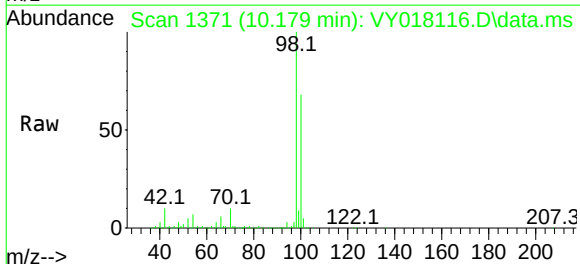

#62

4-Bromofluorobenzene

Concen: 44.549 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. -0.006 min

Lab File: VY018116.D

Acq: 02 May 2024 14:54




Tgt Ion: 95 Resp: 177313


Ion Ratio Lower Upper

95 100

174 89.3 0.0 175.6

176 87.1 0.0 171.4

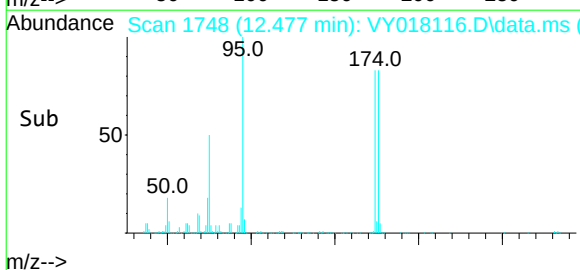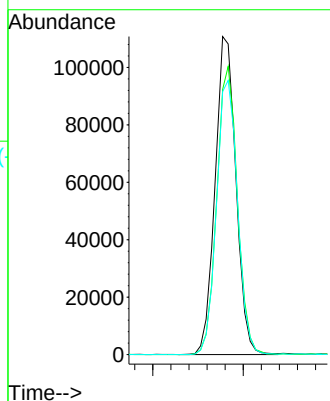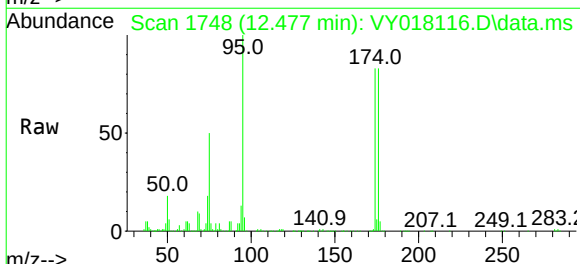

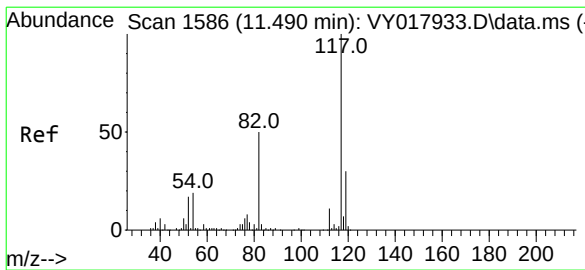

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 15

Delta R.T. 0.001 min

Lab File: VY018116.D

Acq: 02 May 2024 14:54

Instrument :

MSVOA_Y

ClientSampleId :

TP-1





Tgt Ion:117 Resp: 452108

Ion Ratio Lower Upper

117 100

82 49.2 42.4 63.6

119 32.7 25.9 38.9

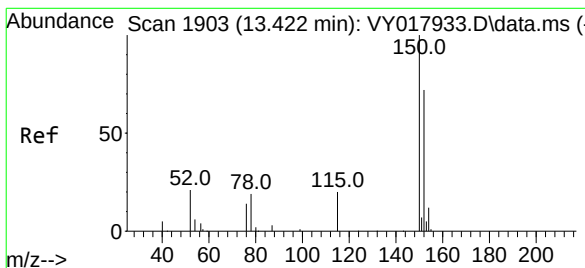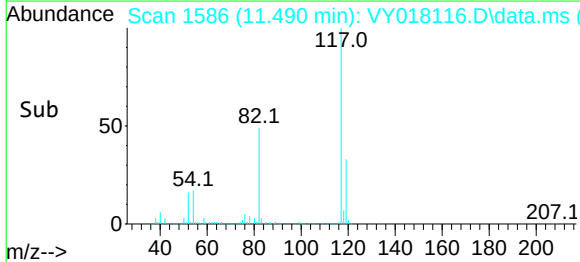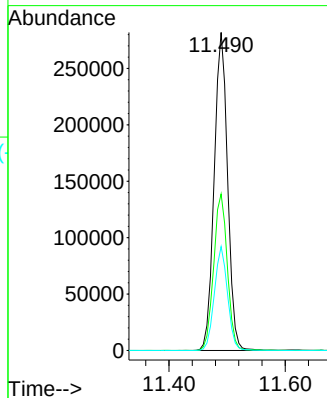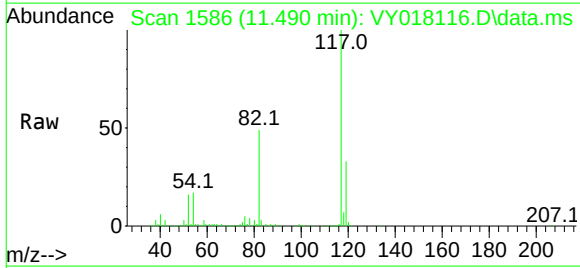

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY018116.D

Acq: 02 May 2024 14:54

Tgt Ion:152 Resp: 181207

Ion Ratio Lower Upper

152 100

115 55.8 28.2 84.7

150 157.3 0.0 345.6

