

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050224\
 Data File : VY018119.D
 Acq On : 02 May 2024 16:05
 Operator : SY/MD
 Sample : P2330-01
 Misc : 6.28g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 B-1(0.5-1.5)

Quant Time: May 02 23:05:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050124S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 01 16:21:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	268516	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	466229	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	403701	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	156238	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	111868	52.854	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	105.700%
35) Dibromofluoromethane	7.710	113	135488	50.569	ug/l	-0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.140%
50) Toluene-d8	10.179	98	512186	48.968	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.940%
62) 4-Bromofluorobenzene	12.477	95	160876	44.692	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	89.380%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050224\
Data File : VY018119.D
Acq On : 02 May 2024 16:05
Operator : SY/MD
Sample : P2330-01
Misc : 6.28g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
B-1(0.5-1.5)

Quant Time: May 02 23:05:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050124S.M
Quant Title : SW846 8260
QLast Update : Wed May 01 16:21:20 2024
Response via : Initial Calibration




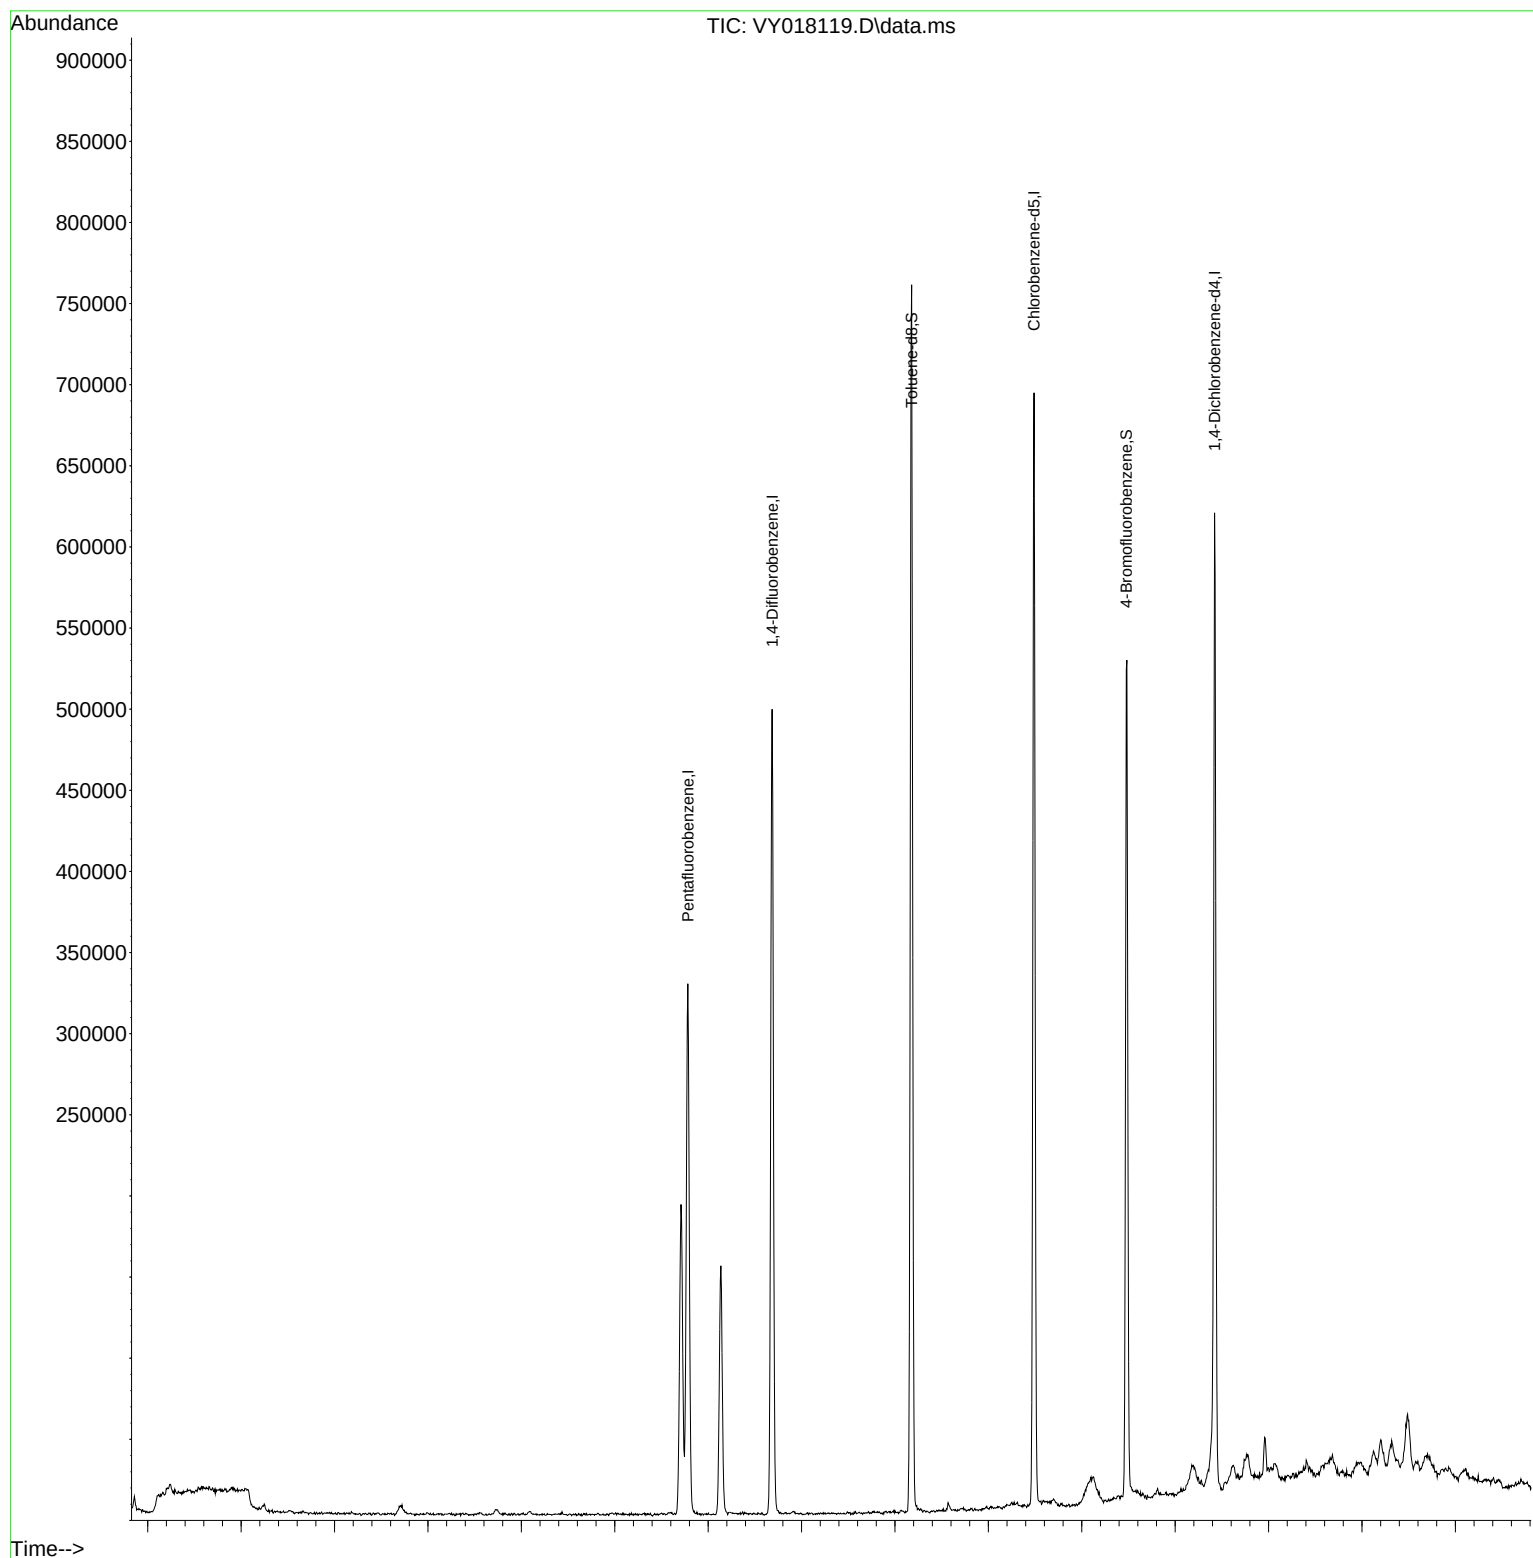


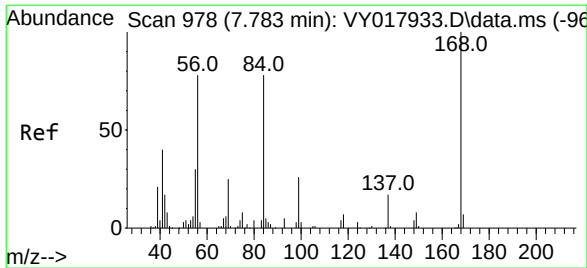

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 97
Delta R.T. -0.006 min
Lab File: VY018119.D
Acq: 02 May 2024 16:05




Instrument :
MSVOA_Y
ClientSampleId :
B-1(0.5-1.5)


Tgt Ion:168 Resp: 268516
Ion Ratio Lower Upper
168 100
99 50.9 39.1 58.7

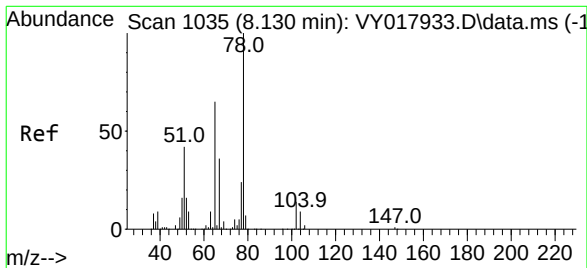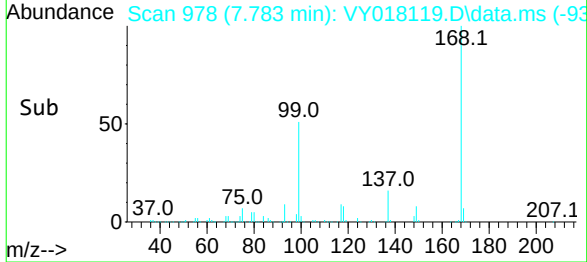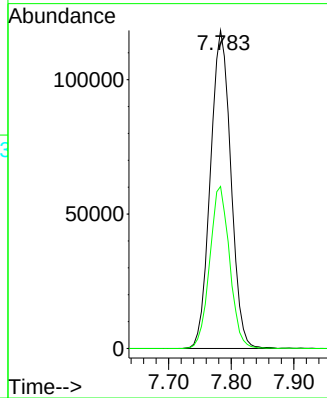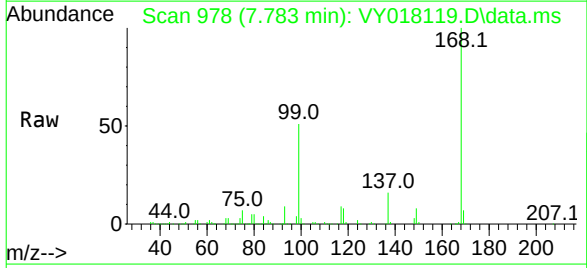

#33
1,2-Dichloroethane-d4
Concen: 52.854 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VY018119.D
Acq: 02 May 2024 16:05

Tgt Ion: 65 Resp: 111868
Ion Ratio Lower Upper
65 100
67 54.7 0.0 109.6


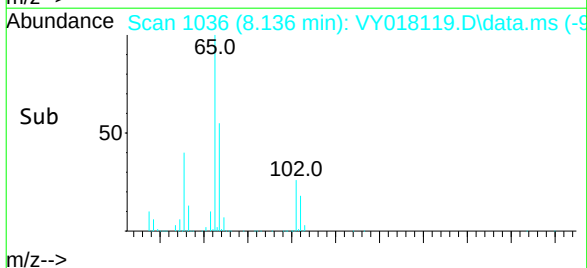
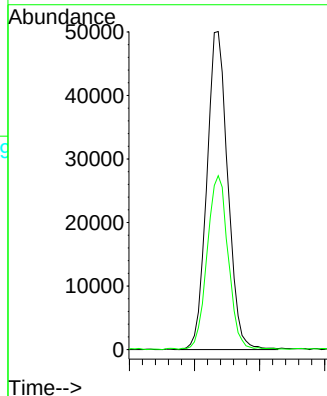
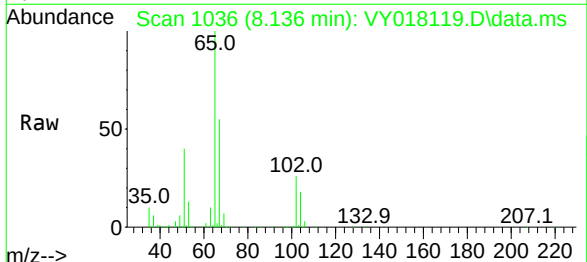


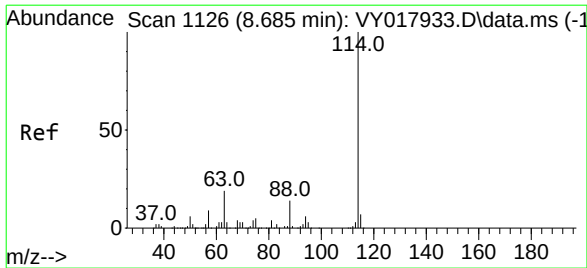

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. -0.006 min
Lab File: VY018119.D
Acq: 02 May 2024 16:05




Instrument :
MSVOA_Y
ClientSampleId :
B-1(0.5-1.5)


Tgt Ion:	114	Resp:	466229
Ion	Ratio	Lower	Upper
114	100		
63	17.0	0.0	35.0
88	14.0	0.0	27.2

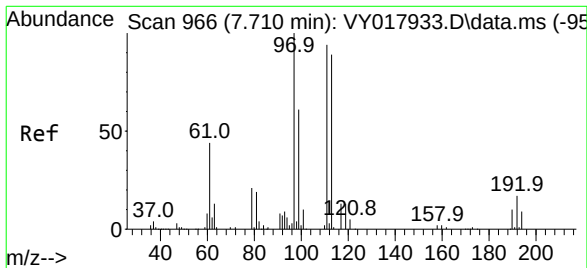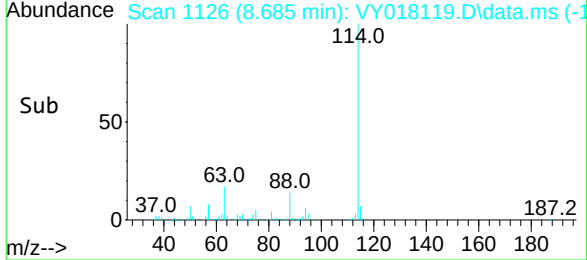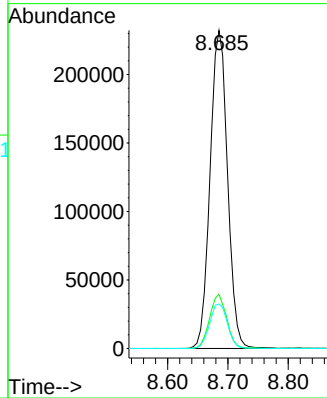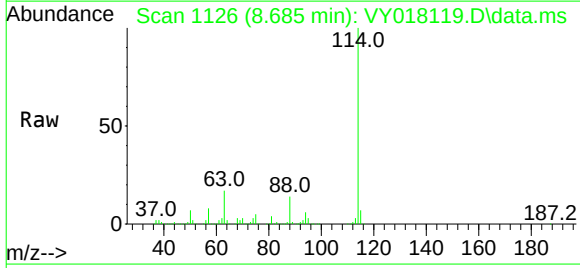

#35
Dibromofluoromethane
Concen: 50.569 ug/l
RT: 7.710 min Scan# 966
Delta R.T. -0.012 min
Lab File: VY018119.D
Acq: 02 May 2024 16:05

Tgt Ion:	113	Resp:	135488
Ion	Ratio	Lower	Upper
113	100		
111	101.9	82.2	123.4
192	21.6	15.9	23.9

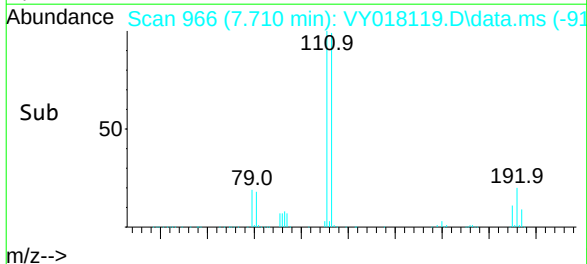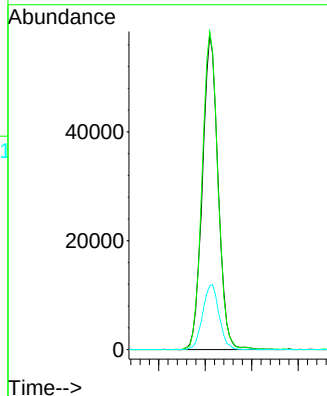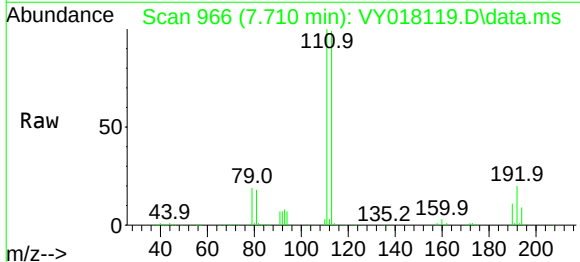

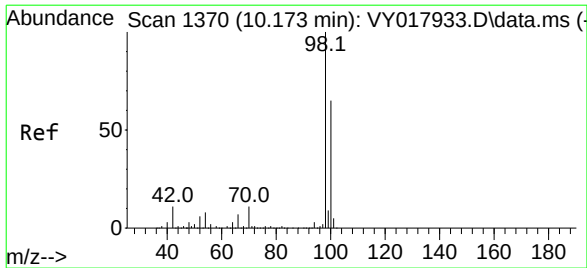

#50

Toluene-d8

Concen: 48.968 ug/l

RT: 10.179 min Scan# 1370

Delta R.T. -0.000 min

Lab File: VY018119.D

Acq: 02 May 2024 16:05

Instrument :

MSVOA_Y

ClientSampleId :





B-1(0.5-1.5)

Tgt Ion: 98 Resp: 512186

Ion Ratio Lower Upper

98 100

100 66.7 52.0 78.0

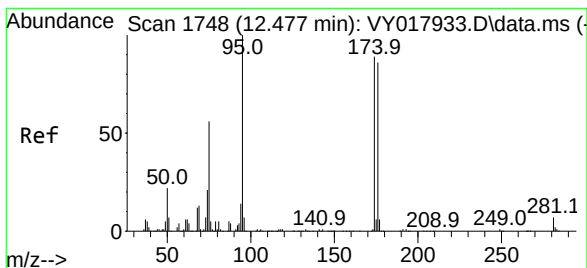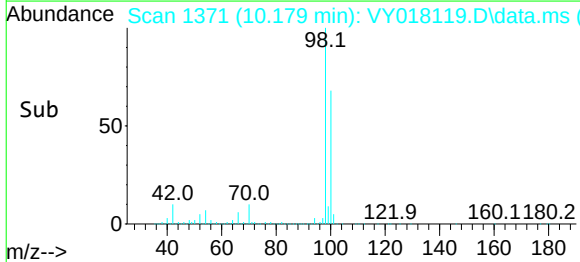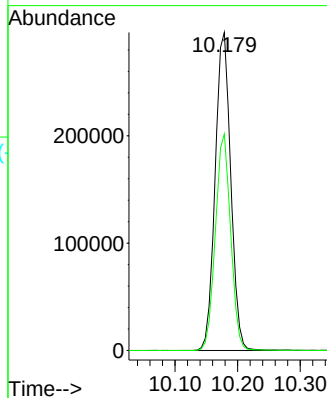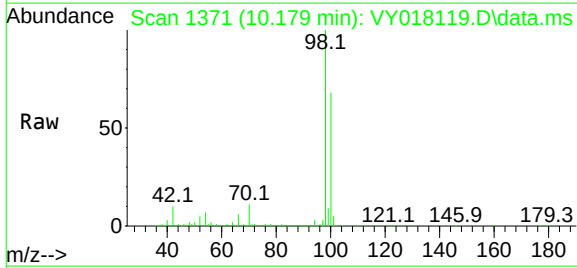

#62

4-Bromofluorobenzene

Concen: 44.692 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. -0.006 min

Lab File: VY018119.D

Acq: 02 May 2024 16:05




Tgt Ion: 95 Resp: 160876


Ion Ratio Lower Upper

95 100

174 86.9 0.0 175.6

176 85.1 0.0 171.4

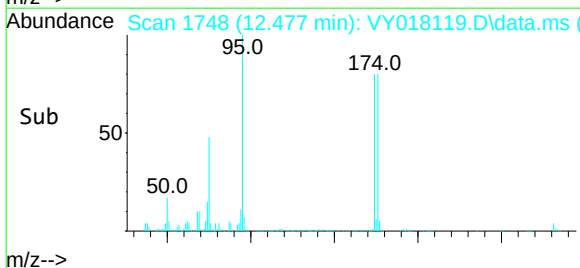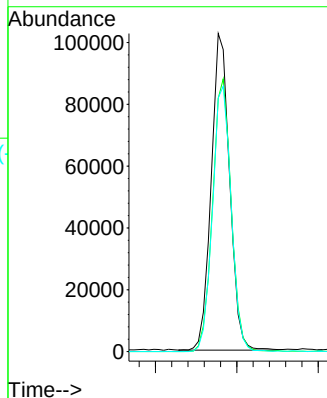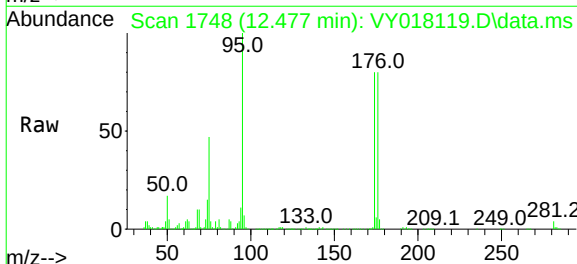

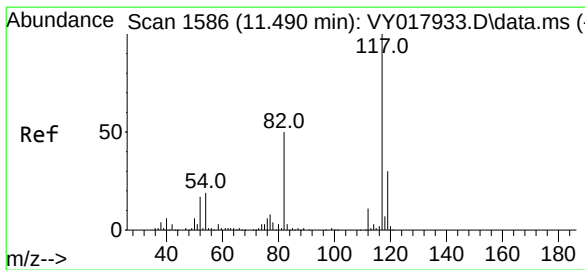

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 1586

Delta R.T. 0.001 min

Lab File: VY018119.D

Acq: 02 May 2024 16:05





Instrument :

MSVOA_Y

ClientSampleId :

B-1(0.5-1.5)

Tgt Ion:	117	Resp:	403701
Ion	Ratio	Lower	Upper
117	100		
82	49.3	42.4	63.6
119	32.4	25.9	38.9

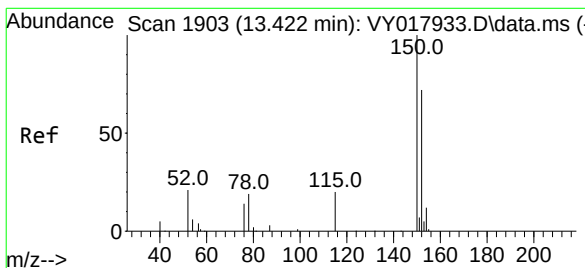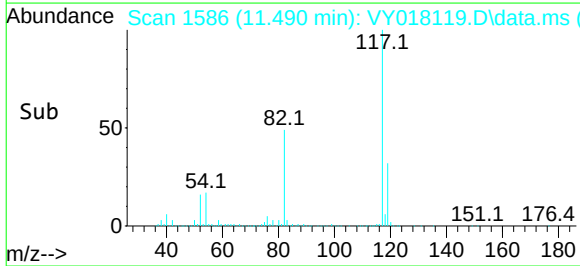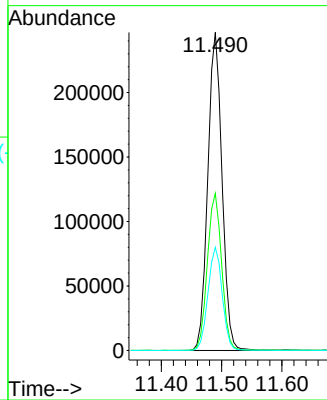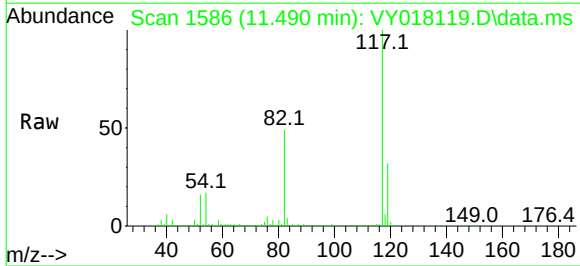

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.006 min

Lab File: VY018119.D

Acq: 02 May 2024 16:05

Tgt Ion:	152	Resp:	156238
Ion	Ratio	Lower	Upper
152	100		
115	56.2	28.2	84.7
150	156.2	0.0	345.6

