
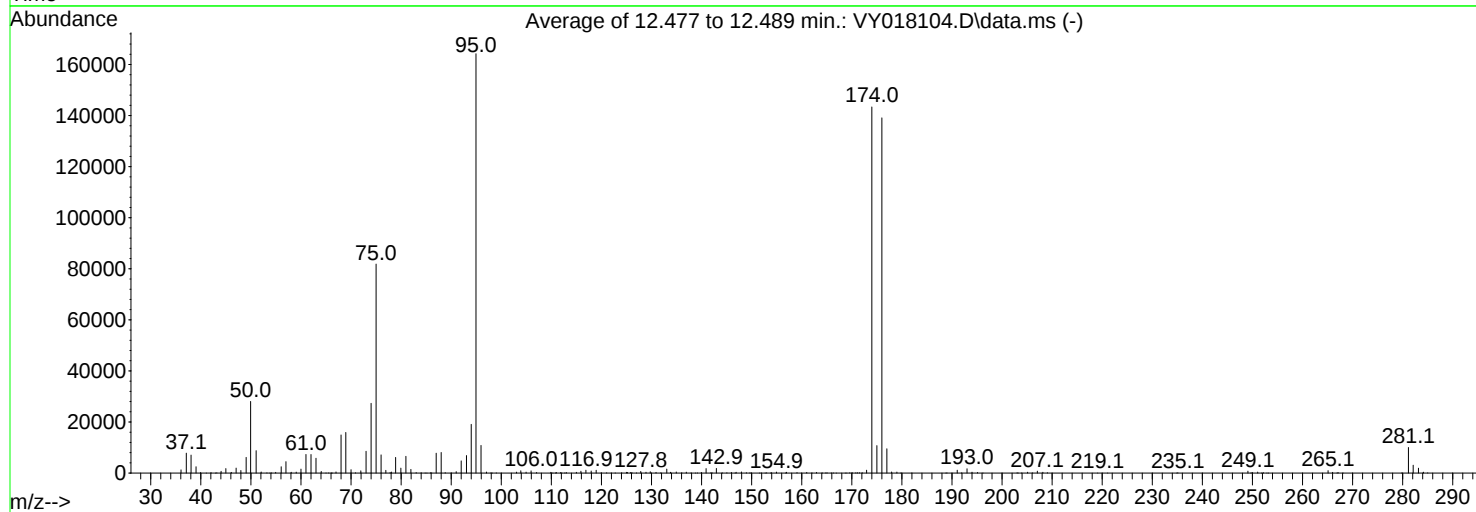


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050224\
Data File : VY018104.D
Acq On : 02 May 2024 08:34
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050124S.M
Title : SW846 8260
Last Update : Wed May 01 16:21:20 2024

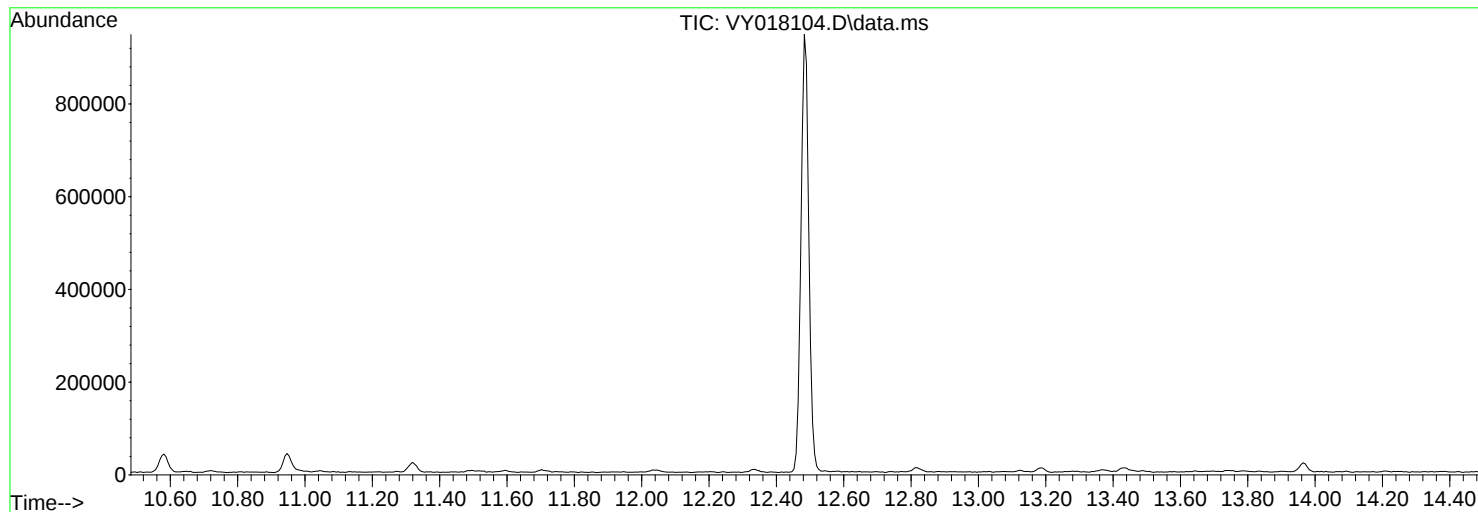

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1735

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	28049	PASS
75	95	30	60	49.8	81853	PASS
95	95	100	100	100.0	164214	PASS
96	95	5	9	6.6	10832	PASS
173	174	0.00	2	0.8	1134	PASS
174	95	50	100	87.3	143373	PASS
175	174	5	9	7.5	10763	PASS
176	174	95	101	97.0	139099	PASS
177	176	5	9	6.8	9504	PASS