
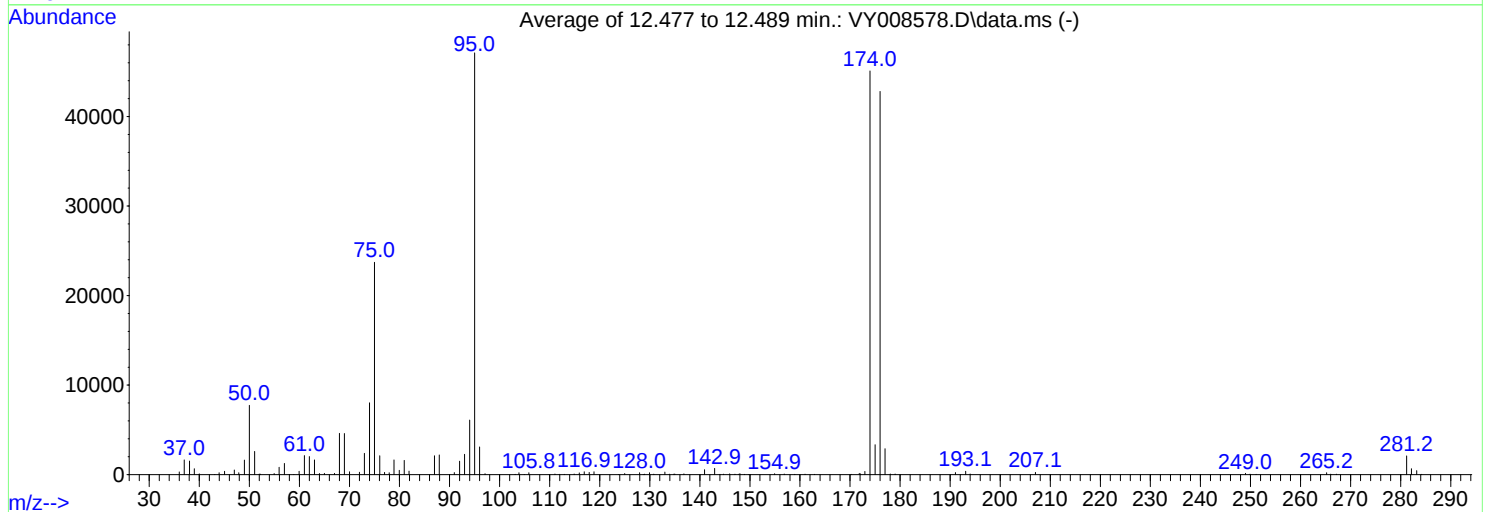


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050322\
 Data File : VY008578.D
 Acq On : 03 May 2022 09:03
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050222S.M
 Title : SW846 8260
 Last Update : Tue May 03 01:57:20 2022

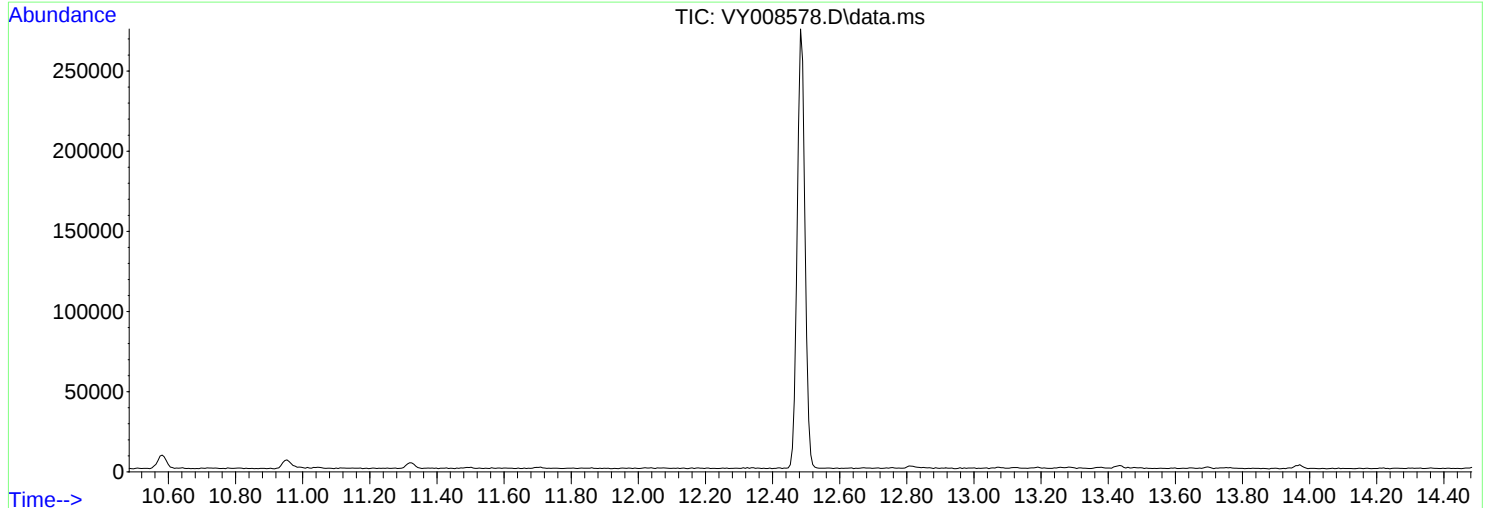

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	7741	PASS
75	95	30	60	50.3	23717	PASS
95	95	100	100	100.0	47112	PASS
96	95	5	9	6.6	3086	PASS
173	174	0.00	2	0.8	362	PASS
174	95	50	100	95.7	45088	PASS
175	174	5	9	7.4	3334	PASS
176	174	95	101	94.9	42795	PASS
177	176	5	9	6.8	2899	PASS