

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050422\
 Data File : VY008616.D
 Acq On : 04 May 2022 16:47
 Operator : KP/MD
 Sample : N2619-09
 Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SS05-1-2-FT

Quant Time: May 05 04:36:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050222S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 03 01:57:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	130166	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	226337	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	229455	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	113887	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	64853	51.262	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	102.520%
35) Dibromofluoromethane	7.722	113	71124	47.490	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	94.980%
50) Toluene-d8	10.179	98	269490	50.790	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	101.580%
62) 4-Bromofluorobenzene	12.483	95	96114	49.422	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	98.840%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050422\
Data File : VY008616.D
Acq On : 04 May 2022 16:47
Operator : KP/MD
Sample : N2619-09
Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SS05-1-2-FT

Quant Time: May 05 04:36:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050222S.M
Quant Title : SW846 8260
QLast Update : Tue May 03 01:57:20 2022
Response via : Initial Calibration




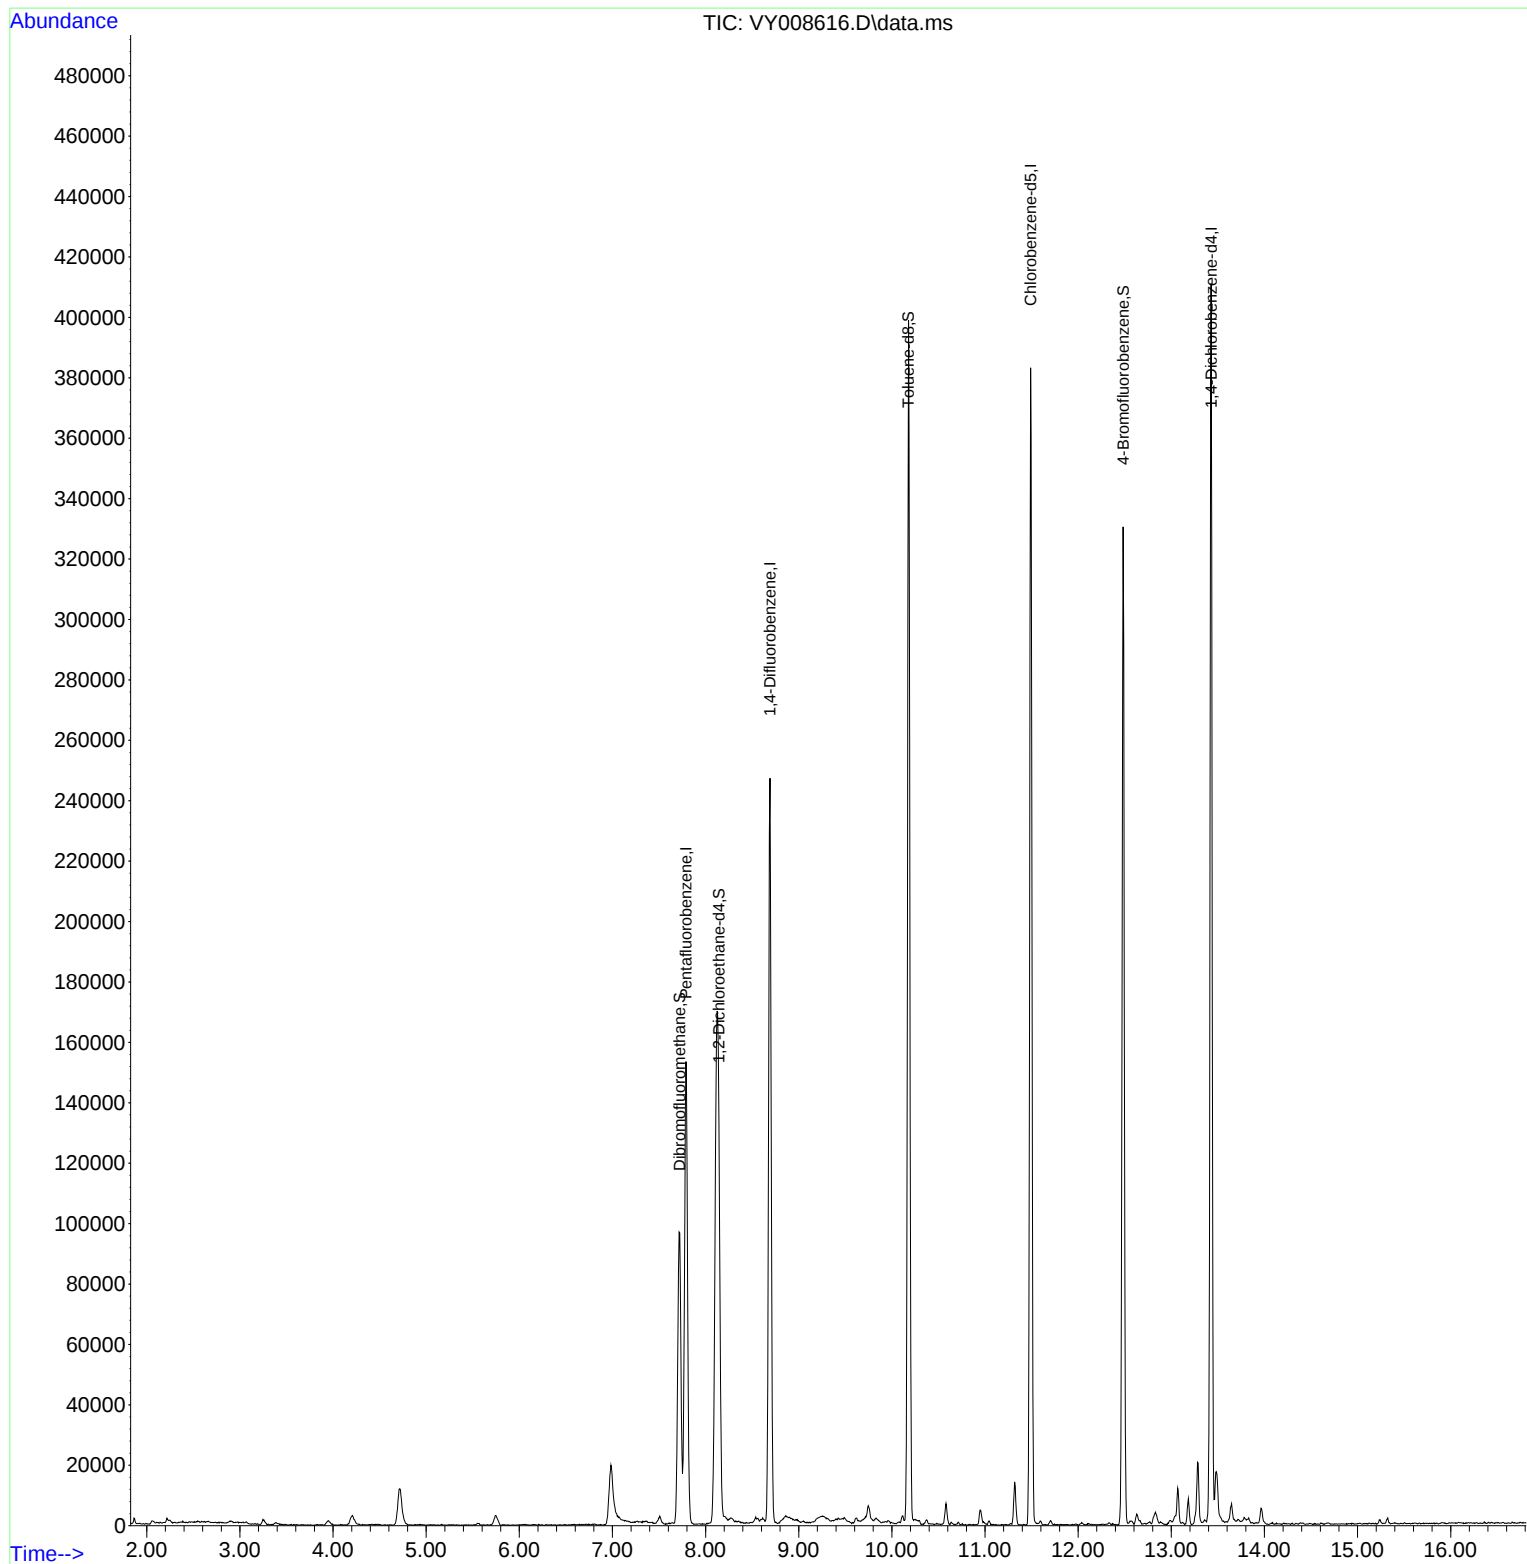


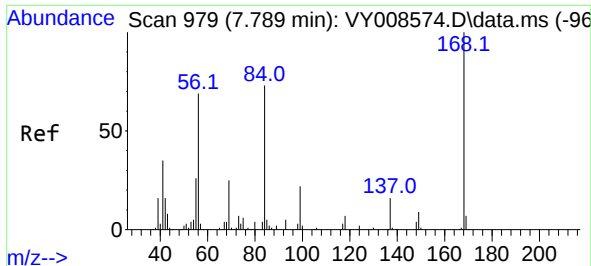

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008616.D
Acq: 04 May 2022 16:47




Instrument :
MSVOA_Y
ClientSampleId :
SS05-1-2-FT


Tgt Ion:168 Resp: 130166
Ion Ratio Lower Upper
168 100
99 48.3 46.9 70.3

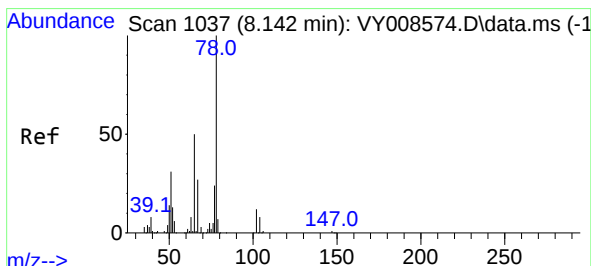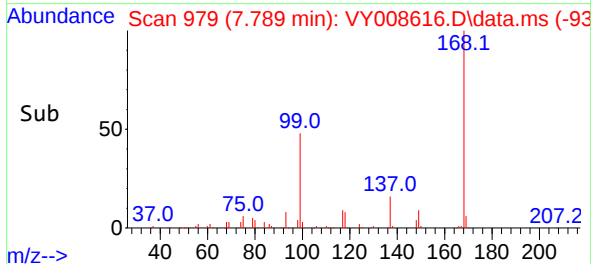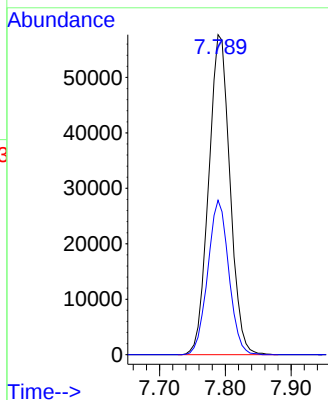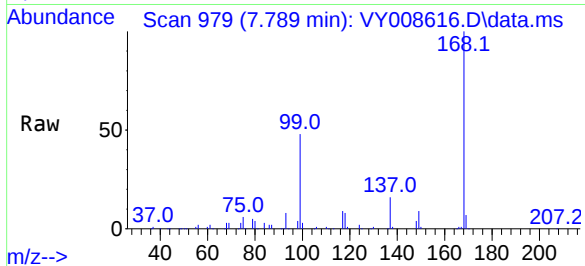

#33
1,2-Dichloroethane-d4
Concen: 51.262 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY008616.D
Acq: 04 May 2022 16:47

Tgt Ion: 65 Resp: 64853
Ion Ratio Lower Upper
65 100
67 57.7 0.0 99.4

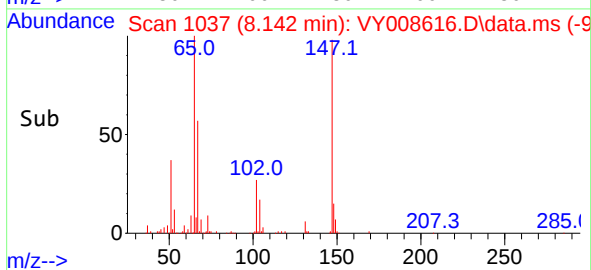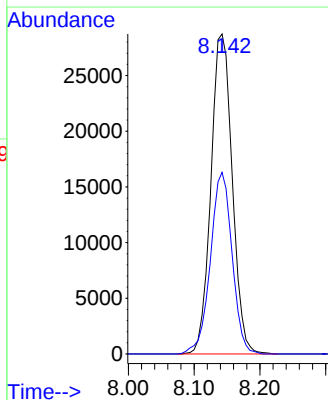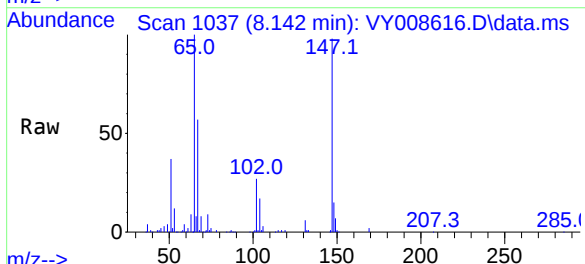

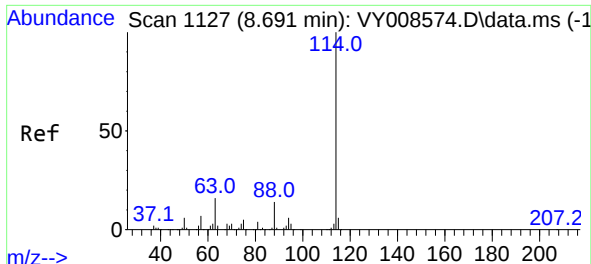

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VY008616.D

Acq: 04 May 2022 16:47

Instrument :

MSVOA_Y

ClientSampleId :

SS05-1-2-FT





Tgt Ion:114 Resp: 226337

Ion Ratio Lower Upper

114 100

63 16.5 0.0 43.2

88 14.5 0.0 31.8

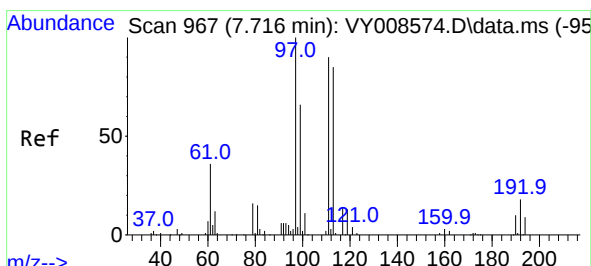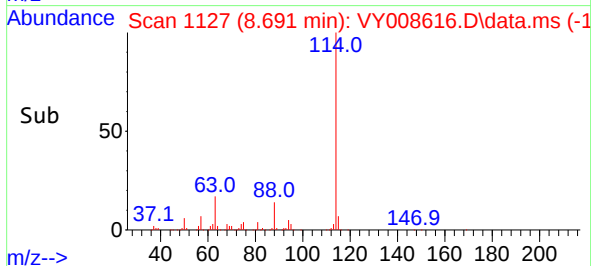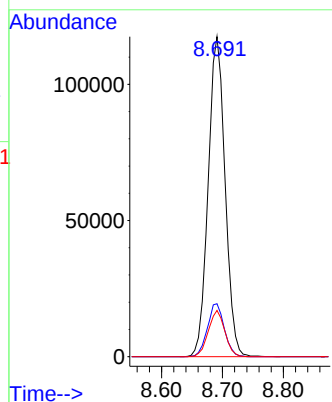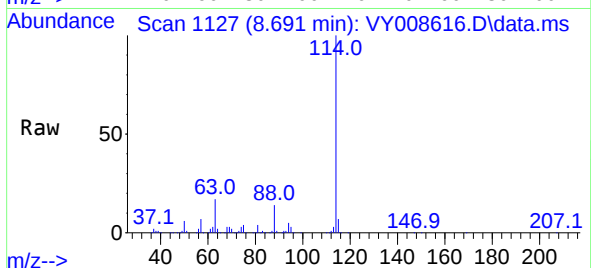

#35

Dibromofluoromethane

Concen: 47.490 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY008616.D

Acq: 04 May 2022 16:47




Tgt Ion:113 Resp: 71124


Ion Ratio Lower Upper

113 100

111 102.5 82.6 124.0

192 21.1 17.6 26.4


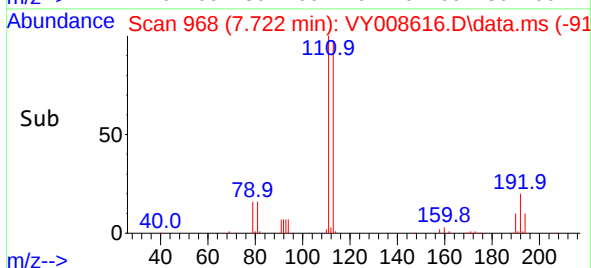
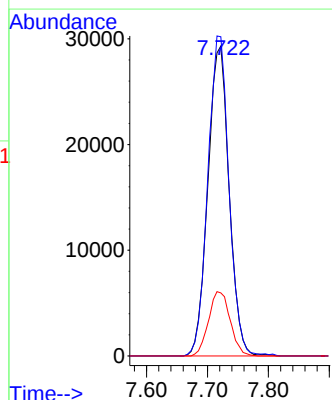
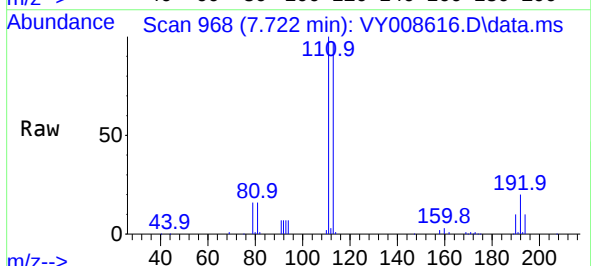


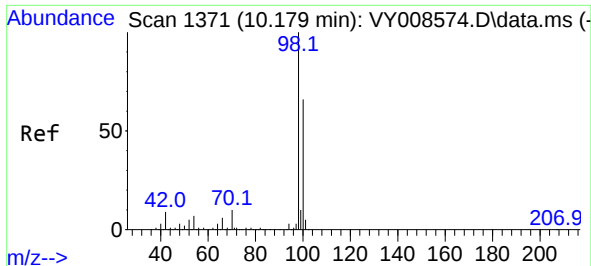

#50
Toluene-d8
Concen: 50.790 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY008616.D
Acq: 04 May 2022 16:47




Instrument :
MSVOA_Y
ClientSampleId :
SS05-1-2-FT


Tgt Ion: 98 Resp: 269490
Ion Ratio Lower Upper
98 100
100 65.5 50.2 75.2

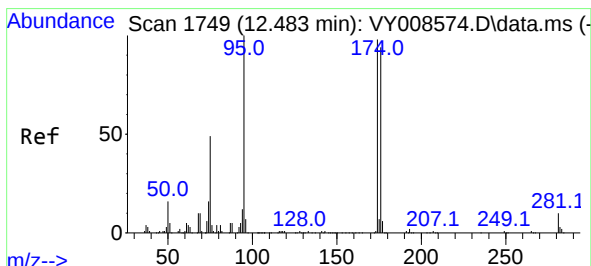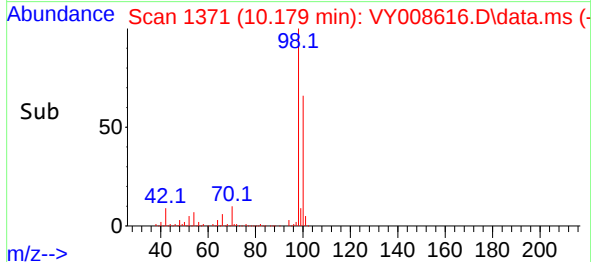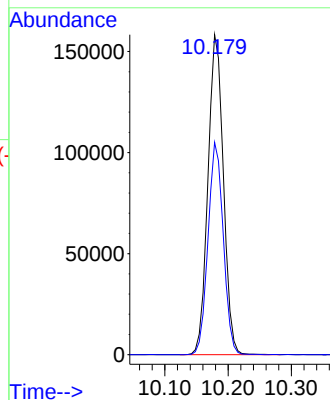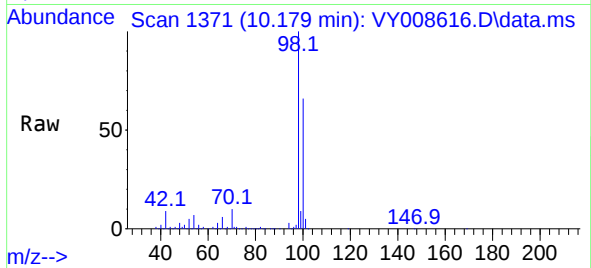

#62
4-Bromofluorobenzene
Concen: 49.422 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY008616.D
Acq: 04 May 2022 16:47

Tgt Ion: 95 Resp: 96114
Ion Ratio Lower Upper
95 100
174 97.2 0.0 177.0
176 93.1 0.0 175.8


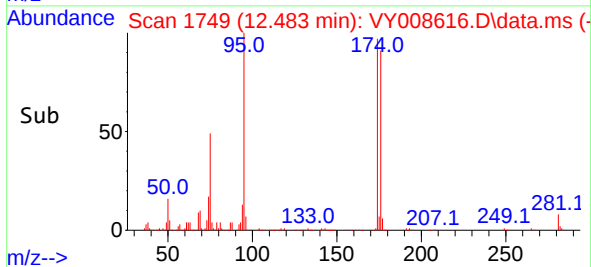
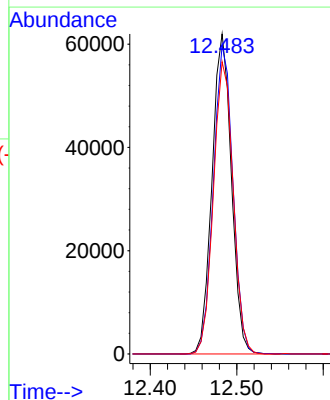
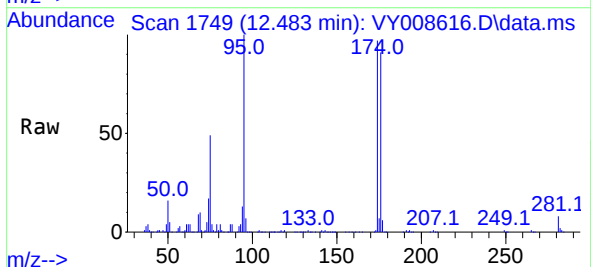


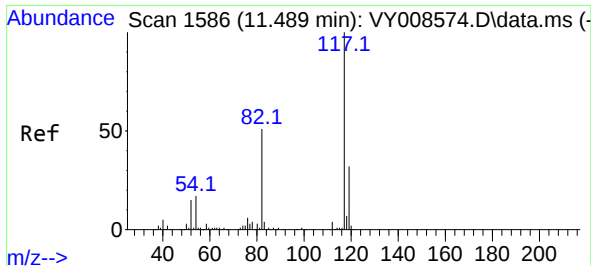

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. -0.000 min
Lab File: VY008616.D
Acq: 04 May 2022 16:47

Instrument :
MSVOA_Y
ClientSampleId :
SS05-1-2-FT

Tgt Ion:117 Resp: 229455
Ion Ratio Lower Upper
117 100
82 49.7 43.0 64.4
119 31.6 25.4 38.0

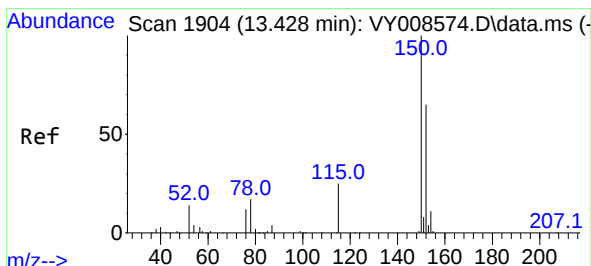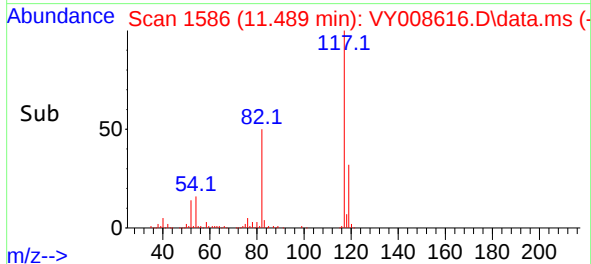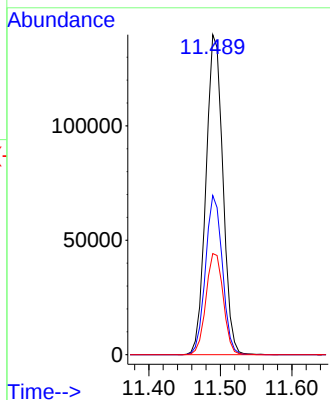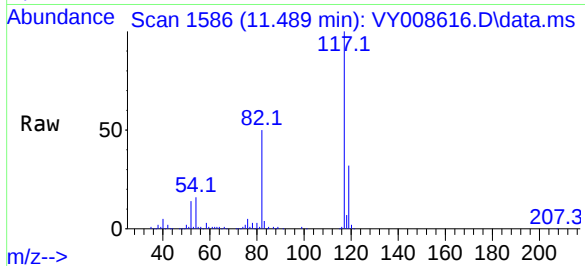

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY008616.D
Acq: 04 May 2022 16:47

Tgt Ion:152 Resp: 113887
Ion Ratio Lower Upper
152 100
115 53.9 28.2 84.7
150 156.6 0.0 347.6

