

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050422\
 Data File : VY008635.D
 Acq On : 05 May 2022 01:17
 Operator : KP/MD
 Sample : N2619-21
 Misc : 4.25g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SS10-1-2-FT

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050222S.M
 Title : SW846 8260

Signal : TIC: VY008635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.716	463	475	487	rBV2	10404	32977	4.86%	0.727%
2	5.741	634	643	653	rBV3	3277	9628	1.42%	0.212%
3	6.978	836	846	859	rBV	15290	56569	8.34%	1.247%
4	7.716	958	967	973	rBV2	99339	237215	34.98%	5.229%
5	7.789	973	979	995	rVB	154714	351073	51.77%	7.738%
6	8.124	1021	1034	1046	rBV2	174375	570449	84.11%	12.574%
7	8.691	1119	1127	1136	rVB	241589	480982	70.92%	10.602%
8	8.862	1139	1155	1156	rBV5	3195	10206	1.50%	0.225%
9	9.746	1289	1300	1311	rBV6	4543	10226	1.51%	0.225%
10	10.179	1363	1371	1379	rVB	404436	678187	100.00%	14.948%
11	10.581	1428	1437	1443	rBV	26254	47293	6.97%	1.042%
12	10.947	1491	1497	1509	rBV	34940	68725	10.13%	1.515%
13	11.319	1552	1558	1564	rVB	13675	21900	3.23%	0.483%
14	11.490	1578	1586	1597	rBV	403487	645031	95.11%	14.218%
15	12.483	1740	1749	1756	rBV	341826	539602	79.57%	11.894%
16	12.825	1797	1805	1812	rBV6	4284	10715	1.58%	0.236%
17	13.069	1835	1845	1851	rVB2	9691	19154	2.82%	0.422%
18	13.178	1857	1863	1870	rBV	5625	8860	1.31%	0.195%
19	13.282	1870	1880	1886	rBV	17721	30244	4.46%	0.667%
20	13.422	1895	1903	1909	rBV	415173	659400	97.23%	14.534%
21	13.483	1909	1913	1924	rVB2	14431	31785	4.69%	0.701%
22	13.648	1932	1940	1945	rBV4	5156	9710	1.43%	0.214%
23	15.318	2209	2214	2220	rVB	4956	6932	1.02%	0.153%


Sum of corrected areas: 4536863

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050422\
Data File : VY008635.D
Acq On : 05 May 2022 01:17
Operator : KP/MD
Sample : N2619-21
Misc : 4.25g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SS10-1-2-FT

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050222S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

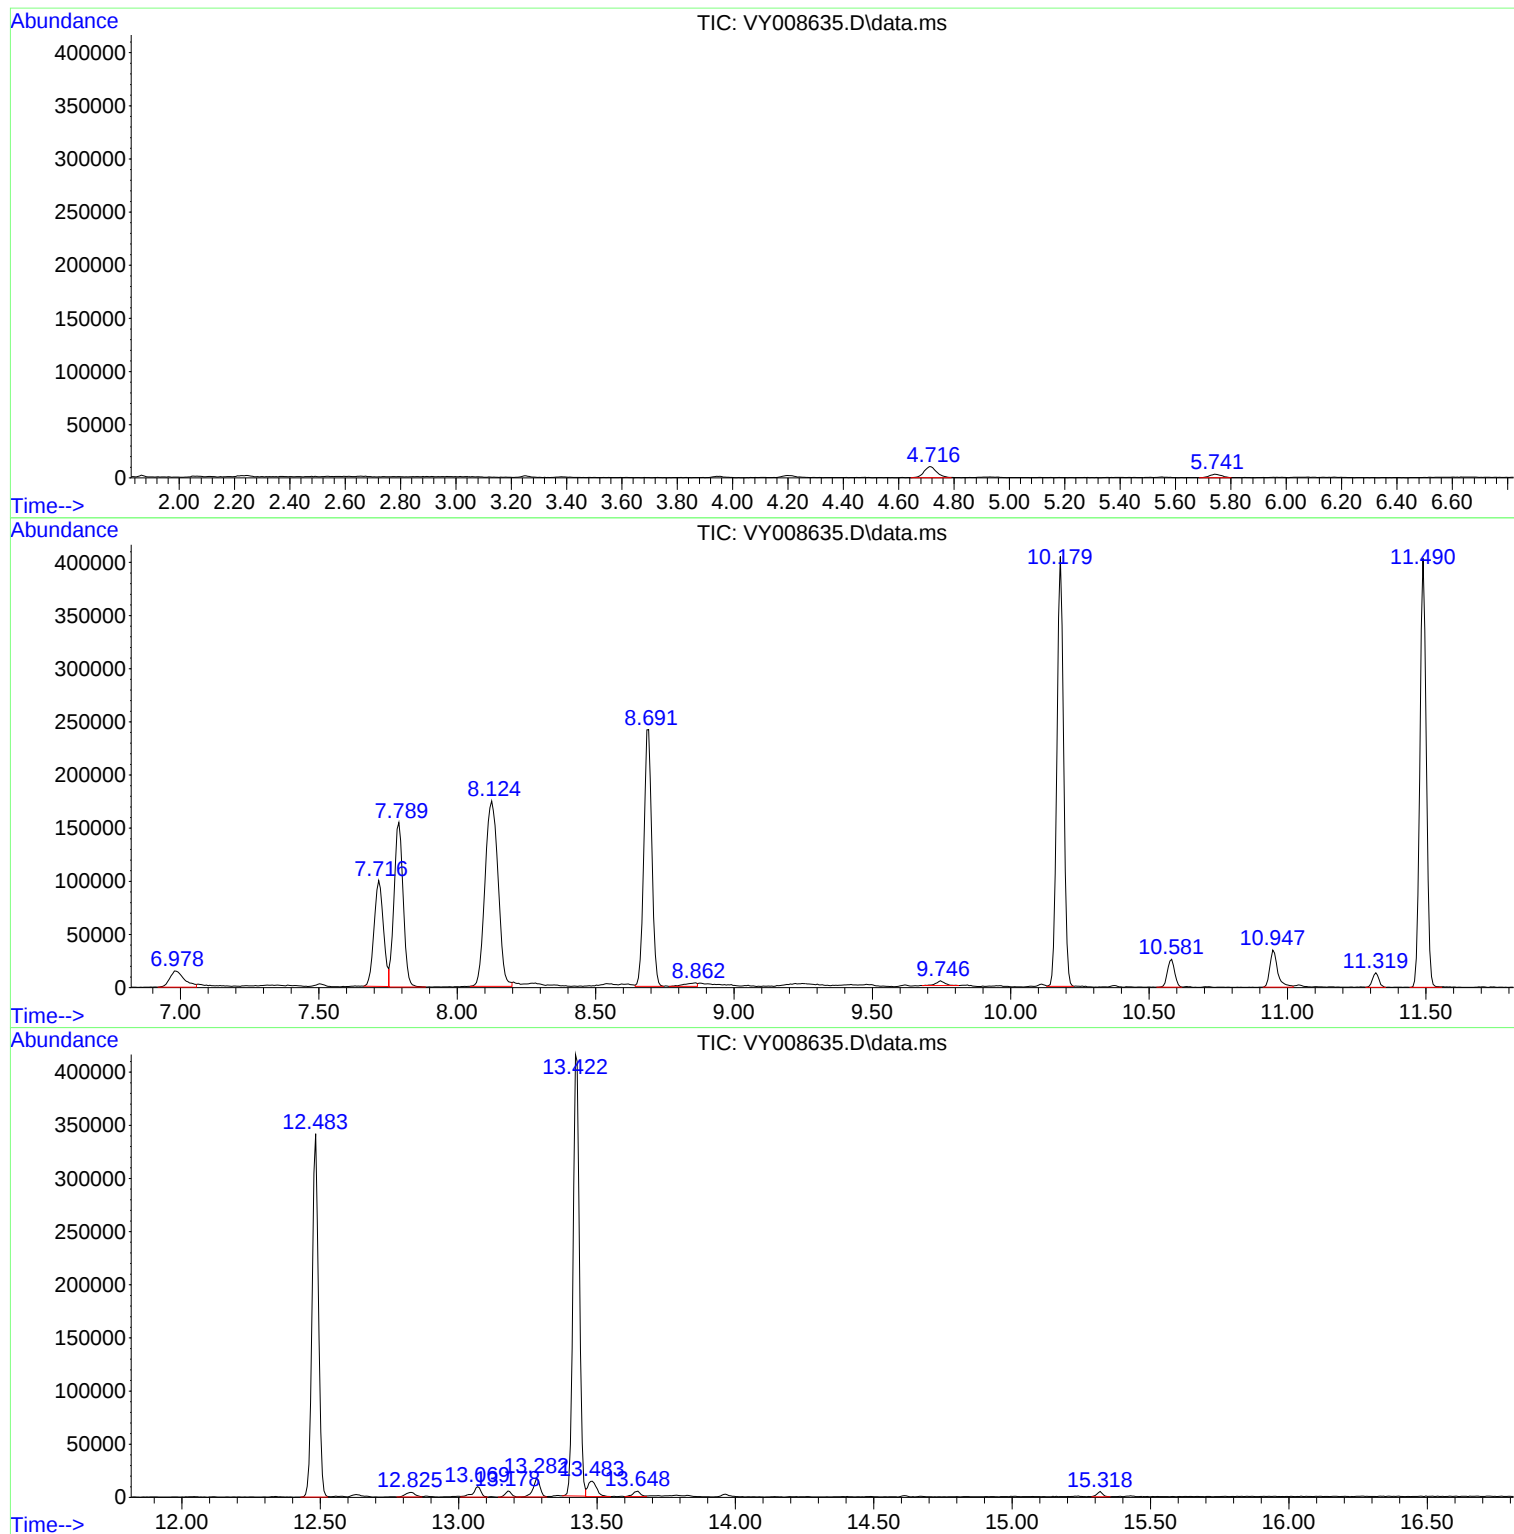

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050422\
Data File : VY008635.D
Acq On : 05 May 2022 01:17
Operator : KP/MD
Sample : N2619-21
Misc : 4.25g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SS10-1-2-FT










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050222S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown10.947 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.947	5.33 ug/l	68725	Chlorobenzene-d5	11.490

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			4-Ethylbenzoic acid, 4-methylpen...	234	C15H22O2	1000293-49-7	17
2			4-Ethylbenzoic acid, cyclohexyl ...	232	C15H20O2	1000293-32-1	12
3			Silane, diethoxydimethyl-	148	C6H16O2Si	000078-62-6	12
4			4-tert-Butyltoluene	148	C11H16	000098-51-1	12
5			Oxalamide, N-(isochroman-1-yl)me...	310	C18H18N2O3	1000304-26-0	10

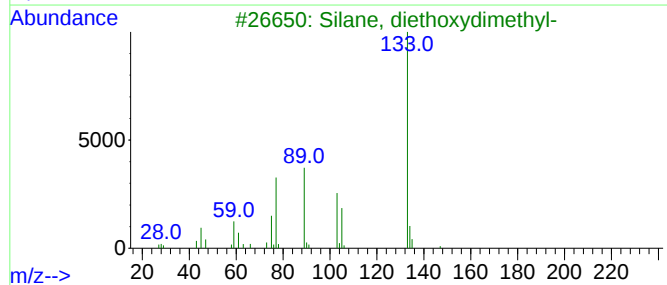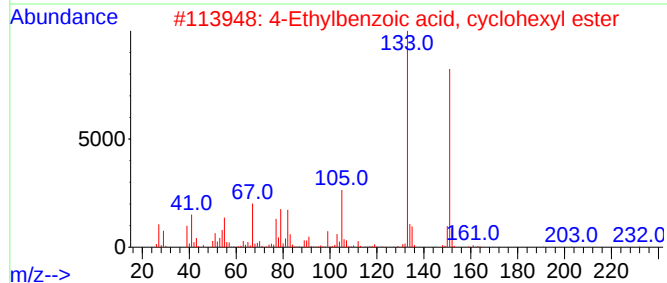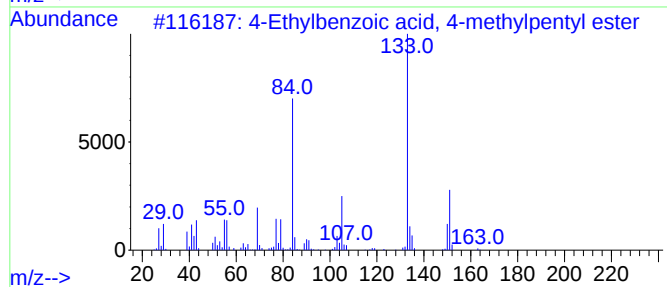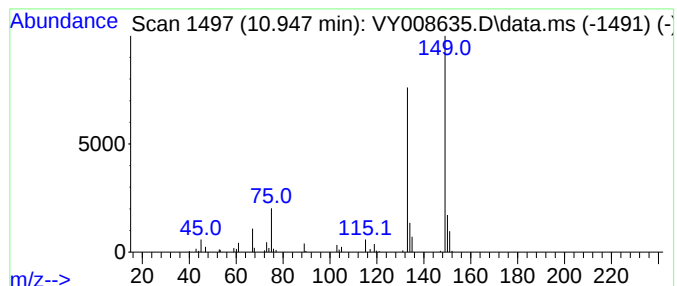

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050422\
Data File : VY008635.D
Acq On : 05 May 2022 01:17
Operator : KP/MD
Sample : N2619-21
Misc : 4.25g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SS10-1-2-FT

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050222S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown10.947	10.947	5.3	ug/l	68725	3	11.490	645031	50.0