

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050525\
 Data File : VY022158.D
 Acq On : 05 May 2025 14:45
 Operator : SY/MD
 Sample : Q1938-08
 Misc : 5.90g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 LOWER-WALL-PILE-D

Quant Time: May 06 05:21:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	233116	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	451914	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	393585	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	137265	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.060	65	115763	53.762	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	107.520%
35) Dibromofluoromethane	7.634	113	150602	50.443	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.880%
50) Toluene-d8	10.109	98	548601	48.740	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.480%
62) 4-Bromofluorobenzene	12.407	95	144387	38.106	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	76.220%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050525\
Data File : VY022158.D
Acq On : 05 May 2025 14:45
Operator : SY/MD
Sample : Q1938-08
Misc : 5.90g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
LOWER-WALL-PILE-D

Quant Time: May 06 05:21:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration



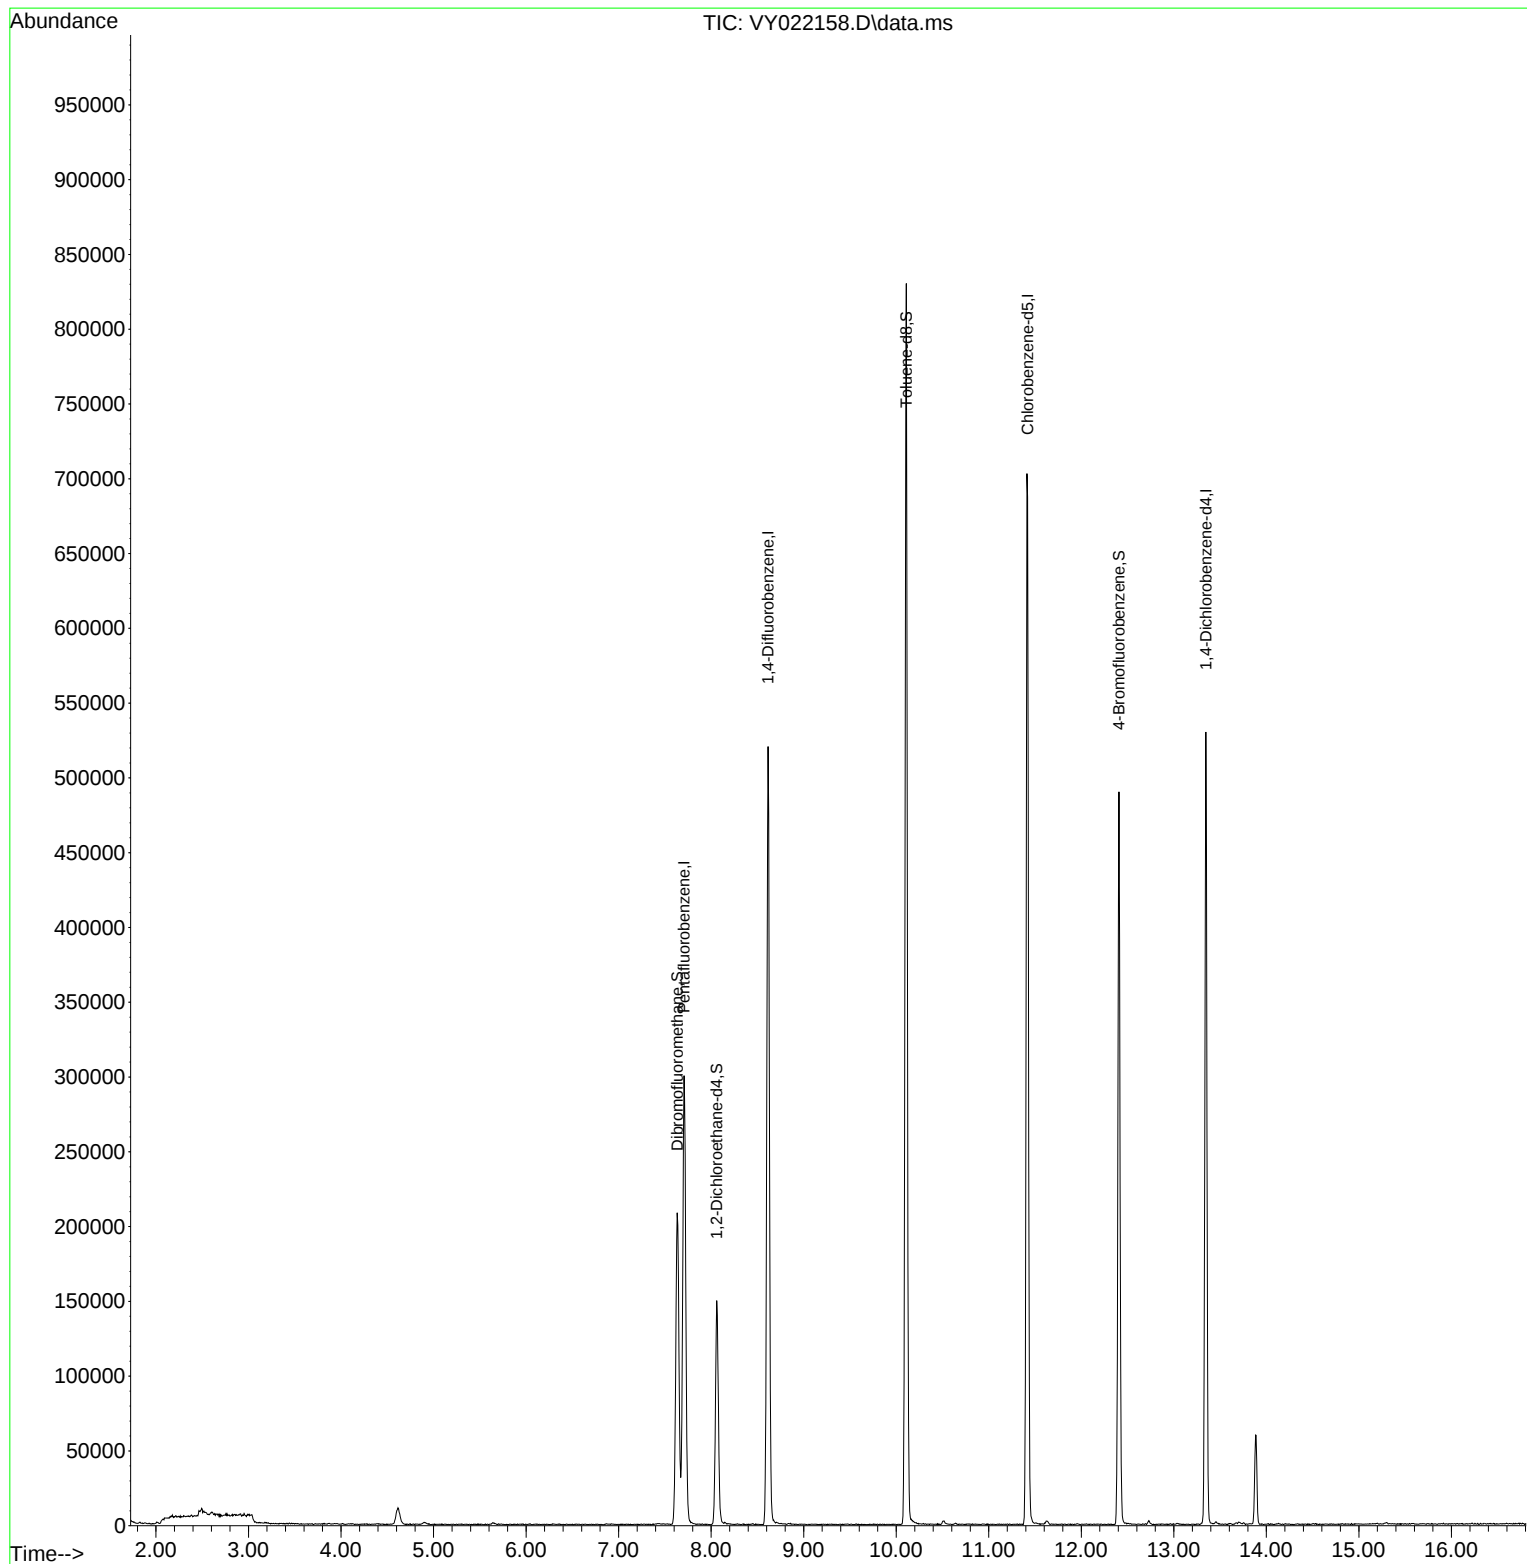




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. -0.000 min
Lab File: VY022158.D
Acq: 05 May 2025 14:45




Instrument :
MSVOA_Y
ClientSampleId :
LOWER-WALL-PILE-D

Tgt Ion:168 Resp: 233116
Ion Ratio Lower Upper
168 100
99 54.2 43.1 64.7

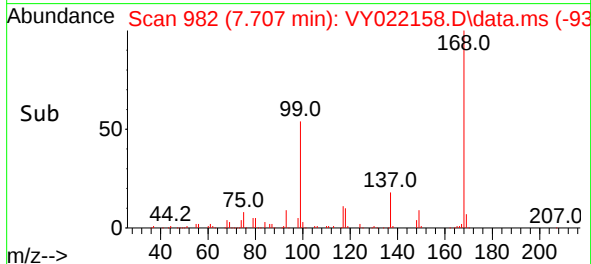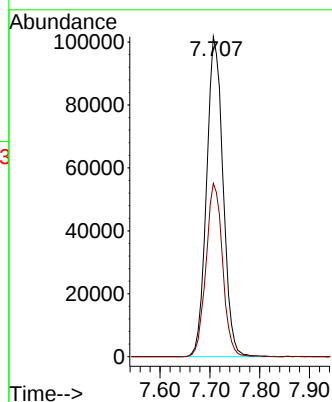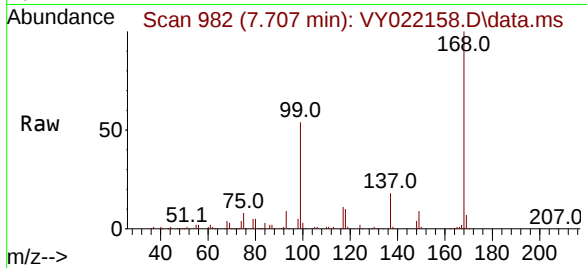

#33
1,2-Dichloroethane-d4
Concen: 53.762 ug/l
RT: 8.060 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY022158.D
Acq: 05 May 2025 14:45

Tgt Ion: 65 Resp: 115763
Ion Ratio Lower Upper
65 100
67 54.2 0.0 105.8


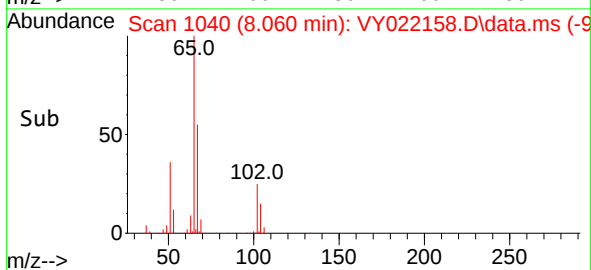
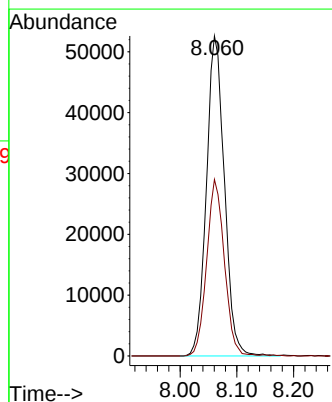
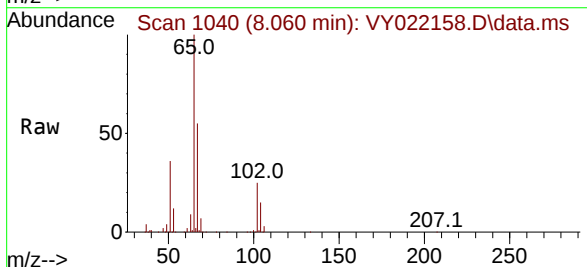




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.615 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VY022158.D
Acq: 05 May 2025 14:45




Instrument :
MSVOA_Y
ClientSampleId :
LOWER-WALL-PILE-D


Tgt Ion:114 Resp: 451914
Ion Ratio Lower Upper
114 100
63 17.7 0.0 35.4
88 14.4 0.0 28.2

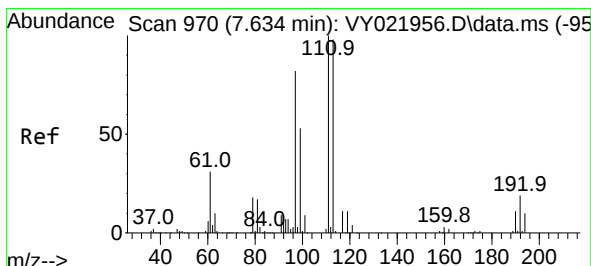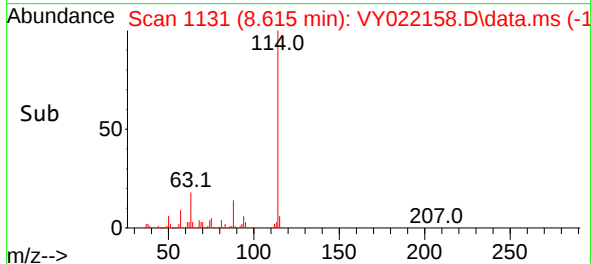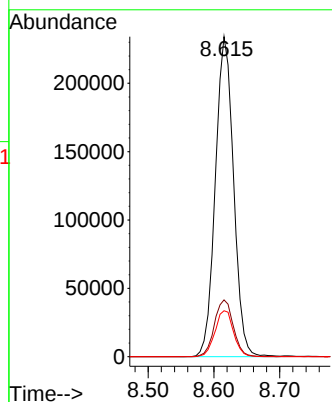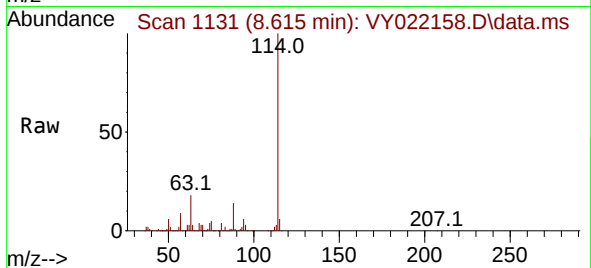

#35
Dibromofluoromethane
Concen: 50.443 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.000 min
Lab File: VY022158.D
Acq: 05 May 2025 14:45

Tgt Ion:113 Resp: 150602
Ion Ratio Lower Upper
113 100
111 102.3 81.8 122.8
192 18.9 15.6 23.4


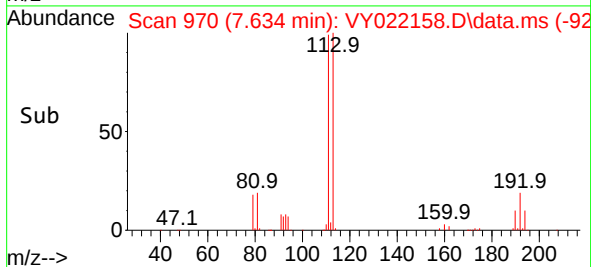
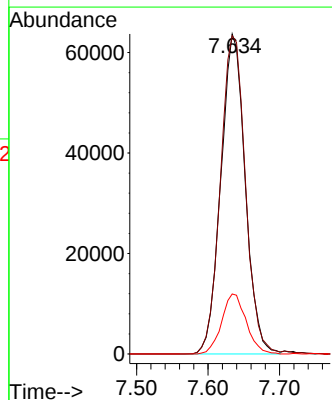
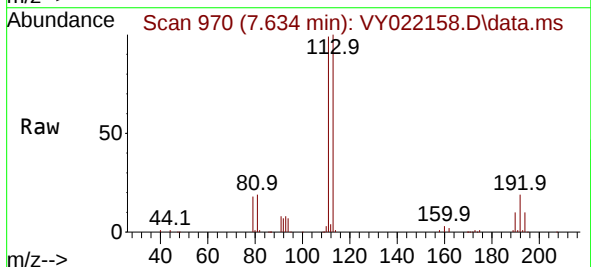


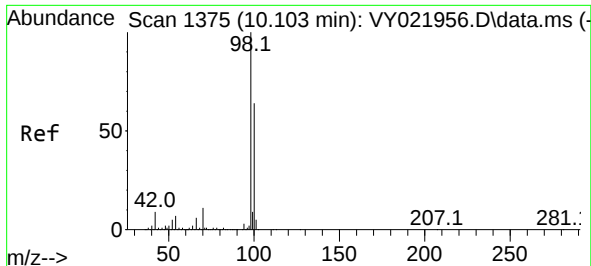

#50
Toluene-d8
Concen: 48.740 ug/l
RT: 10.109 min Scan# 1375
Delta R.T. 0.006 min
Lab File: VY022158.D
Acq: 05 May 2025 14:45




Instrument :
MSVOA_Y
ClientSampleId :
LOWER-WALL-PILE-D


Tgt Ion: 98 Resp: 548601
Ion Ratio Lower Upper
98 100
100 64.1 51.6 77.4

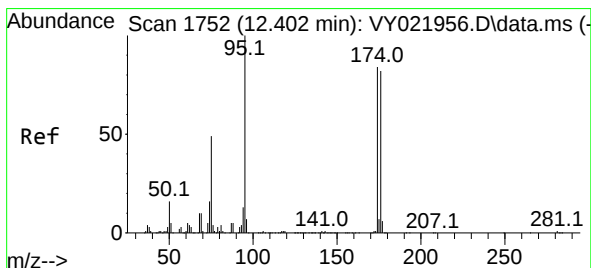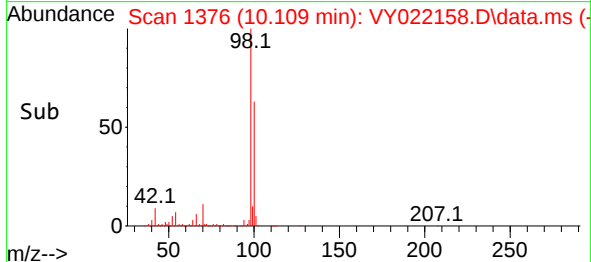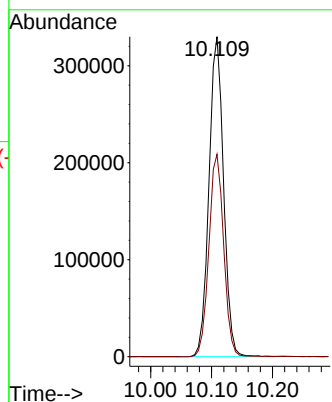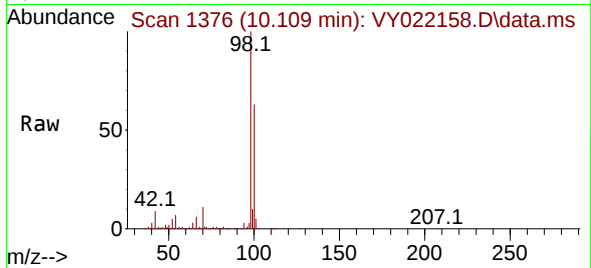

#62
4-Bromofluorobenzene
Concen: 38.106 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY022158.D
Acq: 05 May 2025 14:45

Tgt Ion: 95 Resp: 144387
Ion Ratio Lower Upper
95 100
174 87.1 0.0 179.0
176 82.5 0.0 171.8

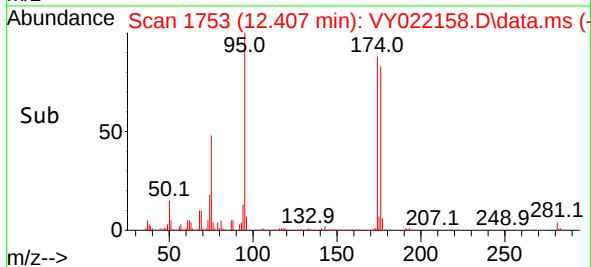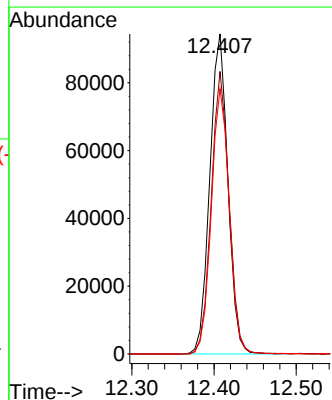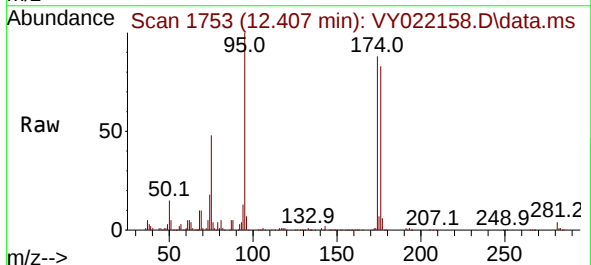

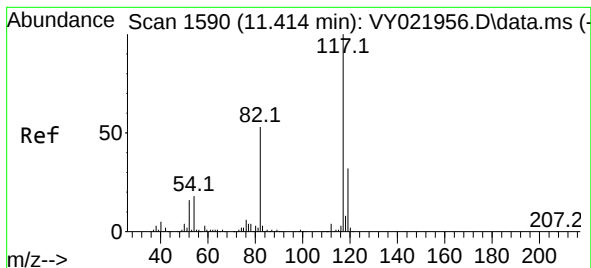

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY022158.D


Acq: 05 May 2025 14:45

Instrument :

MSVOA_Y

ClientSampleId :

LOWER-WALL-PILE-D

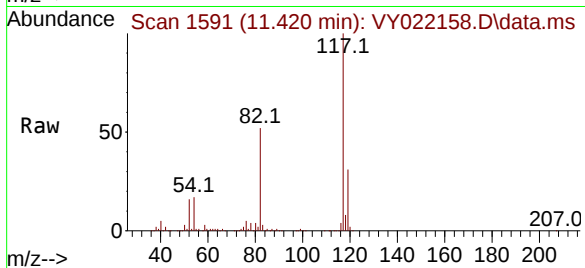




Tgt Ion:117 Resp: 393585

Ion Ratio Lower Upper

117 100

82 51.8 42.1 63.1

119 31.4 25.7 38.5

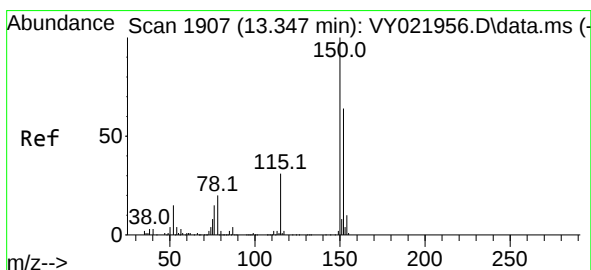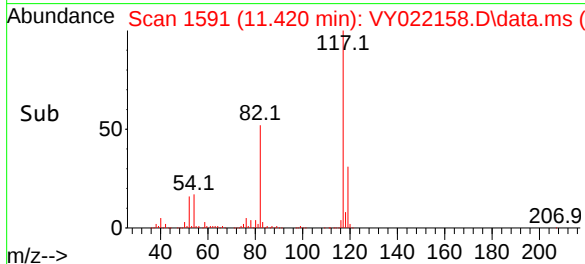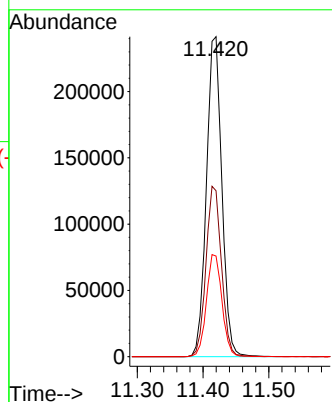

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VY022158.D

Acq: 05 May 2025 14:45

Tgt Ion:152 Resp: 137265

Ion Ratio Lower Upper

152 100

115 57.5 28.0 84.0

150 157.9 0.0 345.6

