

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050525\
 Data File : VY022159.D
 Acq On : 05 May 2025 15:08
 Operator : SY/MD
 Sample : Q1936-04
 Misc : 5.27g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SMALL-PILE-B

Quant Time: May 06 05:22:11 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	228027	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	442358	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	390377	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	141402	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	116031	55.089	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.180%
35) Dibromofluoromethane	7.634	113	147868	50.597	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.200%
50) Toluene-d8	10.109	98	540559	49.063	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	98.120%
62) 4-Bromofluorobenzene	12.407	95	142934	38.537	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	77.080%
Target Compounds						
					Qvalue	
20) Methylene Chloride	4.610	84	9959	3.739	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050525\
Data File : VY022159.D
Acq On : 05 May 2025 15:08
Operator : SY/MD
Sample : Q1936-04
Misc : 5.27g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SMALL-PILE-B

Quant Time: May 06 05:22:11 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration




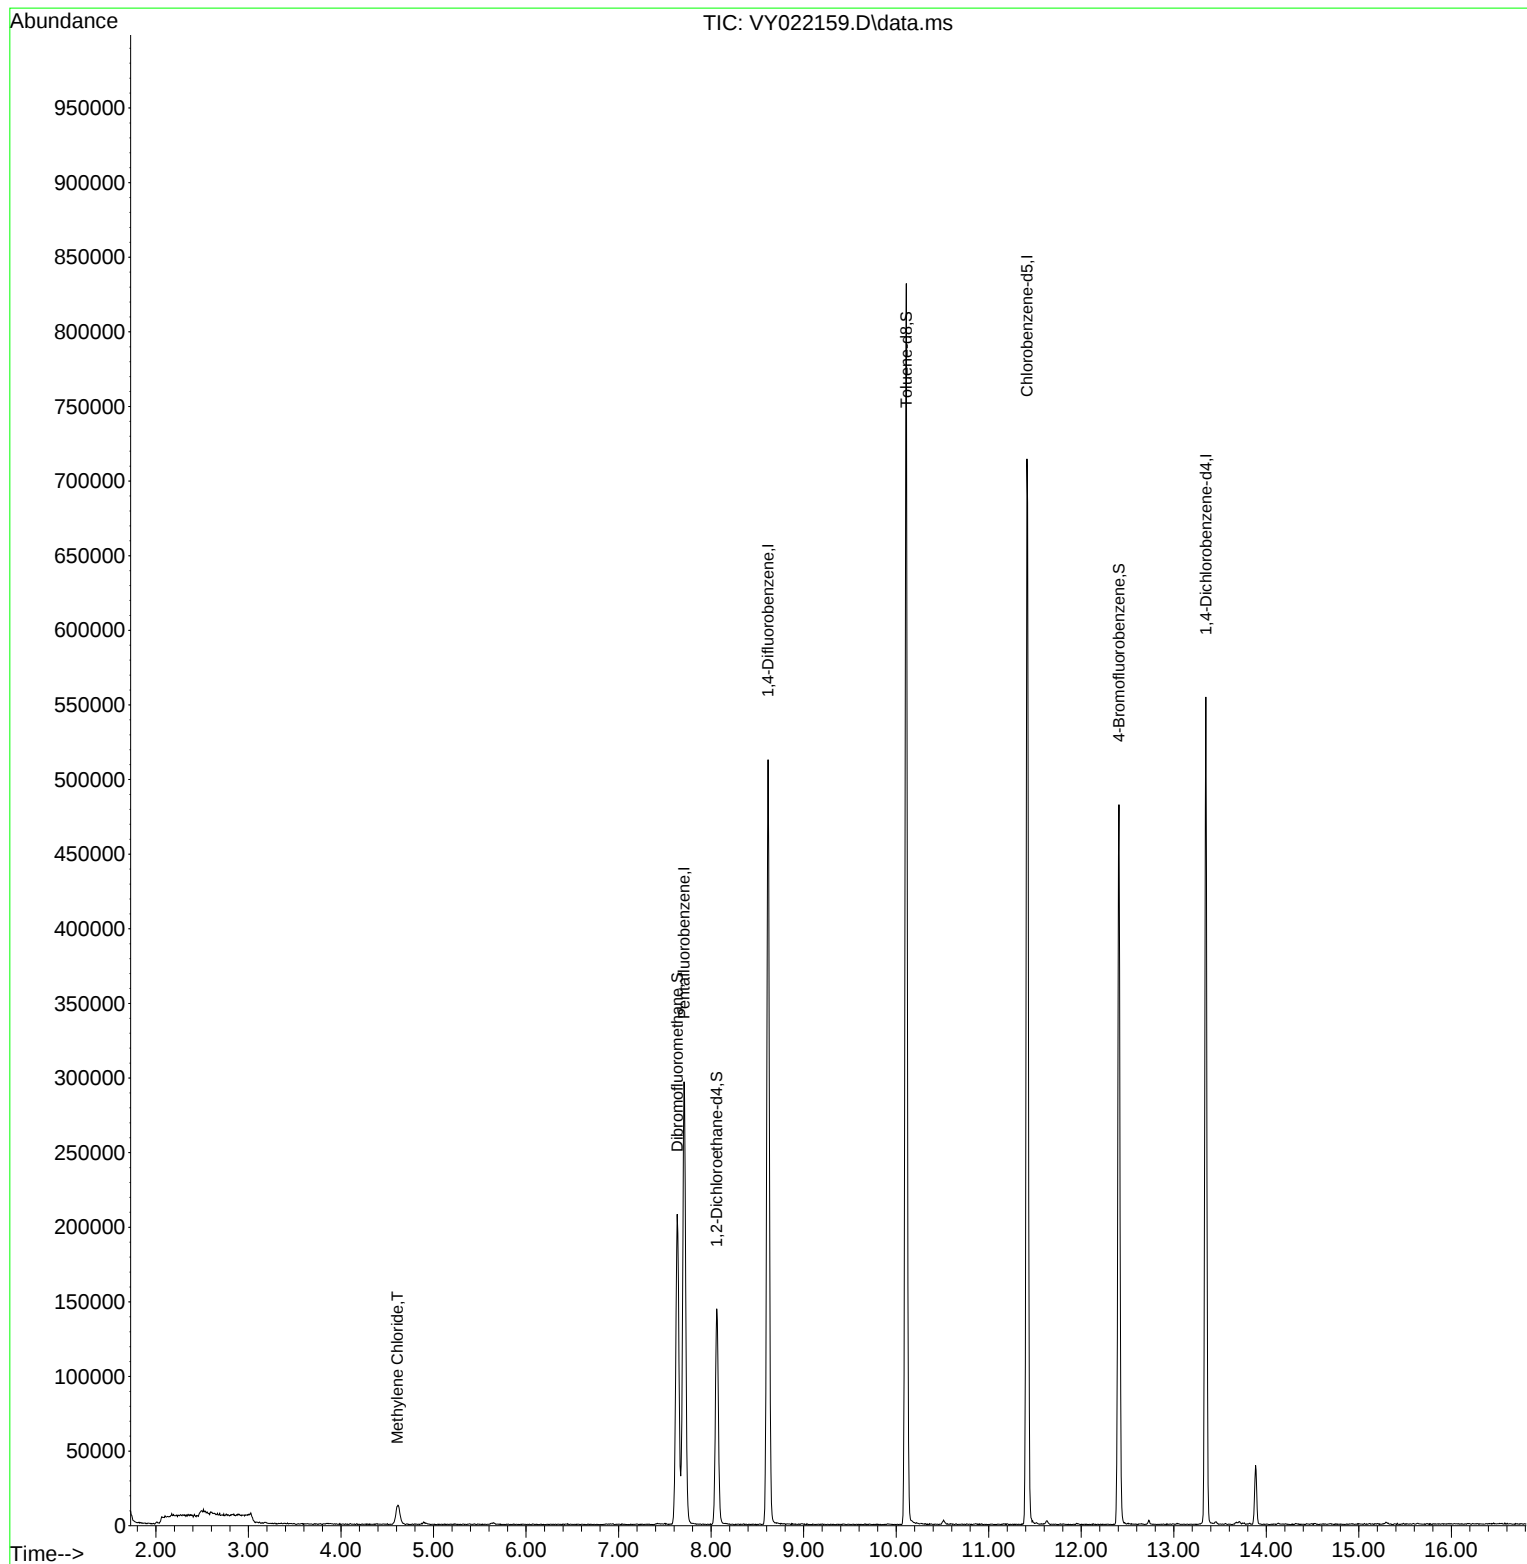


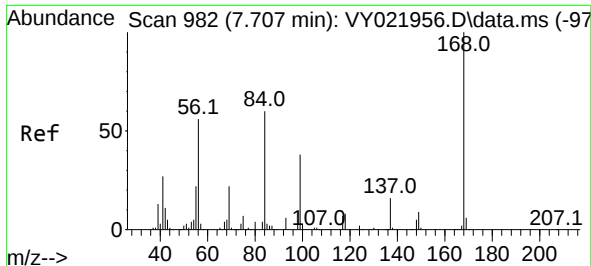

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY022159.D
Acq: 05 May 2025 15:08




Instrument :
MSVOA_Y
ClientSampleId :
SMALL-PILE-B


Tgt Ion:168 Resp: 228027
Ion Ratio Lower Upper
168 100
99 57.5 43.1 64.7

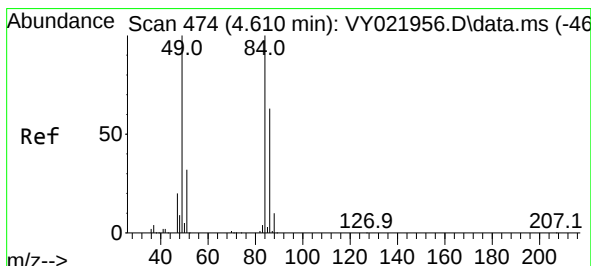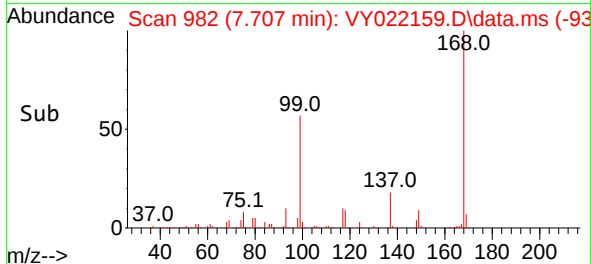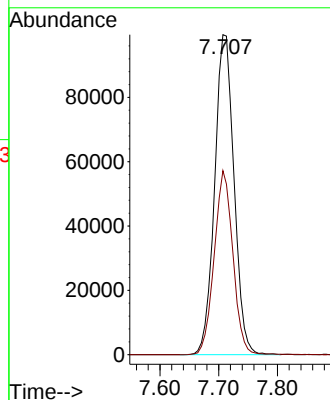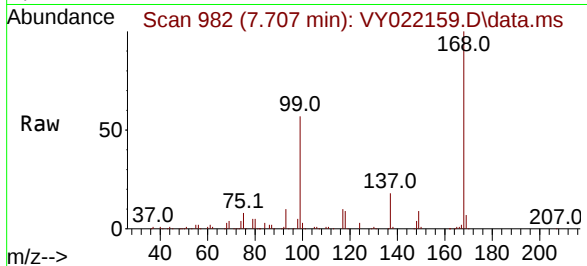

#20
Methylene Chloride
Concen: 3.739 ug/l
RT: 4.610 min Scan# 474
Delta R.T. -0.000 min
Lab File: VY022159.D
Acq: 05 May 2025 15:08

Tgt Ion: 84 Resp: 9959
Ion Ratio Lower Upper
84 100
49 105.3 79.9 119.9
51 31.0 25.4 38.0
86 69.2 50.6 76.0

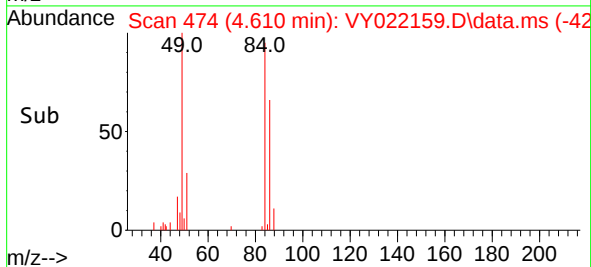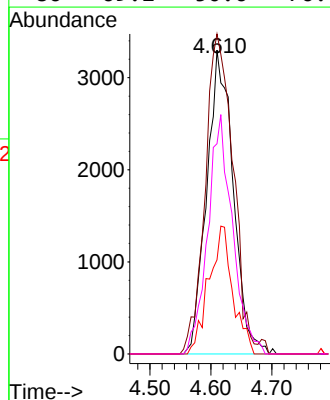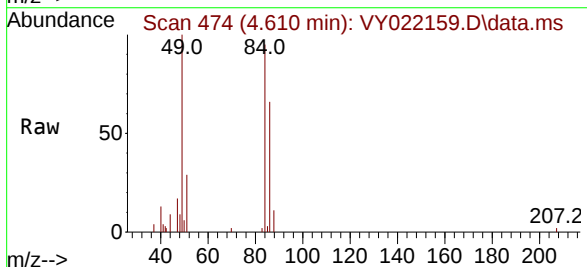

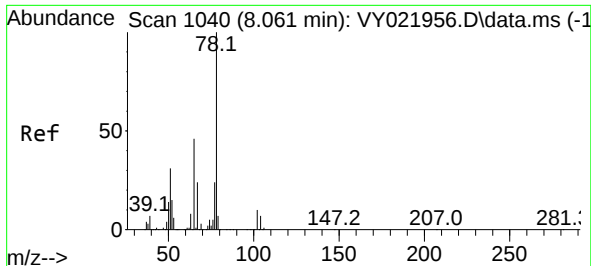

#33

1,2-Dichloroethane-d4

Concen: 55.089 ug/l

RT: 8.061 min Scan# 11040

Delta R.T. -0.000 min

Lab File: VY022159.D

Acq: 05 May 2025 15:08

Instrument :

MSVOA_Y

ClientSampleId :





SMALL-PILE-B

Tgt Ion: 65 Resp: 116031

Ion Ratio Lower Upper

65 100

67 53.0 0.0 105.8

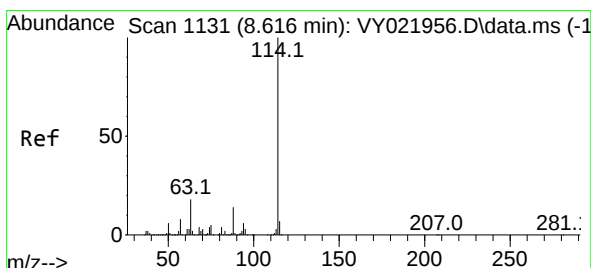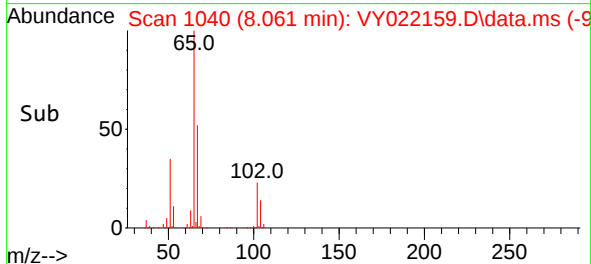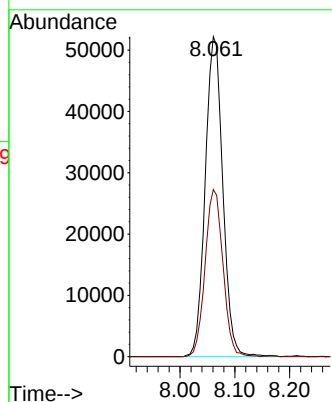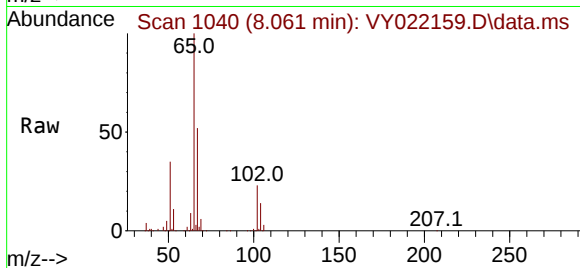

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.615 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VY022159.D

Acq: 05 May 2025 15:08




Tgt Ion:114 Resp: 442358


Ion Ratio Lower Upper

114 100

63 17.7 0.0 35.4

88 15.0 0.0 28.2


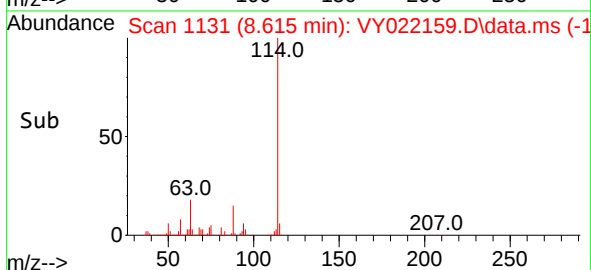
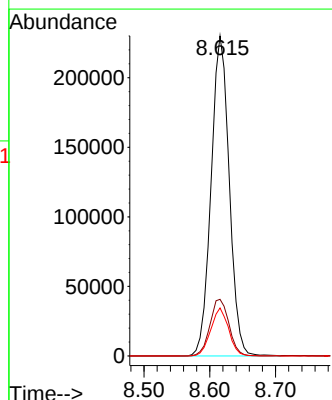
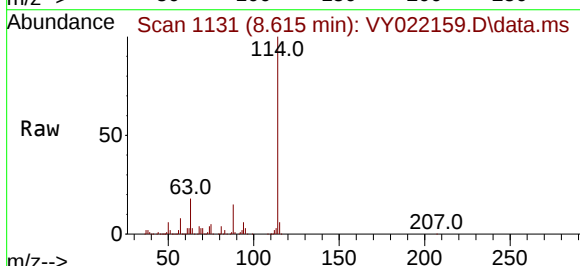


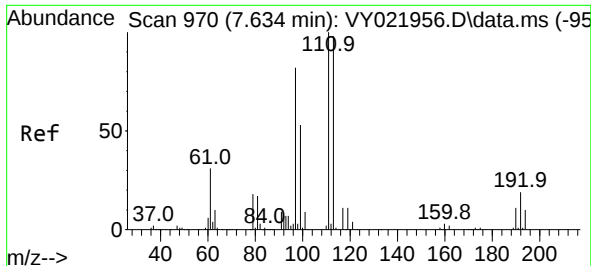

#35
Dibromofluoromethane
Concen: 50.597 ug/l
RT: 7.634 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY022159.D
Acq: 05 May 2025 15:08




Instrument :
MSVOA_Y
ClientSampleId :
SMALL-PILE-B


Tgt Ion:113 Resp: 147868
Ion Ratio Lower Upper
113 100
111 102.2 81.8 122.8
192 19.7 15.6 23.4

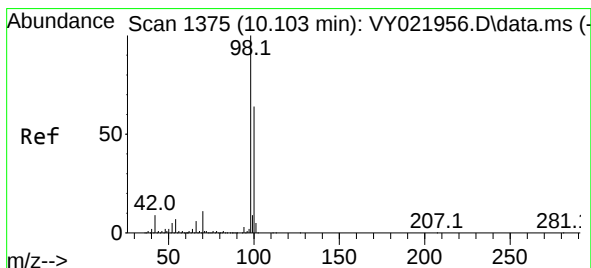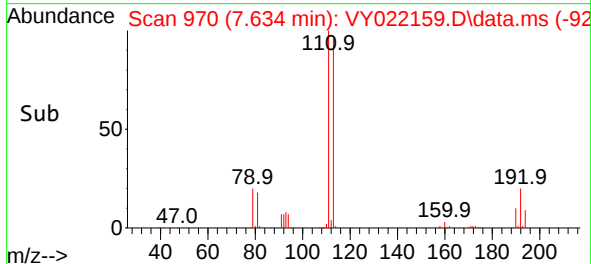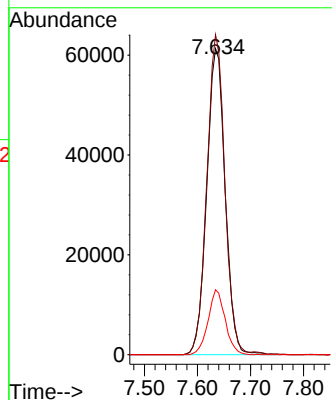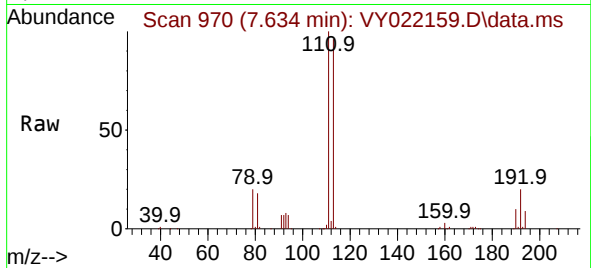

#50
Toluene-d8
Concen: 49.063 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.006 min
Lab File: VY022159.D
Acq: 05 May 2025 15:08

Tgt Ion: 98 Resp: 540559
Ion Ratio Lower Upper
98 100
100 64.2 51.6 77.4


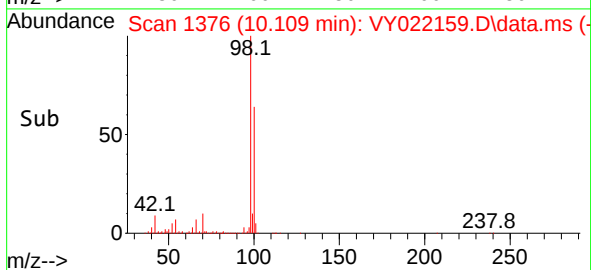
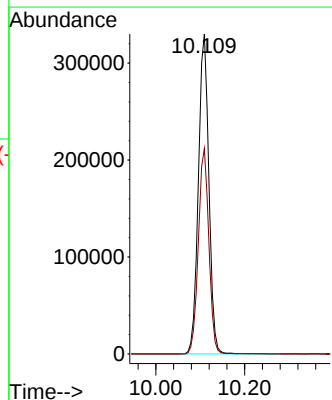
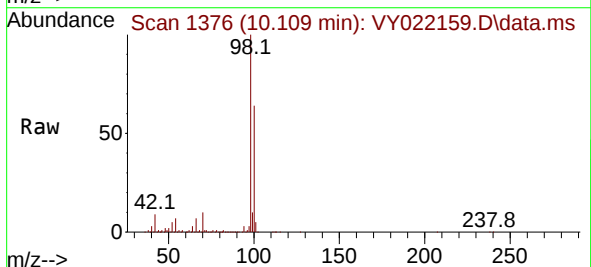


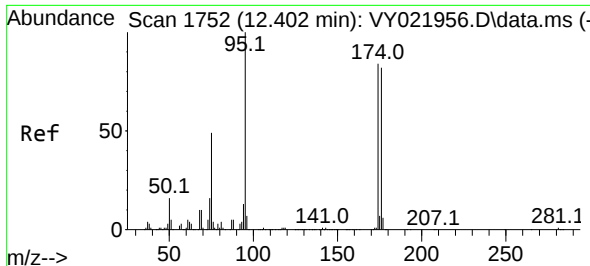

#62
4-Bromofluorobenzene
Concen: 38.537 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY022159.D
Acq: 05 May 2025 15:08




Instrument :
MSVOA_Y
ClientSampleId :
SMALL-PILE-B


Tgt Ion: 95 Resp: 142934
Ion Ratio Lower Upper
95 100
174 88.5 0.0 179.0
176 85.5 0.0 171.8

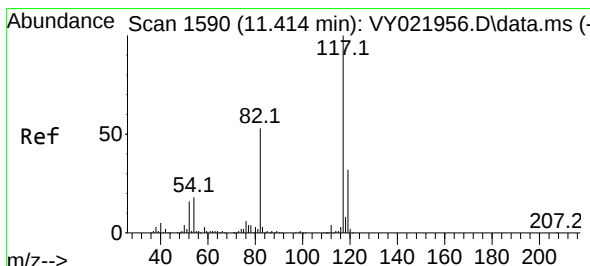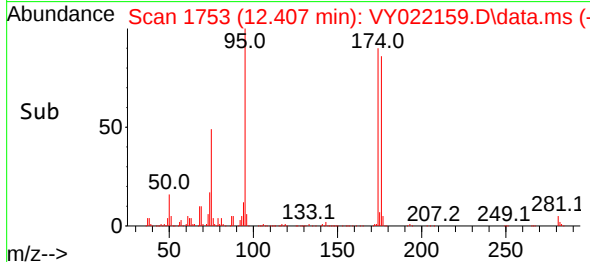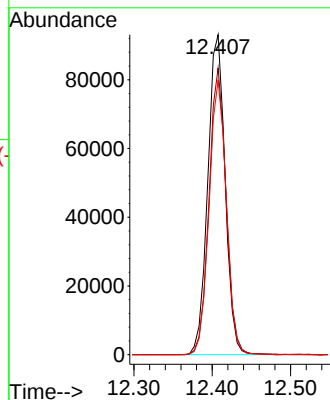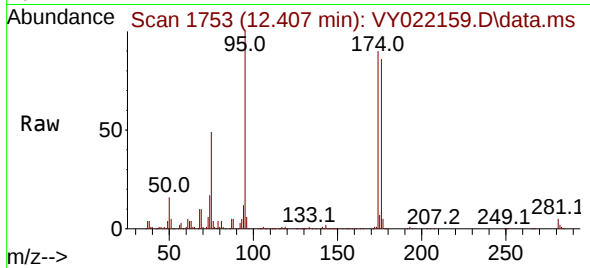

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 1590
Delta R.T. -0.000 min
Lab File: VY022159.D
Acq: 05 May 2025 15:08

Tgt Ion: 117 Resp: 390377
Ion Ratio Lower Upper
117 100
82 54.8 42.1 63.1
119 32.6 25.7 38.5

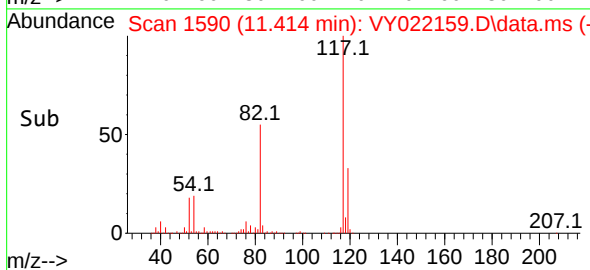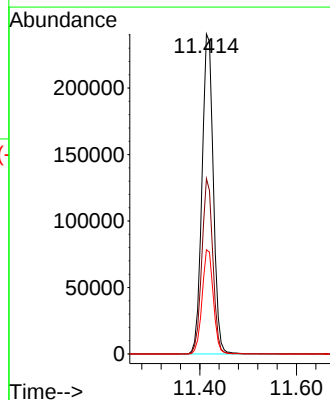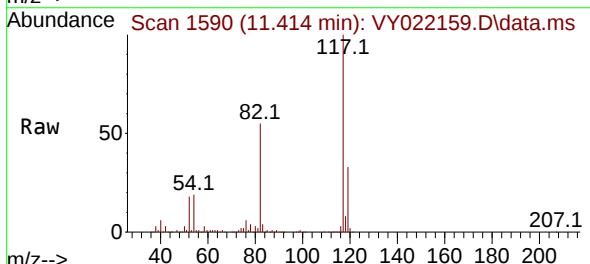

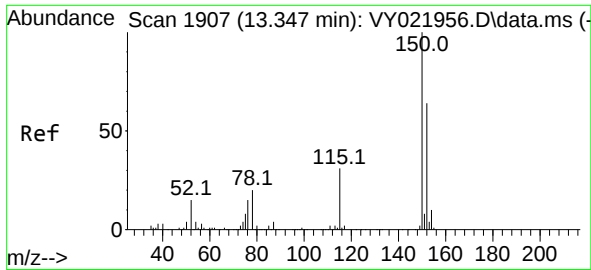

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 1907
 Delta R.T. -0.000 min
 Lab File: VY022159.D
 Acq: 05 May 2025 15:08

Instrument :
 MSVOA_Y
 ClientSampleId :
 SMALL-PILE-B

Tgt Ion:152 Resp: 141402
 Ion Ratio Lower Upper
 152 100
 115 56.8 28.0 84.0
 150 156.8 0.0 345.6

