
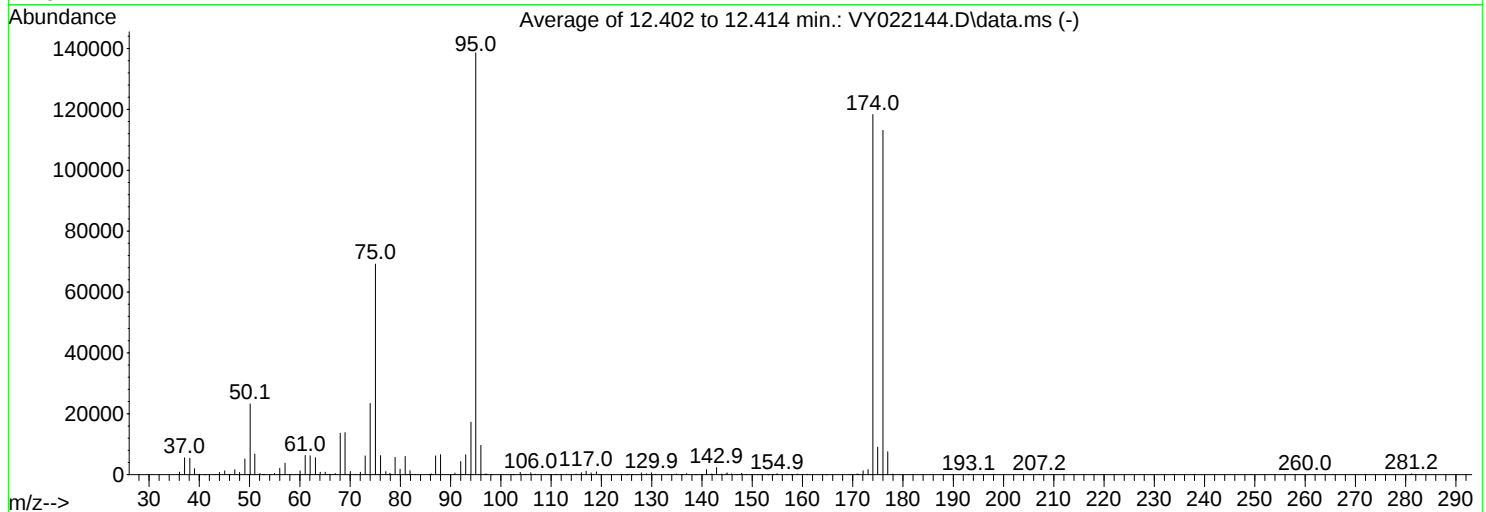


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050525\
Data File : VY022144.D
Acq On : 05 May 2025 08:15
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Title : SW846 8260
Last Update : Wed Apr 23 02:30:30 2025

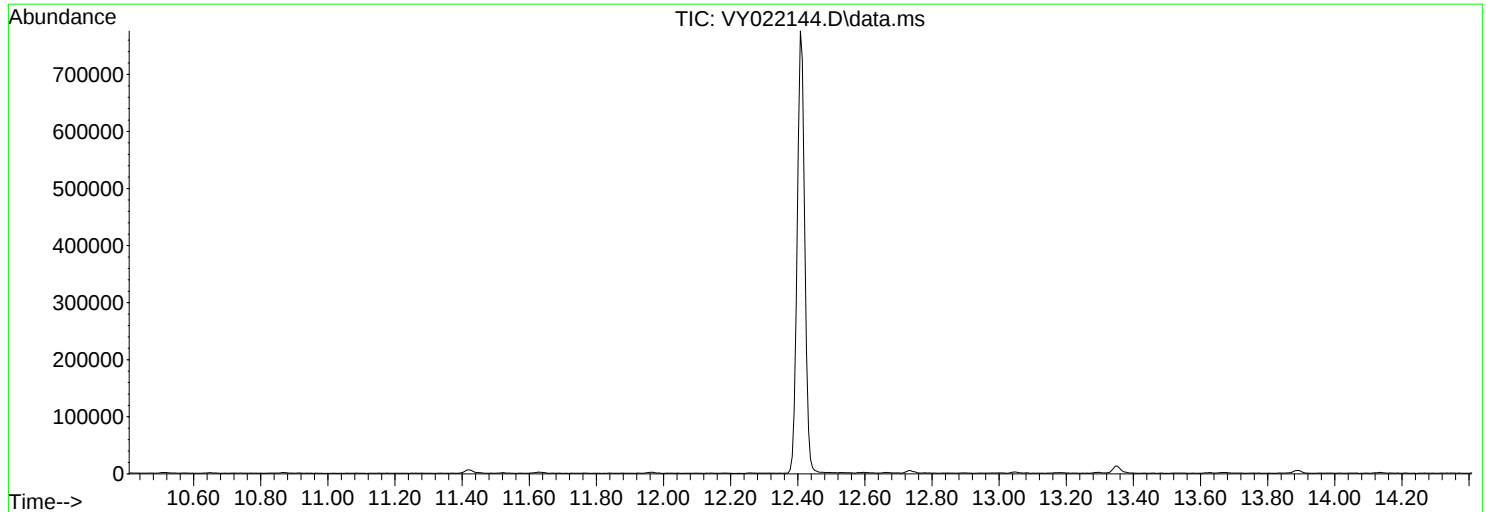

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	23243	PASS
75	95	30	60	49.9	69173	PASS
95	95	100	100	100.0	138573	PASS
96	95	5	9	7.0	9645	PASS
173	174	0.00	2	1.4	1687	PASS
174	95	50	100	85.4	118339	PASS
175	174	5	9	7.7	9061	PASS
176	174	95	101	95.6	113131	PASS
177	176	5	9	6.7	7536	PASS