
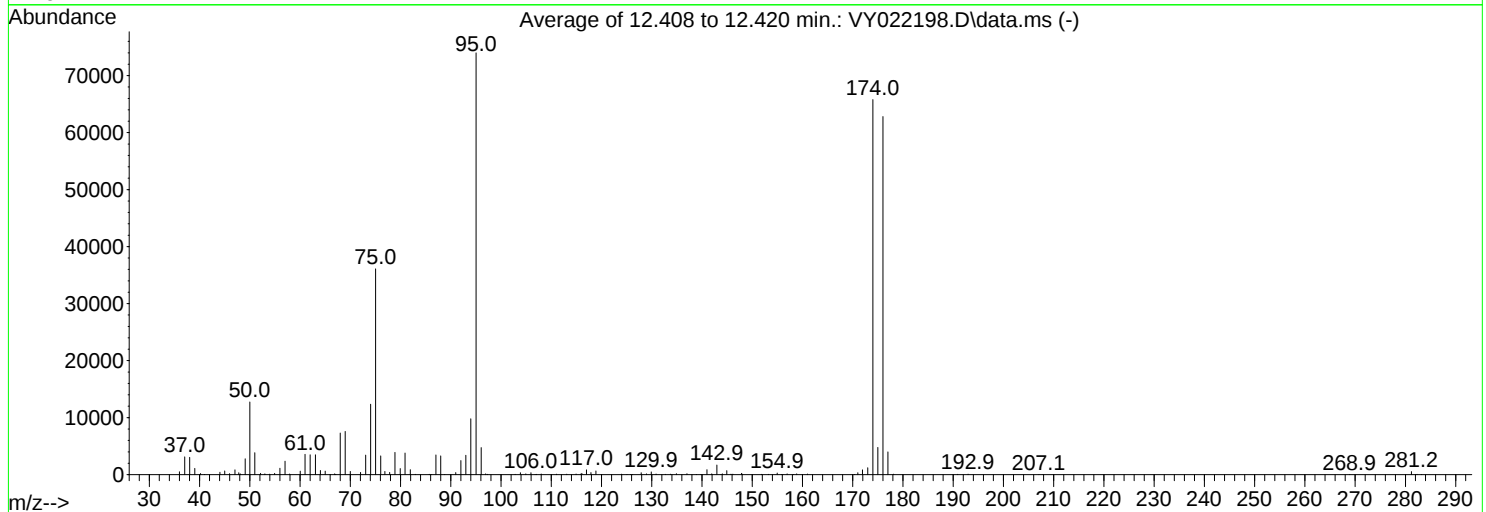


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050825\
Data File : VY022198.D
Acq On : 08 May 2025 08:06
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Title : SW846 8260
Last Update : Wed Apr 23 02:30:30 2025

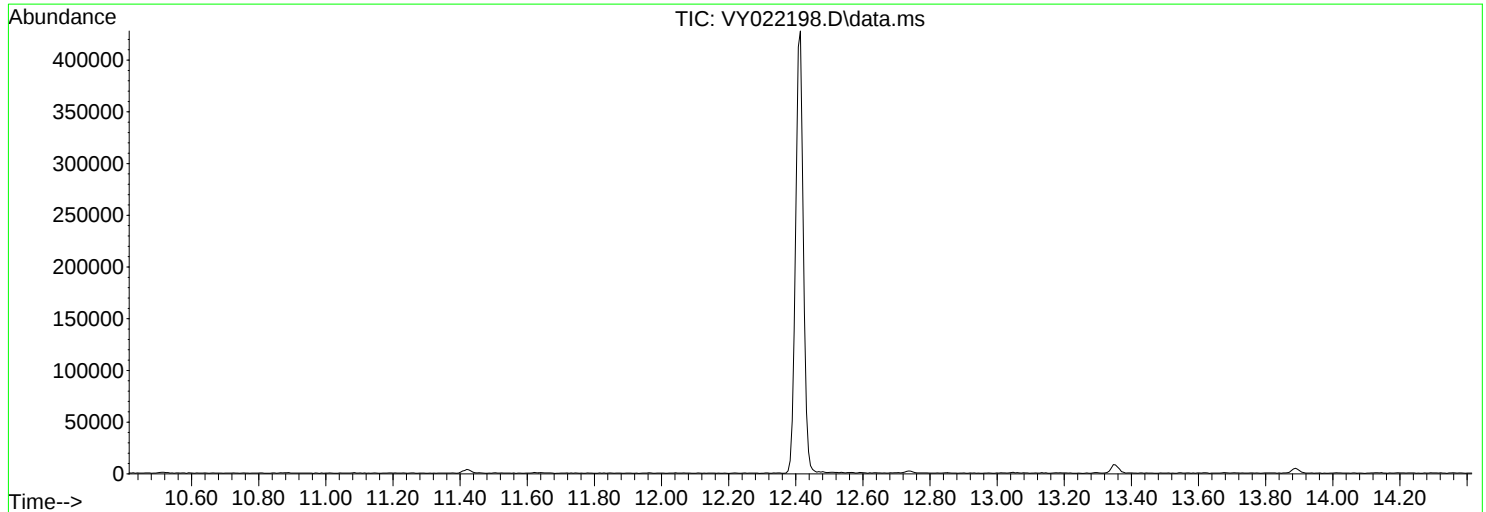

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	12741	PASS
75	95	30	60	48.8	36093	PASS
95	95	100	100	100.0	73995	PASS
96	95	5	9	6.4	4758	PASS
173	174	0.00	2	1.8	1198	PASS
174	95	50	100	88.9	65784	PASS
175	174	5	9	7.2	4767	PASS
176	174	95	101	95.5	62827	PASS
177	176	5	9	6.4	3999	PASS