

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051022\
 Data File : VY008692.D
 Acq On : 10 May 2022 20:04
 Operator : KP/MD
 Sample : N2762-07
 Misc : 5.04g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB17

Quant Time: May 11 04:35:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050922S.M
 Quant Title : SW846 8260
 QLast Update : Mon May 09 19:21:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	29528	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	43267	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	34812	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	13386	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	10642	42.061	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	84.120%
35) Dibromofluoromethane	7.716	113	13519	50.703	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.400%
50) Toluene-d8	10.179	98	47114	50.143	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	100.280%
62) 4-Bromofluorobenzene	12.483	95	12055	35.662	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	71.320%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051022\
Data File : VY008692.D
Acq On : 10 May 2022 20:04
Operator : KP/MD
Sample : N2762-07
Misc : 5.04g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB17

Quant Time: May 11 04:35:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050922S.M
Quant Title : SW846 8260
QLast Update : Mon May 09 19:21:20 2022
Response via : Initial Calibration




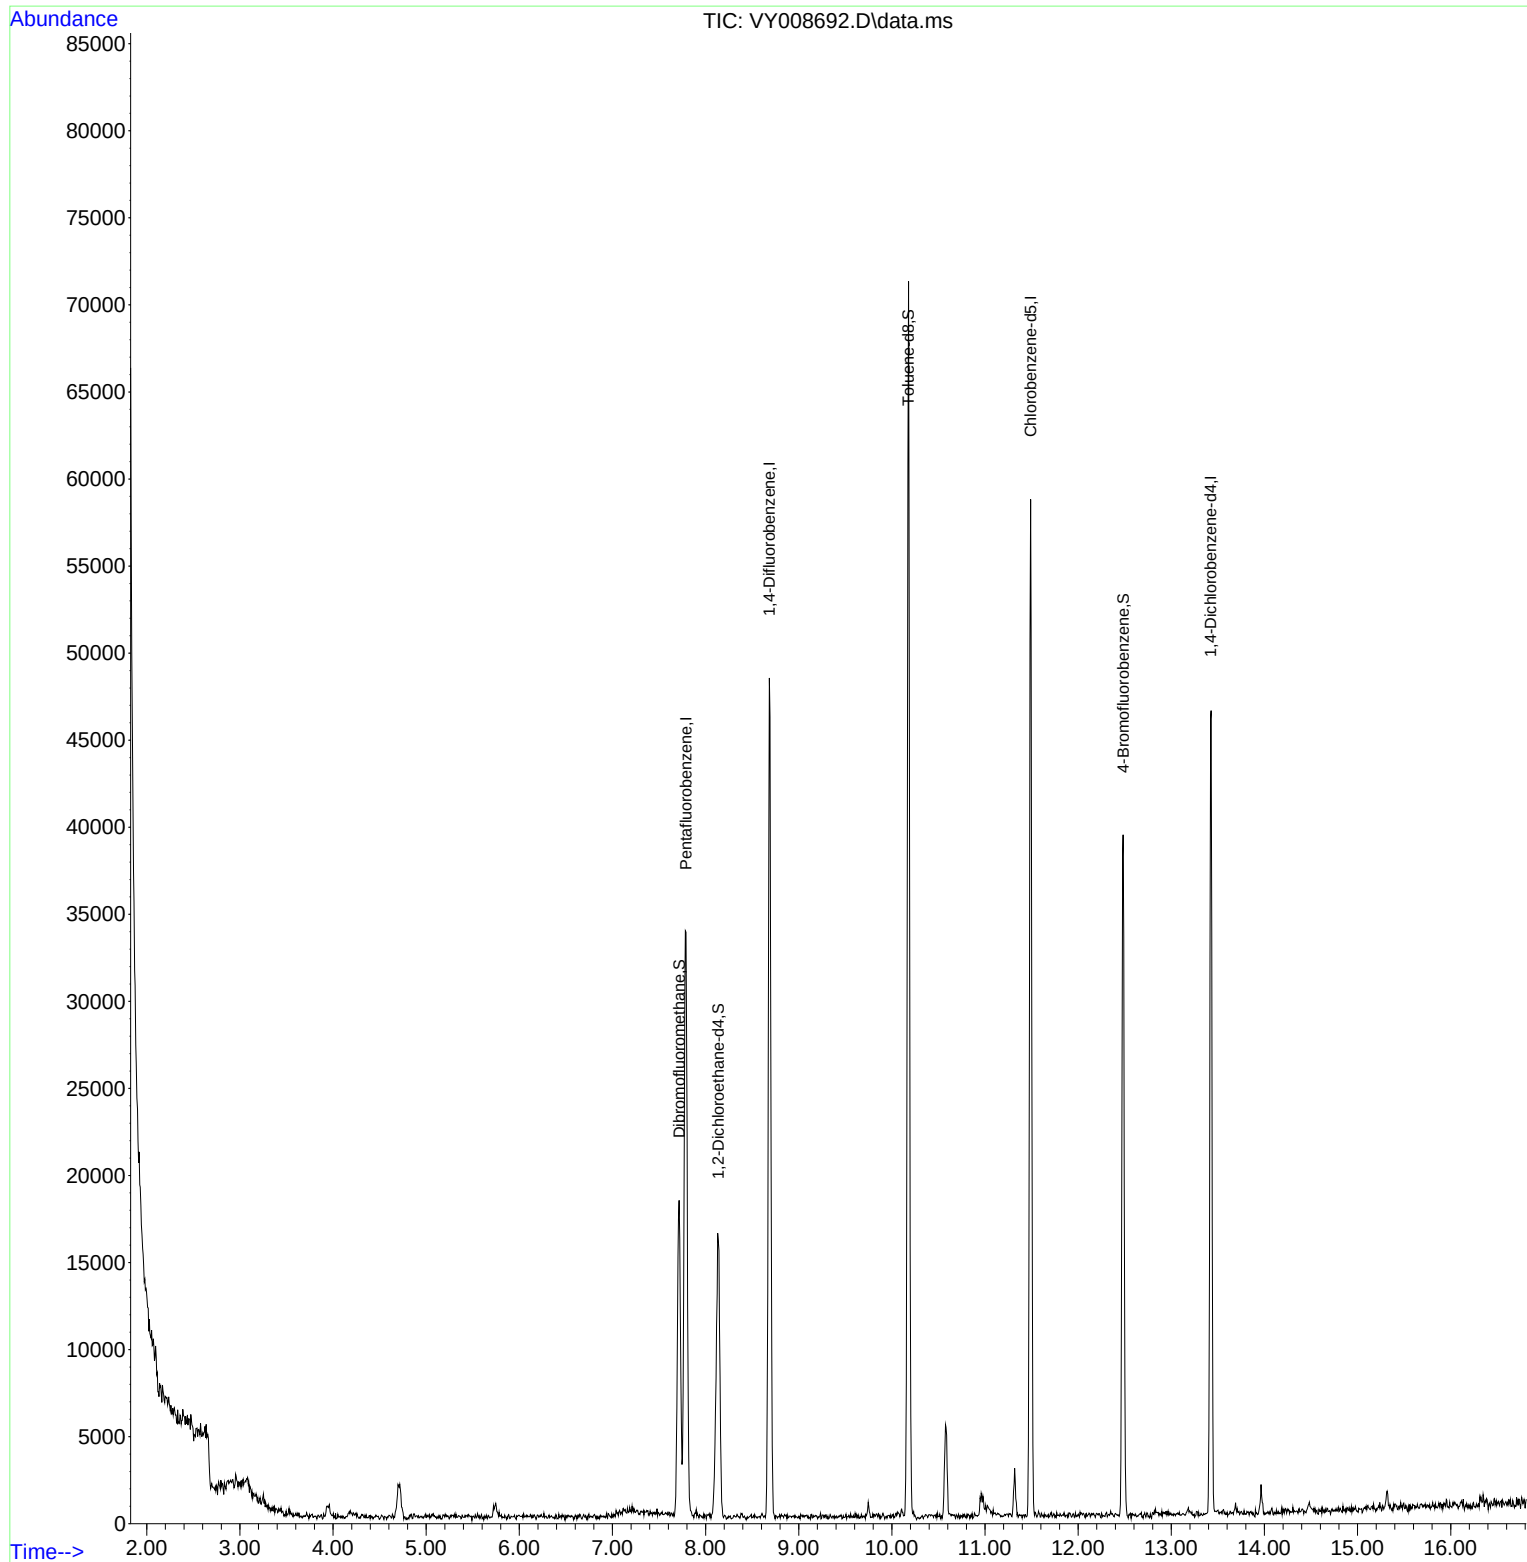


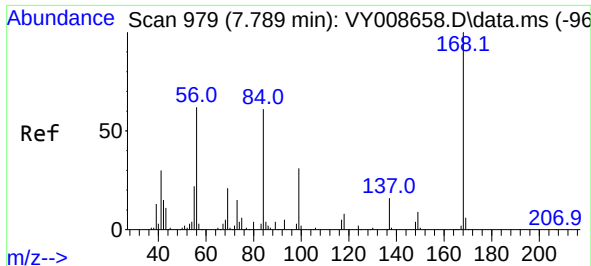

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008692.D
Acq: 10 May 2022 20:04




Instrument :
MSVOA_Y
ClientSampleId :
SB17


Tgt Ion:168 Resp: 29528
Ion Ratio Lower Upper
168 100
99 49.8 46.9 70.3

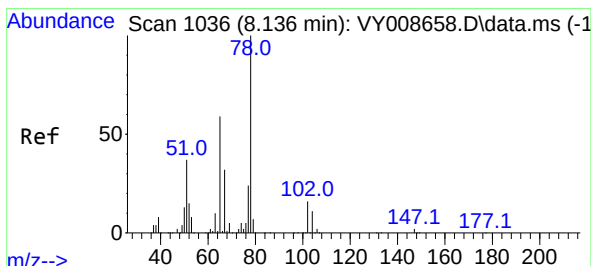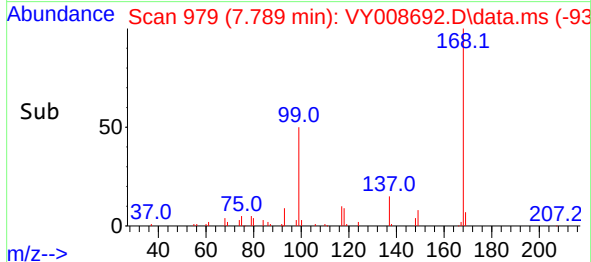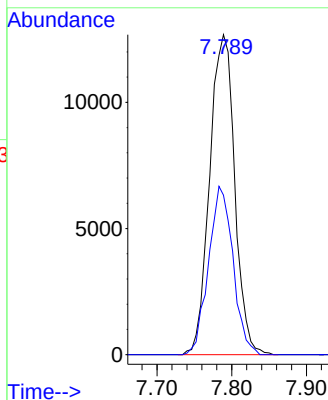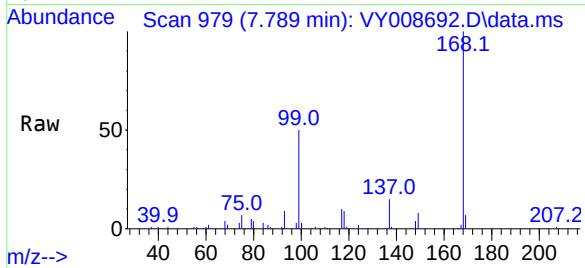

#33
1,2-Dichloroethane-d4
Concen: 42.061 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY008692.D
Acq: 10 May 2022 20:04

Tgt Ion: 65 Resp: 10642
Ion Ratio Lower Upper
65 100
67 57.0 0.0 99.4

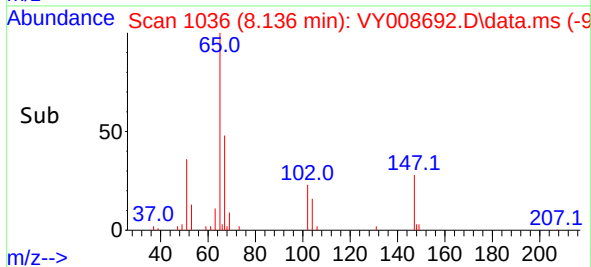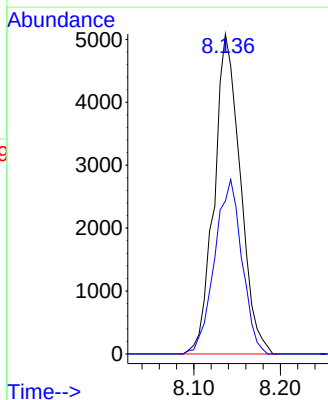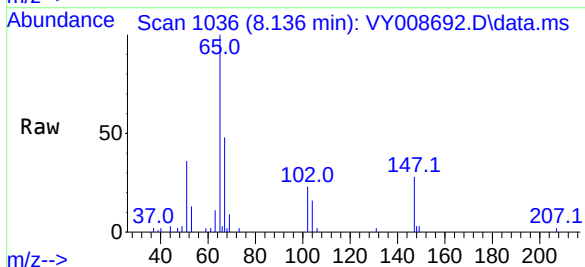

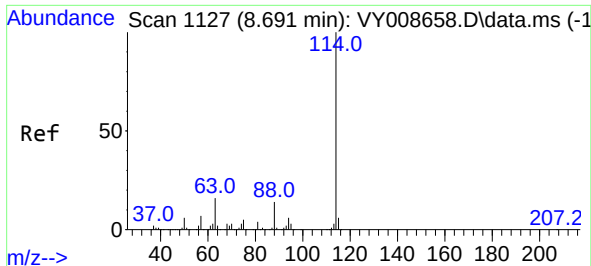

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY008692.D

Acq: 10 May 2022 20:04

Instrument :

MSVOA_Y

ClientSampleId :

SB17





Tgt Ion:114 Resp: 43267

Ion Ratio Lower Upper

114 100

63 18.2 0.0 43.2

88 15.2 0.0 31.8

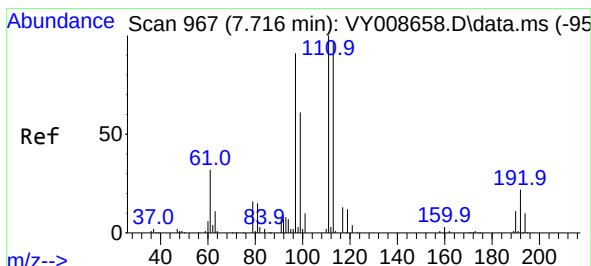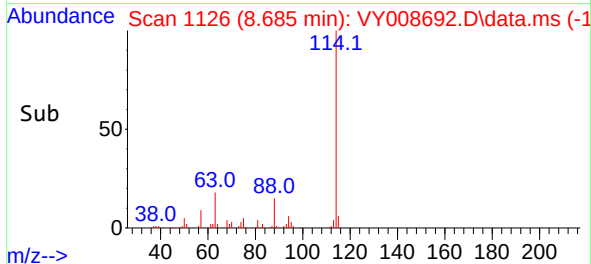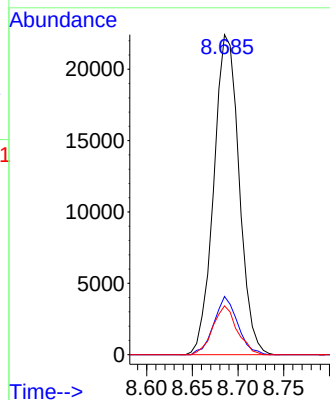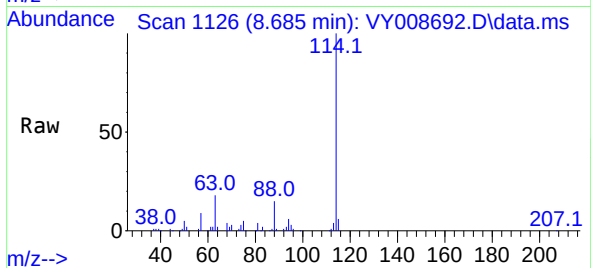

#35

Dibromofluoromethane

Concen: 50.703 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY008692.D

Acq: 10 May 2022 20:04




Tgt Ion:113 Resp: 13519


Ion Ratio Lower Upper

113 100

111 100.8 82.6 124.0

192 19.7 17.6 26.4


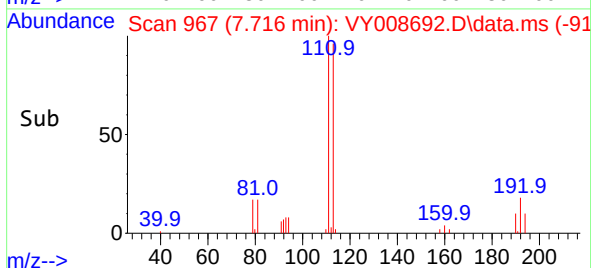
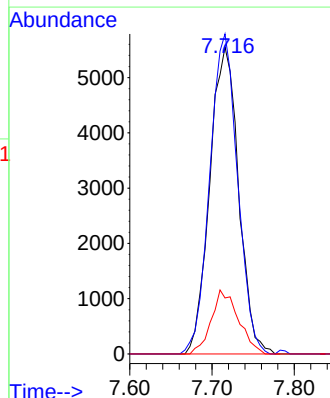
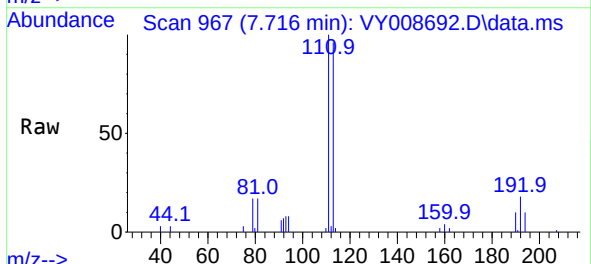


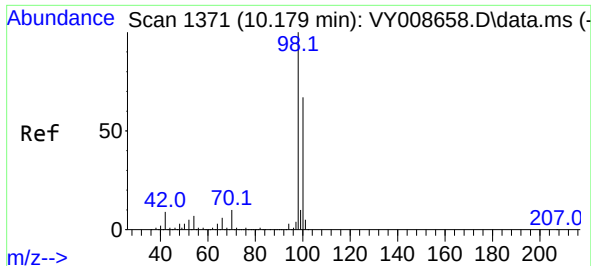

#50
Toluene-d8
Concen: 50.143 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY008692.D
Acq: 10 May 2022 20:04




Instrument :
MSVOA_Y
ClientSampleId :
SB17


Tgt Ion: 98 Resp: 47114
Ion Ratio Lower Upper
98 100
100 64.7 50.2 75.2

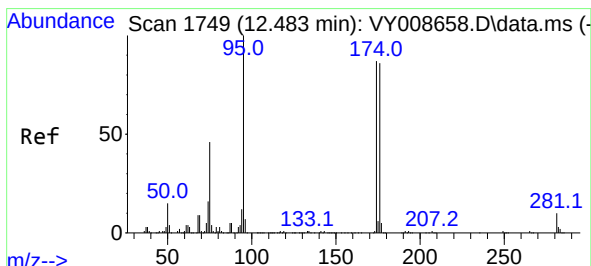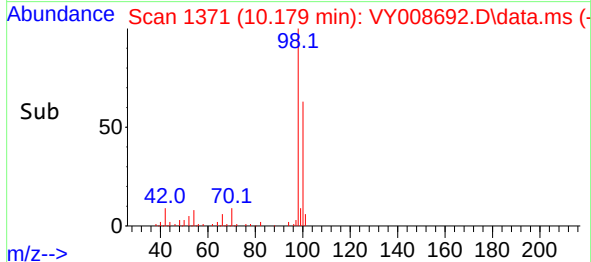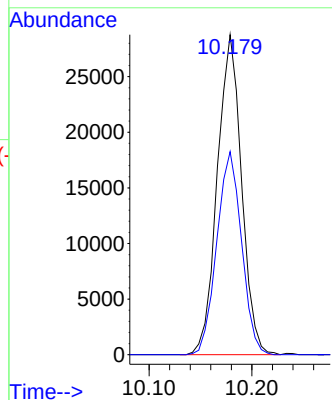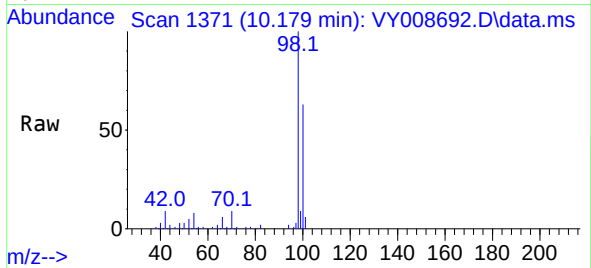

#62
4-Bromofluorobenzene
Concen: 35.662 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008692.D
Acq: 10 May 2022 20:04

Tgt Ion: 95 Resp: 12055
Ion Ratio Lower Upper
95 100
174 92.7 0.0 177.0
176 92.0 0.0 175.8


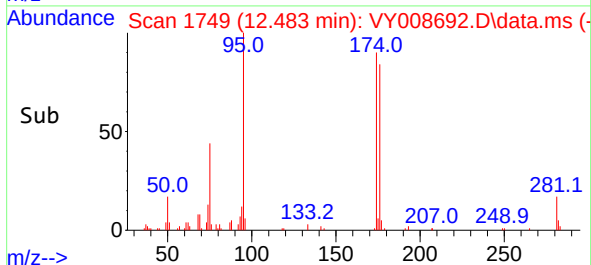
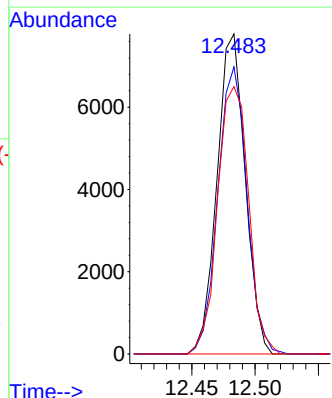
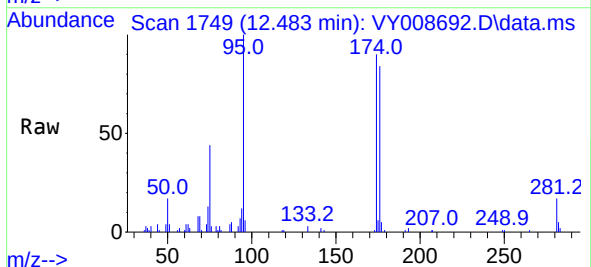


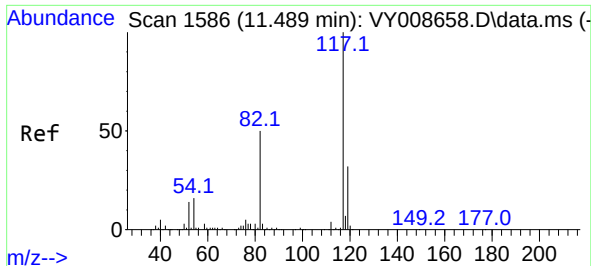

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY008692.D
Acq: 10 May 2022 20:04

Instrument :
MSVOA_Y
ClientSampleId :
SB17

Tgt Ion:	117	Resp:	34812
Ion	Ratio	Lower	Upper
117	100		
82	51.6	43.0	64.4
119	30.8	25.4	38.0

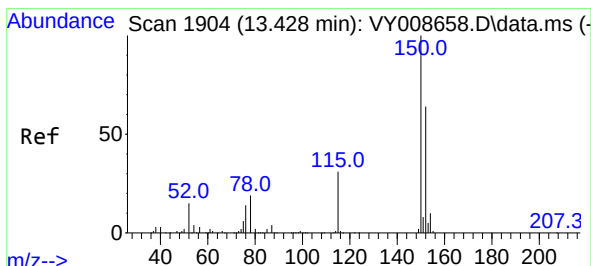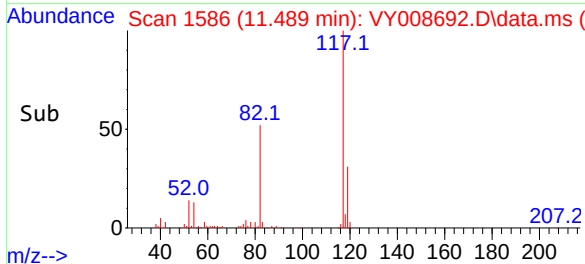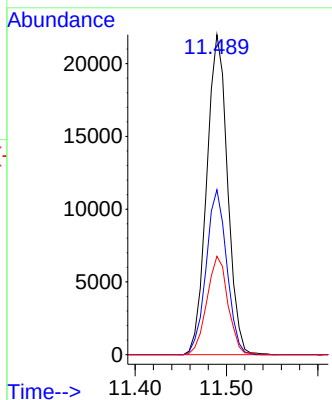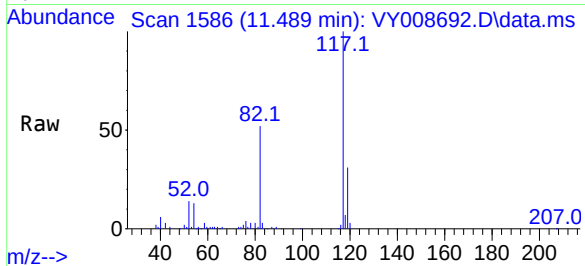

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY008692.D
Acq: 10 May 2022 20:04

Tgt Ion:	152	Resp:	13386
Ion	Ratio	Lower	Upper
152	100		
115	55.8	28.2	84.7
150	160.5	0.0	347.6

