

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051225\
 Data File : VY022223.D
 Acq On : 12 May 2025 14:40
 Operator : SY/MD
 Sample : Q1986-01
 Misc : 5.03g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 COMP-8

Quant Time: May 13 02:20:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	138038	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	245564	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	212412	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	81409	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	77020	60.406	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	120.820%
35) Dibromofluoromethane	7.628	113	89356	55.079	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.160%
50) Toluene-d8	10.109	98	294509	48.153	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.300%
62) 4-Bromofluorobenzene	12.402	95	74668	36.265	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	72.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051225\
Data File : VY022223.D
Acq On : 12 May 2025 14:40
Operator : SY/MD
Sample : Q1986-01
Misc : 5.03g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
COMP-8

Quant Time: May 13 02:20:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration




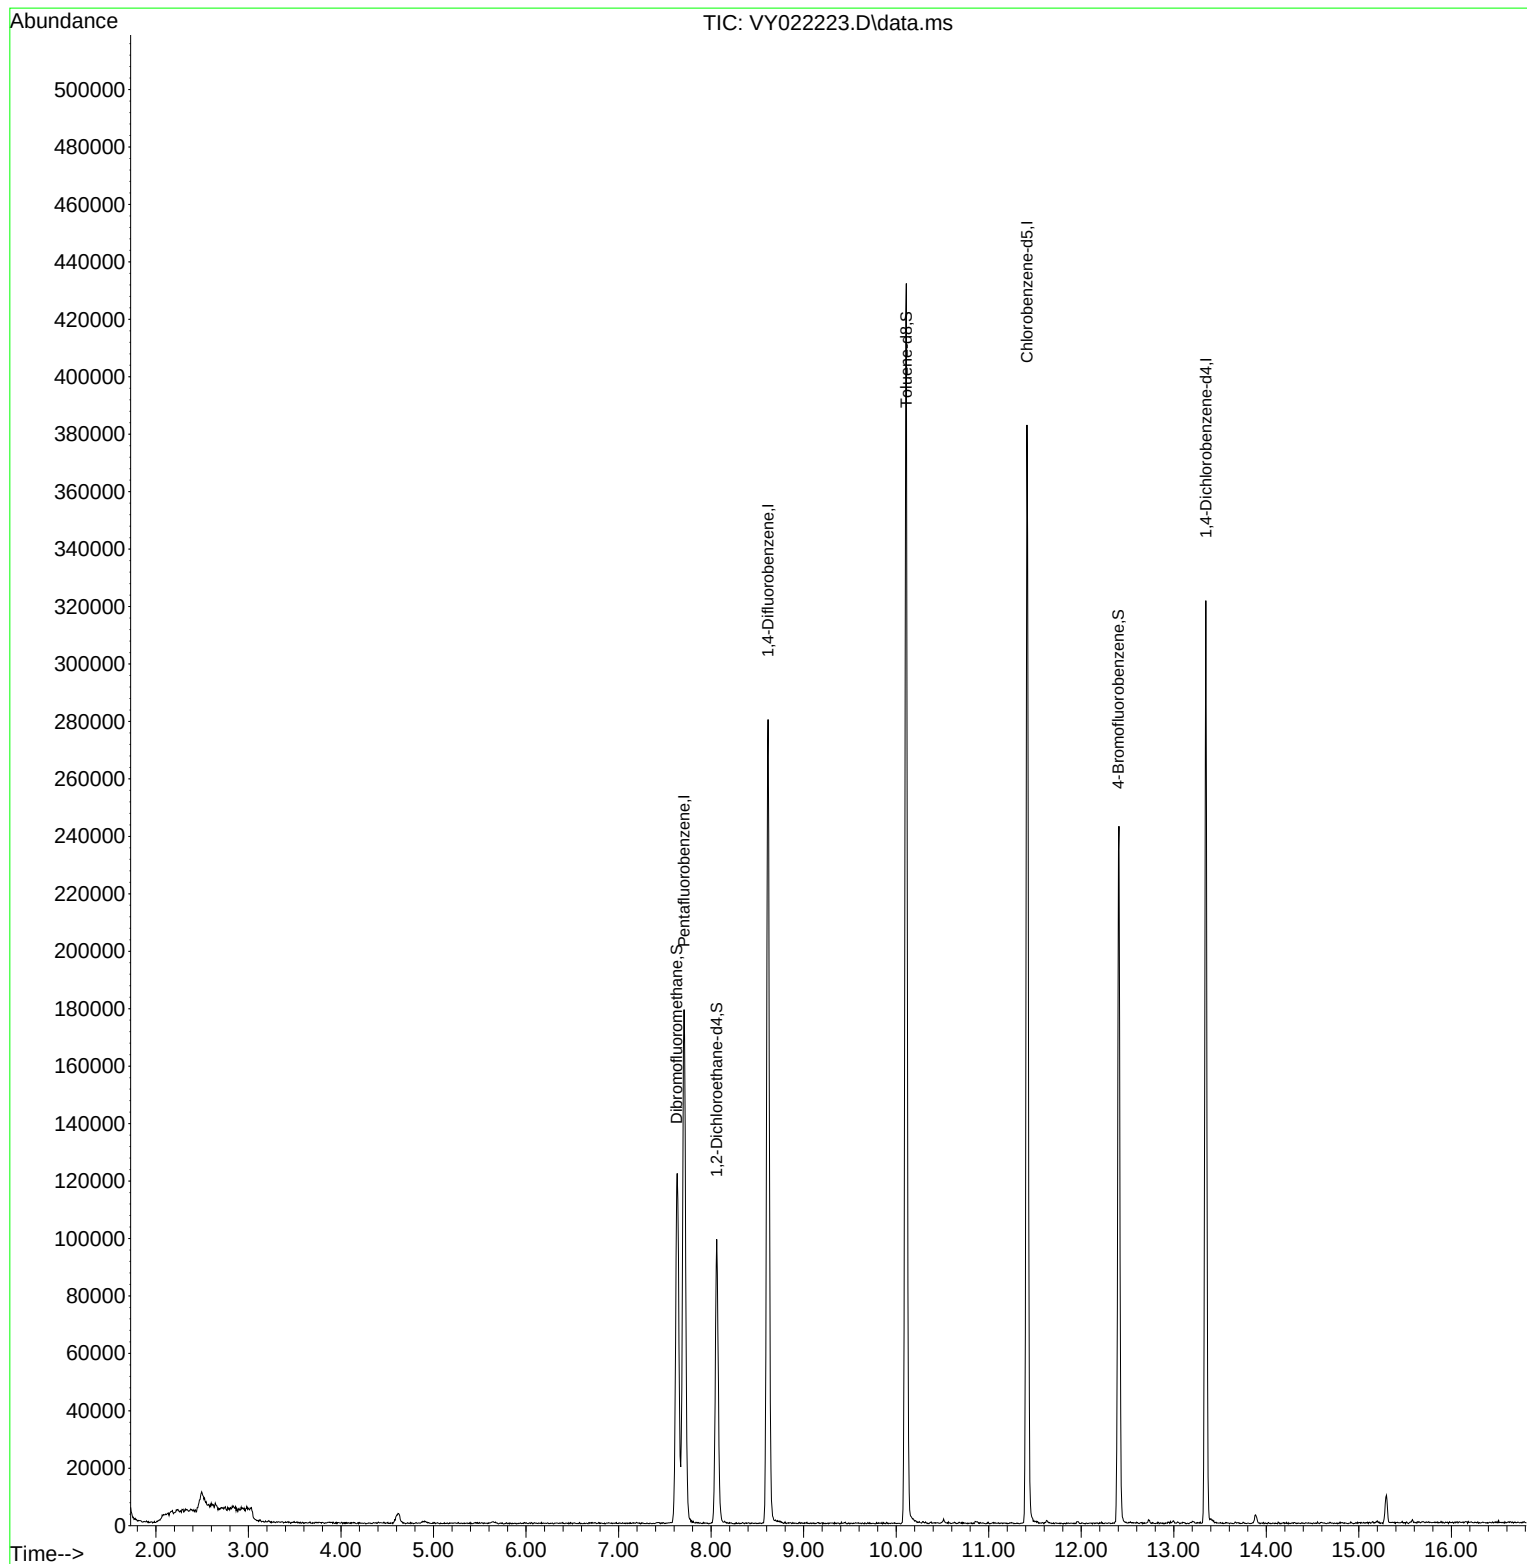


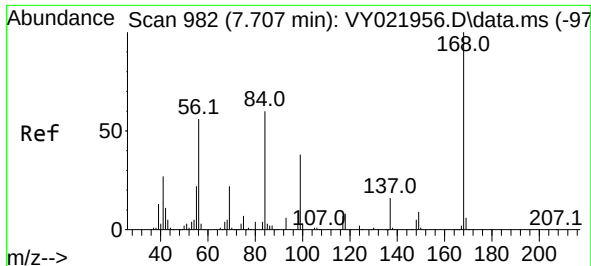

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY022223.D
Acq: 12 May 2025 14:40




Instrument :
MSVOA_Y
ClientSampleId :
COMP-8


Tgt Ion:168 Resp: 138038
Ion Ratio Lower Upper
168 100
99 54.3 43.1 64.7

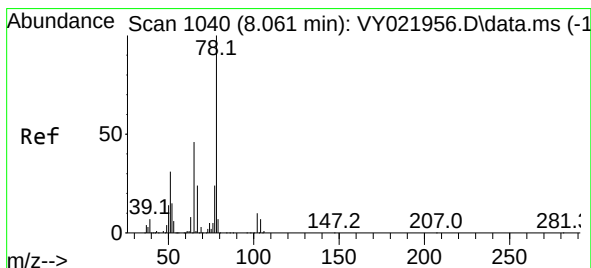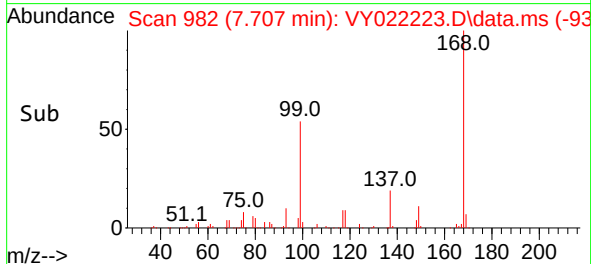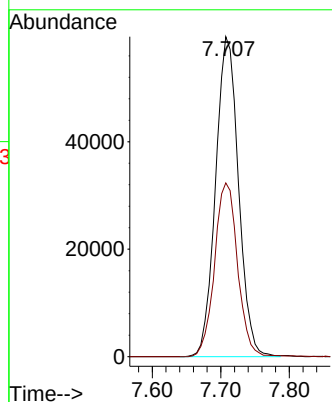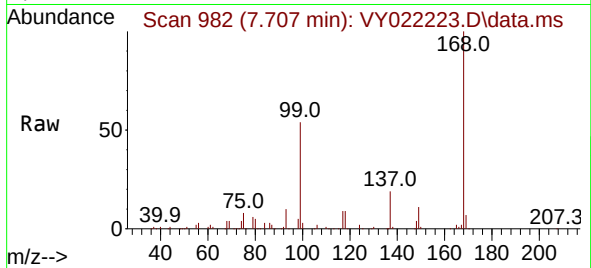

#33
1,2-Dichloroethane-d4
Concen: 60.406 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY022223.D
Acq: 12 May 2025 14:40

Tgt Ion: 65 Resp: 77020
Ion Ratio Lower Upper
65 100
67 52.9 0.0 105.8

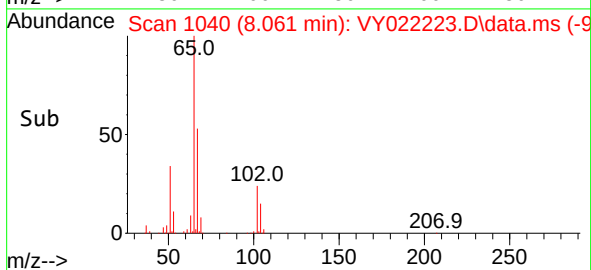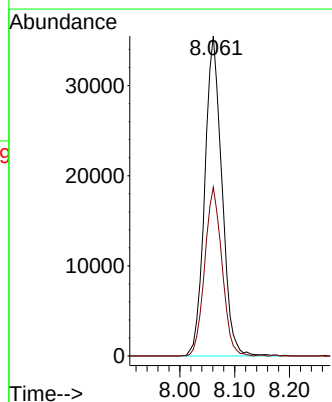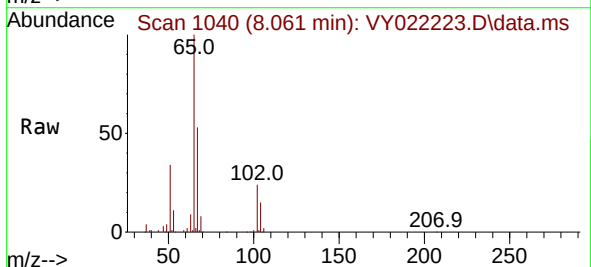

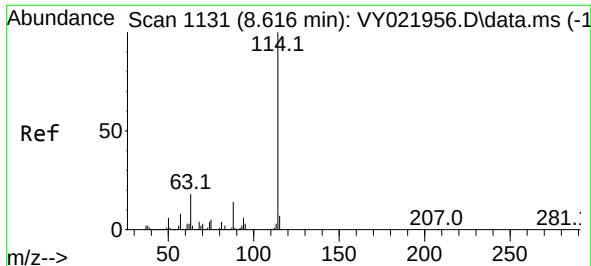

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY022223.D

Acq: 12 May 2025 14:40

Instrument :

MSVOA_Y

ClientSampleId :

COMP-8





Tgt Ion:114 Resp: 245564

Ion Ratio Lower Upper

114 100

63 18.1 0.0 35.4

88 13.7 0.0 28.2

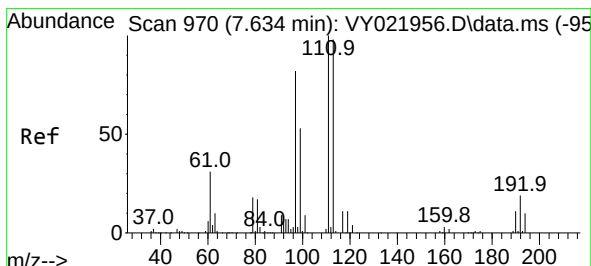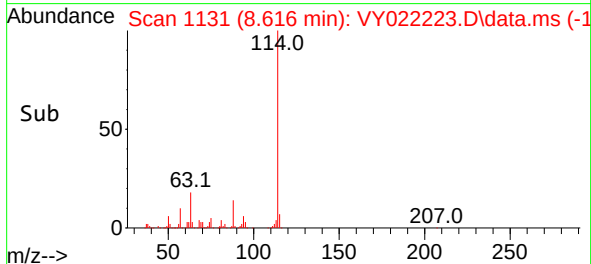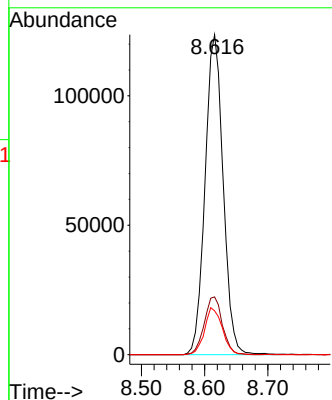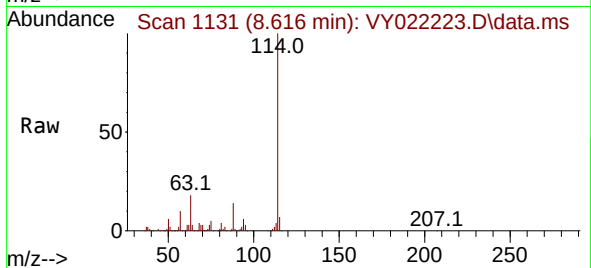

#35

Dibromofluoromethane

Concen: 55.079 ug/l

RT: 7.628 min Scan# 969

Delta R.T. -0.006 min

Lab File: VY022223.D

Acq: 12 May 2025 14:40




Tgt Ion:113 Resp: 89356


Ion Ratio Lower Upper

113 100

111 102.6 81.8 122.8

192 19.9 15.6 23.4


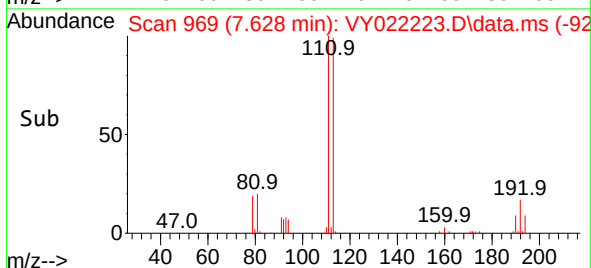
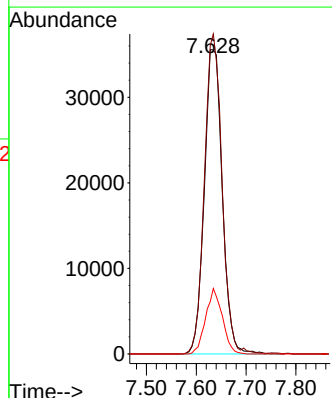
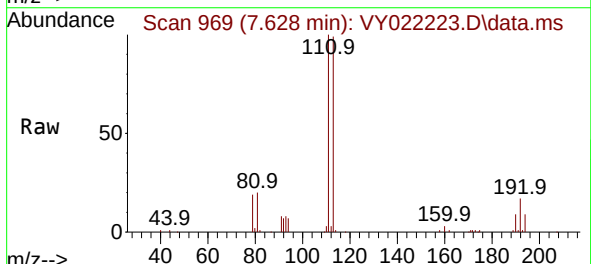


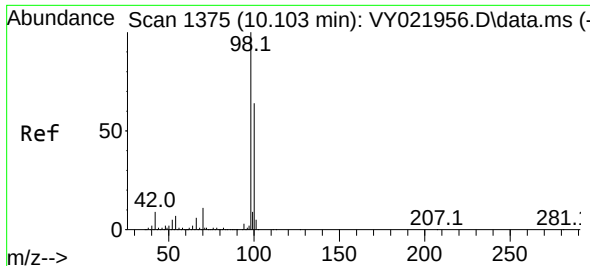

#50
Toluene-d8
Concen: 48.153 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.006 min
Lab File: VY022223.D
Acq: 12 May 2025 14:40




Instrument :
MSVOA_Y
ClientSampleId :
COMP-8


Tgt Ion: 98 Resp: 294509
Ion Ratio Lower Upper
98 100
100 62.7 51.6 77.4

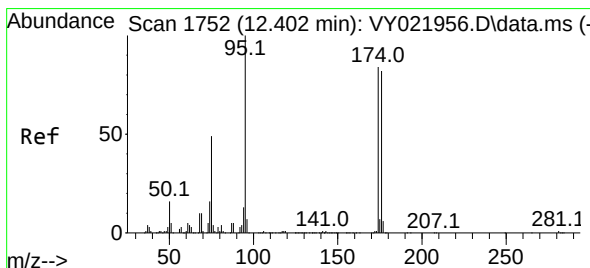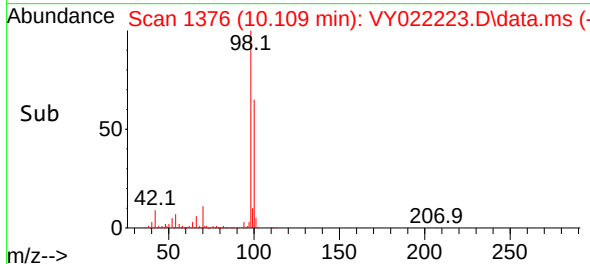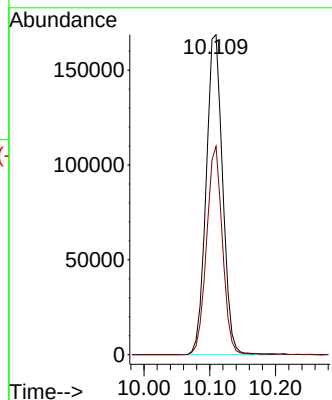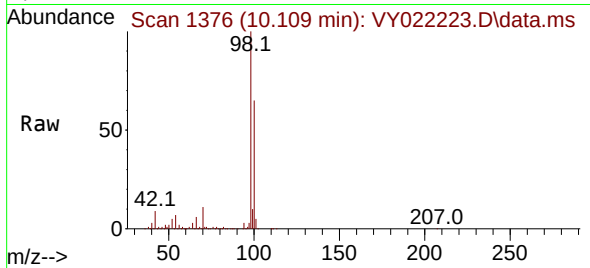

#62
4-Bromofluorobenzene
Concen: 36.265 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY022223.D
Acq: 12 May 2025 14:40

Tgt Ion: 95 Resp: 74668
Ion Ratio Lower Upper
95 100
174 89.6 0.0 179.0
176 83.9 0.0 171.8

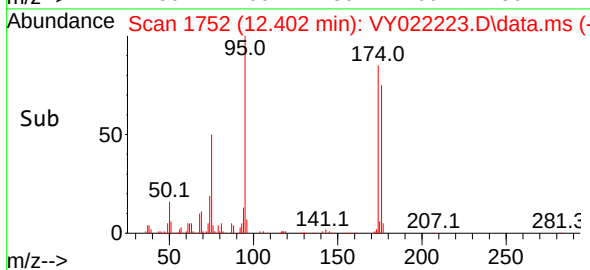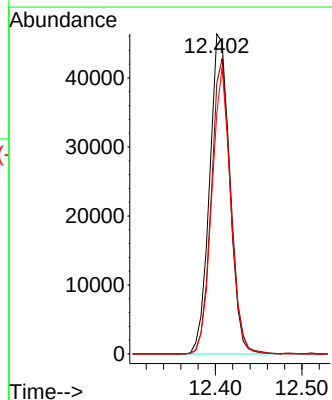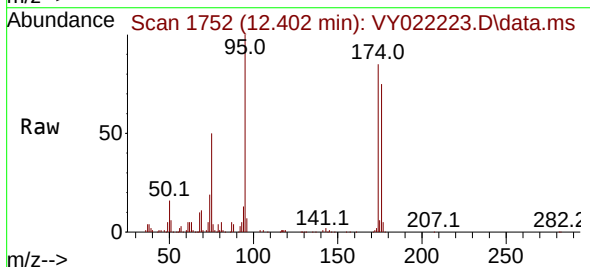

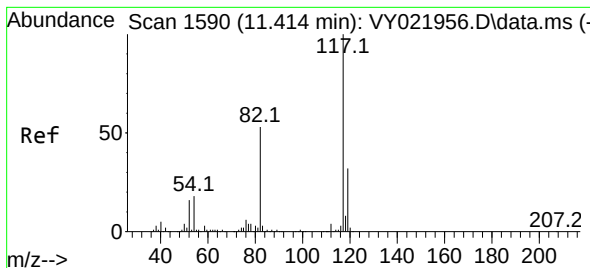

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY022223.D

Acq: 12 May 2025 14:40

Instrument :

MSVOA_Y

ClientSampleId :

COMP-8





Tgt Ion:117 Resp: 212412

Ion Ratio Lower Upper

117 100

82 53.2 42.1 63.1

119 31.9 25.7 38.5

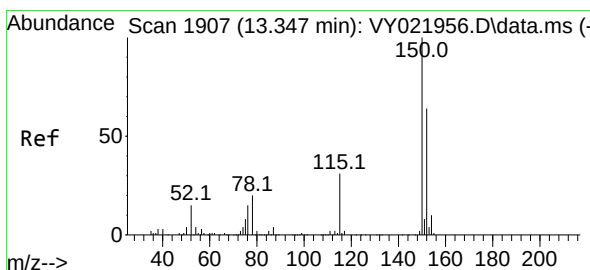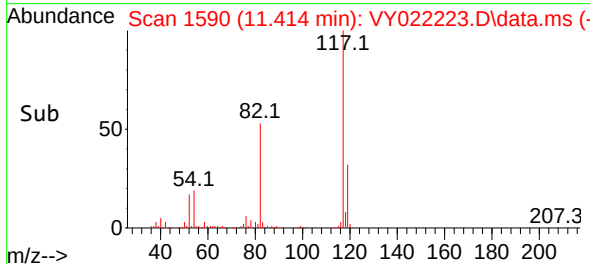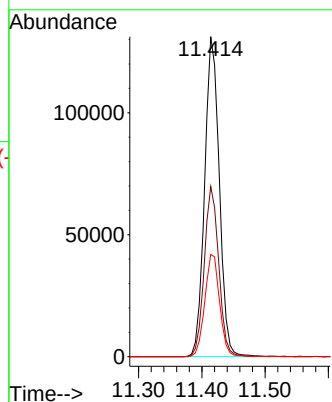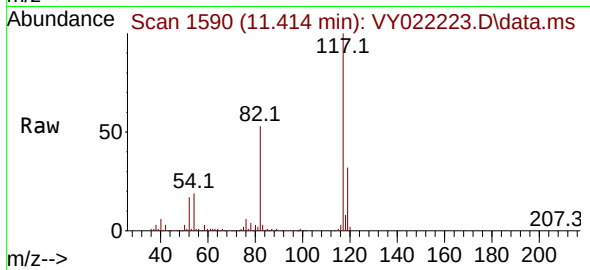

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY022223.D

Acq: 12 May 2025 14:40

Tgt Ion:152 Resp: 81409

Ion Ratio Lower Upper

152 100

115 58.1 28.0 84.0

150 155.8 0.0 345.6

