


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051722\
 Data File : VY008797.D
 Acq On : 18 May 2022 01:20
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051722S.M
 Title : SW846 8260
 Last Update : Wed May 18 07:32:50 2022

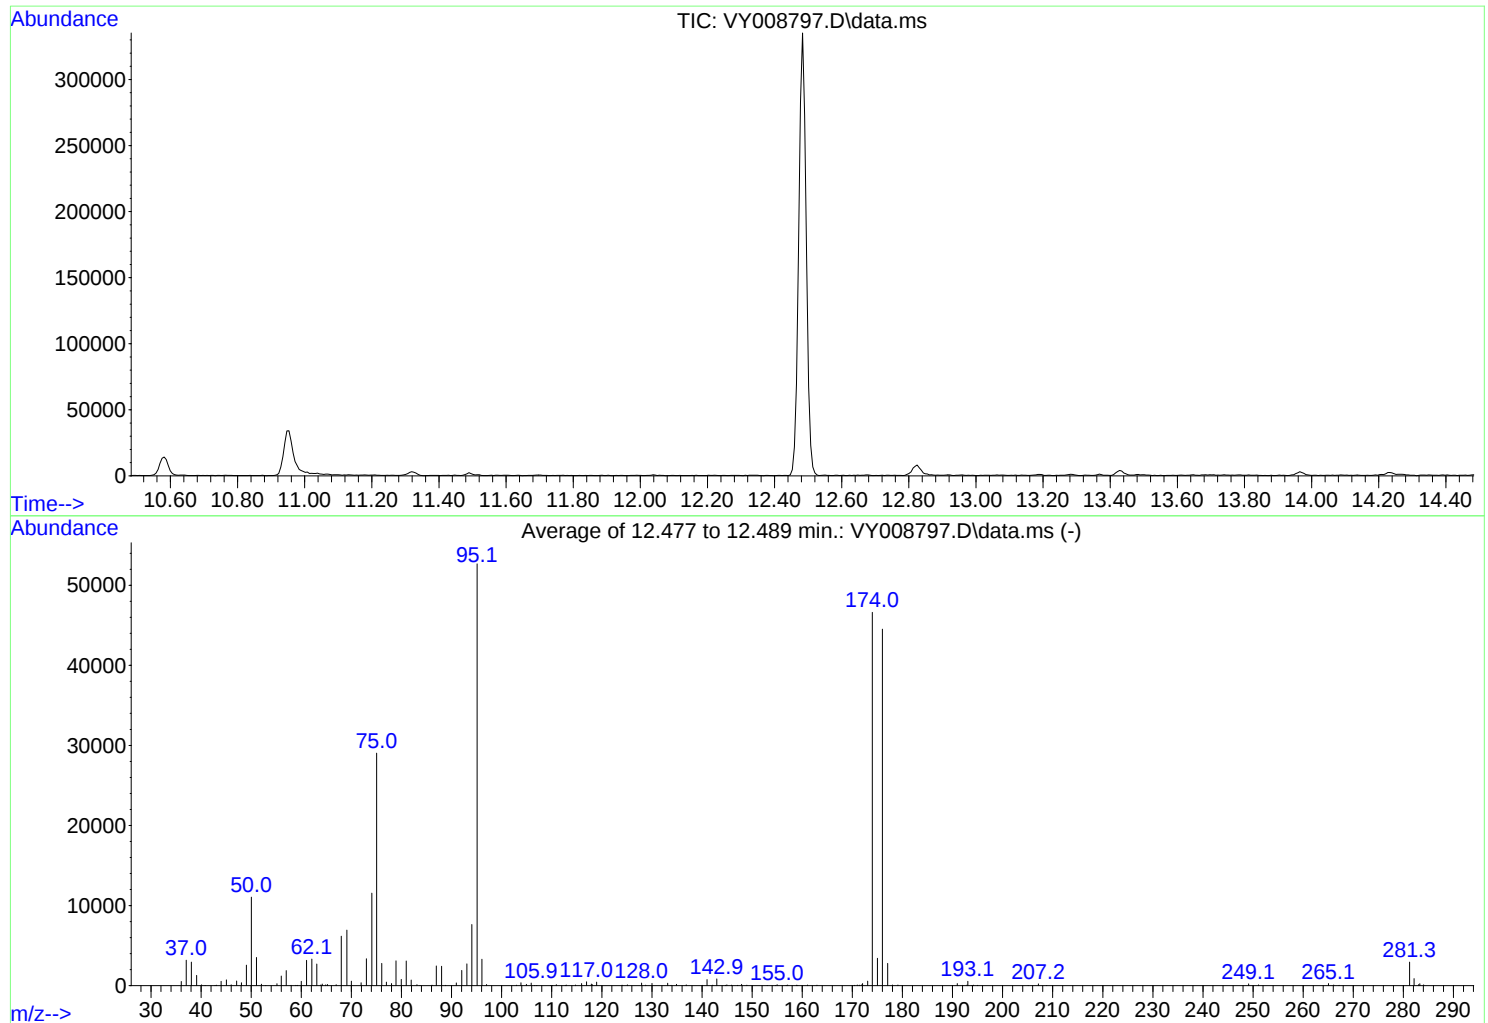

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	11043	PASS
75	95	30	60	55.1	29035	PASS
95	95	100	100	100.0	52677	PASS
96	95	5	9	6.2	3290	PASS
173	174	0.00	2	1.2	566	PASS
174	95	50	100	88.5	46627	PASS
175	174	5	9	7.3	3423	PASS
176	174	95	101	95.5	44523	PASS
177	176	5	9	6.3	2786	PASS