

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051922\
 Data File : VY008860.D
 Acq On : 19 May 2022 12:17
 Operator : KP/MD
 Sample : N2841-18
 Misc : 5.40g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 P009-SS003-1218-01

Quant Time: May 19 17:39:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051722S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 18 07:32:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	153584	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	272104	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	257985	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	109101	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	92033	64.593	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	129.180%
35) Dibromofluoromethane	7.716	113	85175	53.574	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	107.140%
50) Toluene-d8	10.179	98	340763	48.333	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.660%
62) 4-Bromofluorobenzene	12.483	95	99534	40.202	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	80.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051922\
Data File : VY008860.D
Acq On : 19 May 2022 12:17
Operator : KP/MD
Sample : N2841-18
Misc : 5.40g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
P009-SS003-1218-01

Quant Time: May 19 17:39:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051722S.M
Quant Title : SW846 8260
QLast Update : Wed May 18 07:32:50 2022
Response via : Initial Calibration




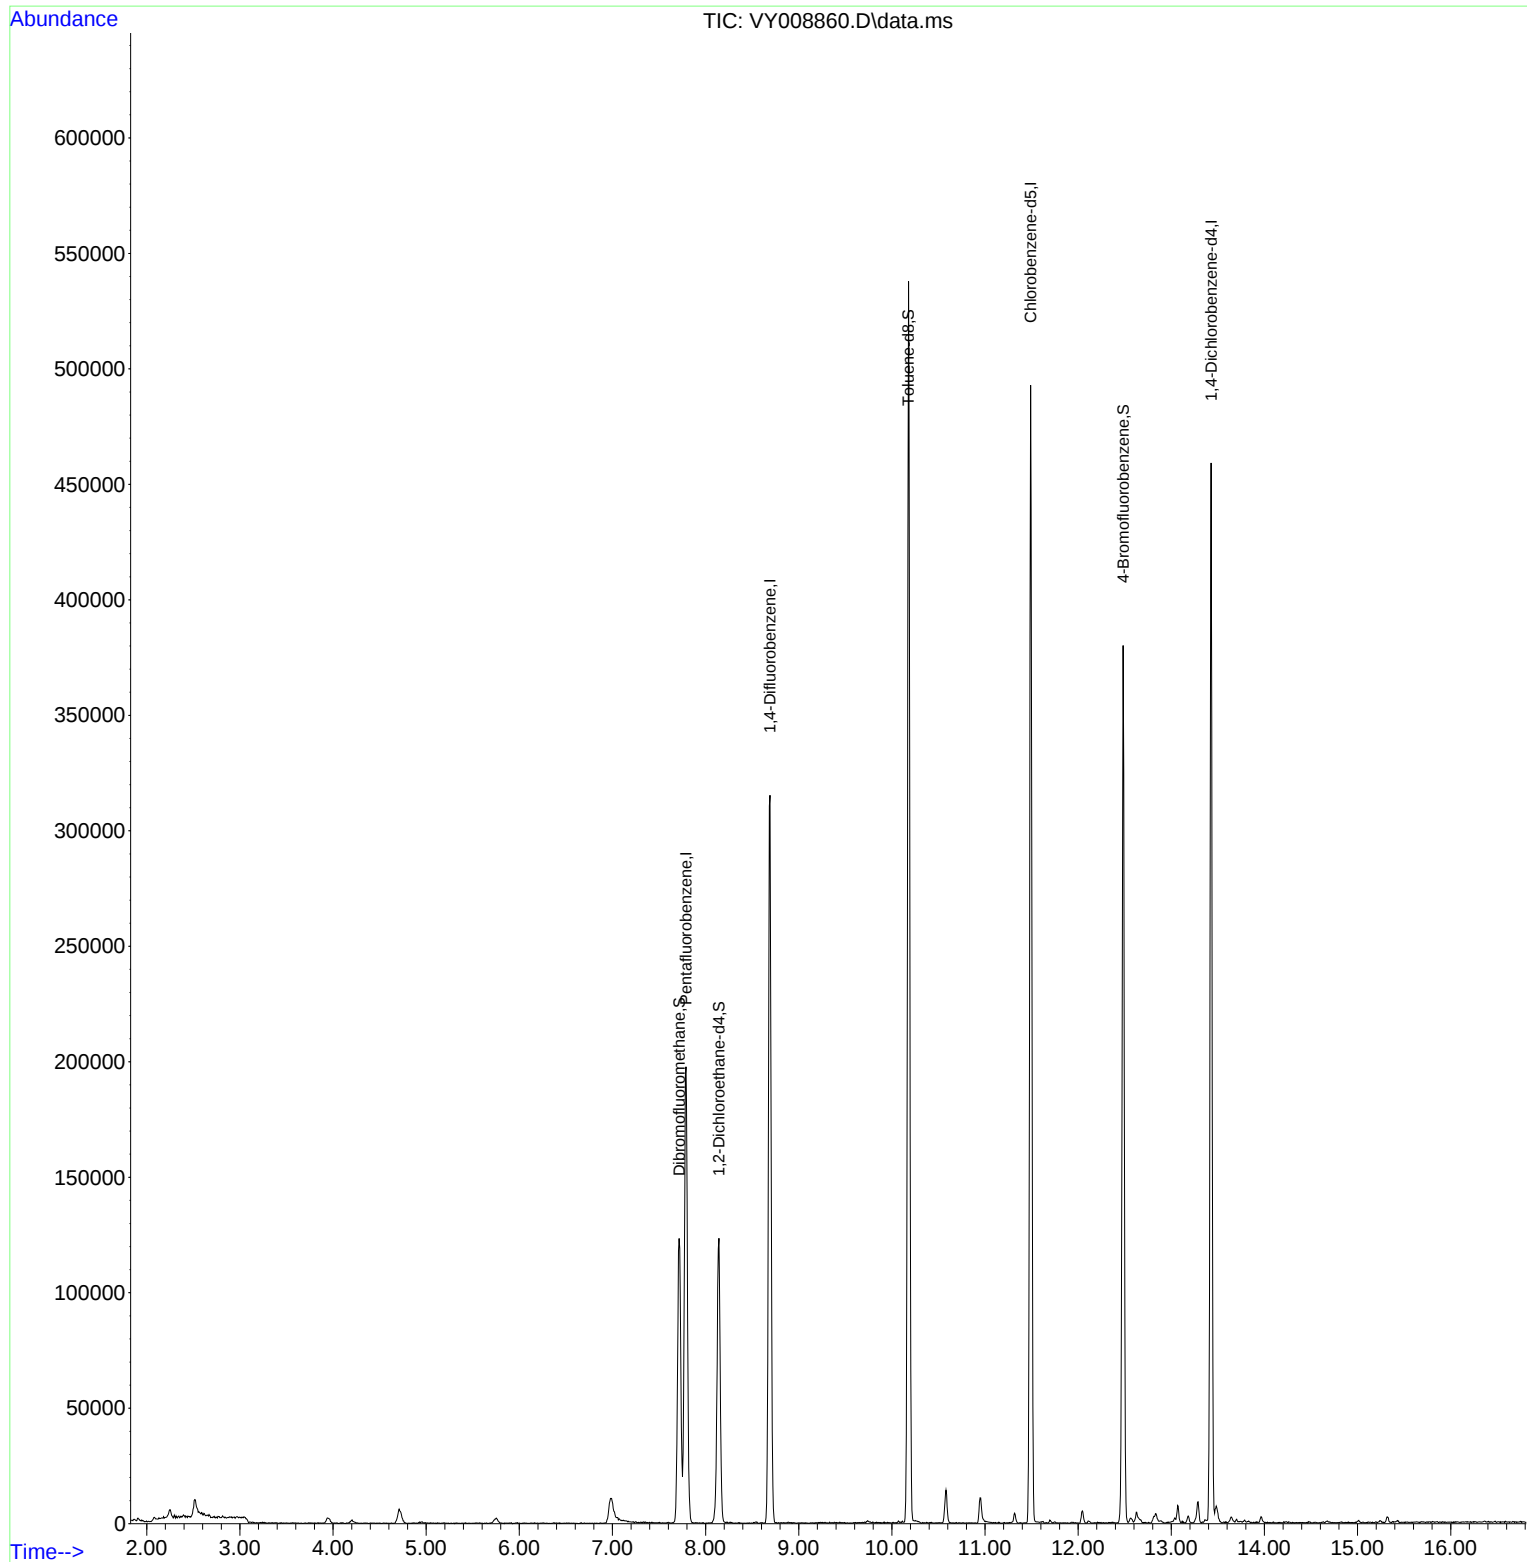


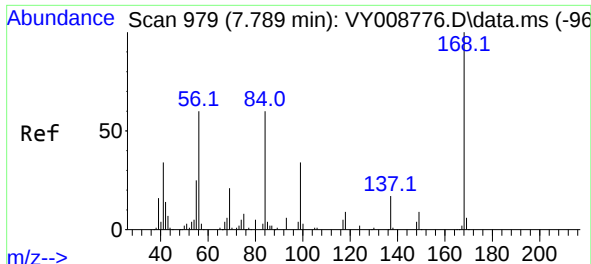

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008860.D
Acq: 19 May 2022 12:17




Instrument :
MSVOA_Y
ClientSampleId :
P009-SS003-1218-01


Tgt Ion:168 Resp: 153584
Ion Ratio Lower Upper
168 100
99 53.2 46.9 70.3

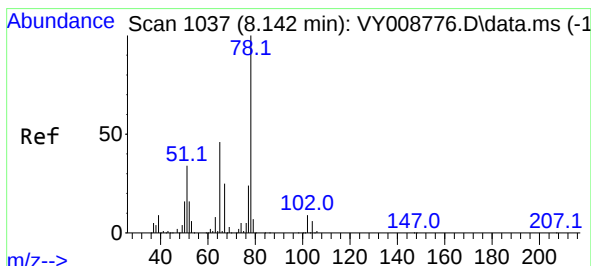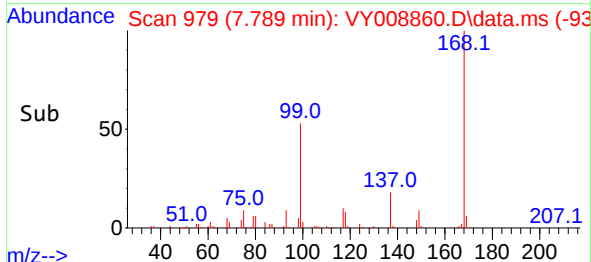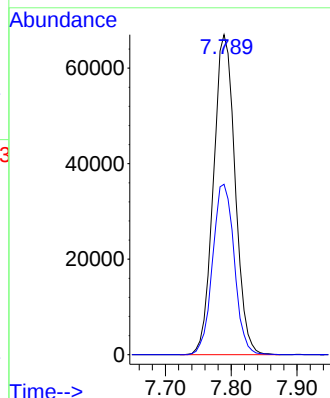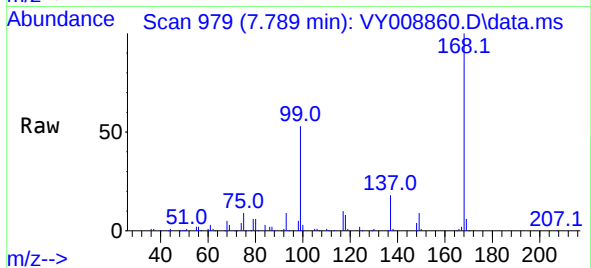

#33
1,2-Dichloroethane-d4
Concen: 64.593 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VY008860.D
Acq: 19 May 2022 12:17

Tgt Ion: 65 Resp: 92033
Ion Ratio Lower Upper
65 100
67 52.1 0.0 99.4

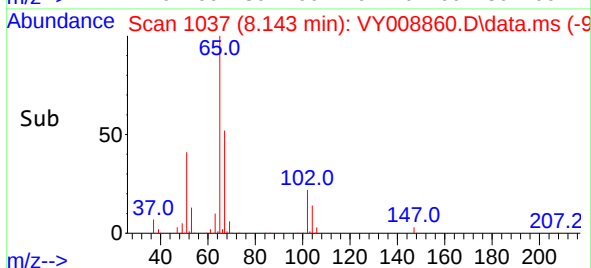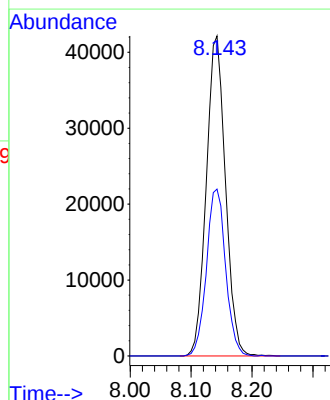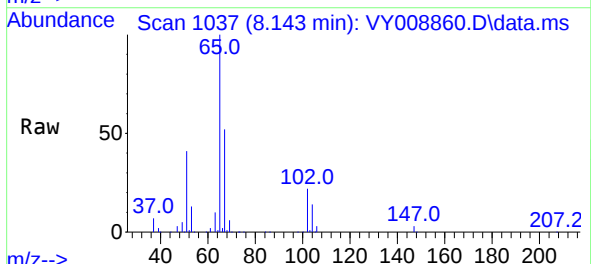

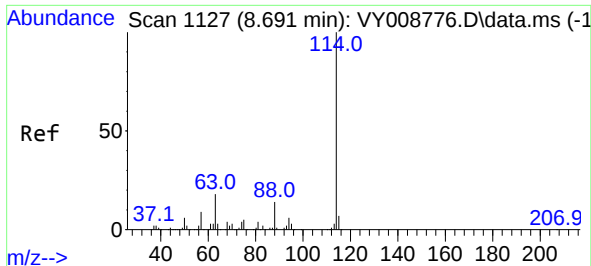

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY008860.D

Acq: 19 May 2022 12:17

Instrument :

MSVOA_Y

ClientSampleId :

P009-SS003-1218-01





Tgt Ion:114 Resp: 272104

Ion Ratio Lower Upper

114 100

63 18.1 0.0 43.2

88 13.8 0.0 31.8

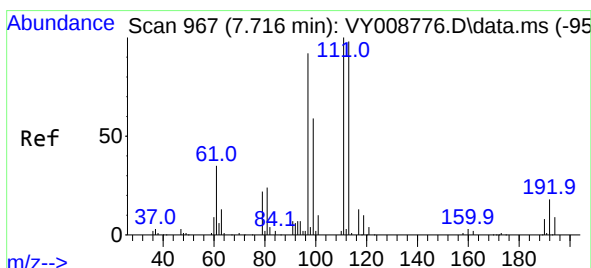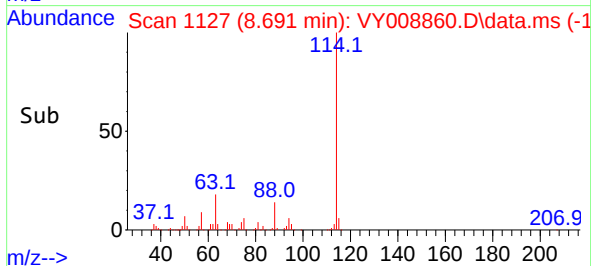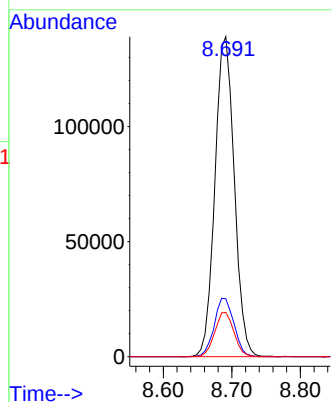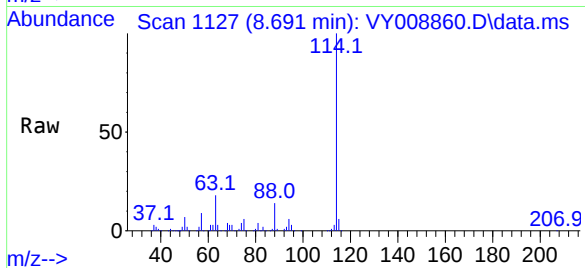

#35

Dibromofluoromethane

Concen: 53.574 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY008860.D

Acq: 19 May 2022 12:17




Tgt Ion:113 Resp: 85175

Ion Ratio Lower Upper

113 100

111 105.5 82.6 124.0

192 20.0 17.6 26.4

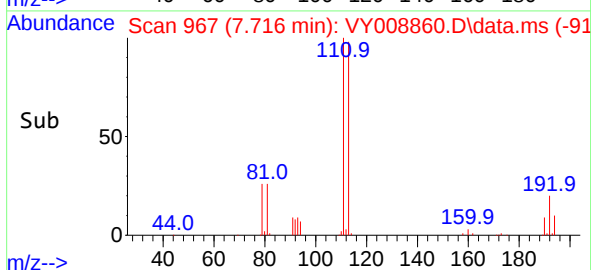
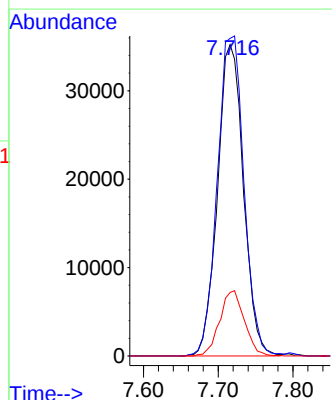
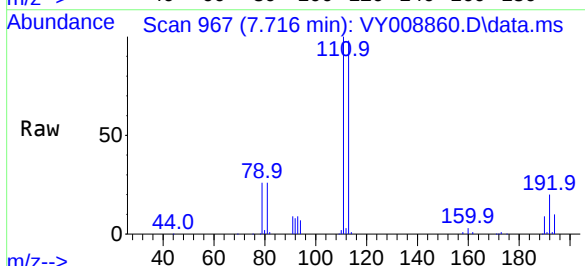




#50
Toluene-d8
Concen: 48.333 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY008860.D
Acq: 19 May 2022 12:17




Instrument :
MSVOA_Y
ClientSampleId :
P009-SS003-1218-01


Tgt Ion: 98 Resp: 340763
Ion Ratio Lower Upper
98 100
100 64.8 50.2 75.2

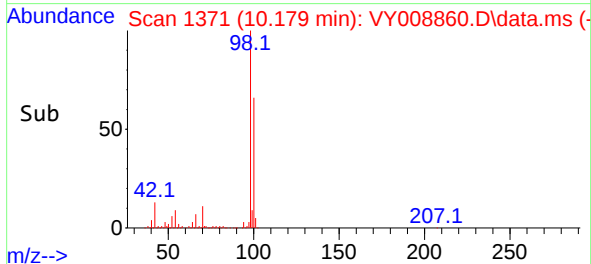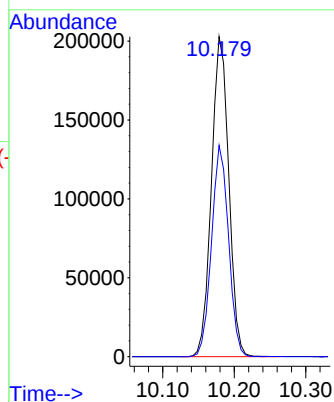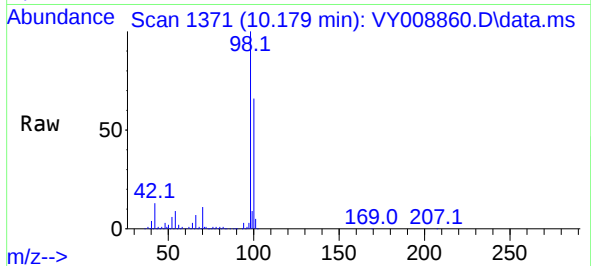

#62
4-Bromofluorobenzene
Concen: 40.202 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008860.D
Acq: 19 May 2022 12:17

Tgt Ion: 95 Resp: 99534
Ion Ratio Lower Upper
95 100
174 91.2 0.0 177.0
176 86.5 0.0 175.8


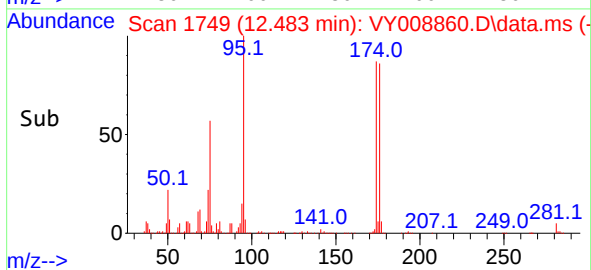
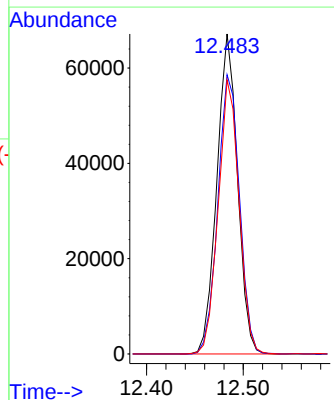
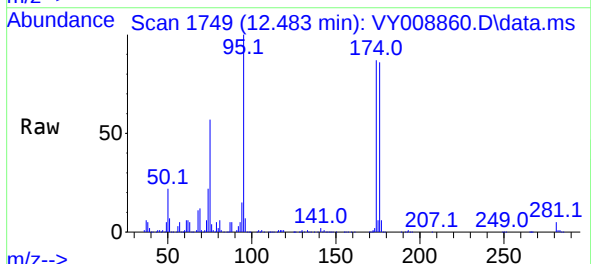


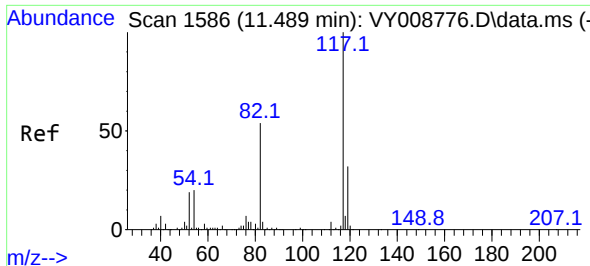

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY008860.D
Acq: 19 May 2022 12:17

Instrument :
MSVOA_Y
ClientSampleId :
P009-SS003-1218-01

Tgt Ion:117 Resp: 257985
Ion Ratio Lower Upper
117 100
82 52.9 43.0 64.4
119 31.0 25.4 38.0

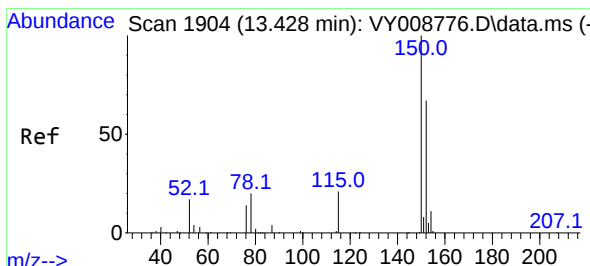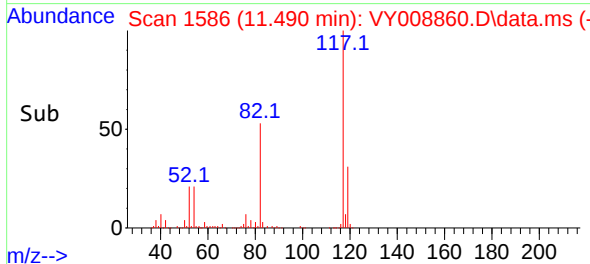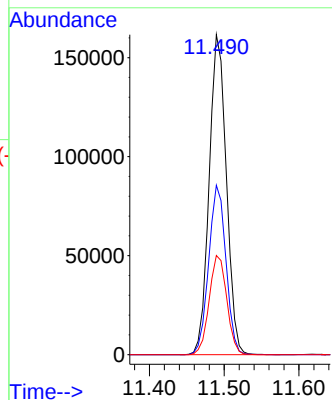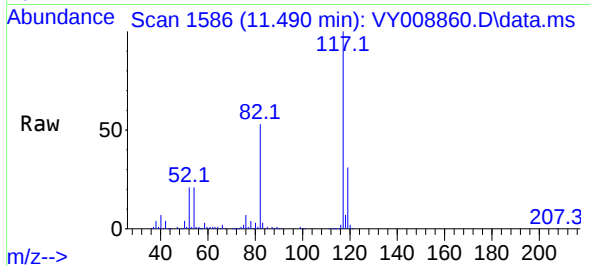

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008860.D
Acq: 19 May 2022 12:17

Tgt Ion:152 Resp: 109101
Ion Ratio Lower Upper
152 100
115 55.6 28.2 84.7
150 157.4 0.0 347.6

