

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051922\
 Data File : VY008867.D
 Acq On : 19 May 2022 15:01
 Operator : KP/MD
 Sample : N2832-09
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB12

Quant Time: May 20 02:52:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051722S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 18 07:32:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	124957	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	229602	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	224806	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	98181	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	83627	72.140	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	144.280%
35) Dibromofluoromethane	7.716	113	74762	55.730	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	111.460%
50) Toluene-d8	10.179	98	292845	49.167	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	98.340%
62) 4-Bromofluorobenzene	12.483	95	87170	41.594	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	83.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051922\
Data File : VY008867.D
Acq On : 19 May 2022 15:01
Operator : KP/MD
Sample : N2832-09
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB12


Quant Time: May 20 02:52:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051722S.M
Quant Title : SW846 8260
QLast Update : Wed May 18 07:32:50 2022
Response via : Initial Calibration

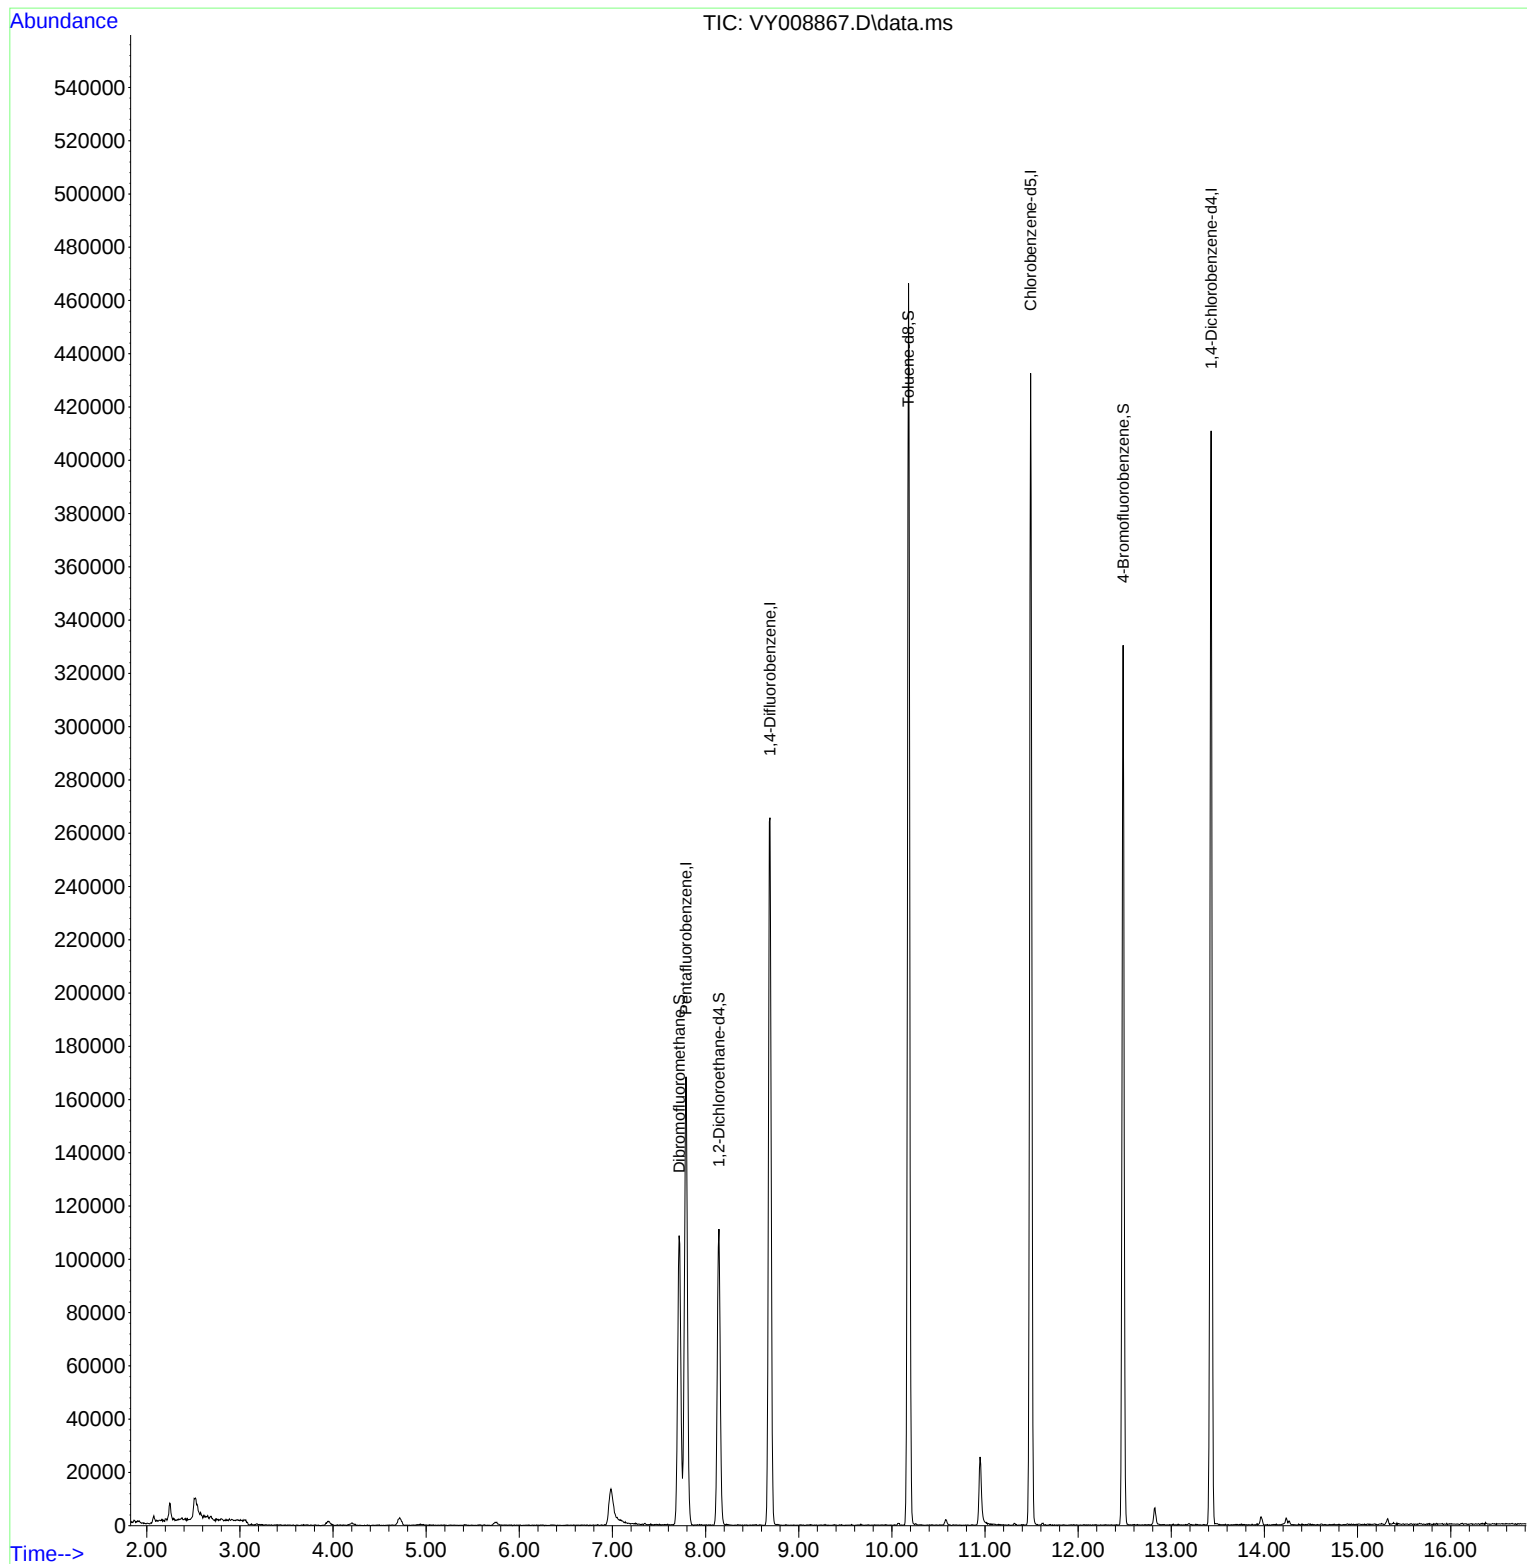



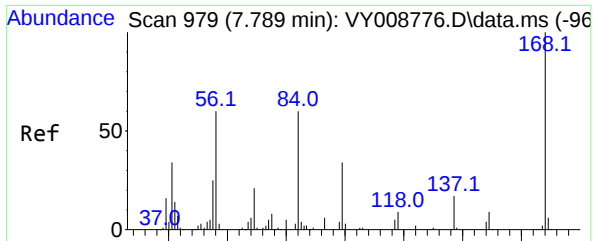


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008867.D
Acq: 19 May 2022 15:01

Instrument :
MSVOA_Y
ClientSampleId :
SB12



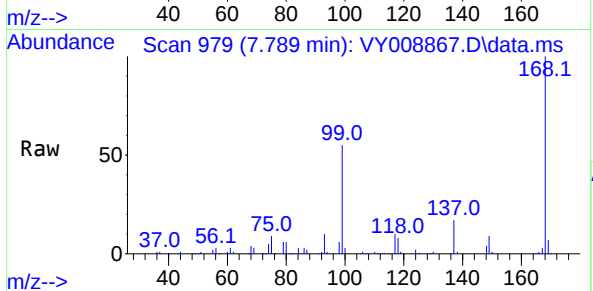



Tgt Ion:168 Resp: 124957
Ion Ratio Lower Upper
168 100
99 55.1 46.9 70.3

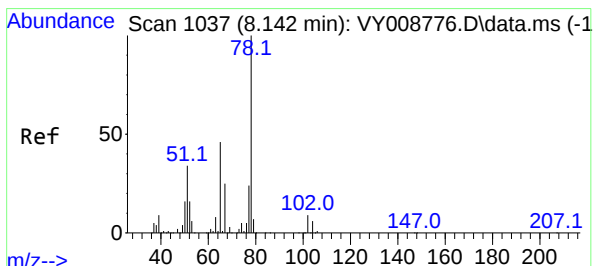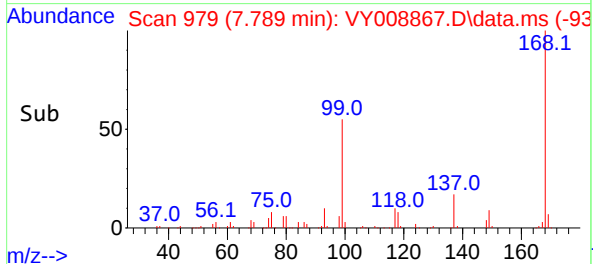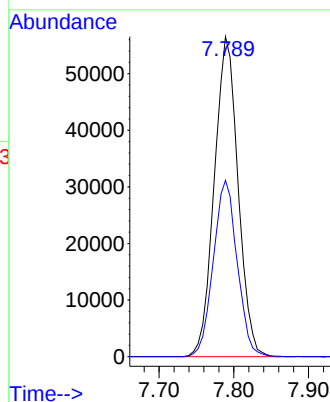

#33
1,2-Dichloroethane-d4
Concen: 72.140 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY008867.D
Acq: 19 May 2022 15:01

Tgt Ion: 65 Resp: 83627
Ion Ratio Lower Upper
65 100
67 52.1 0.0 99.4

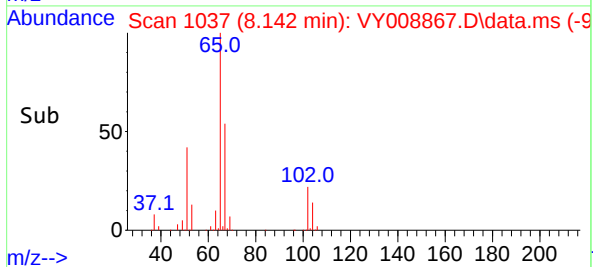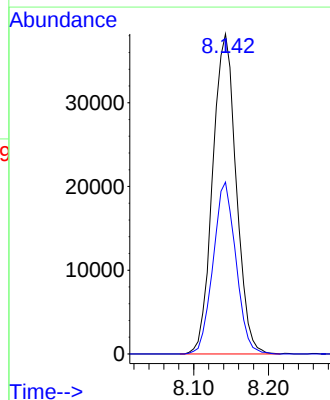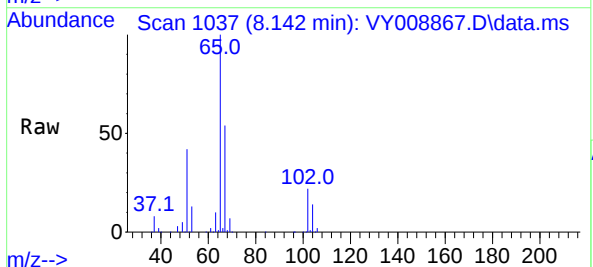

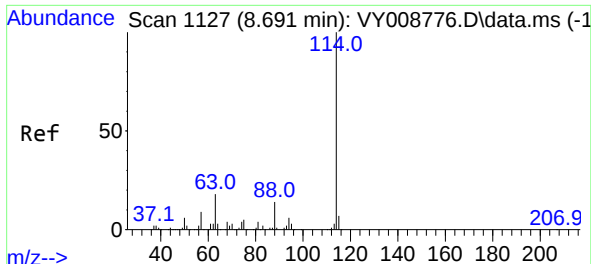

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VY008867.D

Acq: 19 May 2022 15:01

Instrument :

MSVOA_Y

ClientSampleId :

SB12





Tgt Ion:114 Resp: 229602

Ion Ratio Lower Upper

114 100

63 18.6 0.0 43.2

88 13.7 0.0 31.8

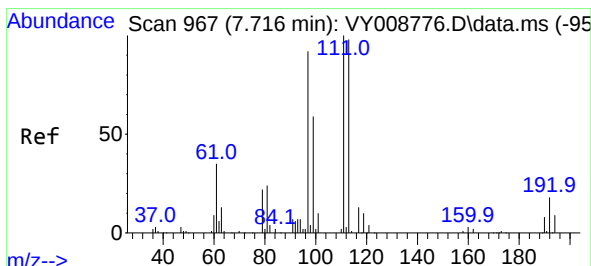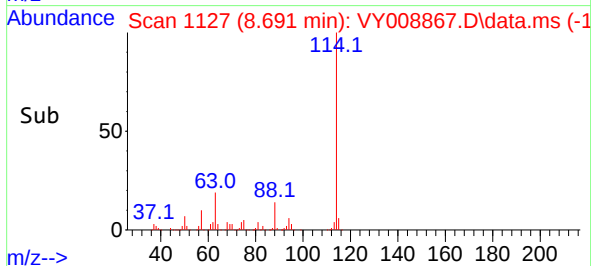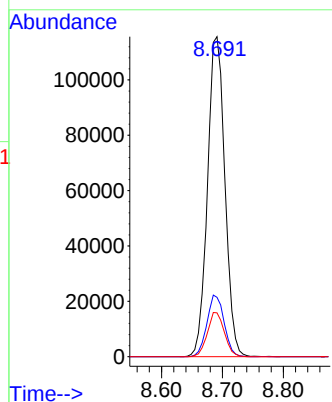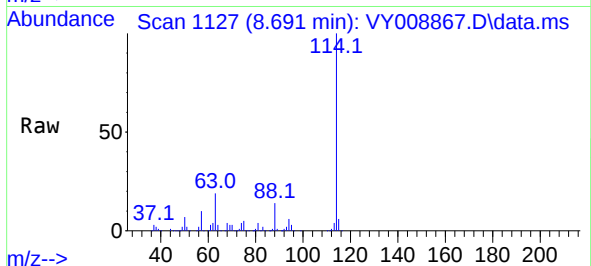

#35

Dibromofluoromethane

Concen: 55.730 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY008867.D

Acq: 19 May 2022 15:01




Tgt Ion:113 Resp: 74762

Ion Ratio Lower Upper

113 100

111 102.5 82.6 124.0

192 19.1 17.6 26.4

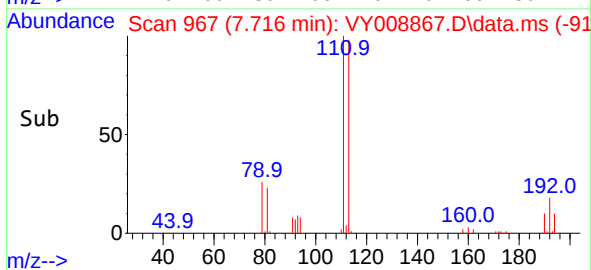
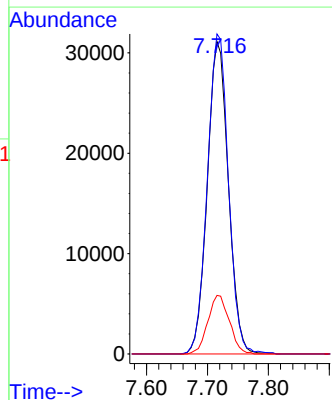
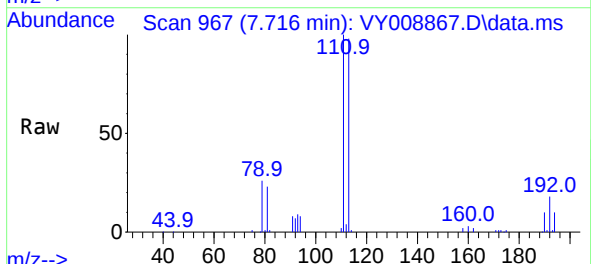




#50
Toluene-d8
Concen: 49.167 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY008867.D
Acq: 19 May 2022 15:01




Instrument :
MSVOA_Y
ClientSampleId :
SB12


Tgt Ion: 98 Resp: 292845
Ion Ratio Lower Upper
98 100
100 64.6 50.2 75.2

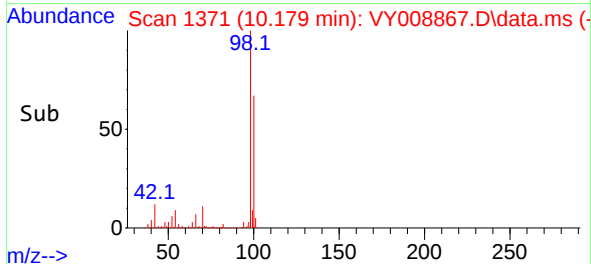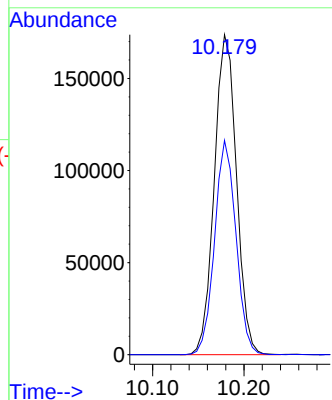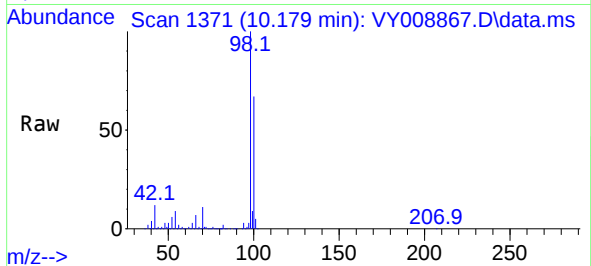

#62
4-Bromofluorobenzene
Concen: 41.594 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008867.D
Acq: 19 May 2022 15:01

Tgt Ion: 95 Resp: 87170
Ion Ratio Lower Upper
95 100
174 91.5 0.0 177.0
176 86.3 0.0 175.8


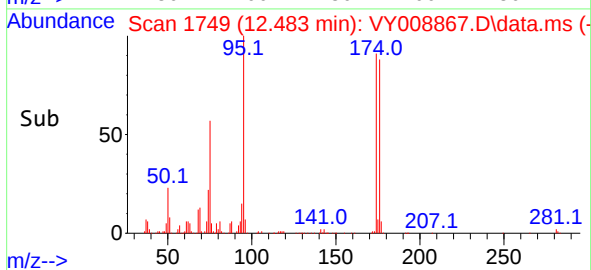
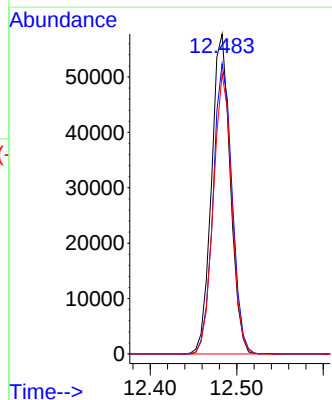
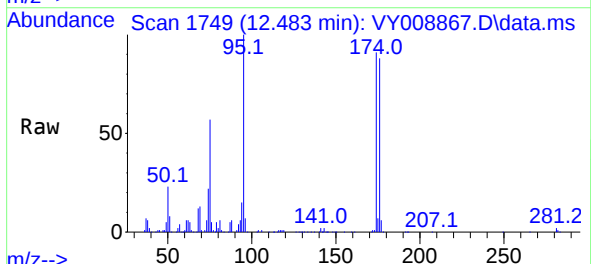


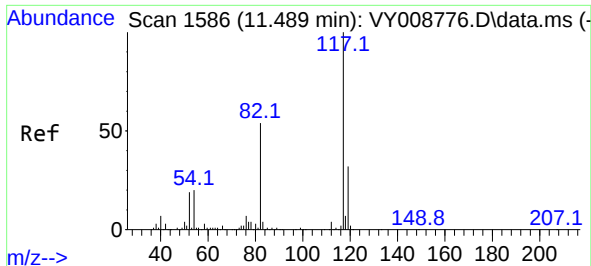

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. -0.000 min
Lab File: VY008867.D
Acq: 19 May 2022 15:01

Instrument :
MSVOA_Y
ClientSampleId :
SB12

Tgt Ion:117 Resp: 224806
Ion Ratio Lower Upper
117 100
82 55.1 43.0 64.4
119 32.1 25.4 38.0

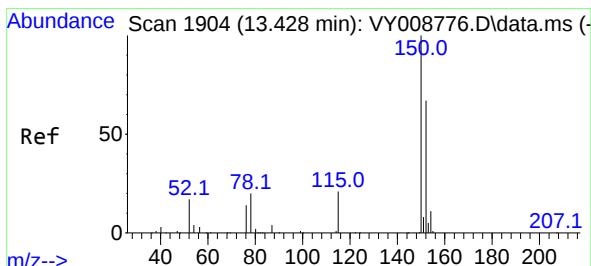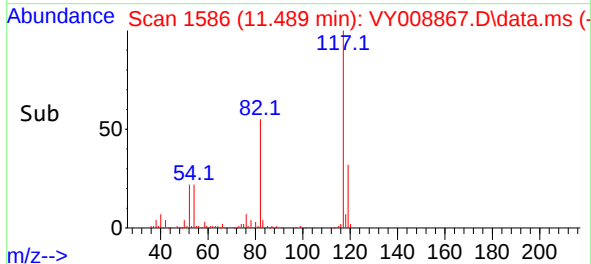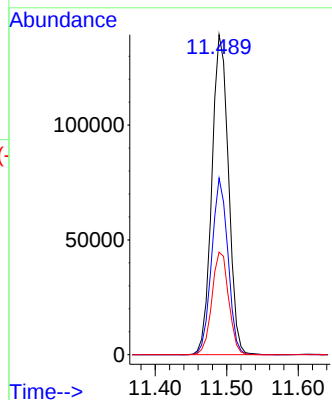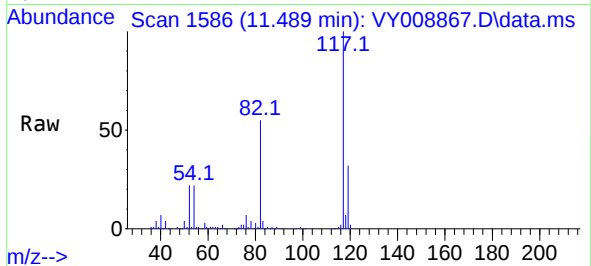

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY008867.D
Acq: 19 May 2022 15:01

Tgt Ion:152 Resp: 98181
Ion Ratio Lower Upper
152 100
115 55.6 28.2 84.7
150 156.2 0.0 347.6

