


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051922\
Data File : VY008884.D
Acq On : 19 May 2022 21:36
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051722S.M
Title : SW846 8260
Last Update : Fri May 20 15:21:19 2022

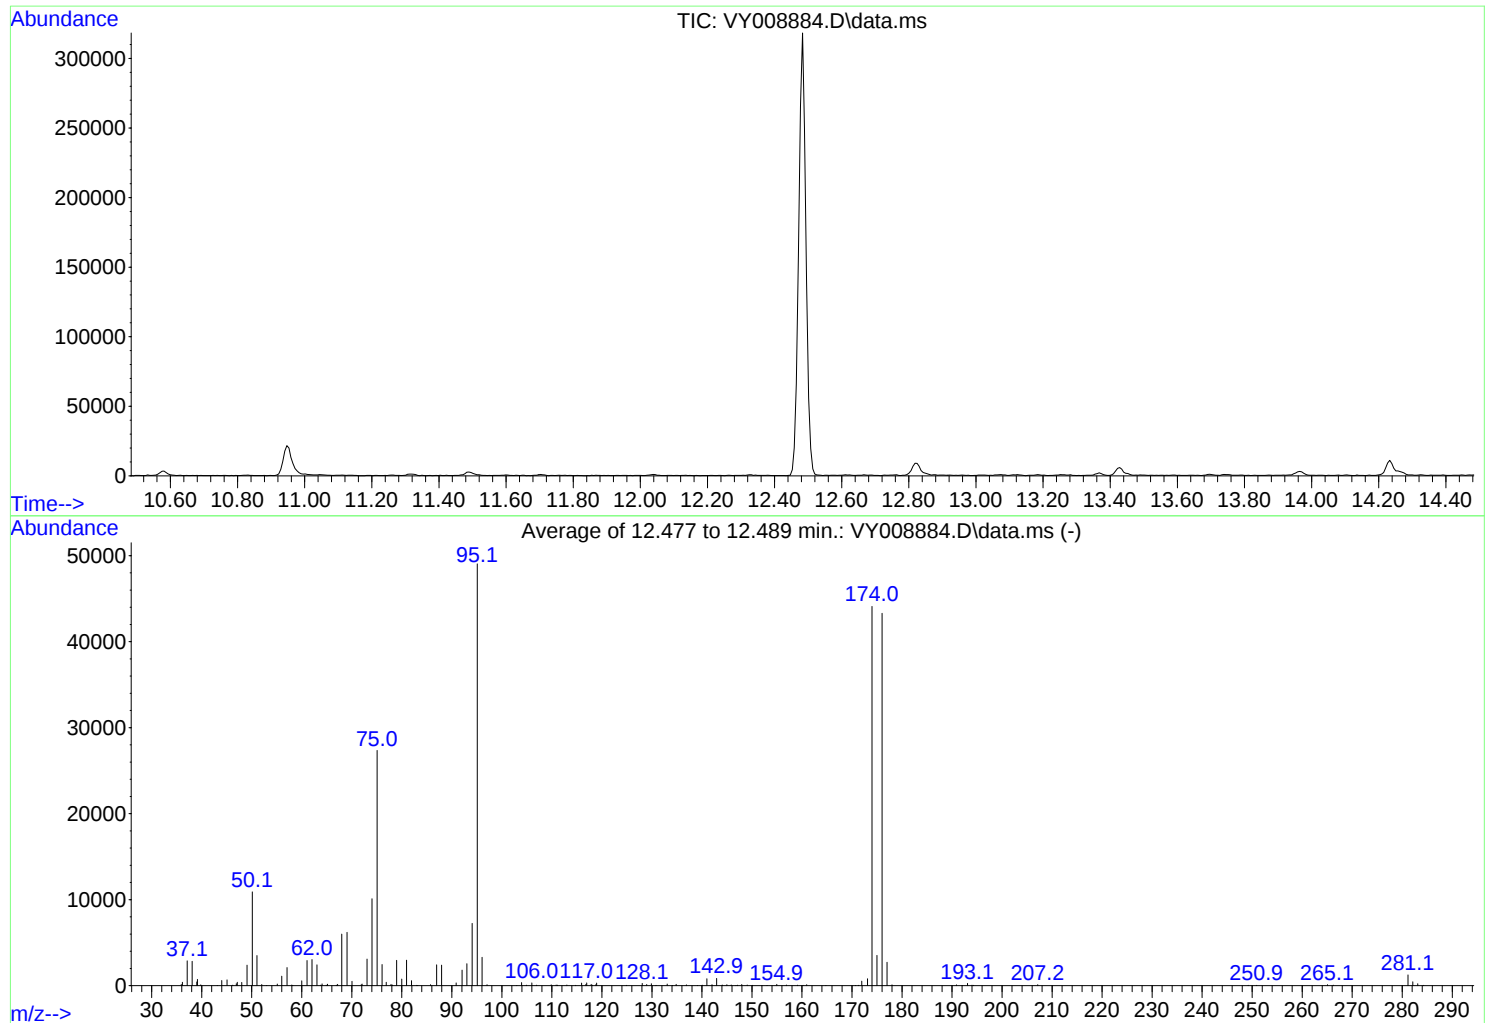

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.2	10896	PASS
75	95	30	60	55.7	27344	PASS
95	95	100	100	100.0	49051	PASS
96	95	5	9	6.7	3295	PASS
173	174	0.00	2	1.8	793	PASS
174	95	50	100	89.9	44107	PASS
175	174	5	9	8.0	3512	PASS
176	174	95	101	98.2	43293	PASS
177	176	5	9	6.3	2722	PASS