
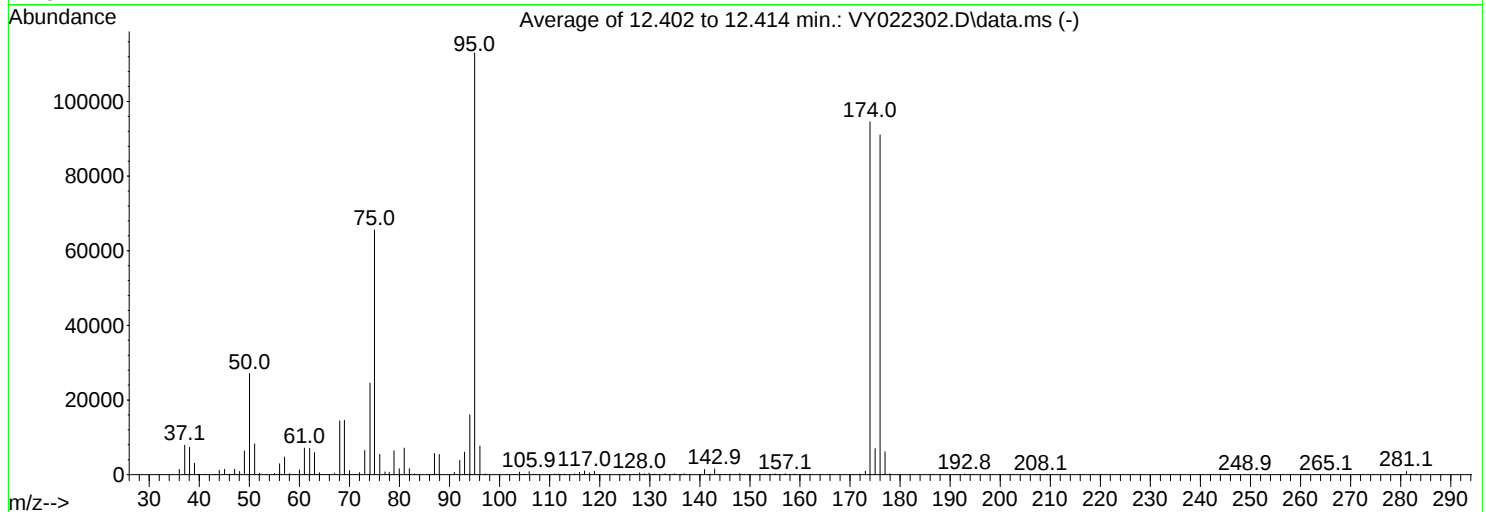


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051925\
Data File : VY022302.D
Acq On : 19 May 2025 07:57
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051525S.M
Title : SW846 8260
Last Update : Fri May 16 01:42:09 2025

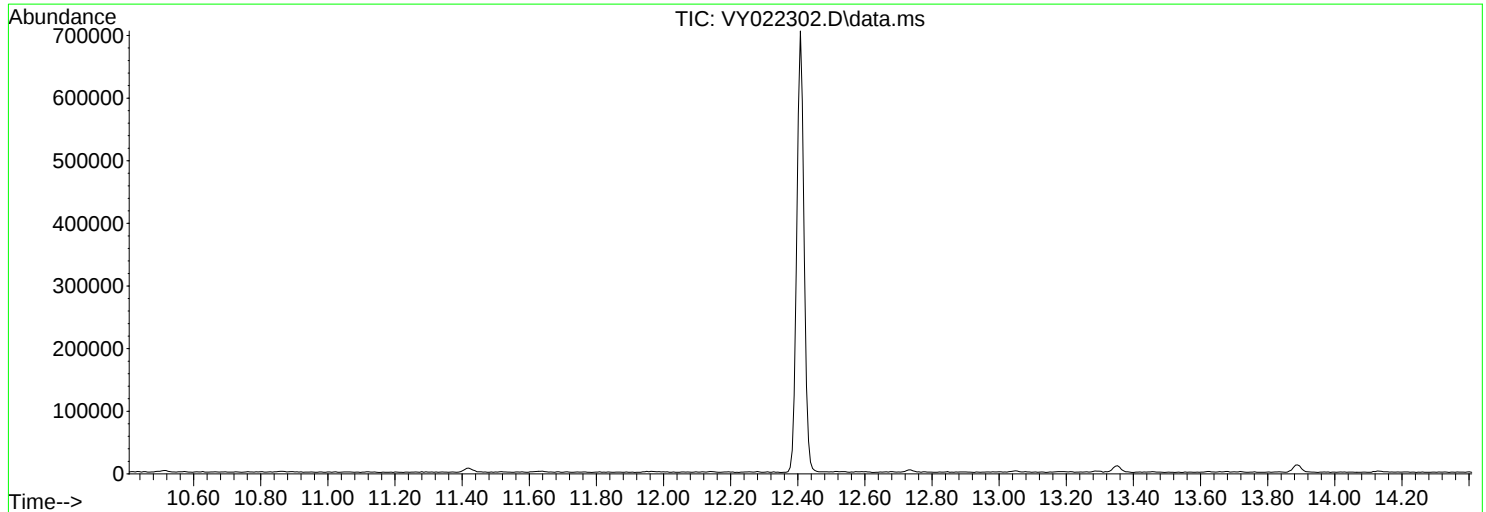

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	27112	PASS
75	95	30	60	58.0	65560	PASS
95	95	100	100	100.0	113035	PASS
96	95	5	9	6.8	7676	PASS
173	174	0.00	2	1.0	967	PASS
174	95	50	100	83.6	94552	PASS
175	174	5	9	7.4	6986	PASS
176	174	95	101	96.3	91027	PASS
177	176	5	9	6.7	6144	PASS